

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031466.D
 Acq On : 08 Jun 2023 22:53
 Operator : SY/MD
 Sample : 03106-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FD6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031466.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	95	rVB	115677	127365	12.24%	1.507%
2	1.532	147	153	165	rVB	114949	134166	12.90%	1.587%
3	2.063	309	318	333	rBV2	237921	358022	34.42%	4.235%
4	2.391	416	420	423	rBV5	473	369	0.04%	0.004%
5	2.610	484	488	490	rBV2	394	294	0.03%	0.003%
6	2.706	510	518	527	rVB8	1879	3385	0.33%	0.040%
7	2.745	527	530	531	rBV	643	317	0.03%	0.004%
8	2.780	539	541	543	rBV3	411	184	0.02%	0.002%
9	2.835	555	558	560	rBV	305	205	0.02%	0.002%
10	2.857	563	565	569	rVB2	332	176	0.02%	0.002%
11	2.928	584	587	589	rBV	378	278	0.03%	0.003%
12	3.192	667	669	673	rVB3	334	219	0.02%	0.003%
13	3.237	680	683	688	rVB3	686	594	0.06%	0.007%
14	3.272	690	694	695	rBV2	236	165	0.02%	0.002%
15	3.343	711	716	717	rBV2	303	200	0.02%	0.002%
16	3.381	725	728	733	rVB3	301	218	0.02%	0.003%
17	3.410	735	737	741	rVB	252	163	0.02%	0.002%
18	3.439	741	746	747	rBV	268	181	0.02%	0.002%
19	3.519	768	771	774	rBV2	291	207	0.02%	0.002%
20	3.581	786	790	791	rBV2	303	193	0.02%	0.002%
21	3.706	825	829	833	rVB3	323	347	0.03%	0.004%
22	3.799	848	858	884	rBV	81901	265500	25.52%	3.141%
23	4.256	986	1000	1026	rBV2	170398	443203	42.61%	5.243%
24	4.706	1138	1140	1142	rBV3	446	238	0.02%	0.003%
25	4.777	1159	1162	1167	rBV	556	390	0.04%	0.005%
26	4.799	1167	1169	1173	rVV2	389	217	0.02%	0.003%
27	4.831	1176	1179	1182	rVV2	386	286	0.03%	0.003%
28	4.963	1202	1220	1244	rBV2	389371	1040250	100.00%	12.306%
29	5.243	1304	1307	1310	rVB4	678	432	0.04%	0.005%
30	5.275	1314	1317	1320	rBV2	502	431	0.04%	0.005%
31	5.323	1328	1332	1334	rBV3	639	518	0.05%	0.006%
32	5.384	1348	1351	1354	rVB4	492	301	0.03%	0.004%
33	5.420	1361	1362	1368	rVB3	529	351	0.03%	0.004%
34	5.462	1372	1375	1377	rBV	514	215	0.02%	0.003%
35	5.542	1388	1400	1422	rBV	276601	579978	55.75%	6.861%
36	5.838	1477	1492	1524	rBV3	324719	703012	67.58%	8.317%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031466.D
 Acq On : 08 Jun 2023 22:53
 Operator : SY/MD
 Sample : 03106-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FD6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	5.995	1528	1541	1564	rBV	245416	509440	48.97%	6.027%
38	6.320	1640	1642	1646	rVB4	688	457	0.04%	0.005%
39	6.391	1660	1664	1670	rBV5	871	766	0.07%	0.009%
40	6.561	1706	1717	1719	rBV4	1630	1985	0.19%	0.023%
41	6.706	1760	1762	1765	rVV2	501	301	0.03%	0.004%
42	6.722	1765	1767	1769	rVB2	409	192	0.02%	0.002%
43	6.754	1775	1777	1783	rVB4	842	767	0.07%	0.009%
44	6.825	1796	1799	1801	rBV	333	208	0.02%	0.002%
45	6.918	1818	1828	1863	rBV	108220	217036	20.86%	2.568%
46	7.249	1920	1931	1956	rBV	415849	742468	71.37%	8.783%
47	7.558	2017	2027	2052	rBV	84216	155316	14.93%	1.837%
48	7.886	2121	2129	2135	rBV4	2447	3867	0.37%	0.046%
49	8.034	2165	2175	2213	rBV3	226040	514887	49.50%	6.091%
50	8.394	2284	2287	2289	rBV2	767	485	0.05%	0.006%
51	8.455	2304	2306	2309	rBV2	445	275	0.03%	0.003%
52	8.645	2363	2365	2368	rBV3	547	355	0.03%	0.004%
53	8.680	2373	2376	2380	rVB2	767	615	0.06%	0.007%
54	8.709	2382	2385	2390	rVB4	510	459	0.04%	0.005%
55	8.789	2396	2410	2438	rBV	443745	753359	72.42%	8.912%
56	9.008	2475	2478	2482	rBV4	485	333	0.03%	0.004%
57	9.153	2520	2523	2526	rVB3	372	216	0.02%	0.003%
58	9.201	2535	2538	2541	rBV3	487	283	0.03%	0.003%
59	9.223	2543	2545	2549	rVV2	604	324	0.03%	0.004%
60	9.320	2571	2575	2579	rBV3	451	356	0.03%	0.004%
61	9.342	2580	2582	2587	rVB4	567	424	0.04%	0.005%
62	9.458	2616	2618	2621	rBV2	405	313	0.03%	0.004%
63	9.516	2634	2636	2644	rBV3	469	482	0.05%	0.006%
64	9.548	2644	2646	2648	rBV2	628	362	0.03%	0.004%
65	9.693	2688	2691	2692	rBV	336	216	0.02%	0.003%
66	9.735	2702	2704	2707	rBV2	291	204	0.02%	0.002%
67	9.760	2709	2712	2714	rVB	444	233	0.02%	0.003%
68	9.802	2722	2725	2727	rBV2	497	317	0.03%	0.004%
69	9.821	2729	2731	2733	rBV	457	194	0.02%	0.002%
70	9.870	2742	2746	2747	rBV3	760	426	0.04%	0.005%
71	10.159	2823	2836	2855	rBV	291313	465193	44.72%	5.503%
72	10.336	2882	2891	2903	rBV2	5052	7908	0.76%	0.094%
73	10.481	2933	2936	2941	rVB3	666	447	0.04%	0.005%
74	10.571	2962	2964	2967	rBV3	350	214	0.02%	0.003%
75	10.657	2988	2991	2993	rBV	403	236	0.02%	0.003%
76	10.751	3018	3020	3025	rBV2	391	257	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031466.D
 Acq On : 08 Jun 2023 22:53
 Operator : SY/MD
 Sample : 03106-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FD6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.860	3051	3054	3056	rBV3	540	331	0.03%	0.004%
78	10.895	3063	3065	3068	rBV	632	378	0.04%	0.004%
79	11.133	3133	3139	3145	rVB4	619	770	0.07%	0.009%
80	11.191	3145	3157	3184	rBV	432554	687320	66.07%	8.131%
81	11.458	3238	3240	3243	rBV	435	267	0.03%	0.003%
82	11.567	3262	3274	3291	rBV	448813	713377	68.58%	8.439%
83	11.757	3332	3333	3336	rBV	620	281	0.03%	0.003%
84	11.773	3336	3338	3340	rVB	475	161	0.02%	0.002%
85	11.886	3371	3373	3377	rBV2	463	423	0.04%	0.005%
86	12.037	3413	3420	3421	rBV4	437	508	0.05%	0.006%
87	12.326	3508	3510	3516	rBV3	372	235	0.02%	0.003%
88	12.484	3557	3559	3561	rBV2	361	206	0.02%	0.002%
89	12.554	3579	3581	3586	rBV4	581	465	0.04%	0.006%
90	12.580	3586	3589	3591	rBV2	447	260	0.02%	0.003%
91	12.622	3599	3602	3603	rBV	582	294	0.03%	0.003%
92	12.789	3652	3654	3655	rBV	494	199	0.02%	0.002%
93	12.857	3672	3675	3677	rBV	341	178	0.02%	0.002%
94	13.210	3782	3785	3787	rBV3	399	254	0.02%	0.003%
95	13.458	3858	3862	3864	rVV3	710	516	0.05%	0.006%
96	13.741	3948	3950	3953	rBV2	445	157	0.02%	0.002%
97	13.931	4006	4009	4014	rBV3	657	641	0.06%	0.008%
98	14.014	4034	4035	4038	rVB	727	269	0.03%	0.003%
99	14.345	4135	4138	4139	rBV2	797	433	0.04%	0.005%
100	14.660	4233	4236	4237	rBV3	713	425	0.04%	0.005%




Sum of corrected areas: 8453094

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031466.D
Acq On : 08 Jun 2023 22:53
Operator : SY/MD
Sample : 03106-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FD6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

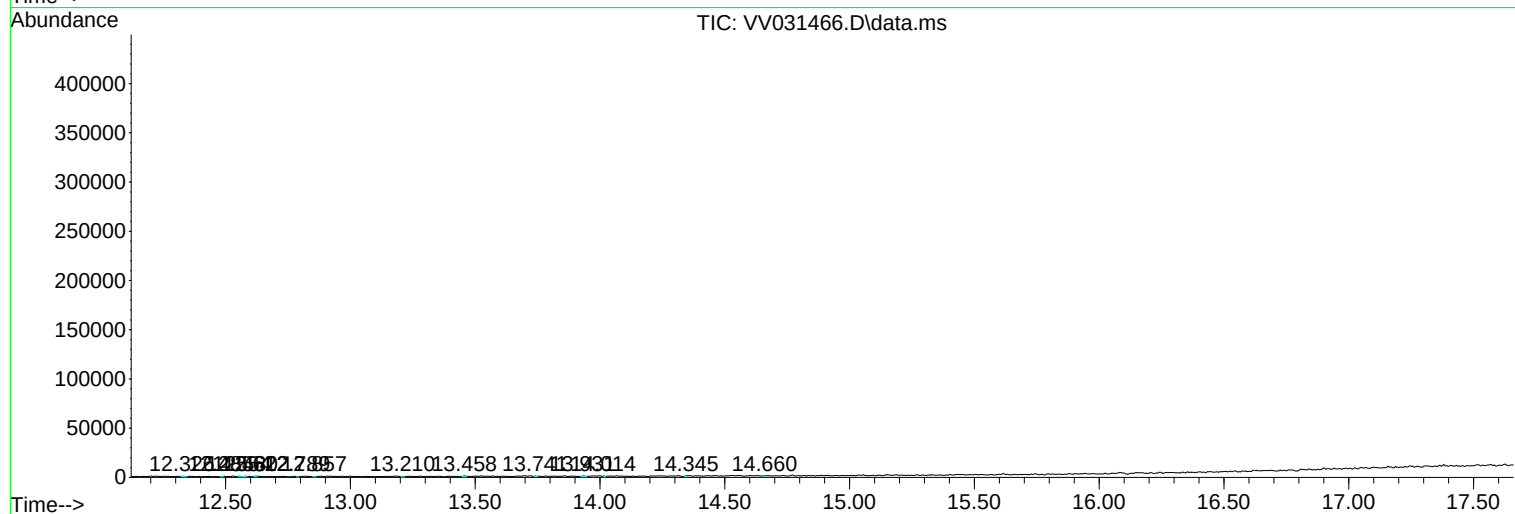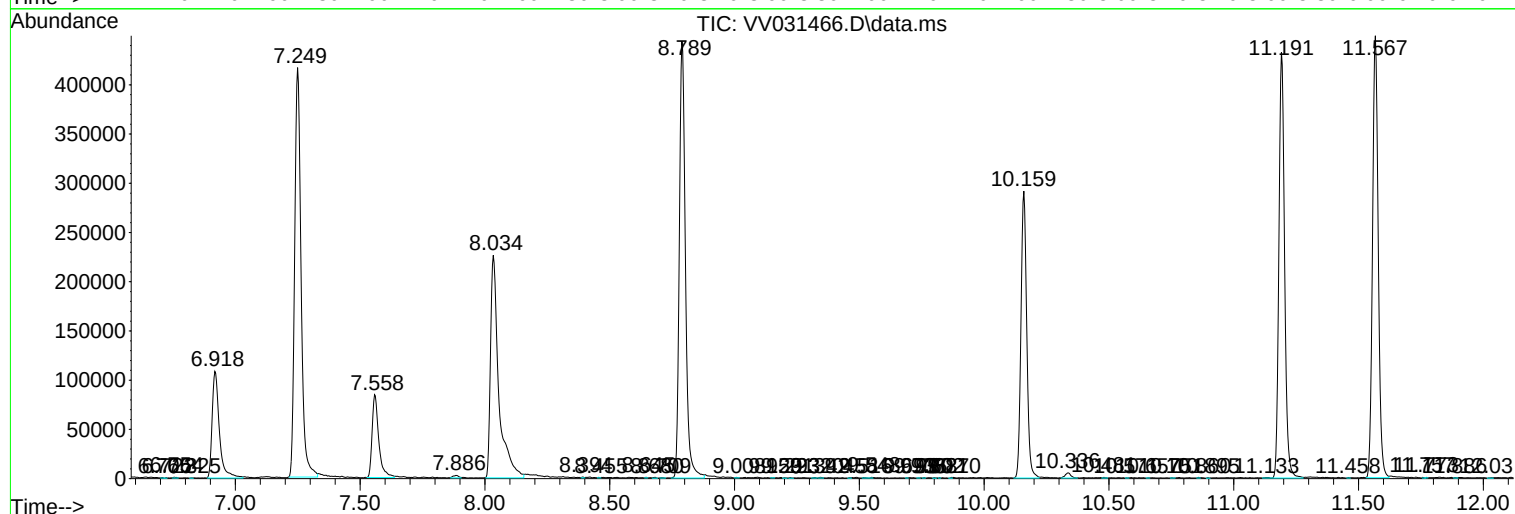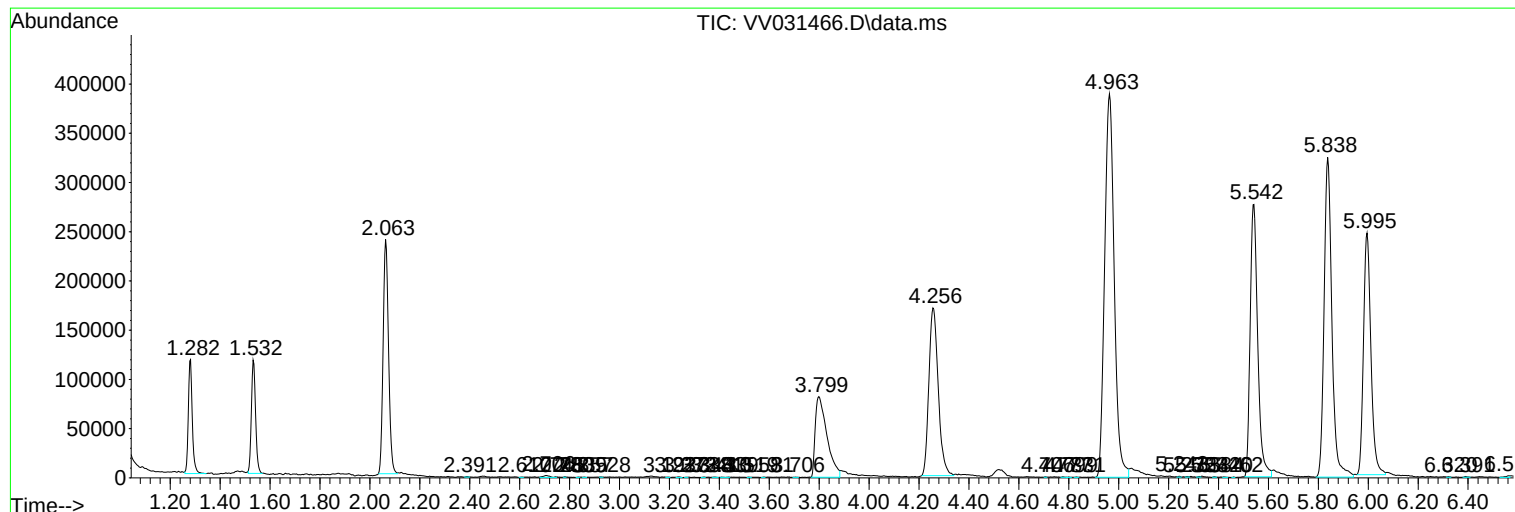

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031466.D
Acq On : 08 Jun 2023 22:53
Operator : SY/MD
Sample : 03106-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FD6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031466.D
Acq On : 08 Jun 2023 22:53
Operator : SY/MD
Sample : 03106-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FD6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------