

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031467.D
 Acq On : 08 Jun 2023 23:16
 Operator : SY/MD
 Sample : 03106-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FD8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031467.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	87	rVB	115987	127656	11.76%	1.585%
2	1.532	147	153	168	rVB	121047	144696	13.33%	1.796%
3	2.063	308	318	332	rBV	235416	346611	31.94%	4.303%
4	2.397	417	422	423	rBV3	597	433	0.04%	0.005%
5	2.423	428	430	434	rVB3	403	242	0.02%	0.003%
6	2.452	434	439	441	rBV4	941	846	0.08%	0.011%
7	2.539	462	466	467	rBV2	368	256	0.02%	0.003%
8	2.564	472	474	477	rBV2	362	202	0.02%	0.003%
9	2.603	485	486	489	rBV	489	297	0.03%	0.004%
10	2.693	511	514	516	rBV3	421	306	0.03%	0.004%
11	2.748	528	531	534	rVB2	629	326	0.03%	0.004%
12	2.860	562	566	568	rBV3	341	275	0.03%	0.003%
13	3.227	678	680	684	rBV	540	337	0.03%	0.004%
14	3.275	691	695	700	rBV3	341	346	0.03%	0.004%
15	3.365	721	723	727	rBV	265	195	0.02%	0.002%
16	3.388	727	730	732	rBV	288	206	0.02%	0.003%
17	3.609	796	799	802	rBV2	257	187	0.02%	0.002%
18	3.719	830	833	834	rBV	407	198	0.02%	0.002%
19	3.738	834	839	842	rBV3	367	411	0.04%	0.005%
20	3.796	848	857	902	rBV	82642	259000	23.86%	3.215%
21	4.256	978	1000	1027	rBV2	178499	474016	43.67%	5.885%
22	4.513	1076	1080	1084	rBV4	902	938	0.09%	0.012%
23	4.593	1103	1105	1106	rBV4	490	208	0.02%	0.003%
24	4.635	1116	1118	1121	rVB	772	369	0.03%	0.005%
25	4.654	1121	1124	1125	rBV	361	174	0.02%	0.002%
26	4.680	1129	1132	1136	rVB	397	254	0.02%	0.003%
27	4.777	1159	1162	1163	rBV	424	288	0.03%	0.004%
28	4.828	1176	1178	1184	rVV2	385	289	0.03%	0.004%
29	4.857	1184	1187	1189	rVV2	545	340	0.03%	0.004%
30	4.870	1189	1191	1193	rVB2	453	196	0.02%	0.002%
31	4.886	1193	1196	1197	rBV2	384	197	0.02%	0.002%
32	4.963	1202	1220	1245	rBV2	408521	1085345	100.00%	13.474%
33	5.249	1307	1309	1311	rVB	651	235	0.02%	0.003%
34	5.349	1338	1340	1343	rBV2	577	339	0.03%	0.004%
35	5.375	1346	1348	1351	rVV3	506	264	0.02%	0.003%
36	5.445	1366	1370	1374	rBV3	771	530	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031467.D
 Acq On : 08 Jun 2023 23:16
 Operator : SY/MD
 Sample : 03106-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FD8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	5.542	1386	1400	1417	rBV	280653	586496	54.04%	7.281%
38	5.831	1478	1490	1514	rBV6	45930	108696	10.01%	1.349%
39	5.995	1526	1541	1577	rBV	251746	541949	49.93%	6.728%
40	6.320	1641	1642	1645	rVB2	721	373	0.03%	0.005%
41	6.693	1755	1758	1760	rBV	575	313	0.03%	0.004%
42	6.731	1766	1770	1771	rBV	437	289	0.03%	0.004%
43	6.770	1779	1782	1788	rBV2	484	549	0.05%	0.007%
44	6.825	1797	1799	1801	rBV2	264	178	0.02%	0.002%
45	6.918	1817	1828	1853	rBV	115176	224159	20.65%	2.783%
46	7.104	1882	1886	1888	rBV3	1154	1041	0.10%	0.013%
47	7.249	1919	1931	1967	rBV	431785	774835	71.39%	9.619%
48	7.558	2018	2027	2055	rBV	84760	156985	14.46%	1.949%
49	7.805	2102	2104	2107	rBV3	668	386	0.04%	0.005%
50	7.886	2121	2129	2133	rBV4	1496	2133	0.20%	0.026%
51	7.966	2150	2154	2157	rBV3	435	403	0.04%	0.005%
52	8.034	2165	2175	2219	rBV2	234014	544629	50.18%	6.761%
53	8.317	2260	2263	2268	rBV4	952	704	0.06%	0.009%
54	8.497	2317	2319	2322	rVB2	431	263	0.02%	0.003%
55	8.571	2339	2342	2344	rBV	301	227	0.02%	0.003%
56	8.632	2358	2361	2364	rVB2	466	249	0.02%	0.003%
57	8.751	2395	2398	2399	rBV	391	193	0.02%	0.002%
58	8.789	2399	2410	2435	rBV	451812	757023	69.75%	9.398%
59	9.043	2485	2489	2491	rBV2	493	414	0.04%	0.005%
60	9.088	2497	2503	2508	rBV4	709	800	0.07%	0.010%
61	9.162	2520	2526	2531	rVB3	546	605	0.06%	0.008%
62	9.188	2531	2534	2539	rBV2	380	430	0.04%	0.005%
63	9.297	2567	2568	2572	rVB	432	181	0.02%	0.002%
64	9.320	2572	2575	2578	rBV2	296	250	0.02%	0.003%
65	9.358	2583	2587	2590	rBV2	390	345	0.03%	0.004%
66	9.407	2598	2602	2604	rBV	491	431	0.04%	0.005%
67	9.455	2615	2617	2622	rBV3	407	304	0.03%	0.004%
68	9.522	2634	2638	2643	rBV7	825	822	0.08%	0.010%
69	9.548	2644	2646	2650	rVB3	696	347	0.03%	0.004%
70	9.757	2707	2711	2712	rBV2	549	398	0.04%	0.005%
71	9.870	2744	2746	2748	rBV2	696	408	0.04%	0.005%
72	9.956	2770	2773	2775	rBV	401	259	0.02%	0.003%
73	10.027	2791	2795	2798	rBV2	452	306	0.03%	0.004%
74	10.111	2819	2821	2824	rBV3	294	188	0.02%	0.002%
75	10.159	2825	2836	2856	rVV	298154	472708	43.55%	5.868%
76	10.265	2866	2869	2873	rBV3	457	414	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031467.D
 Acq On : 08 Jun 2023 23:16
 Operator : SY/MD
 Sample : 03106-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FD8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.339	2884	2892	2904	rVB4	3166	5320	0.49%	0.066%
78	10.474	2929	2934	2935	rBV2	392	301	0.03%	0.004%
79	10.538	2951	2954	2957	rVB2	500	315	0.03%	0.004%
80	10.590	2966	2970	2973	rBV3	547	402	0.04%	0.005%
81	10.609	2974	2976	2979	rBV2	497	257	0.02%	0.003%
82	10.718	3008	3010	3014	rVB3	517	309	0.03%	0.004%
83	10.783	3027	3030	3032	rBV2	323	186	0.02%	0.002%
84	10.911	3067	3070	3075	rVB2	534	294	0.03%	0.004%
85	11.008	3098	3100	3102	rBV2	446	176	0.02%	0.002%
86	11.027	3103	3106	3111	rVV2	422	380	0.04%	0.005%
87	11.191	3146	3157	3176	rBV	437290	682641	62.90%	8.474%
88	11.519	3256	3259	3261	rVB2	458	191	0.02%	0.002%
89	11.567	3261	3274	3296	rBV	453165	732091	67.45%	9.088%
90	11.767	3333	3336	3338	rBV2	423	234	0.02%	0.003%
91	11.940	3388	3390	3394	rBV3	563	342	0.03%	0.004%
92	11.982	3400	3403	3405	rBV2	464	317	0.03%	0.004%
93	12.066	3426	3429	3432	rVB	432	212	0.02%	0.003%
94	12.918	3692	3694	3696	rBV	462	231	0.02%	0.003%
95	12.985	3712	3715	3717	rBV	414	328	0.03%	0.004%
96	13.017	3723	3725	3728	rVB2	705	289	0.03%	0.004%
97	13.365	3831	3833	3839	rBV3	576	474	0.04%	0.006%
98	13.869	3986	3990	3992	rBV3	668	580	0.05%	0.007%
99	13.886	3993	3995	3997	rVV2	535	236	0.02%	0.003%
100	14.400	4151	4155	4156	rBV3	740	531	0.05%	0.007%




Sum of corrected areas: 8055328

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031467.D
Acq On : 08 Jun 2023 23:16
Operator : SY/MD
Sample : 03106-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FD8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

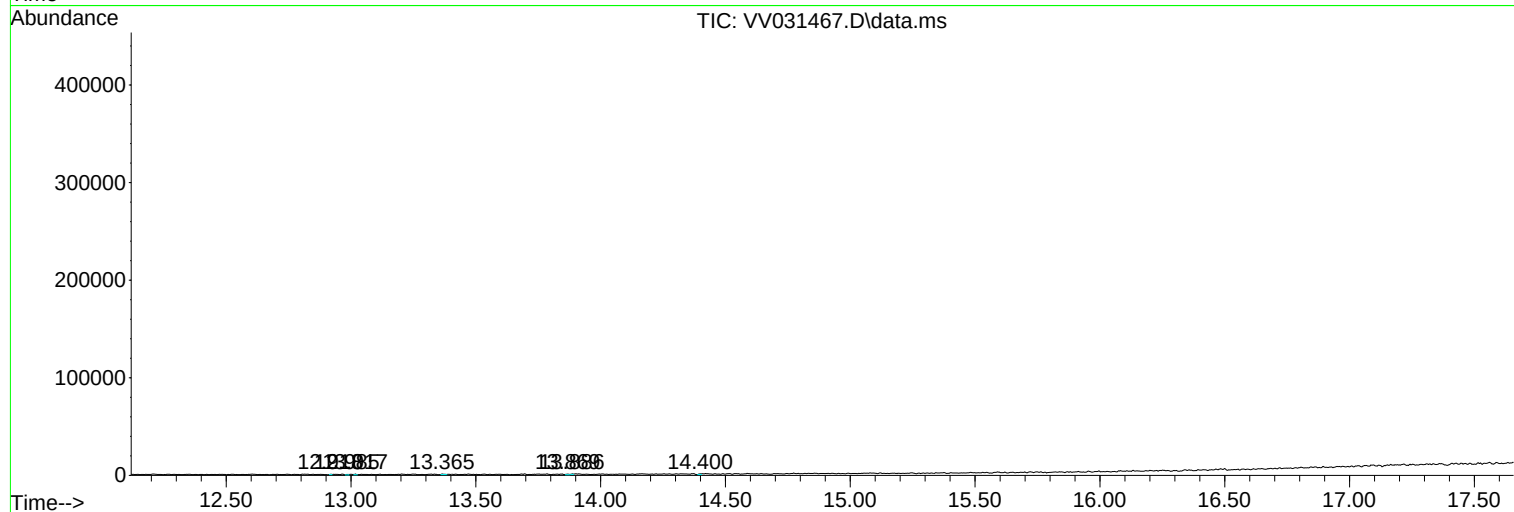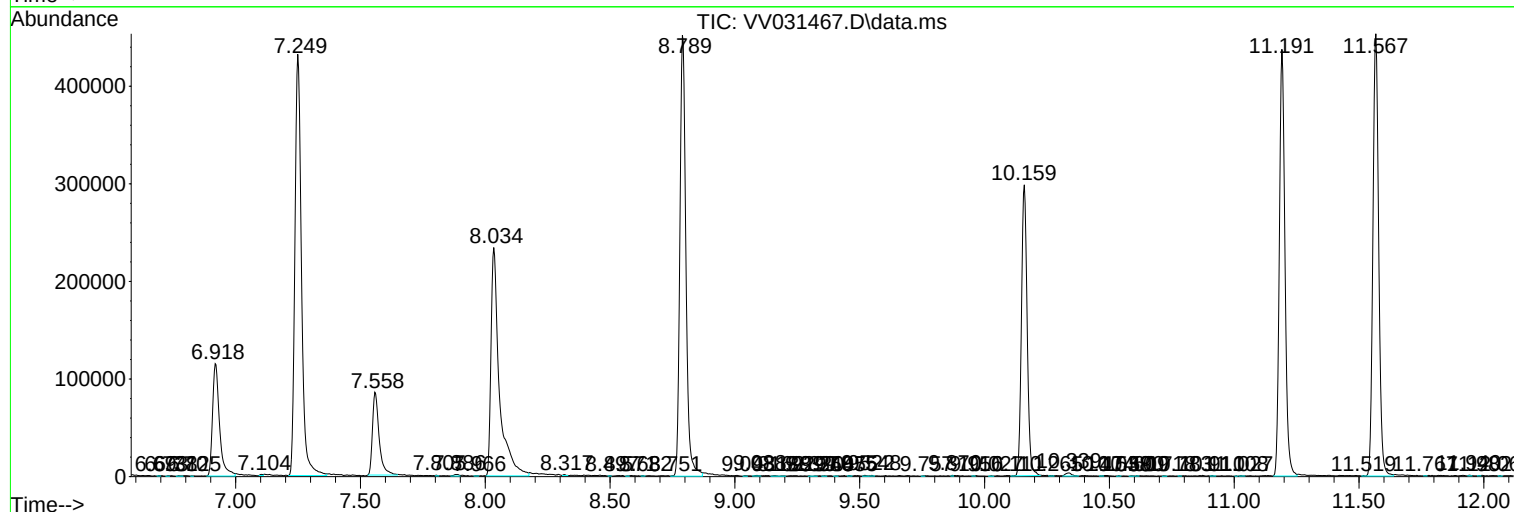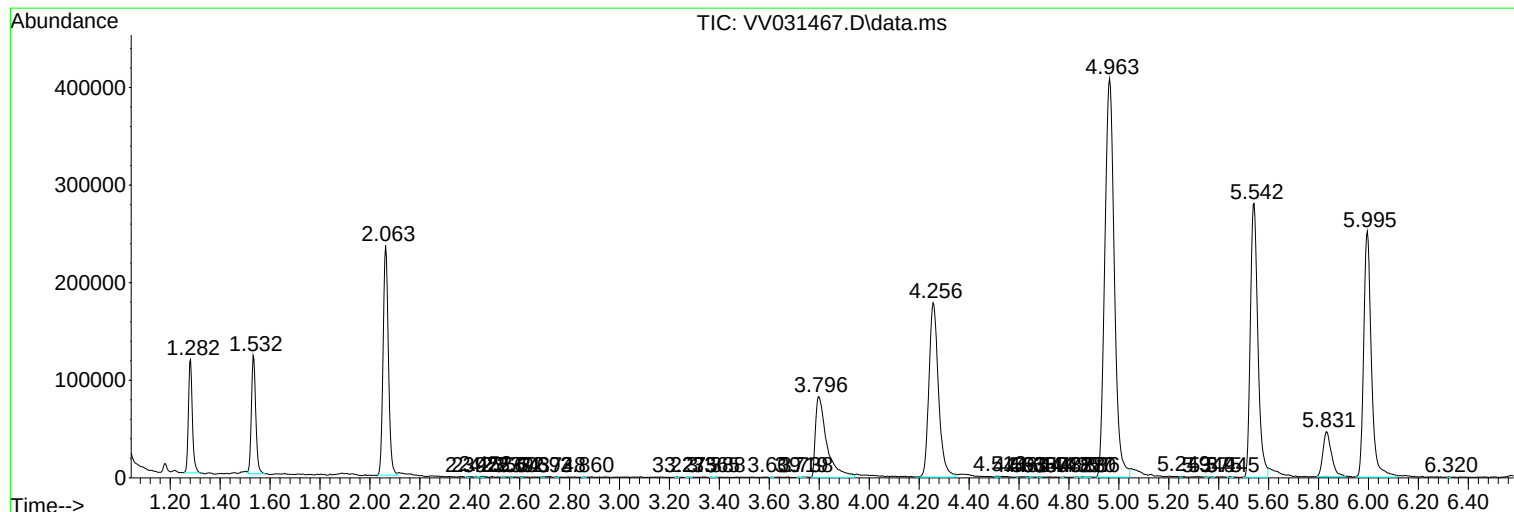

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031467.D
Acq On : 08 Jun 2023 23:16
Operator : SY/MD
Sample : 03106-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FD8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031467.D
Acq On : 08 Jun 2023 23:16
Operator : SY/MD
Sample : 03106-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FD8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
