

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031468.D
 Acq On : 08 Jun 2023 23:40
 Operator : SY/MD
 Sample : 03106-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FD9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031468.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	92	rVB	120635	132595	12.16%	1.654%
2	1.535	147	154	170	rVB	123044	147167	13.49%	1.835%
3	2.063	309	318	332	rBV	237984	345686	31.69%	4.311%
4	2.535	463	465	470	rVB	603	423	0.04%	0.005%
5	2.558	470	472	477	rBV2	493	523	0.05%	0.007%
6	2.606	484	487	488	rBV2	346	208	0.02%	0.003%
7	2.793	544	545	547	rVB	581	169	0.02%	0.002%
8	2.805	547	549	553	rVB2	304	159	0.01%	0.002%
9	2.892	573	576	579	rBV2	275	166	0.02%	0.002%
10	2.918	582	584	589	rVB3	295	239	0.02%	0.003%
11	3.082	633	635	636	rBV	244	99	0.01%	0.001%
12	3.117	643	646	649	rBV3	370	293	0.03%	0.004%
13	3.201	668	672	673	rBV2	226	193	0.02%	0.002%
14	3.240	681	684	688	rBV3	354	253	0.02%	0.003%
15	3.288	697	699	703	rVB	711	368	0.03%	0.005%
16	3.310	704	706	708	rBV	358	165	0.02%	0.002%
17	3.346	713	717	718	rBV2	289	206	0.02%	0.003%
18	3.352	718	719	721	rVB	381	88	0.01%	0.001%
19	3.384	728	729	731	rVB	267	86	0.01%	0.001%
20	3.413	736	738	741	rBV2	203	114	0.01%	0.001%
21	3.439	744	746	750	rBV	350	211	0.02%	0.003%
22	3.458	750	752	754	rVB2	258	120	0.01%	0.001%
23	3.471	754	756	757	rBV2	209	77	0.01%	0.001%
24	3.542	776	778	779	rBV2	276	124	0.01%	0.002%
25	3.638	803	808	813	rBV3	515	346	0.03%	0.004%
26	3.661	813	815	819	rVB	282	190	0.02%	0.002%
27	3.686	819	823	824	rBV	321	162	0.01%	0.002%
28	3.719	831	833	837	rBV2	168	131	0.01%	0.002%
29	3.799	846	858	886	rBV2	86599	250833	23.00%	3.128%
30	4.256	985	1000	1027	rBV2	179065	473466	43.41%	5.905%
31	4.645	1119	1121	1124	rBV4	379	274	0.03%	0.003%
32	4.793	1165	1167	1173	rBV3	208	205	0.02%	0.003%
33	4.844	1180	1183	1185	rBV2	581	314	0.03%	0.004%
34	4.963	1203	1220	1241	rBV2	414861	1090753	100.00%	13.603%
35	5.468	1374	1377	1380	rBV3	807	444	0.04%	0.006%
36	5.542	1387	1400	1419	rBV	276293	581075	53.27%	7.247%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031468.D
 Acq On : 08 Jun 2023 23:40
 Operator : SY/MD
 Sample : 03106-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FD9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	5.776	1471	1473	1475	rBV3	423	186	0.02%	0.002%
38	5.831	1478	1490	1511	rBV5	43187	100416	9.21%	1.252%
39	5.934	1519	1522	1525	rVB3	819	463	0.04%	0.006%
40	5.995	1528	1541	1560	rBV	252276	533339	48.90%	6.651%
41	6.342	1647	1649	1653	rVB3	536	296	0.03%	0.004%
42	6.362	1653	1655	1656	rBV2	264	116	0.01%	0.001%
43	6.423	1671	1674	1676	rBV	464	236	0.02%	0.003%
44	6.500	1695	1698	1703	rBV	361	238	0.02%	0.003%
45	6.526	1703	1706	1709	rBV2	493	314	0.03%	0.004%
46	6.558	1712	1716	1717	rBV2	1124	795	0.07%	0.010%
47	6.712	1762	1764	1767	rVB3	472	294	0.03%	0.004%
48	6.728	1767	1769	1772	rBV	445	200	0.02%	0.002%
49	6.854	1803	1808	1810	rBV3	331	315	0.03%	0.004%
50	6.918	1817	1828	1856	rBV	114547	223689	20.51%	2.790%
51	7.249	1920	1931	1963	rBV	430902	773476	70.91%	9.646%
52	7.558	2018	2027	2049	rBV	86716	158866	14.56%	1.981%
53	7.773	2091	2094	2098	rVB5	507	382	0.04%	0.005%
54	7.866	2120	2123	2124	rBV	559	315	0.03%	0.004%
55	7.940	2144	2146	2148	rBV2	367	153	0.01%	0.002%
56	7.989	2157	2161	2162	rBV2	467	259	0.02%	0.003%
57	8.034	2165	2175	2210	rBV2	238799	555331	50.91%	6.926%
58	8.583	2344	2346	2348	rBV3	721	392	0.04%	0.005%
59	8.686	2376	2378	2380	rBV2	441	226	0.02%	0.003%
60	8.738	2391	2394	2395	rBV	338	164	0.02%	0.002%
61	8.789	2398	2410	2438	rBV	440270	755411	69.26%	9.421%
62	9.088	2500	2503	2506	rBV2	932	627	0.06%	0.008%
63	9.201	2536	2538	2541	rBV2	487	232	0.02%	0.003%
64	9.384	2591	2595	2599	rBV3	556	457	0.04%	0.006%
65	9.423	2604	2607	2610	rBV3	448	330	0.03%	0.004%
66	9.461	2615	2619	2623	rBV2	467	401	0.04%	0.005%
67	9.484	2623	2626	2627	rBV2	310	165	0.02%	0.002%
68	9.496	2627	2630	2633	rBV2	674	469	0.04%	0.006%
69	9.625	2668	2670	2672	rBV2	390	151	0.01%	0.002%
70	9.718	2695	2699	2704	rBV4	406	446	0.04%	0.006%
71	9.815	2726	2729	2731	rBV2	481	262	0.02%	0.003%
72	9.828	2731	2733	2735	rBV	365	226	0.02%	0.003%
73	10.008	2787	2789	2792	rBV2	274	216	0.02%	0.003%
74	10.053	2801	2803	2809	rVB2	385	354	0.03%	0.004%
75	10.078	2809	2811	2813	rBV2	192	96	0.01%	0.001%
76	10.159	2824	2836	2855	rBV	295689	479332	43.95%	5.978%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031468.D
 Acq On : 08 Jun 2023 23:40
 Operator : SY/MD
 Sample : 03106-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FD9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.387	2905	2907	2911	rVB2	441	216	0.02%	0.003%
78	10.413	2914	2915	2916	rBV2	306	87	0.01%	0.001%
79	10.509	2942	2945	2947	rBV	340	230	0.02%	0.003%
80	10.628	2979	2982	2984	rBV	368	214	0.02%	0.003%
81	10.686	2999	3000	3003	rBV2	341	164	0.02%	0.002%
82	10.712	3006	3008	3012	rVV3	529	272	0.02%	0.003%
83	10.844	3047	3049	3051	rBV	320	125	0.01%	0.002%
84	10.863	3053	3055	3057	rBV2	320	174	0.02%	0.002%
85	10.908	3067	3069	3070	rBV	277	105	0.01%	0.001%
86	11.017	3101	3103	3107	rBV2	359	281	0.03%	0.004%
87	11.107	3129	3131	3135	rBV2	317	284	0.03%	0.004%
88	11.191	3146	3157	3177	rBV	417457	656453	60.18%	8.187%
89	11.349	3204	3206	3208	rBV2	532	258	0.02%	0.003%
90	11.567	3262	3274	3292	rBV	467634	739098	67.76%	9.218%
91	11.873	3367	3369	3371	rBV	552	248	0.02%	0.003%
92	12.323	3506	3509	3511	rBV3	502	249	0.02%	0.003%
93	12.567	3584	3585	3586	rBV3	302	79	0.01%	0.001%
94	12.599	3592	3595	3602	rVB3	709	636	0.06%	0.008%
95	12.641	3602	3608	3609	rBV2	476	376	0.03%	0.005%
96	12.815	3660	3662	3664	rVB	350	122	0.01%	0.002%
97	12.905	3688	3690	3692	rBV	336	155	0.01%	0.002%
98	13.030	3727	3729	3734	rBV2	426	306	0.03%	0.004%
99	13.078	3741	3744	3745	rBV2	453	191	0.02%	0.002%
100	14.040	4041	4043	4047	rVB5	971	493	0.05%	0.006%




Sum of corrected areas: 8018377

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031468.D
Acq On : 08 Jun 2023 23:40
Operator : SY/MD
Sample : 03106-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

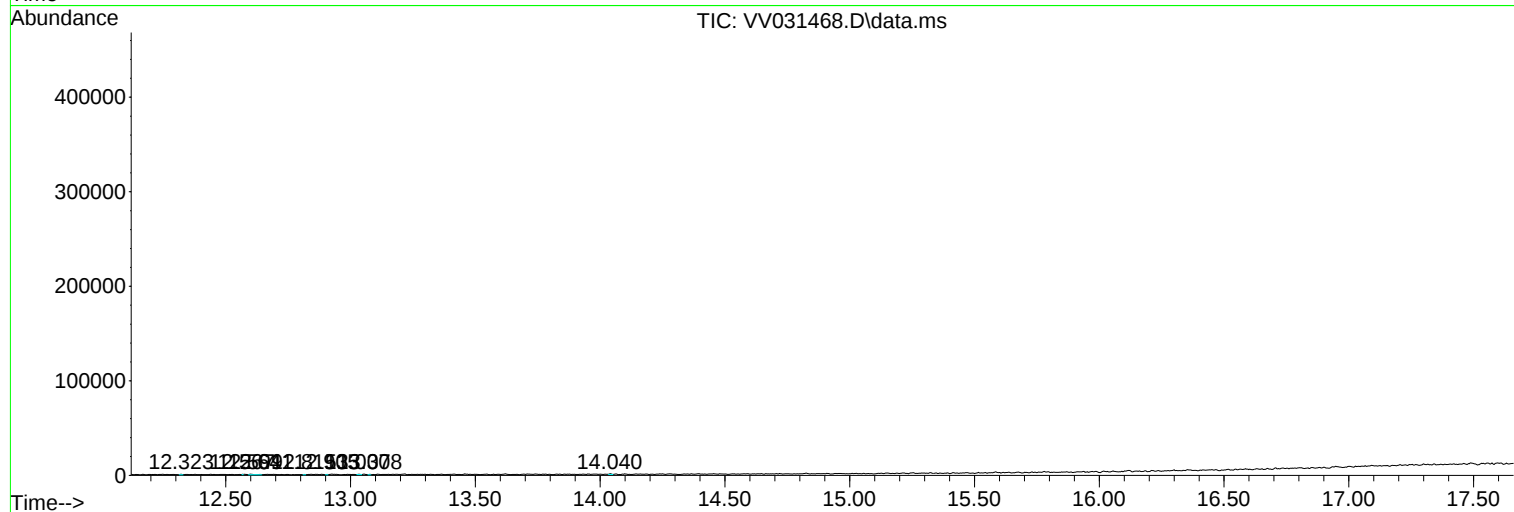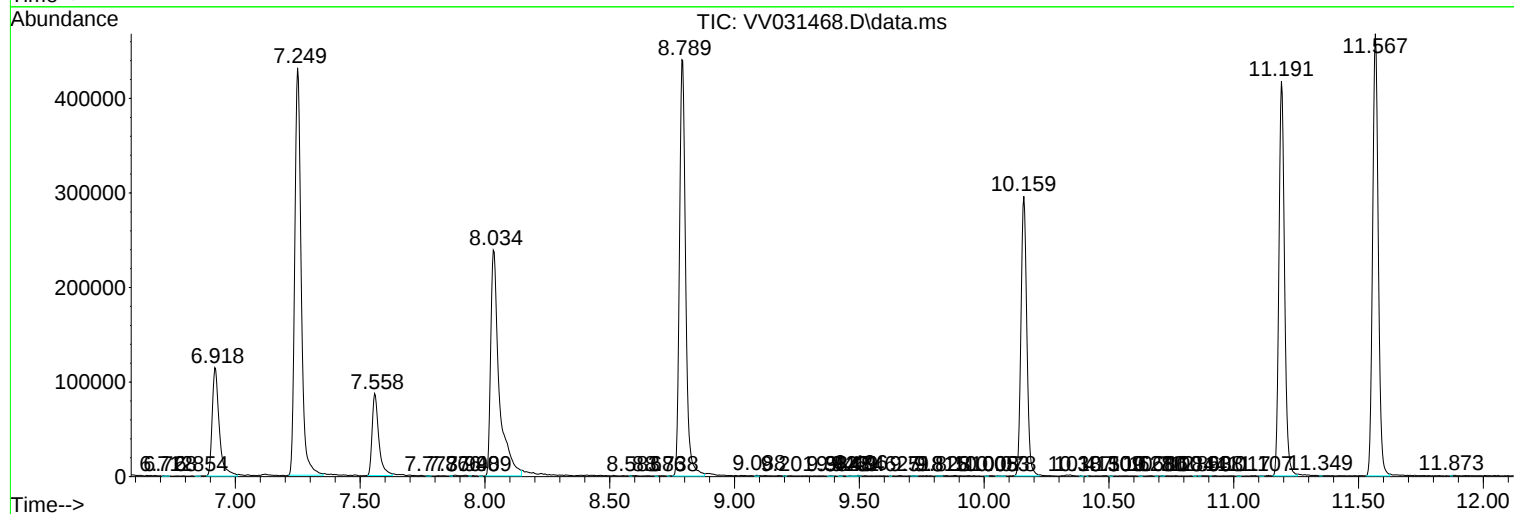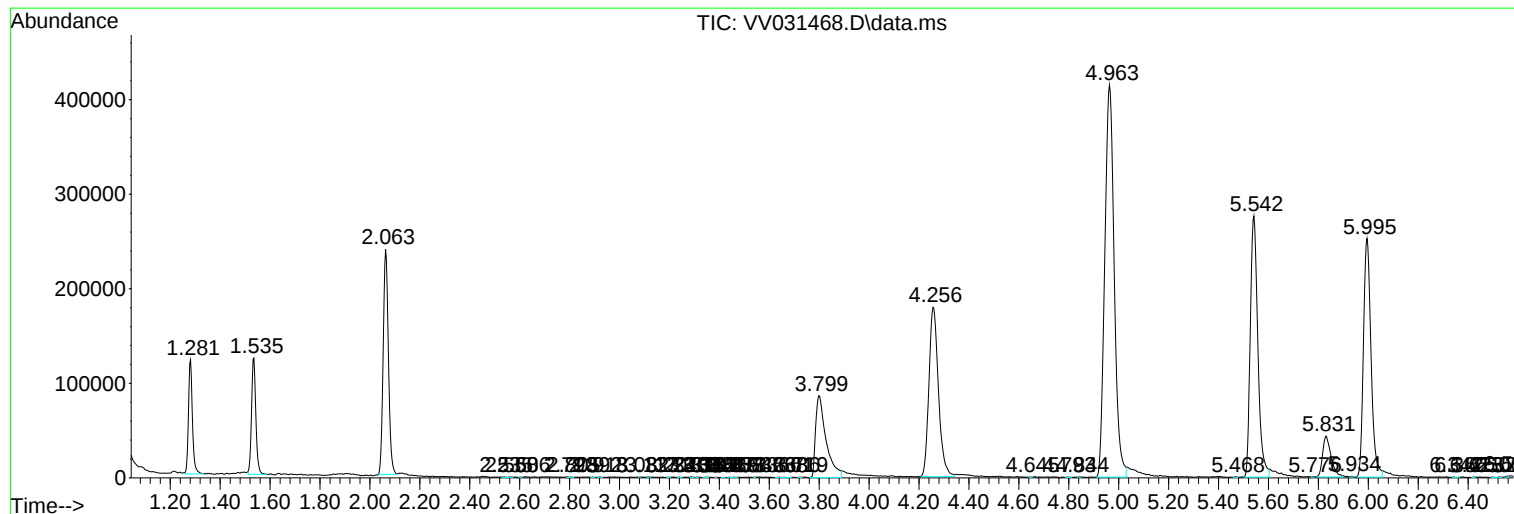

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031468.D
Acq On : 08 Jun 2023 23:40
Operator : SY/MD
Sample : 03106-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031468.D
Acq On : 08 Jun 2023 23:40
Operator : SY/MD
Sample : 03106-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc