

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031470.D
 Acq On : 09 Jun 2023 00:28
 Operator : SY/MD
 Sample : 03106-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FE2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031470.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	112314	122007	11.74%	1.473%
2	1.532	146	153	166	rVB	119376	138319	13.31%	1.670%
3	2.063	307	318	332	rBV2	232734	362316	34.86%	4.374%
4	2.359	407	410	413	rBV3	468	382	0.04%	0.005%
5	2.539	465	466	467	rBV3	234	78	0.01%	0.001%
6	2.600	483	485	488	rVB3	521	270	0.03%	0.003%
7	2.667	502	506	508	rBV2	723	410	0.04%	0.005%
8	2.741	528	529	530	rBV2	212	69	0.01%	0.001%
9	2.751	530	532	534	rVB2	518	187	0.02%	0.002%
10	2.854	561	564	569	rBV	334	307	0.03%	0.004%
11	2.928	584	587	589	rBV2	375	251	0.02%	0.003%
12	3.082	633	635	640	rBV3	552	407	0.04%	0.005%
13	3.371	719	725	726	rBV3	264	243	0.02%	0.003%
14	3.420	736	740	745	rBV3	310	325	0.03%	0.004%
15	3.442	745	747	751	rBV3	184	93	0.01%	0.001%
16	3.465	751	754	756	rBV2	312	221	0.02%	0.003%
17	3.571	785	787	790	rBV	137	88	0.01%	0.001%
18	3.603	794	797	801	rBV2	288	235	0.02%	0.003%
19	3.641	806	809	811	rBV	286	219	0.02%	0.003%
20	3.654	811	813	815	rBV2	221	120	0.01%	0.001%
21	3.686	821	823	827	rVB2	425	217	0.02%	0.003%
22	3.731	834	837	841	rVB2	436	366	0.04%	0.004%
23	3.757	841	845	846	rBV	268	165	0.02%	0.002%
24	3.796	847	857	888	rBV	78236	242163	23.30%	2.923%
25	4.256	986	1000	1025	rBV	173585	450139	43.31%	5.434%
26	4.670	1127	1129	1131	rBV2	593	288	0.03%	0.003%
27	4.719	1142	1144	1146	rBV	347	103	0.01%	0.001%
28	4.963	1203	1220	1246	rBV2	387326	1039295	100.00%	12.546%
29	5.400	1353	1356	1361	rBV4	645	565	0.05%	0.007%
30	5.474	1376	1379	1380	rBV2	347	199	0.02%	0.002%
31	5.542	1386	1400	1427	rBV	263551	557491	53.64%	6.730%
32	5.838	1477	1492	1527	rBV3	372436	806048	77.56%	9.730%
33	5.995	1529	1541	1573	rVB2	244539	514991	49.55%	6.217%
34	6.256	1620	1622	1627	rVB3	691	289	0.03%	0.003%
35	6.281	1627	1630	1631	rVB	458	210	0.02%	0.003%
36	6.329	1643	1645	1647	rBV2	456	207	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031470.D
 Acq On : 09 Jun 2023 00:28
 Operator : SY/MD
 Sample : 03106-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FE2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	6.432	1675	1677	1679	rBV	549	277	0.03%	0.003%
38	6.670	1749	1751	1752	rBV2	297	156	0.02%	0.002%
39	6.747	1773	1775	1780	rBV3	478	292	0.03%	0.004%
40	6.802	1791	1792	1797	rVB2	459	292	0.03%	0.004%
41	6.918	1816	1828	1850	rBV	109297	213855	20.58%	2.582%
42	7.249	1920	1931	1965	rBV	402460	713536	68.66%	8.614%
43	7.558	2017	2027	2049	rBV2	81382	151662	14.59%	1.831%
44	7.831	2109	2112	2113	rBV	389	172	0.02%	0.002%
45	7.876	2123	2126	2129	rBV4	1313	939	0.09%	0.011%
46	8.034	2165	2175	2213	rBV2	213571	497459	47.87%	6.005%
47	8.484	2311	2315	2321	rBV4	466	522	0.05%	0.006%
48	8.590	2346	2348	2350	rBV3	485	275	0.03%	0.003%
49	8.635	2360	2362	2363	rBV	253	123	0.01%	0.001%
50	8.741	2391	2395	2398	rBV3	277	232	0.02%	0.003%
51	8.789	2398	2410	2436	rBV	418860	704011	67.74%	8.499%
52	9.030	2483	2485	2487	rBV	485	186	0.02%	0.002%
53	9.136	2514	2518	2521	rVB5	642	453	0.04%	0.005%
54	9.297	2564	2568	2569	rBV	460	313	0.03%	0.004%
55	9.429	2604	2609	2612	rBV2	437	494	0.05%	0.006%
56	9.455	2615	2617	2619	rVB	460	152	0.01%	0.002%
57	9.535	2640	2642	2644	rVB	560	196	0.02%	0.002%
58	9.593	2659	2660	2663	rBV	295	139	0.01%	0.002%
59	9.664	2679	2682	2684	rBV2	299	185	0.02%	0.002%
60	9.699	2691	2693	2695	rBV	173	96	0.01%	0.001%
61	9.751	2706	2709	2710	rBV	627	238	0.02%	0.003%
62	9.915	2758	2760	2763	rVB3	535	310	0.03%	0.004%
63	9.992	2782	2784	2786	rBV	478	225	0.02%	0.003%
64	10.030	2792	2796	2797	rBV	408	290	0.03%	0.004%
65	10.078	2810	2811	2812	rBV	115	26	0.00%	0.000%
66	10.159	2825	2836	2861	rBV	284268	457508	44.02%	5.523%
67	10.339	2886	2892	2895	rBV4	1385	1566	0.15%	0.019%
68	10.400	2909	2911	2916	rVB3	538	422	0.04%	0.005%
69	10.429	2917	2920	2923	rBV	380	270	0.03%	0.003%
70	10.451	2925	2927	2929	rBV2	449	256	0.02%	0.003%
71	10.635	2980	2984	2986	rBV	471	310	0.03%	0.004%
72	10.677	2994	2997	2999	rBV2	404	281	0.03%	0.003%
73	10.744	3013	3018	3022	rBV3	367	416	0.04%	0.005%
74	10.950	3079	3082	3088	rBV2	444	467	0.04%	0.006%
75	10.979	3088	3091	3095	rVB3	379	251	0.02%	0.003%
76	11.024	3104	3105	3107	rBV2	182	58	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031470.D
 Acq On : 09 Jun 2023 00:28
 Operator : SY/MD
 Sample : 03106-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FE2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	11.140	3135	3141	3144	rBV3	740	745	0.07%	0.009%
78	11.191	3146	3157	3183	rVV	390472	619031	59.56%	7.473%
79	11.567	3262	3274	3293	rBV	417601	672301	64.69%	8.116%
80	11.905	3378	3379	3384	rVB3	452	272	0.03%	0.003%
81	12.159	3455	3458	3459	rBV	525	250	0.02%	0.003%
82	12.329	3509	3511	3515	rBV2	379	287	0.03%	0.003%
83	12.361	3519	3521	3525	rBV3	574	446	0.04%	0.005%
84	12.564	3580	3584	3585	rBV2	439	329	0.03%	0.004%
85	12.593	3591	3593	3595	rBV	397	205	0.02%	0.002%
86	12.947	3701	3703	3705	rBV2	370	149	0.01%	0.002%
87	13.072	3738	3742	3744	rBV2	307	275	0.03%	0.003%
88	13.114	3753	3755	3757	rBV	424	213	0.02%	0.003%
89	13.262	3799	3801	3803	rBV	457	196	0.02%	0.002%
90	13.647	3917	3921	3924	rBV4	488	375	0.04%	0.005%
91	13.699	3934	3937	3938	rBV2	728	300	0.03%	0.004%
92	13.805	3968	3970	3972	rBV	561	284	0.03%	0.003%




Sum of corrected areas: 8283852

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031470.D
Acq On : 09 Jun 2023 00:28
Operator : SY/MD
Sample : 03106-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FE2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

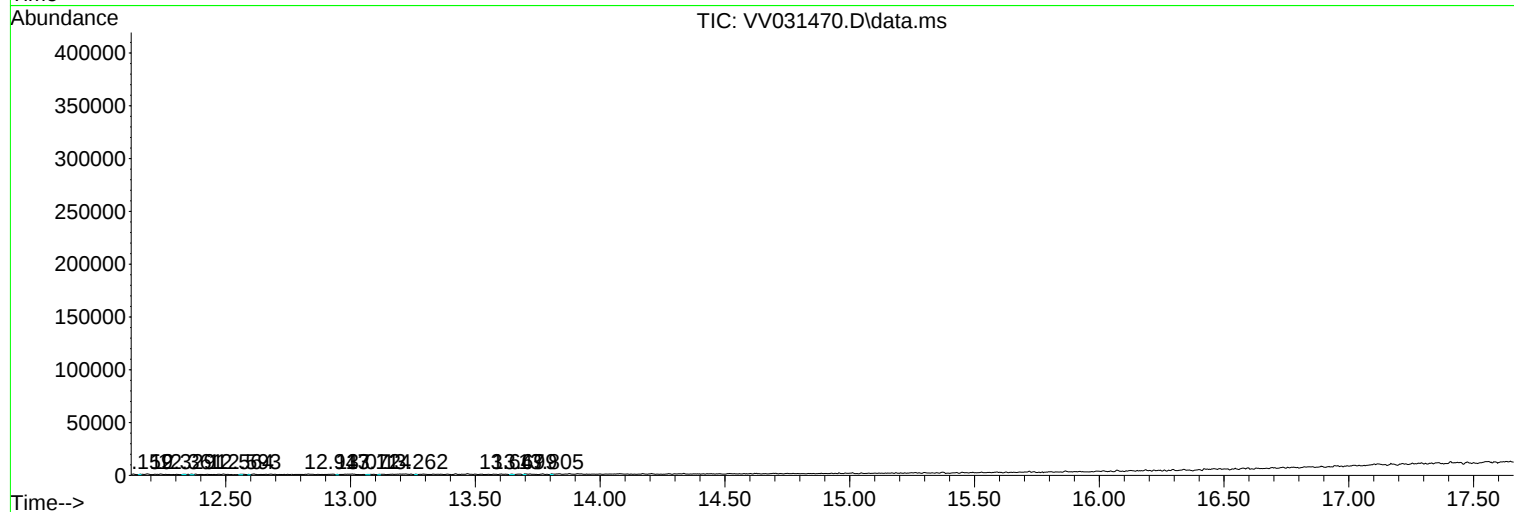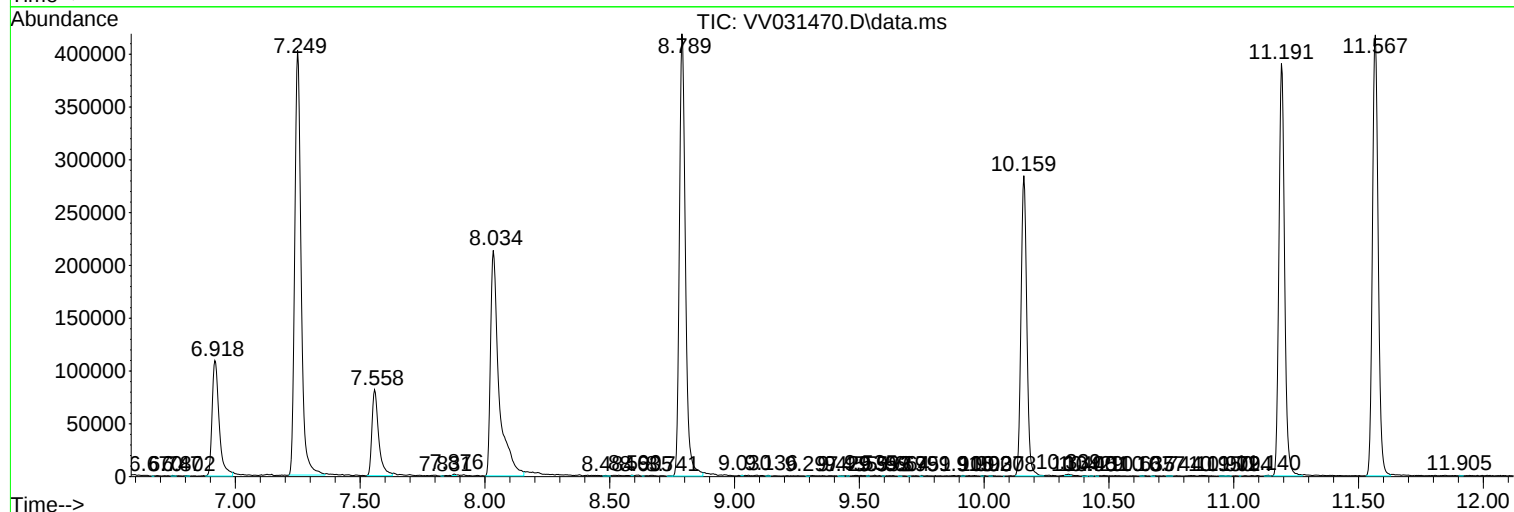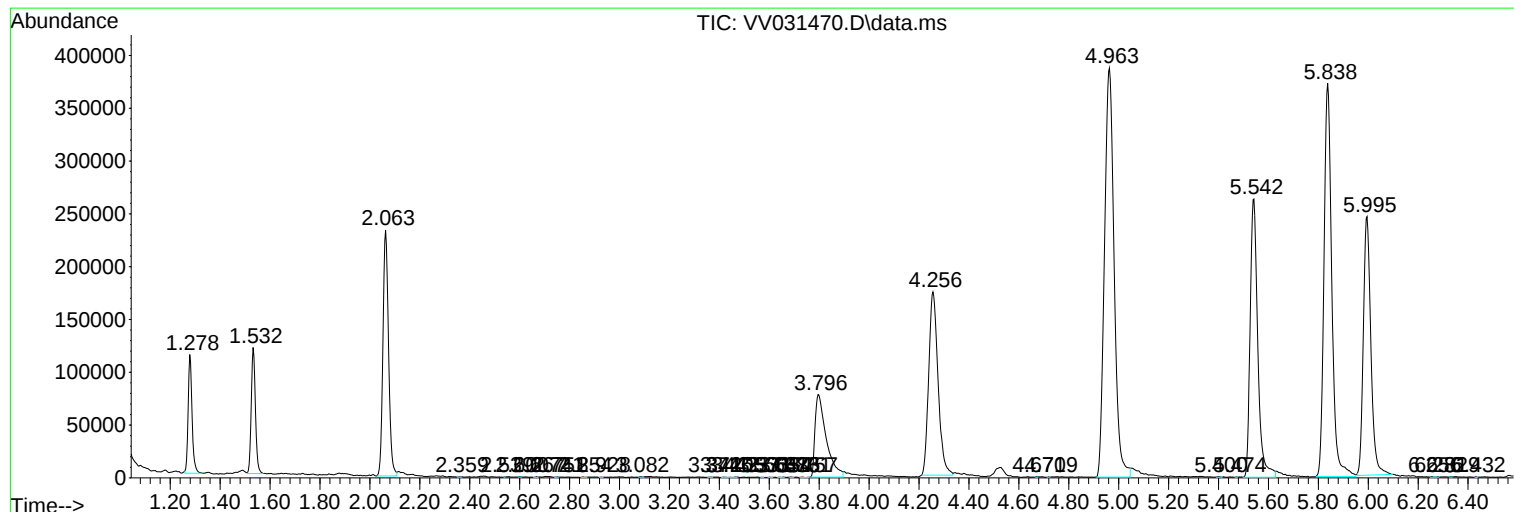

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031470.D
Acq On : 09 Jun 2023 00:28
Operator : SY/MD
Sample : 03106-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FE2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031470.D
Acq On : 09 Jun 2023 00:28
Operator : SY/MD
Sample : 03106-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FE2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------