

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031471.D
 Acq On : 09 Jun 2023 00:51
 Operator : SY/MD
 Sample : 03106-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FE4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031471.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	114107	125968	12.25%	1.678%
2	1.532	146	153	164	rVB	117015	134384	13.07%	1.790%
3	2.063	308	318	332	rBV	225838	329528	32.04%	4.390%
4	2.397	419	422	423	rBV	360	234	0.02%	0.003%
5	2.474	443	446	448	rBV	445	238	0.02%	0.003%
6	2.523	459	461	463	rBV2	268	82	0.01%	0.001%
7	2.616	487	490	492	rBV2	473	232	0.02%	0.003%
8	2.748	529	531	534	rVB2	385	183	0.02%	0.002%
9	2.809	548	550	552	rBV3	297	133	0.01%	0.002%
10	2.831	556	557	561	rBV2	337	206	0.02%	0.003%
11	2.892	570	576	577	rBV2	594	631	0.06%	0.008%
12	3.005	610	611	614	rBV	456	259	0.03%	0.003%
13	3.105	638	642	644	rBV3	642	458	0.04%	0.006%
14	3.156	655	658	662	rBV3	275	194	0.02%	0.003%
15	3.188	665	668	669	rBV	314	178	0.02%	0.002%
16	3.310	704	706	707	rBV	386	159	0.02%	0.002%
17	3.397	730	733	734	rBV2	267	129	0.01%	0.002%
18	3.420	737	740	743	rVB2	370	183	0.02%	0.002%
19	3.516	768	770	772	rBV	185	83	0.01%	0.001%
20	3.568	784	786	788	rBV	150	68	0.01%	0.001%
21	3.593	792	794	801	rVB2	550	419	0.04%	0.006%
22	3.651	810	812	815	rBV	290	125	0.01%	0.002%
23	3.706	827	829	831	rBV	243	123	0.01%	0.002%
24	3.722	832	834	838	rVB2	476	283	0.03%	0.004%
25	3.741	838	840	841	rBV2	321	95	0.01%	0.001%
26	3.796	848	857	890	rBV2	77285	229686	22.33%	3.060%
27	4.256	985	1000	1026	rBV	172221	440445	42.83%	5.867%
28	4.523	1079	1083	1087	rBV3	695	754	0.07%	0.010%
29	4.561	1093	1095	1096	rBV	690	211	0.02%	0.003%
30	4.616	1110	1112	1114	rVB2	414	161	0.02%	0.002%
31	4.632	1114	1117	1121	rBV3	574	413	0.04%	0.006%
32	4.735	1146	1149	1152	rBV2	414	334	0.03%	0.004%
33	4.748	1152	1153	1157	rVV2	643	263	0.03%	0.004%
34	4.809	1169	1172	1175	rVB3	327	208	0.02%	0.003%
35	4.822	1175	1176	1180	rBV2	404	191	0.02%	0.003%
36	4.851	1180	1185	1188	rVB4	525	412	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031471.D
 Acq On : 09 Jun 2023 00:51
 Operator : SY/MD
 Sample : 03106-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FE4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	4.863	1188	1189	1190	rBV4	354	130	0.01%	0.002%
38	4.963	1203	1220	1247	rBV2	384552	1028456	100.00%	13.700%
39	5.304	1323	1326	1328	rVB2	415	266	0.03%	0.004%
40	5.378	1347	1349	1352	rVB2	397	163	0.02%	0.002%
41	5.413	1355	1360	1364	rVB4	711	720	0.07%	0.010%
42	5.442	1364	1369	1370	rBV	547	347	0.03%	0.005%
43	5.539	1387	1399	1419	rBV	259923	544942	52.99%	7.259%
44	5.828	1478	1489	1511	rBV2	31569	70965	6.90%	0.945%
45	5.995	1527	1541	1563	rBV	239565	504354	49.04%	6.718%
46	6.252	1618	1621	1624	rBV2	723	430	0.04%	0.006%
47	6.269	1624	1626	1631	rVB3	575	357	0.03%	0.005%
48	6.404	1666	1668	1674	rVB3	479	375	0.04%	0.005%
49	6.436	1675	1678	1680	rBV2	445	213	0.02%	0.003%
50	6.568	1711	1719	1720	rBV4	1840	1691	0.16%	0.023%
51	6.693	1756	1758	1760	rVB2	484	221	0.02%	0.003%
52	6.709	1760	1763	1766	rVB3	342	178	0.02%	0.002%
53	6.738	1768	1772	1774	rBV2	423	267	0.03%	0.004%
54	6.805	1791	1793	1794	rVB2	257	72	0.01%	0.001%
55	6.850	1805	1807	1809	rVB	198	64	0.01%	0.001%
56	6.860	1809	1810	1812	rBV	282	120	0.01%	0.002%
57	6.918	1817	1828	1849	rBV	109554	206697	20.10%	2.753%
58	7.175	1906	1908	1910	rBV3	837	367	0.04%	0.005%
59	7.249	1919	1931	1957	rBV	400712	721357	70.14%	9.609%
60	7.503	2009	2010	2013	rBV3	374	159	0.02%	0.002%
61	7.558	2017	2027	2048	rBV	78990	148588	14.45%	1.979%
62	7.802	2101	2103	2107	rVB3	391	292	0.03%	0.004%
63	7.822	2107	2109	2111	rBV2	381	134	0.01%	0.002%
64	7.915	2134	2138	2141	rBV3	727	614	0.06%	0.008%
65	8.034	2165	2175	2205	rBV2	219436	491617	47.80%	6.549%
66	8.551	2334	2336	2340	rBV3	517	366	0.04%	0.005%
67	8.789	2396	2410	2438	rBV	418362	710140	69.05%	9.460%
68	9.124	2510	2514	2517	rBV2	549	451	0.04%	0.006%
69	9.153	2522	2523	2525	rVB2	411	155	0.02%	0.002%
70	9.256	2550	2555	2557	rBV2	584	460	0.04%	0.006%
71	9.275	2558	2561	2564	rBV3	620	433	0.04%	0.006%
72	9.336	2578	2580	2581	rBV	288	121	0.01%	0.002%
73	9.384	2592	2595	2598	rBB2	492	401	0.04%	0.005%
74	9.429	2606	2609	2613	rBV2	561	448	0.04%	0.006%
75	9.625	2668	2670	2673	rBV2	153	101	0.01%	0.001%
76	9.712	2693	2697	2699	rVB2	401	249	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031471.D
 Acq On : 09 Jun 2023 00:51
 Operator : SY/MD
 Sample : 03106-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FE4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	9.751	2707	2709	2710	rBV2	395	174	0.02%	0.002%
78	9.828	2731	2733	2734	rBV2	319	74	0.01%	0.001%
79	9.870	2743	2746	2748	rBV2	547	409	0.04%	0.005%
80	9.915	2758	2760	2765	rBB2	442	236	0.02%	0.003%
81	9.960	2772	2774	2777	rVB2	539	196	0.02%	0.003%
82	10.014	2789	2791	2792	rBV2	248	120	0.01%	0.002%
83	10.082	2807	2812	2814	rBV2	441	346	0.03%	0.005%
84	10.159	2824	2836	2853	rBV	288380	460711	44.80%	6.137%
85	10.680	2994	2998	3002	rBV2	678	524	0.05%	0.007%
86	10.854	3049	3052	3053	rBV	505	305	0.03%	0.004%
87	10.953	3079	3083	3089	rBV4	552	673	0.07%	0.009%
88	10.985	3090	3093	3094	rBV	516	247	0.02%	0.003%
89	11.191	3146	3157	3176	rBV	399064	639615	62.19%	8.520%
90	11.567	3262	3274	3292	rBV	438270	695079	67.58%	9.259%
91	11.738	3324	3327	3329	rBV2	906	468	0.05%	0.006%
92	12.368	3520	3523	3525	rBV2	571	237	0.02%	0.003%
93	12.538	3573	3576	3578	rBV2	377	241	0.02%	0.003%
94	12.841	3668	3670	3673	rBV3	546	403	0.04%	0.005%
95	13.008	3720	3722	3725	rVB	505	195	0.02%	0.003%
96	13.169	3769	3772	3775	rBV3	473	380	0.04%	0.005%
97	13.635	3915	3917	3920	rBV2	601	315	0.03%	0.004%
98	14.152	4076	4078	4079	rBV2	753	339	0.03%	0.005%
99	14.625	4223	4225	4228	rBV3	1041	557	0.05%	0.007%




Sum of corrected areas: 7506978

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031471.D
Acq On : 09 Jun 2023 00:51
Operator : SY/MD
Sample : 03106-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FE4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

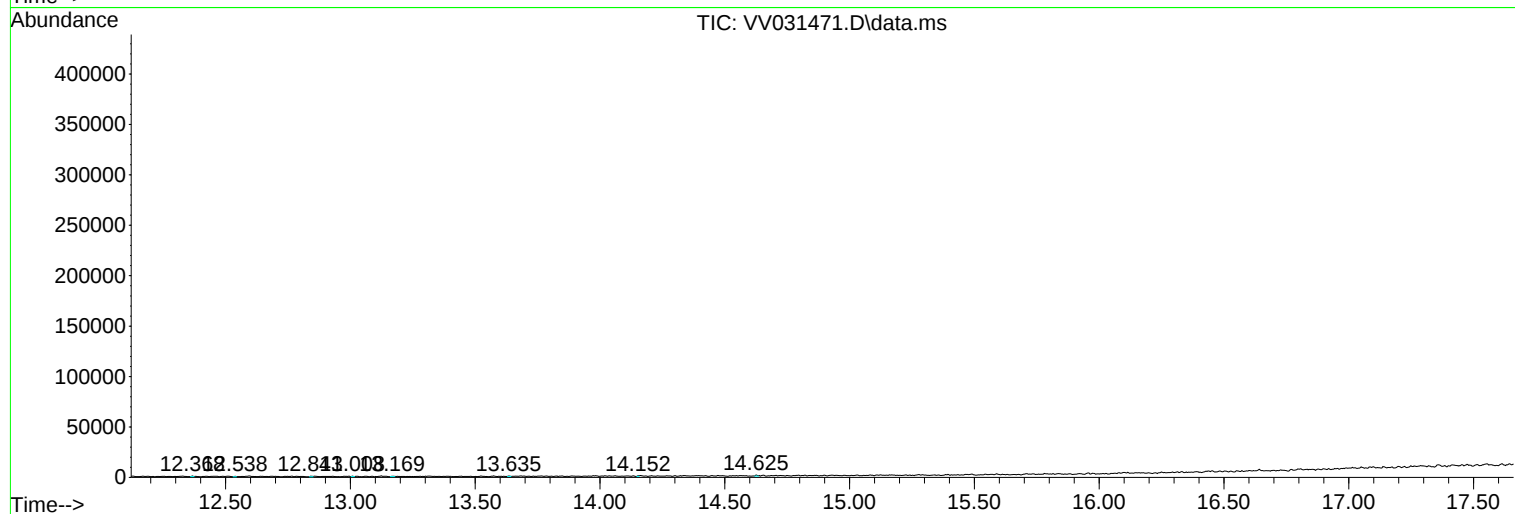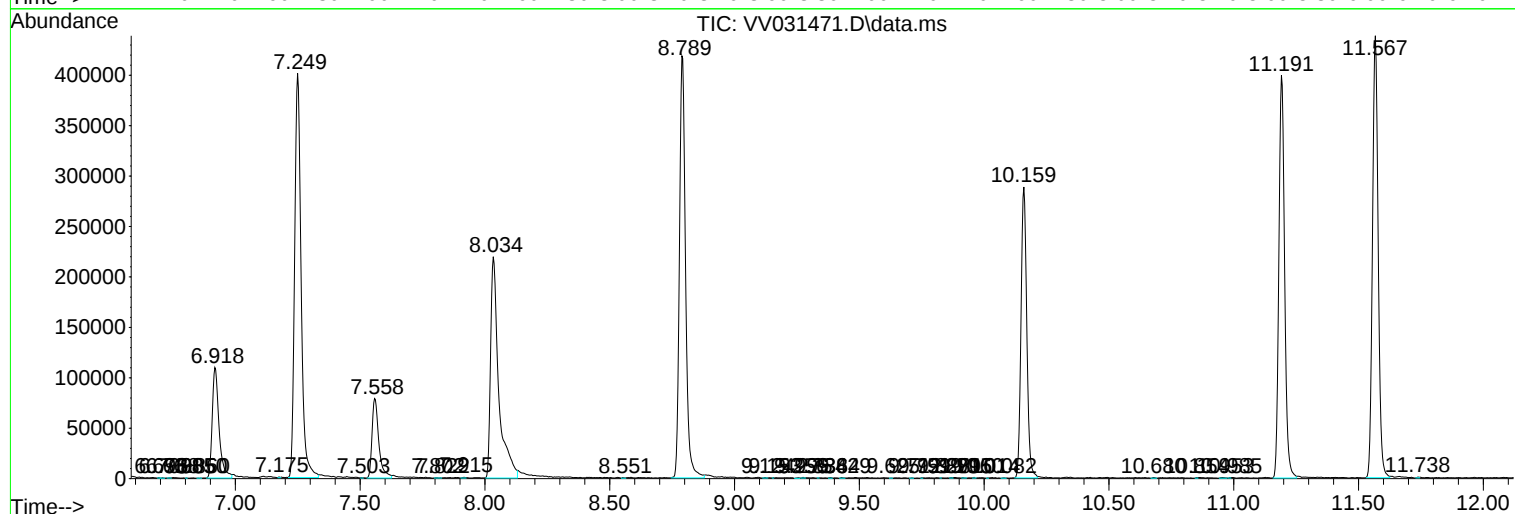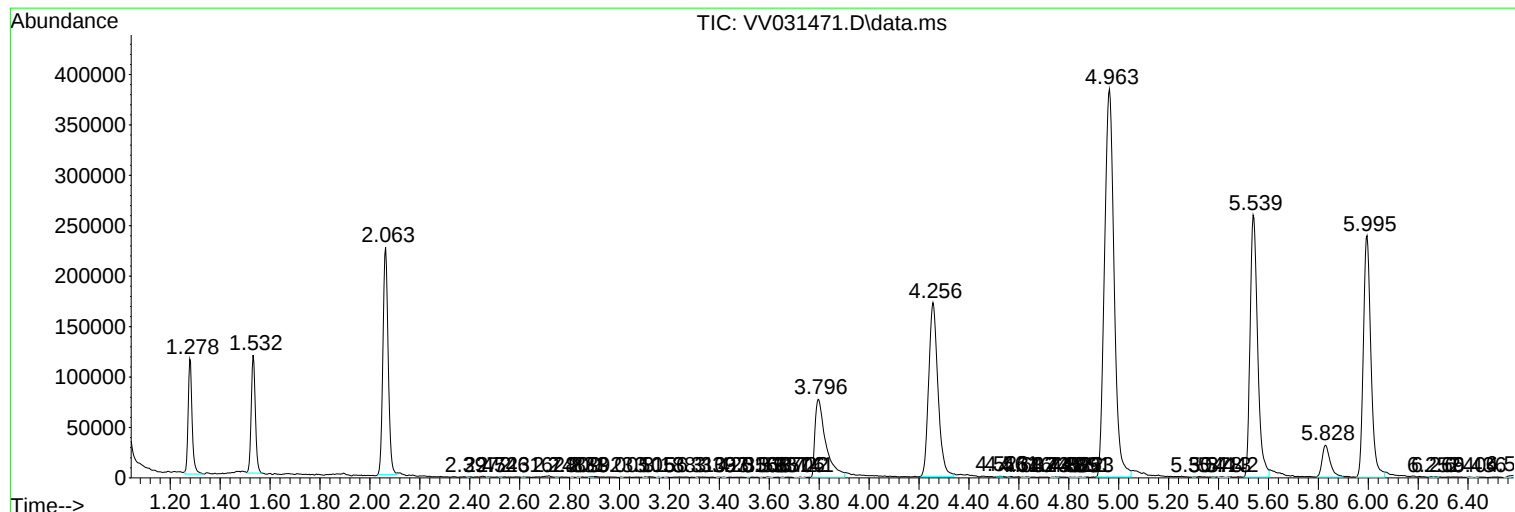

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031471.D
Acq On : 09 Jun 2023 00:51
Operator : SY/MD
Sample : 03106-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FE4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031471.D
Acq On : 09 Jun 2023 00:51
Operator : SY/MD
Sample : 03106-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FE4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------