

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031472.D
 Acq On : 09 Jun 2023 01:15
 Operator : SY/MD
 Sample : 03106-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FE5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031472.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	113301	121186	11.68%	1.564%
2	1.532	146	153	170	rVB	119237	140084	13.50%	1.808%
3	2.063	308	318	333	rBV	225833	332171	32.01%	4.287%
4	2.523	456	461	464	rBV2	541	437	0.04%	0.006%
5	2.687	509	512	513	rBV2	501	296	0.03%	0.004%
6	2.844	557	561	564	rBV3	364	300	0.03%	0.004%
7	2.863	564	567	571	rVB3	491	394	0.04%	0.005%
8	2.892	572	576	579	rBV3	666	609	0.06%	0.008%
9	2.921	583	585	588	rBV	190	122	0.01%	0.002%
10	2.947	591	593	595	rBV	289	114	0.01%	0.001%
11	3.047	622	624	628	rBV2	300	194	0.02%	0.003%
12	3.153	655	657	661	rVB2	404	221	0.02%	0.003%
13	3.410	733	737	738	rBV2	443	233	0.02%	0.003%
14	3.432	742	744	749	rVB2	355	229	0.02%	0.003%
15	3.477	757	758	762	rVB	260	106	0.01%	0.001%
16	3.529	770	774	776	rVB	178	96	0.01%	0.001%
17	3.561	782	784	785	rBV	388	141	0.01%	0.002%
18	3.590	789	793	794	rBV	368	262	0.03%	0.003%
19	3.661	813	815	818	rBV2	323	182	0.02%	0.002%
20	3.674	818	819	823	rVB	321	94	0.01%	0.001%
21	3.693	823	825	828	rBV	200	95	0.01%	0.001%
22	3.709	828	830	833	rBV	326	288	0.03%	0.004%
23	3.748	839	842	843	rBV	150	77	0.01%	0.001%
24	3.754	843	844	846	rBV2	363	116	0.01%	0.001%
25	3.796	848	857	890	rBV2	79108	236841	22.82%	3.057%
26	4.256	986	1000	1027	rBV	170905	436982	42.11%	5.640%
27	4.757	1152	1156	1158	rBV2	562	426	0.04%	0.005%
28	4.818	1173	1175	1177	rVB2	335	141	0.01%	0.002%
29	4.841	1180	1182	1183	rBV	234	93	0.01%	0.001%
30	4.963	1202	1220	1243	rBV2	386326	1037831	100.00%	13.394%
31	5.407	1355	1358	1363	rBV3	603	542	0.05%	0.007%
32	5.429	1363	1365	1367	rVB2	398	140	0.01%	0.002%
33	5.484	1380	1382	1386	rVB3	499	310	0.03%	0.004%
34	5.539	1387	1399	1439	rBV	273283	588055	56.66%	7.589%
35	5.783	1473	1475	1477	rBV3	574	298	0.03%	0.004%
36	5.834	1477	1491	1509	rVV5	53766	129590	12.49%	1.672%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031472.D
 Acq On : 09 Jun 2023 01:15
 Operator : SY/MD
 Sample : 03106-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FE5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	5.995	1528	1541	1559	rBV	246017	509371	49.08%	6.574%
38	6.368	1656	1657	1660	rBV	221	125	0.01%	0.002%
39	6.407	1667	1669	1675	rBV3	601	495	0.05%	0.006%
40	6.516	1701	1703	1705	rVB2	305	130	0.01%	0.002%
41	6.532	1705	1708	1710	rBV	421	209	0.02%	0.003%
42	6.574	1710	1721	1722	rBV5	1638	2672	0.26%	0.034%
43	6.686	1754	1756	1759	rBV	277	151	0.01%	0.002%
44	6.722	1765	1767	1770	rBV2	565	263	0.03%	0.003%
45	6.815	1795	1796	1798	rBV2	356	144	0.01%	0.002%
46	6.847	1804	1806	1807	rBV2	165	68	0.01%	0.001%
47	6.918	1817	1828	1858	rBV2	106043	209785	20.21%	2.707%
48	7.249	1919	1931	1951	rBV	409844	730246	70.36%	9.424%
49	7.500	2007	2009	2011	rVB2	536	203	0.02%	0.003%
50	7.558	2016	2027	2053	rBV	80475	156799	15.11%	2.024%
51	7.780	2094	2096	2098	rBV2	398	208	0.02%	0.003%
52	7.821	2107	2109	2112	rVB2	540	264	0.03%	0.003%
53	7.915	2134	2138	2140	rBV4	535	430	0.04%	0.006%
54	8.034	2165	2175	2212	rBV2	225150	521915	50.29%	6.736%
55	8.481	2311	2314	2315	rBV	470	243	0.02%	0.003%
56	8.596	2348	2350	2353	rVB2	663	265	0.03%	0.003%
57	8.612	2353	2355	2357	rBV2	396	202	0.02%	0.003%
58	8.715	2385	2387	2392	rBV3	568	460	0.04%	0.006%
59	8.789	2396	2410	2436	rBV	431714	740068	71.31%	9.551%
60	9.014	2477	2480	2482	rBV2	510	305	0.03%	0.004%
61	9.024	2482	2483	2486	rVV4	440	221	0.02%	0.003%
62	9.149	2520	2522	2525	rVB3	533	260	0.03%	0.003%
63	9.397	2597	2599	2601	rBV	266	111	0.01%	0.001%
64	9.525	2633	2639	2643	rBV3	488	630	0.06%	0.008%
65	9.583	2654	2657	2659	rBV	586	307	0.03%	0.004%
66	9.712	2694	2697	2700	rBV	586	361	0.03%	0.005%
67	9.866	2743	2745	2746	rBV	542	161	0.02%	0.002%
68	9.937	2766	2767	2770	rBV	310	124	0.01%	0.002%
69	10.027	2792	2795	2797	rBV2	373	267	0.03%	0.003%
70	10.159	2824	2836	2862	rVB	292122	466285	44.93%	6.018%
71	10.249	2862	2864	2868	rVB3	406	218	0.02%	0.003%
72	10.275	2870	2872	2875	rBV2	545	319	0.03%	0.004%
73	10.593	2970	2971	2974	rBV2	513	283	0.03%	0.004%
74	10.667	2992	2994	2997	rBV2	556	340	0.03%	0.004%
75	10.709	3004	3007	3010	rBV	627	397	0.04%	0.005%
76	10.805	3032	3037	3040	rBV2	545	530	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031472.D
 Acq On : 09 Jun 2023 01:15
 Operator : SY/MD
 Sample : 03106-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FE5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.834	3042	3046	3049	rBV2	589	598	0.06%	0.008%
78	11.027	3103	3106	3107	rBV	195	113	0.01%	0.001%
79	11.059	3112	3116	3121	rBV2	477	518	0.05%	0.007%
80	11.123	3134	3136	3138	rBV2	269	114	0.01%	0.001%
81	11.191	3145	3157	3181	rBV	427138	664187	64.00%	8.572%
82	11.358	3208	3209	3211	rBV2	455	163	0.02%	0.002%
83	11.567	3262	3274	3292	rBV	444319	705063	67.94%	9.099%
84	11.873	3366	3369	3370	rBV	410	212	0.02%	0.003%
85	12.011	3410	3412	3413	rBV	520	189	0.02%	0.002%
86	12.551	3576	3580	3582	rBV2	456	357	0.03%	0.005%
87	12.625	3598	3603	3608	rVB3	692	661	0.06%	0.009%
88	12.648	3608	3610	3614	rBV2	359	344	0.03%	0.004%
89	13.381	3836	3838	3839	rBV2	342	139	0.01%	0.002%
90	13.490	3870	3872	3873	rBV2	346	141	0.01%	0.002%
91	13.519	3878	3881	3884	rBV2	619	453	0.04%	0.006%




Sum of corrected areas: 7748383

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031472.D
Acq On : 09 Jun 2023 01:15
Operator : SY/MD
Sample : 03106-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FE5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

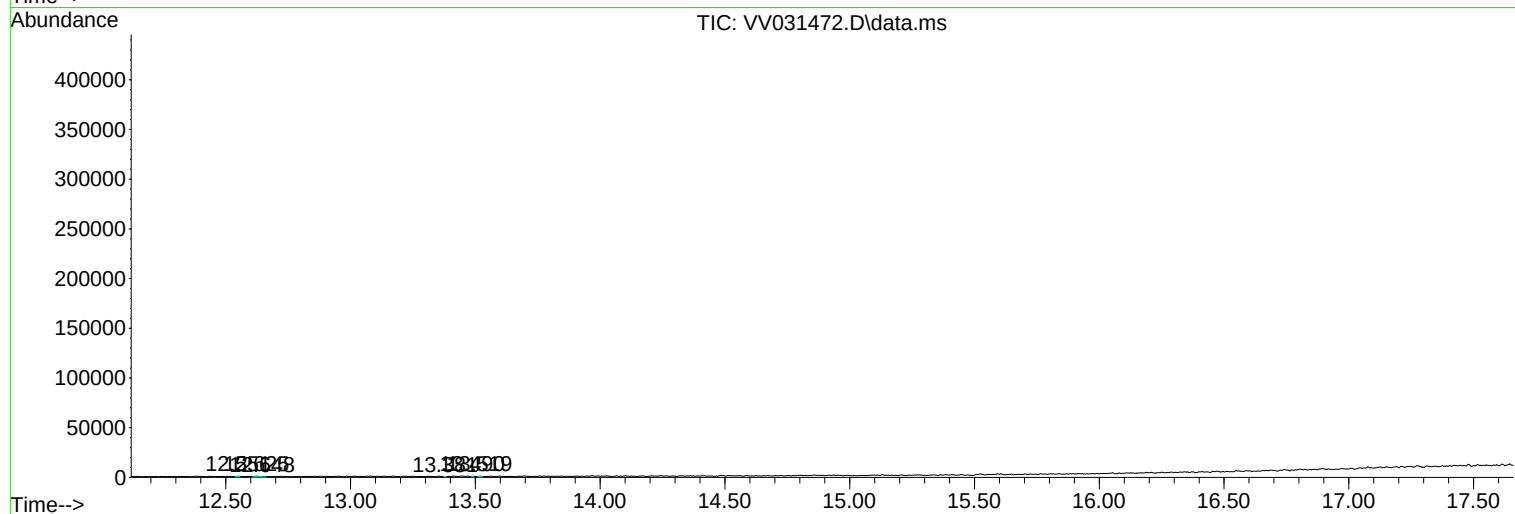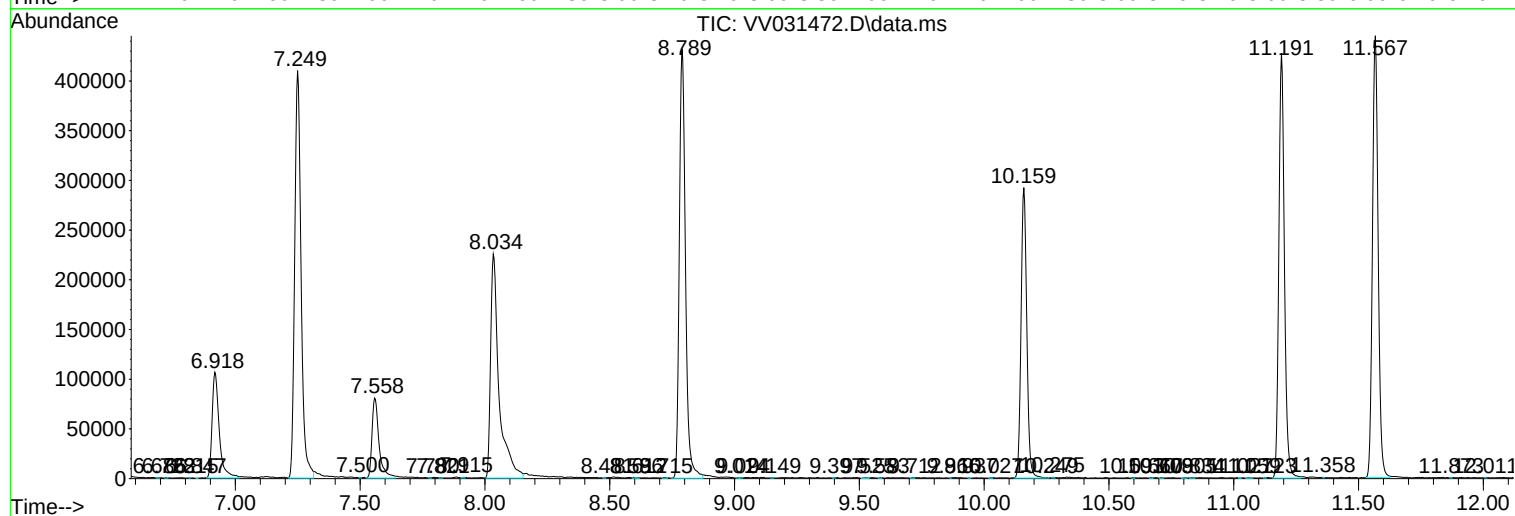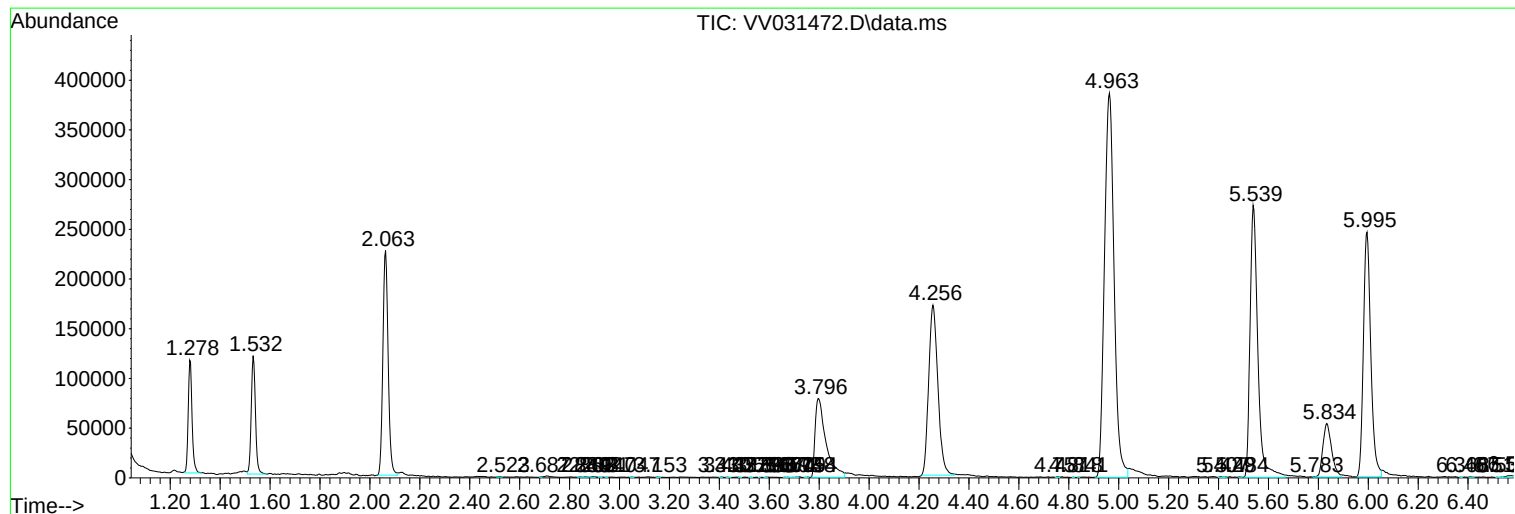

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031472.D
Acq On : 09 Jun 2023 01:15
Operator : SY/MD
Sample : 03106-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FE5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031472.D
Acq On : 09 Jun 2023 01:15
Operator : SY/MD
Sample : 03106-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FE5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------