

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031473.D
 Acq On : 09 Jun 2023 01:39
 Operator : SY/MD
 Sample : 03106-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FE7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031473.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rVB	111563	117707	11.41%	1.534%
2	1.532	146	153	167	rVB	118019	136891	13.27%	1.785%
3	2.063	308	318	332	rBV	221981	324905	31.49%	4.236%
4	2.429	429	432	434	rBV2	456	260	0.03%	0.003%
5	2.548	464	469	470	rBV2	493	295	0.03%	0.004%
6	2.671	503	507	509	rBV2	355	279	0.03%	0.004%
7	2.777	537	540	544	rVB3	618	364	0.04%	0.005%
8	3.011	611	613	617	rVB2	551	372	0.04%	0.005%
9	3.040	617	622	625	rBV3	494	532	0.05%	0.007%
10	3.118	642	646	651	rBV3	432	454	0.04%	0.006%
11	3.503	762	766	768	rBV	407	305	0.03%	0.004%
12	3.519	768	771	774	rVV	383	296	0.03%	0.004%
13	3.629	799	805	809	rBV3	614	509	0.05%	0.007%
14	3.690	819	824	827	rBV2	495	399	0.04%	0.005%
15	3.799	848	858	891	rBV2	79884	236501	22.92%	3.083%
16	4.256	985	1000	1028	rBV	171482	449392	43.55%	5.858%
17	4.545	1087	1090	1093	rBV2	708	520	0.05%	0.007%
18	4.738	1147	1150	1153	rBV4	332	239	0.02%	0.003%
19	4.831	1176	1179	1180	rBV	491	242	0.02%	0.003%
20	4.851	1184	1185	1194	rVB3	583	552	0.05%	0.007%
21	4.892	1194	1198	1201	rBV3	453	390	0.04%	0.005%
22	4.963	1202	1220	1244	rBV2	384619	1031928	100.00%	13.453%
23	5.294	1320	1323	1327	rVB4	1018	652	0.06%	0.008%
24	5.314	1327	1329	1330	rBV2	617	271	0.03%	0.004%
25	5.478	1377	1380	1383	rVB3	603	374	0.04%	0.005%
26	5.539	1387	1399	1424	rBV	275918	575070	55.73%	7.497%
27	5.828	1478	1489	1514	rBV3	37160	82342	7.98%	1.073%
28	5.995	1527	1541	1579	rBV	240323	514425	49.85%	6.706%
29	6.195	1601	1603	1607	rBV4	449	275	0.03%	0.004%
30	6.301	1633	1636	1639	rBV3	480	342	0.03%	0.004%
31	6.426	1673	1675	1676	rBV	749	275	0.03%	0.004%
32	6.564	1712	1718	1719	rBV3	1265	1070	0.10%	0.014%
33	6.715	1763	1765	1769	rVB2	514	239	0.02%	0.003%
34	6.918	1814	1828	1853	rBV	107182	210018	20.35%	2.738%
35	7.098	1881	1884	1886	rBV2	699	431	0.04%	0.006%
36	7.249	1919	1931	1965	rBV	404786	732500	70.98%	9.549%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031473.D
 Acq On : 09 Jun 2023 01:39
 Operator : SY/MD
 Sample : 03106-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FE7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	7.558	2018	2027	2058	rBV	79007	150538	14.59%	1.962%
38	7.744	2083	2085	2088	rVB3	723	339	0.03%	0.004%
39	7.764	2088	2091	2095	rBV3	646	651	0.06%	0.008%
40	7.870	2121	2124	2125	rBV	494	255	0.02%	0.003%
41	7.953	2147	2150	2152	rVB	398	274	0.03%	0.004%
42	7.982	2152	2159	2164	rBV4	696	951	0.09%	0.012%
43	8.034	2164	2175	2215	rBV2	219357	521763	50.56%	6.802%
44	8.667	2368	2372	2373	rBV2	573	371	0.04%	0.005%
45	8.748	2395	2397	2399	rBV2	632	312	0.03%	0.004%
46	8.789	2399	2410	2441	rBV	441284	743835	72.08%	9.697%
47	9.027	2482	2484	2489	rVB4	579	489	0.05%	0.006%
48	9.056	2489	2493	2498	rBV3	858	690	0.07%	0.009%
49	9.085	2498	2502	2504	rBV3	568	509	0.05%	0.007%
50	9.246	2548	2552	2553	rBV3	419	251	0.02%	0.003%
51	9.329	2574	2578	2582	rBV3	695	580	0.06%	0.008%
52	9.384	2590	2595	2599	rBV2	400	306	0.03%	0.004%
53	9.420	2603	2606	2607	rBV	368	235	0.02%	0.003%
54	9.548	2644	2646	2650	rVB	557	365	0.04%	0.005%
55	9.629	2667	2671	2673	rBV4	476	348	0.03%	0.005%
56	9.667	2679	2683	2685	rBV2	574	366	0.04%	0.005%
57	9.680	2685	2687	2691	rVB3	382	241	0.02%	0.003%
58	9.702	2691	2694	2695	rBV2	388	242	0.02%	0.003%
59	9.773	2710	2716	2717	rBV3	595	479	0.05%	0.006%
60	9.866	2742	2745	2746	rBV2	488	266	0.03%	0.003%
61	9.915	2756	2760	2763	rBV3	702	519	0.05%	0.007%
62	9.969	2774	2777	2779	rBV	658	397	0.04%	0.005%
63	10.008	2786	2789	2793	rBV2	376	392	0.04%	0.005%
64	10.085	2811	2813	2816	rBV2	439	252	0.02%	0.003%
65	10.108	2818	2820	2822	rVB2	720	268	0.03%	0.003%
66	10.159	2824	2836	2858	rVV	287540	451769	43.78%	5.889%
67	10.236	2858	2860	2863	rVB3	912	394	0.04%	0.005%
68	10.288	2874	2876	2882	rBV2	325	264	0.03%	0.003%
69	10.320	2883	2886	2887	rBV3	438	248	0.02%	0.003%
70	10.394	2906	2909	2911	rBV	427	262	0.03%	0.003%
71	10.490	2936	2939	2942	rBV	456	333	0.03%	0.004%
72	10.548	2955	2957	2964	rVB2	418	342	0.03%	0.004%
73	10.612	2975	2977	2981	rVB3	373	251	0.02%	0.003%
74	10.719	3006	3010	3013	rBV2	409	268	0.03%	0.003%
75	10.744	3015	3018	3020	rBV3	441	254	0.02%	0.003%
76	10.828	3040	3044	3049	rBV3	646	694	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW060823\
 Data File : VW031473.D
 Acq On : 09 Jun 2023 01:39
 Operator : SY/MD
 Sample : 03106-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FE7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.863	3049	3055	3060	rBV4	1035	919	0.09%	0.012%
78	11.108	3129	3131	3136	rVB3	425	237	0.02%	0.003%
79	11.130	3136	3138	3145	rBV4	750	687	0.07%	0.009%
80	11.191	3145	3157	3177	rBV	418312	666980	64.63%	8.695%
81	11.452	3234	3238	3242	rBV3	443	421	0.04%	0.005%
82	11.567	3262	3274	3292	rBV	431157	691156	66.98%	9.010%
83	11.773	3333	3338	3341	rBV3	680	675	0.07%	0.009%
84	11.841	3356	3359	3362	rBV2	344	265	0.03%	0.003%
85	11.937	3384	3389	3390	rBV3	442	349	0.03%	0.005%
86	12.185	3461	3466	3469	rBV2	649	676	0.07%	0.009%
87	12.648	3607	3610	3612	rBV	517	291	0.03%	0.004%
88	12.812	3659	3661	3663	rBV	369	236	0.02%	0.003%
89	12.863	3674	3677	3679	rBV2	562	331	0.03%	0.004%
90	12.927	3695	3697	3701	rVB	459	274	0.03%	0.004%
91	12.963	3706	3708	3714	rVB3	556	392	0.04%	0.005%
92	13.169	3769	3772	3774	rBV	478	303	0.03%	0.004%
93	13.204	3781	3783	3789	rBV2	414	342	0.03%	0.004%
94	13.259	3798	3800	3805	rBV3	586	512	0.05%	0.007%
95	13.406	3844	3846	3852	rBV2	705	577	0.06%	0.008%
96	13.503	3873	3876	3877	rBV2	454	251	0.02%	0.003%
97	13.779	3958	3962	3964	rBV2	516	380	0.04%	0.005%
98	13.828	3974	3977	3982	rVB4	549	358	0.03%	0.005%
99	13.876	3990	3992	3996	rVB3	596	318	0.03%	0.004%
100	14.336	4132	4135	4140	rBV4	636	712	0.07%	0.009%




Sum of corrected areas: 7670821

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031473.D
Acq On : 09 Jun 2023 01:39
Operator : SY/MD
Sample : 03106-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FE7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

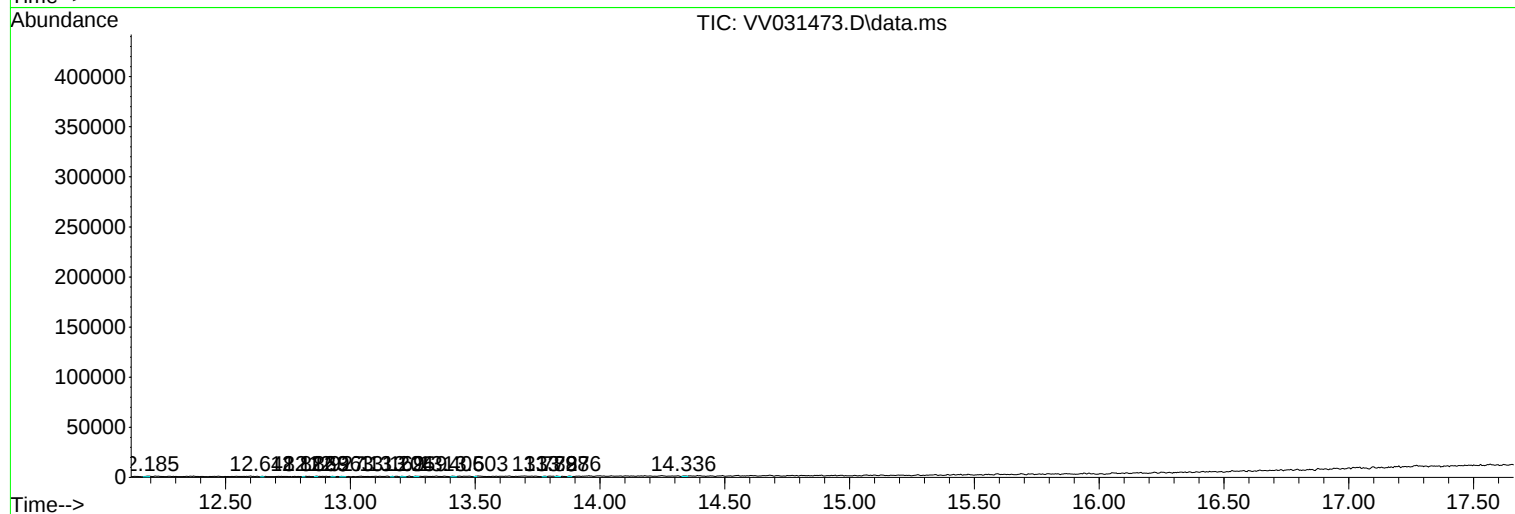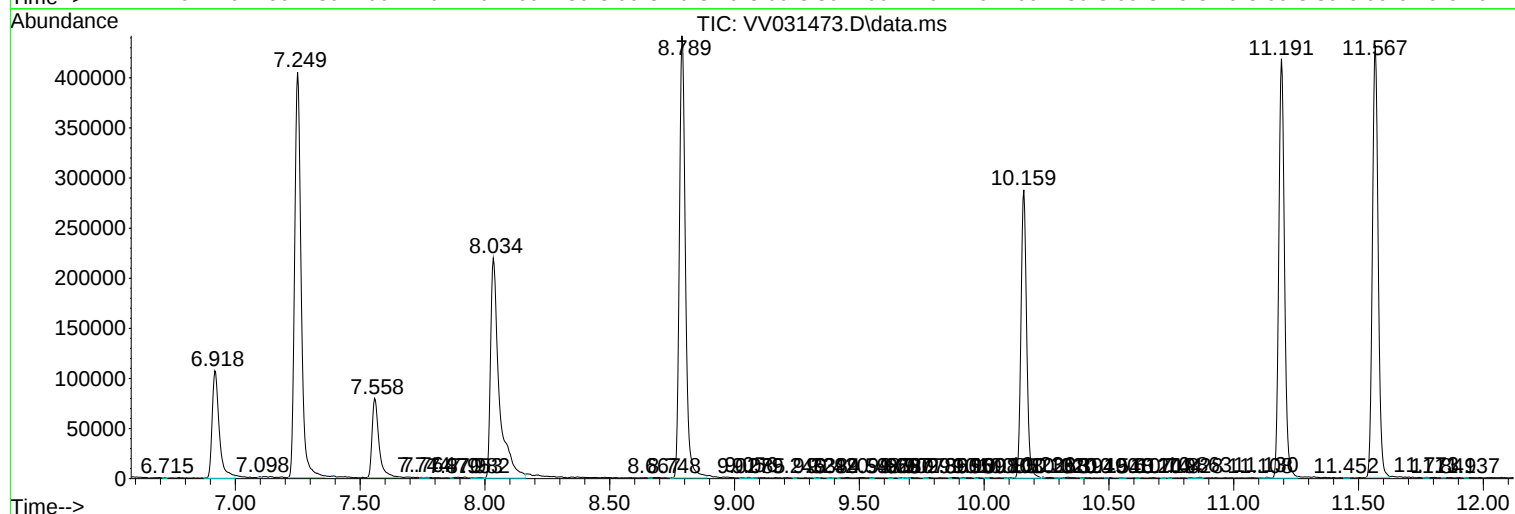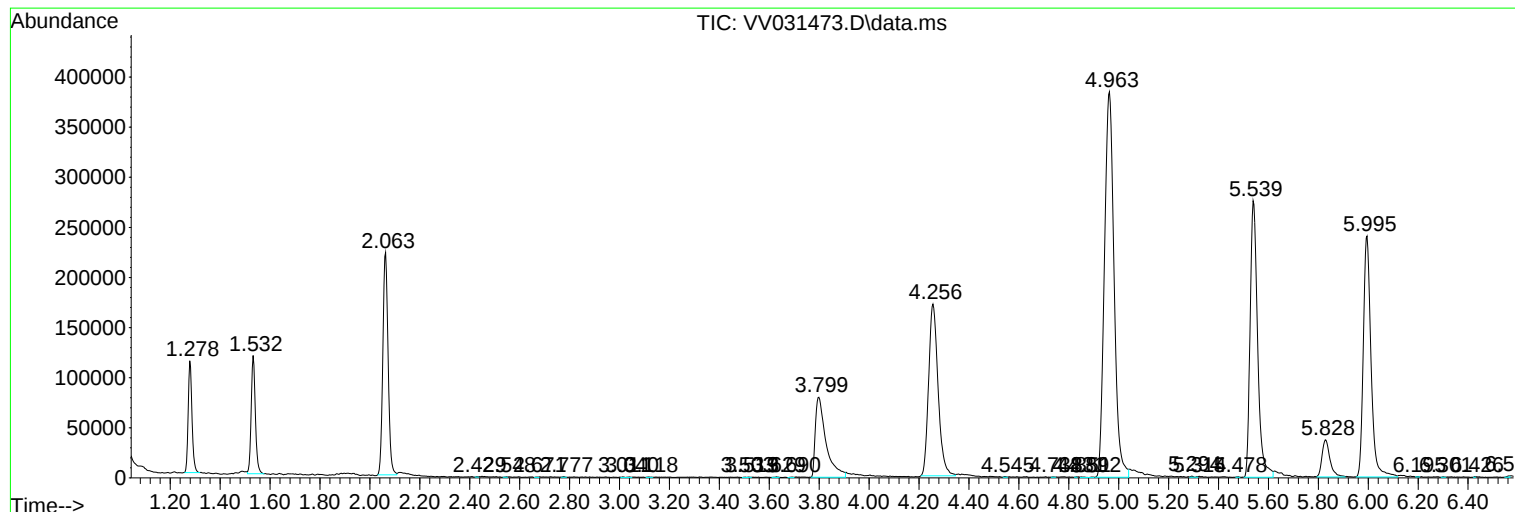

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031473.D
Acq On : 09 Jun 2023 01:39
Operator : SY/MD
Sample : 03106-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FE7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031473.D
Acq On : 09 Jun 2023 01:39
Operator : SY/MD
Sample : 03106-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FE7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------