

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031474.D
 Acq On : 09 Jun 2023 02:03
 Operator : SY/MD
 Sample : 03106-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FE8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031474.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	109924	118336	11.60%	1.571%
2	1.532	146	153	167	rVB	117338	139915	13.71%	1.858%
3	2.063	308	318	332	rBV	219457	322818	31.64%	4.287%
4	2.535	462	465	467	rBV	508	266	0.03%	0.004%
5	2.780	539	541	546	rBV3	316	234	0.02%	0.003%
6	2.850	560	563	566	rBV	267	219	0.02%	0.003%
7	2.912	575	582	584	rBV2	316	388	0.04%	0.005%
8	2.928	584	587	591	rVB3	503	420	0.04%	0.006%
9	3.024	614	617	618	rBV	377	229	0.02%	0.003%
10	3.169	659	662	666	rBV4	280	233	0.02%	0.003%
11	3.214	673	676	680	rBV2	211	208	0.02%	0.003%
12	3.326	709	711	714	rBV	361	224	0.02%	0.003%
13	3.715	826	832	833	rVB2	358	226	0.02%	0.003%
14	3.725	833	835	838	rBV2	352	256	0.03%	0.003%
15	3.796	848	857	888	rBV	77976	229114	22.46%	3.042%
16	4.256	984	1000	1028	rBV	167170	444289	43.55%	5.900%
17	4.587	1102	1103	1108	rBV2	359	237	0.02%	0.003%
18	4.616	1111	1112	1117	rVB2	445	213	0.02%	0.003%
19	4.638	1117	1119	1122	rVB2	513	248	0.02%	0.003%
20	4.661	1122	1126	1131	rVB3	442	398	0.04%	0.005%
21	4.702	1135	1139	1142	rVB3	407	331	0.03%	0.004%
22	4.802	1165	1170	1171	rBV	336	261	0.03%	0.003%
23	4.834	1178	1180	1184	rVV2	638	476	0.05%	0.006%
24	4.857	1184	1187	1190	rVB2	497	334	0.03%	0.004%
25	4.895	1196	1199	1201	rBV2	325	212	0.02%	0.003%
26	4.963	1202	1220	1243	rBV2	380656	1020175	100.00%	13.547%
27	5.207	1294	1296	1297	rBV	621	221	0.02%	0.003%
28	5.426	1363	1364	1369	rVB2	455	267	0.03%	0.004%
29	5.452	1369	1372	1375	rBV3	333	270	0.03%	0.004%
30	5.542	1385	1400	1424	rBV	265851	563818	55.27%	7.487%
31	5.754	1464	1466	1470	rVB2	688	399	0.04%	0.005%
32	5.773	1470	1472	1478	rBV5	898	892	0.09%	0.012%
33	5.828	1478	1489	1505	rBV2	38732	85487	8.38%	1.135%
34	5.995	1527	1541	1557	rBV	240212	496385	48.66%	6.591%
35	6.243	1615	1618	1622	rBV2	445	332	0.03%	0.004%
36	6.291	1631	1633	1635	rBV2	529	216	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031474.D
 Acq On : 09 Jun 2023 02:03
 Operator : SY/MD
 Sample : 03106-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FE8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	6.378	1658	1660	1665	rBV3	402	229	0.02%	0.003%
38	6.416	1669	1672	1675	rBV2	350	279	0.03%	0.004%
39	6.468	1683	1688	1689	rBV2	302	206	0.02%	0.003%
40	6.561	1710	1717	1718	rBV3	1286	1273	0.12%	0.017%
41	6.622	1733	1736	1741	rVB6	779	780	0.08%	0.010%
42	6.657	1745	1747	1749	rVV2	673	268	0.03%	0.004%
43	6.699	1756	1760	1764	rBV2	497	312	0.03%	0.004%
44	6.731	1768	1770	1773	rBV2	394	262	0.03%	0.003%
45	6.767	1779	1781	1785	rBV2	652	292	0.03%	0.004%
46	6.825	1796	1799	1802	rBV2	516	367	0.04%	0.005%
47	6.918	1817	1828	1852	rBV	104545	204744	20.07%	2.719%
48	7.249	1919	1931	1954	rBV	408297	718975	70.48%	9.547%
49	7.558	2018	2027	2051	rBV	79134	147838	14.49%	1.963%
50	7.821	2105	2109	2114	rBV5	825	758	0.07%	0.010%
51	7.870	2120	2124	2126	rBV2	684	435	0.04%	0.006%
52	8.034	2165	2175	2217	rBV2	219290	516562	50.63%	6.859%
53	8.429	2294	2298	2300	rBV3	569	427	0.04%	0.006%
54	8.497	2317	2319	2323	rBV3	518	434	0.04%	0.006%
55	8.570	2340	2342	2344	rBV	518	254	0.02%	0.003%
56	8.699	2378	2382	2384	rBV3	473	320	0.03%	0.004%
57	8.747	2395	2397	2399	rBV	402	211	0.02%	0.003%
58	8.789	2399	2410	2444	rBV	430036	728184	71.38%	9.669%
59	9.226	2544	2546	2547	rBV	468	218	0.02%	0.003%
60	9.246	2550	2552	2556	rVB	644	333	0.03%	0.004%
61	9.262	2556	2557	2561	rBV2	282	213	0.02%	0.003%
62	9.310	2570	2572	2575	rVB2	481	282	0.03%	0.004%
63	9.445	2612	2614	2616	rVB	552	235	0.02%	0.003%
64	9.554	2646	2648	2657	rVB2	323	297	0.03%	0.004%
65	9.593	2657	2660	2662	rBV3	329	220	0.02%	0.003%
66	9.644	2674	2676	2680	rVB3	454	230	0.02%	0.003%
67	9.709	2695	2696	2702	rVB3	523	442	0.04%	0.006%
68	9.799	2722	2724	2727	rVB2	488	215	0.02%	0.003%
69	9.876	2745	2748	2750	rBV2	481	318	0.03%	0.004%
70	10.043	2797	2800	2802	rBV	642	385	0.04%	0.005%
71	10.107	2818	2820	2823	rBV2	394	320	0.03%	0.004%
72	10.159	2824	2836	2853	rVV	273617	435472	42.69%	5.783%
73	10.397	2906	2910	2913	rVB2	494	303	0.03%	0.004%
74	10.432	2917	2921	2924	rVV4	460	290	0.03%	0.004%
75	10.484	2935	2937	2941	rBV2	396	288	0.03%	0.004%
76	10.670	2990	2995	2997	rBV2	302	254	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031474.D
 Acq On : 09 Jun 2023 02:03
 Operator : SY/MD
 Sample : 03106-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FE8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.770	3020	3026	3028	rBV3	483	532	0.05%	0.007%
78	10.795	3032	3034	3037	rBV	395	238	0.02%	0.003%
79	10.866	3053	3056	3060	rVB2	623	451	0.04%	0.006%
80	10.895	3060	3065	3067	rBV3	425	421	0.04%	0.006%
81	10.963	3083	3086	3090	rBV	496	408	0.04%	0.005%
82	11.017	3100	3103	3106	rBV2	381	325	0.03%	0.004%
83	11.191	3145	3157	3176	rBV	410237	640061	62.74%	8.499%
84	11.358	3206	3209	3215	rVB3	632	661	0.06%	0.009%
85	11.506	3250	3255	3260	rBV4	604	603	0.06%	0.008%
86	11.567	3262	3274	3293	rBV	431937	690710	67.71%	9.172%
87	11.712	3316	3319	3320	rBV2	467	252	0.02%	0.003%
88	11.930	3384	3387	3390	rVB	424	210	0.02%	0.003%
89	11.956	3390	3395	3396	rBV2	511	361	0.04%	0.005%
90	12.098	3437	3439	3442	rBV4	475	260	0.03%	0.003%
91	12.197	3467	3470	3472	rBV2	489	231	0.02%	0.003%
92	12.287	3496	3498	3500	rBV2	288	208	0.02%	0.003%
93	12.400	3528	3533	3534	rBV	336	249	0.02%	0.003%
94	12.799	3654	3657	3659	rBV	319	239	0.02%	0.003%
95	12.930	3695	3698	3700	rBV	453	277	0.03%	0.004%
96	13.258	3797	3800	3802	rBV2	411	242	0.02%	0.003%
97	13.548	3886	3890	3891	rBV2	421	281	0.03%	0.004%
98	13.860	3985	3987	3992	rVB2	713	406	0.04%	0.005%
99	13.885	3992	3995	3996	rBV	741	443	0.04%	0.006%
100	13.950	4013	4015	4019	rBV3	590	487	0.05%	0.006%




Sum of corrected areas: 7530828

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031474.D
Acq On : 09 Jun 2023 02:03
Operator : SY/MD
Sample : 03106-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FE8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

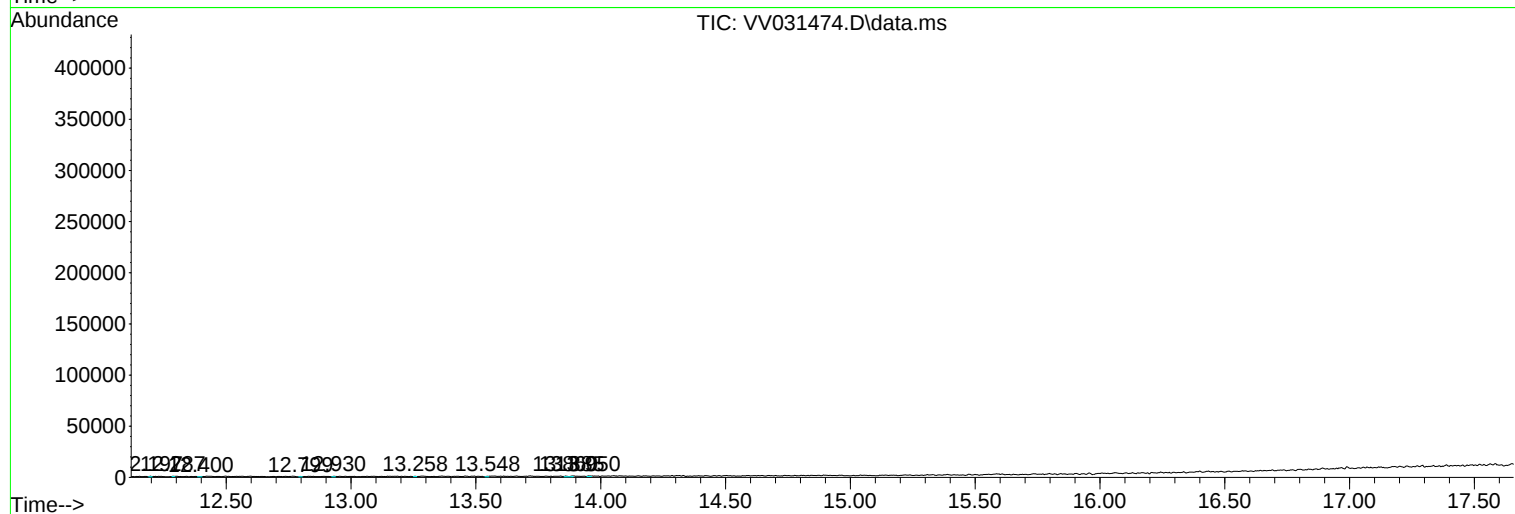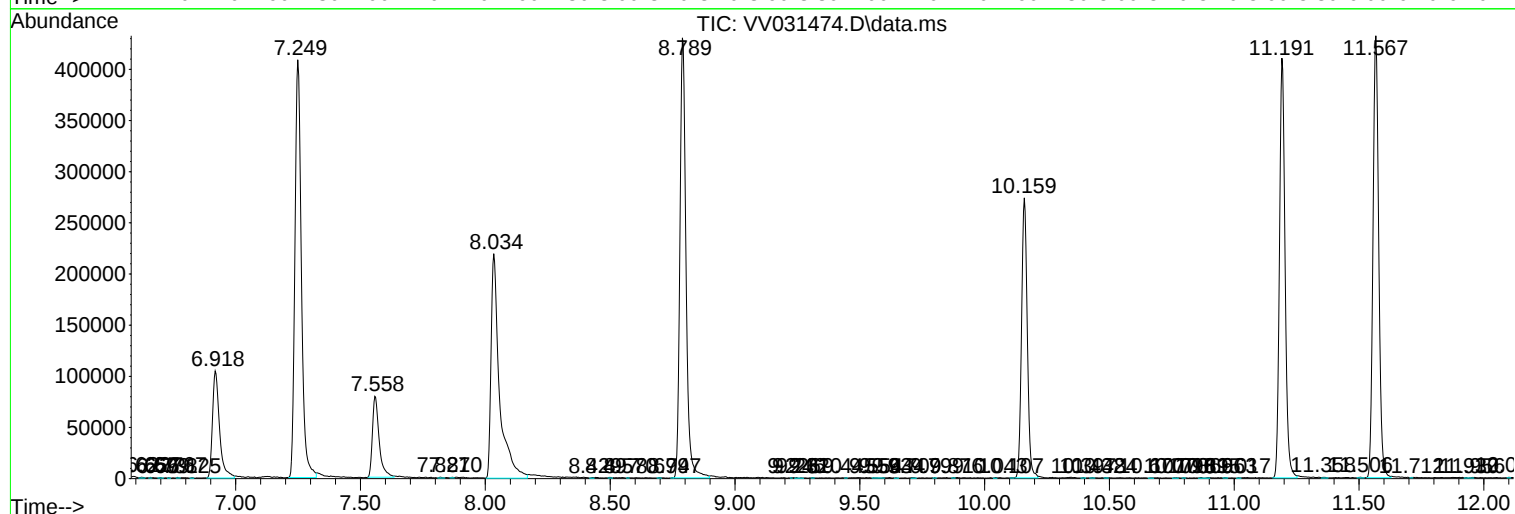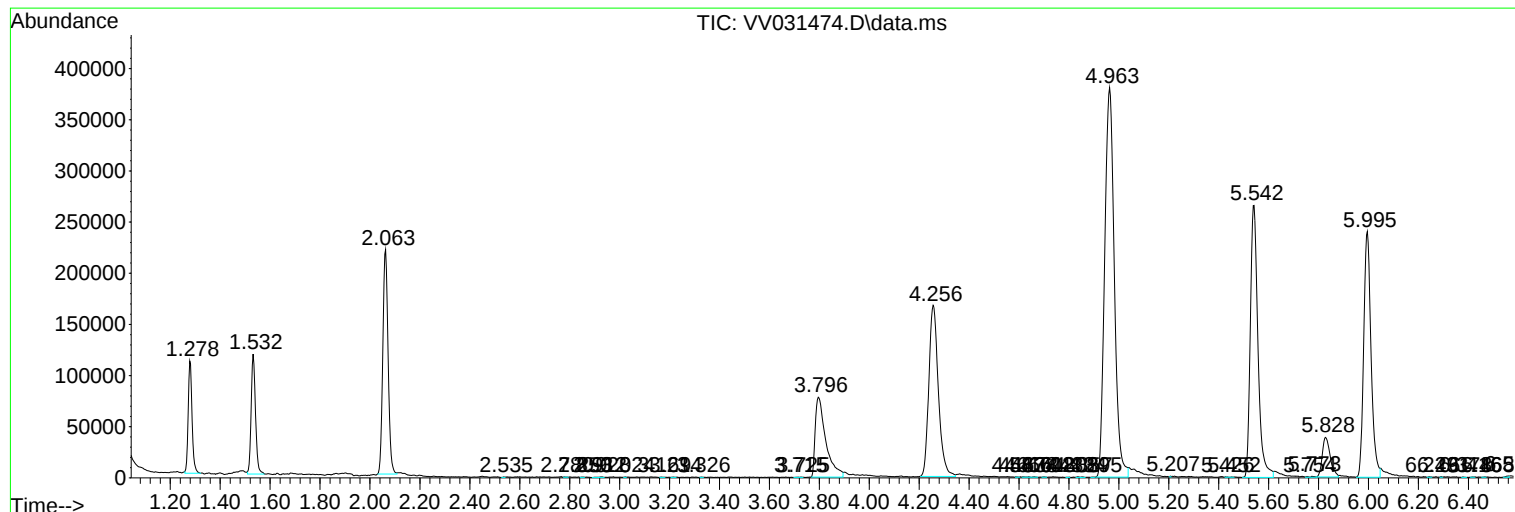

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031474.D
Acq On : 09 Jun 2023 02:03
Operator : SY/MD
Sample : 03106-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FE8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031474.D
Acq On : 09 Jun 2023 02:03
Operator : SY/MD
Sample : 03106-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FE8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------