

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031475.D
 Acq On : 09 Jun 2023 02:26
 Operator : SY/MD
 Sample : 03106-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FF0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031475.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rVB	110338	117915	11.37%	1.523%
2	1.532	146	153	171	rVB	119108	140488	13.55%	1.815%
3	2.063	307	318	336	rBV	226152	343058	33.08%	4.432%
4	2.371	412	414	416	rBV2	610	283	0.03%	0.004%
5	2.442	432	436	438	rBV3	577	476	0.05%	0.006%
6	2.658	500	503	505	rBV2	391	212	0.02%	0.003%
7	2.748	529	531	534	rVB3	391	154	0.01%	0.002%
8	2.992	605	607	609	rBV2	467	245	0.02%	0.003%
9	3.050	621	625	626	rBV	644	345	0.03%	0.004%
10	3.076	631	633	635	rVB2	351	186	0.02%	0.002%
11	3.195	668	670	672	rVB2	336	153	0.01%	0.002%
12	3.214	672	676	682	rVB4	562	457	0.04%	0.006%
13	3.252	682	688	689	rBV2	351	233	0.02%	0.003%
14	3.281	695	697	700	rBV2	389	246	0.02%	0.003%
15	3.304	702	704	710	rVB3	388	330	0.03%	0.004%
16	3.333	710	713	714	rBV	287	147	0.01%	0.002%
17	3.355	718	720	723	rVB2	250	146	0.01%	0.002%
18	3.407	733	736	739	rBV4	347	289	0.03%	0.004%
19	3.494	761	763	766	rVB3	277	142	0.01%	0.002%
20	3.519	769	771	773	rBV	265	161	0.02%	0.002%
21	3.539	773	777	778	rBV2	432	281	0.03%	0.004%
22	3.625	802	804	806	rVB	542	249	0.02%	0.003%
23	3.645	806	810	814	rBV3	322	256	0.02%	0.003%
24	3.664	814	816	819	rBV	278	153	0.01%	0.002%
25	3.744	838	841	844	rBV	400	234	0.02%	0.003%
26	3.802	848	859	890	rBV2	81078	257956	24.88%	3.332%
27	4.256	984	1000	1027	rBV	172308	447571	43.16%	5.782%
28	4.658	1124	1125	1128	rVB	325	143	0.01%	0.002%
29	4.677	1128	1131	1134	rBV2	394	271	0.03%	0.004%
30	4.732	1143	1148	1149	rBV3	427	340	0.03%	0.004%
31	4.754	1153	1155	1158	rVB3	401	193	0.02%	0.002%
32	4.773	1158	1161	1163	rBV2	479	261	0.03%	0.003%
33	4.818	1170	1175	1177	rBV3	583	452	0.04%	0.006%
34	4.963	1202	1220	1245	rBV2	386834	1036905	100.00%	13.395%
35	5.288	1317	1321	1324	rBV5	809	767	0.07%	0.010%
36	5.539	1386	1399	1424	rBV	284610	594733	57.36%	7.683%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031475.D
 Acq On : 09 Jun 2023 02:26
 Operator : SY/MD
 Sample : 03106-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FF0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	5.831	1477	1490	1511	rBV7	34638	80840	7.80%	1.044%
38	5.995	1527	1541	1565	rBV2	239184	507326	48.93%	6.554%
39	6.297	1632	1635	1638	rBV4	586	404	0.04%	0.005%
40	6.346	1645	1650	1651	rBV2	465	347	0.03%	0.004%
41	6.429	1674	1676	1679	rVB	334	163	0.02%	0.002%
42	6.445	1679	1681	1682	rBV2	409	191	0.02%	0.002%
43	6.481	1690	1692	1695	rVB2	343	188	0.02%	0.002%
44	6.500	1695	1698	1699	rBV	330	194	0.02%	0.003%
45	6.535	1707	1709	1712	rBV2	470	294	0.03%	0.004%
46	6.561	1713	1717	1718	rBB3	226	266	0.03%	0.003%
47	6.706	1758	1762	1765	rVB3	530	384	0.04%	0.005%
48	6.722	1765	1767	1770	rVB3	506	290	0.03%	0.004%
49	6.838	1801	1803	1805	rBV2	248	160	0.02%	0.002%
50	6.866	1810	1812	1814	rBV	238	139	0.01%	0.002%
51	6.918	1817	1828	1844	rBV	106849	202510	19.53%	2.616%
52	7.249	1918	1931	1955	rBV	403129	723246	69.75%	9.343%
53	7.516	2012	2014	2016	rBV	411	191	0.02%	0.002%
54	7.558	2016	2027	2050	rBV	78392	150934	14.56%	1.950%
55	7.799	2100	2102	2107	rVB3	408	309	0.03%	0.004%
56	7.825	2107	2110	2112	rBV2	766	411	0.04%	0.005%
57	7.883	2121	2128	2131	rBV4	667	956	0.09%	0.012%
58	7.966	2151	2154	2157	rBV3	296	224	0.02%	0.003%
59	8.034	2165	2175	2218	rBV2	223563	520577	50.20%	6.725%
60	8.493	2315	2318	2320	rBV2	546	298	0.03%	0.004%
61	8.612	2354	2355	2357	rVB	379	134	0.01%	0.002%
62	8.738	2390	2394	2397	rBV4	450	346	0.03%	0.004%
63	8.789	2398	2410	2434	rBV	445465	754667	72.78%	9.749%
64	9.037	2484	2487	2493	rVB3	719	569	0.05%	0.007%
65	9.079	2498	2500	2503	rBV2	595	421	0.04%	0.005%
66	9.153	2519	2523	2525	rBV3	518	360	0.03%	0.005%
67	9.320	2571	2575	2577	rBV2	344	239	0.02%	0.003%
68	9.403	2599	2601	2603	rBV2	500	244	0.02%	0.003%
69	9.503	2630	2632	2635	rVB3	473	250	0.02%	0.003%
70	9.834	2732	2735	2736	rBV	405	187	0.02%	0.002%
71	9.924	2760	2763	2764	rVB2	343	137	0.01%	0.002%
72	9.934	2764	2766	2770	rVB2	425	241	0.02%	0.003%
73	9.992	2783	2784	2788	rBV	272	163	0.02%	0.002%
74	10.021	2791	2793	2795	rBV2	403	189	0.02%	0.002%
75	10.159	2822	2836	2858	rBV	289466	457462	44.12%	5.910%
76	10.294	2876	2878	2881	rBV2	406	266	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031475.D
 Acq On : 09 Jun 2023 02:26
 Operator : SY/MD
 Sample : 03106-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FF0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.480	2934	2936	2937	rBV2	391	138	0.01%	0.002%
78	10.686	2996	3000	3002	rBV	336	237	0.02%	0.003%
79	10.699	3002	3004	3006	rVV3	418	188	0.02%	0.002%
80	10.841	3045	3048	3049	rBV	381	220	0.02%	0.003%
81	11.053	3111	3114	3116	rBV2	315	167	0.02%	0.002%
82	11.095	3123	3127	3128	rBV2	441	318	0.03%	0.004%
83	11.191	3143	3157	3179	rBV	431551	685365	66.10%	8.854%
84	11.384	3213	3217	3220	rBV2	626	492	0.05%	0.006%
85	11.567	3262	3274	3297	rBV	436136	695147	67.04%	8.980%
86	12.069	3428	3430	3432	rBV	323	155	0.01%	0.002%
87	12.194	3465	3469	3472	rBV3	682	478	0.05%	0.006%
88	12.538	3574	3576	3580	rBV4	607	437	0.04%	0.006%
89	12.587	3588	3591	3594	rVB3	751	353	0.03%	0.005%
90	13.005	3718	3721	3724	rBV2	280	212	0.02%	0.003%
91	13.062	3734	3739	3742	rBV3	543	536	0.05%	0.007%
92	13.146	3763	3765	3769	rBV	449	330	0.03%	0.004%
93	13.233	3791	3792	3797	rBV2	354	289	0.03%	0.004%
94	13.368	3831	3834	3837	rBV	333	287	0.03%	0.004%
95	13.464	3860	3864	3869	rBV4	868	851	0.08%	0.011%
96	13.567	3893	3896	3897	rBV2	443	246	0.02%	0.003%
97	13.599	3904	3906	3907	rBV	359	168	0.02%	0.002%
98	13.738	3944	3949	3951	rBV2	519	441	0.04%	0.006%
99	14.037	4040	4042	4045	rVB2	513	231	0.02%	0.003%
100	14.117	4064	4067	4070	rBV2	398	315	0.03%	0.004%




Sum of corrected areas: 7740749

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031475.D
Acq On : 09 Jun 2023 02:26
Operator : SY/MD
Sample : 03106-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FF0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

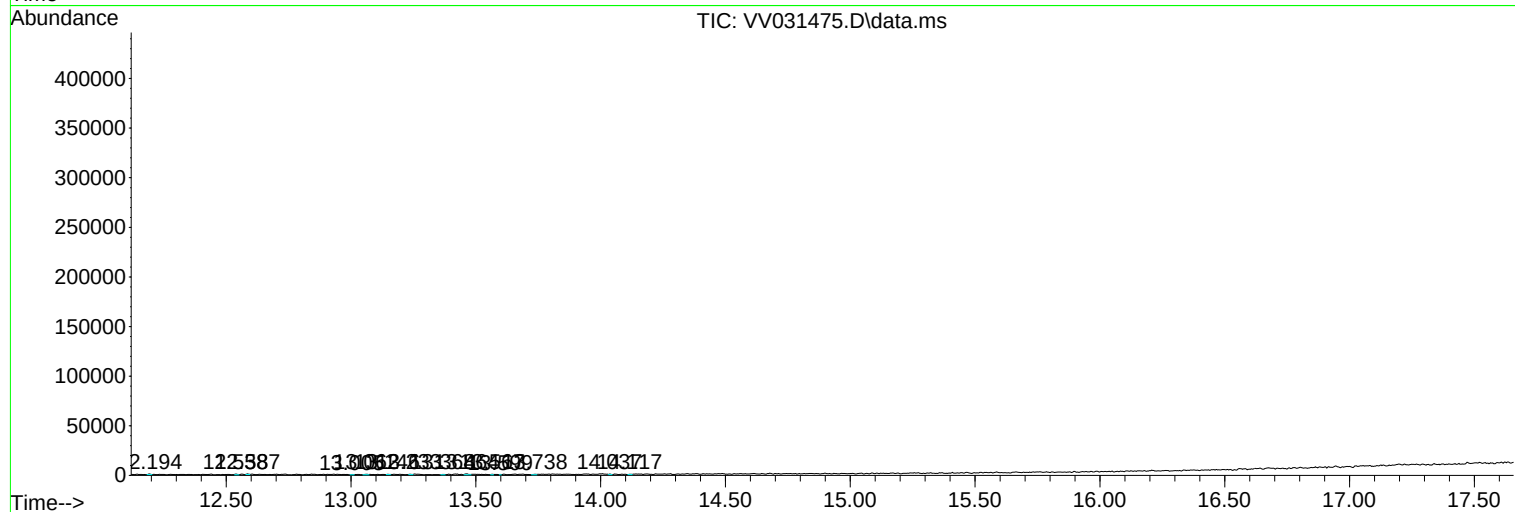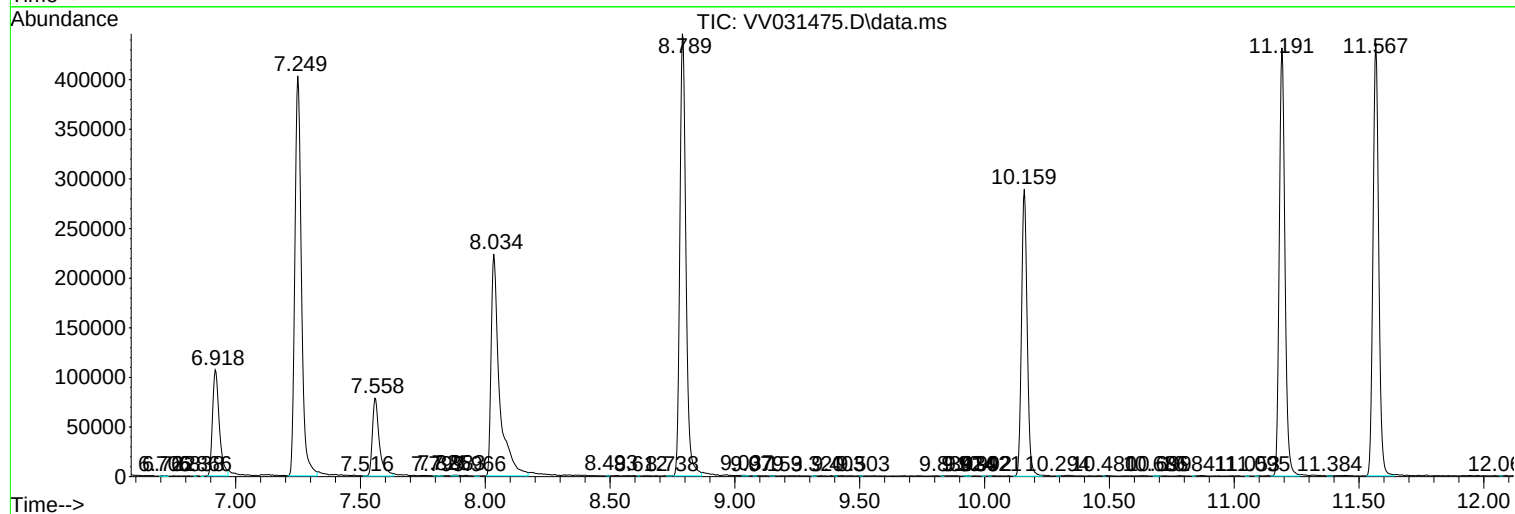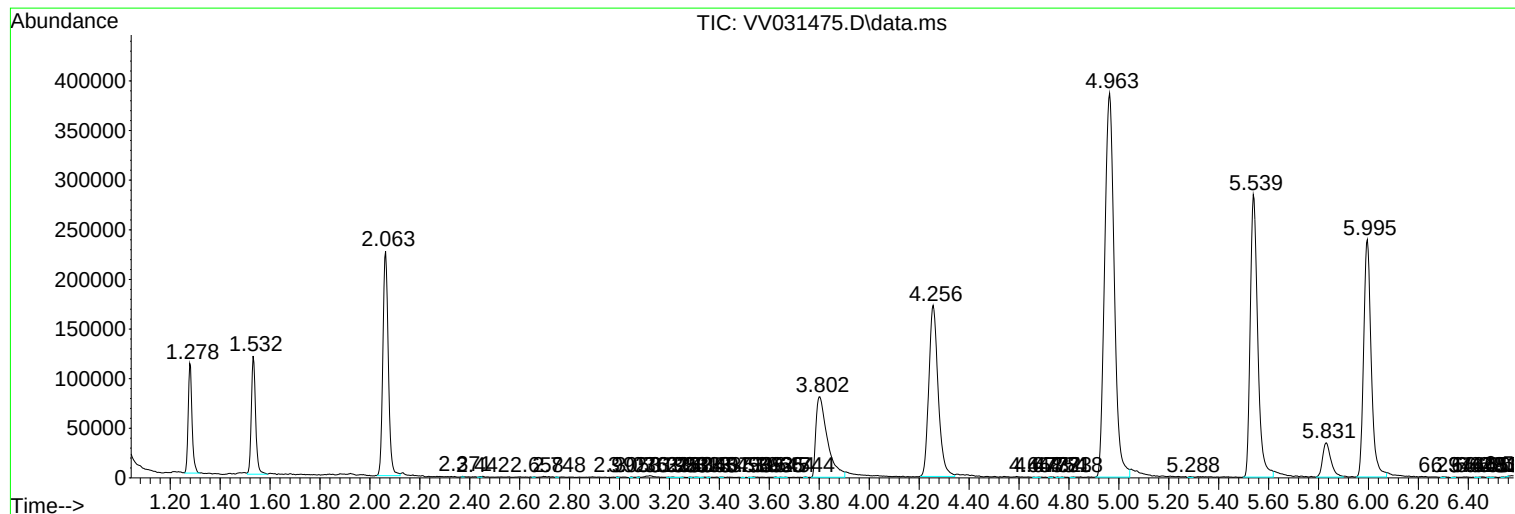

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031475.D
Acq On : 09 Jun 2023 02:26
Operator : SY/MD
Sample : 03106-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FF0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031475.D
Acq On : 09 Jun 2023 02:26
Operator : SY/MD
Sample : 03106-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FF0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------