

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031476.D
 Acq On : 09 Jun 2023 02:50
 Operator : SY/MD
 Sample : 03106-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031476.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	85	rVB	113993	119915	11.33%	1.416%
2	1.532	147	153	168	rVB	120621	142034	13.42%	1.677%
3	2.063	308	318	333	rBV2	237180	366272	34.59%	4.325%
4	2.349	404	407	410	rVB4	611	331	0.03%	0.004%
5	2.407	421	425	430	rVB4	605	562	0.05%	0.007%
6	2.809	545	550	551	rBV3	369	277	0.03%	0.003%
7	2.895	574	577	580	rBV3	268	179	0.02%	0.002%
8	2.979	599	603	605	rBV2	225	192	0.02%	0.002%
9	3.082	633	635	636	rBV	479	172	0.02%	0.002%
10	3.162	658	660	664	rVB	323	182	0.02%	0.002%
11	3.207	672	674	677	rBV3	298	166	0.02%	0.002%
12	3.262	687	691	693	rBV2	582	345	0.03%	0.004%
13	3.275	693	695	699	rVB2	365	193	0.02%	0.002%
14	3.442	744	747	749	rBV2	288	193	0.02%	0.002%
15	3.500	761	765	769	rVB2	388	298	0.03%	0.004%
16	3.580	788	790	793	rVB2	389	205	0.02%	0.002%
17	3.638	804	808	810	rBV2	324	164	0.02%	0.002%
18	3.670	814	818	821	rBV3	352	310	0.03%	0.004%
19	3.799	848	858	889	rBV2	83035	274578	25.93%	3.243%
20	4.256	983	1000	1027	rBV	173681	456032	43.07%	5.385%
21	4.619	1110	1113	1115	rBV2	530	320	0.03%	0.004%
22	4.693	1133	1136	1139	rBV3	424	234	0.02%	0.003%
23	4.821	1173	1176	1177	rBV	339	214	0.02%	0.003%
24	4.886	1194	1196	1201	rVB2	468	315	0.03%	0.004%
25	4.963	1202	1220	1247	rBV2	396993	1058759	100.00%	12.503%
26	5.329	1331	1334	1336	rVB3	555	246	0.02%	0.003%
27	5.342	1336	1338	1340	rBV2	549	294	0.03%	0.003%
28	5.439	1365	1368	1370	rBV2	486	309	0.03%	0.004%
29	5.490	1382	1384	1387	rBV2	376	262	0.02%	0.003%
30	5.538	1387	1399	1421	rBV	273404	568713	53.72%	6.716%
31	5.837	1476	1492	1527	rBV2	341855	740441	69.93%	8.744%
32	5.995	1529	1541	1569	rVB	250294	509054	48.08%	6.012%
33	6.191	1598	1602	1603	rBV2	934	581	0.05%	0.007%
34	6.345	1648	1650	1654	rBV	421	268	0.03%	0.003%
35	6.387	1658	1663	1665	rBV4	568	359	0.03%	0.004%
36	6.435	1675	1678	1680	rBV2	720	443	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031476.D
 Acq On : 09 Jun 2023 02:50
 Operator : SY/MD
 Sample : 03106-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	6.493	1692	1696	1700	rVB3	357	252	0.02%	0.003%
38	6.574	1713	1721	1724	rBV3	1646	2291	0.22%	0.027%
39	6.696	1757	1759	1764	rVB4	676	537	0.05%	0.006%
40	6.722	1764	1767	1771	rBV3	622	452	0.04%	0.005%
41	6.741	1771	1773	1777	rVB2	514	295	0.03%	0.003%
42	6.815	1793	1796	1799	rBV3	240	184	0.02%	0.002%
43	6.918	1817	1828	1854	rBV	106203	213800	20.19%	2.525%
44	7.249	1919	1931	1956	rBV	412722	744163	70.29%	8.788%
45	7.558	2017	2027	2049	rBV	81649	153124	14.46%	1.808%
46	7.937	2142	2145	2148	rBV3	566	258	0.02%	0.003%
47	8.034	2165	2175	2213	rBV2	219710	523503	49.44%	6.182%
48	8.554	2334	2337	2338	rBV2	626	309	0.03%	0.004%
49	8.593	2346	2349	2353	rVB2	750	486	0.05%	0.006%
50	8.612	2353	2355	2357	rBV2	356	195	0.02%	0.002%
51	8.625	2357	2359	2363	rBV2	424	287	0.03%	0.003%
52	8.702	2380	2383	2385	rBV3	500	345	0.03%	0.004%
53	8.789	2396	2410	2433	rBV	434858	741136	70.00%	8.752%
54	9.075	2497	2499	2501	rBV2	342	223	0.02%	0.003%
55	9.220	2541	2544	2551	rBV3	484	419	0.04%	0.005%
56	9.271	2557	2560	2565	rVB4	337	226	0.02%	0.003%
57	9.297	2565	2568	2570	rVB2	601	254	0.02%	0.003%
58	9.371	2588	2591	2593	rBV3	371	179	0.02%	0.002%
59	9.387	2593	2596	2599	rVB4	342	203	0.02%	0.002%
60	9.410	2599	2603	2605	rBV2	632	468	0.04%	0.006%
61	9.439	2609	2612	2615	rVB2	503	329	0.03%	0.004%
62	9.541	2640	2644	2647	rBV3	404	404	0.04%	0.005%
63	9.615	2665	2667	2671	rBV	526	388	0.04%	0.005%
64	9.660	2678	2681	2684	rBV2	428	354	0.03%	0.004%
65	9.696	2690	2692	2695	rBV2	431	299	0.03%	0.004%
66	9.812	2724	2728	2729	rBV2	484	222	0.02%	0.003%
67	9.857	2740	2742	2744	rVB2	578	204	0.02%	0.002%
68	9.869	2744	2746	2748	rBV3	493	261	0.02%	0.003%
69	10.021	2791	2793	2796	rBV2	468	281	0.03%	0.003%
70	10.159	2824	2836	2855	rBV	289077	463527	43.78%	5.474%
71	10.262	2866	2868	2873	rBV4	679	574	0.05%	0.007%
72	10.426	2916	2919	2922	rVB3	460	326	0.03%	0.004%
73	10.551	2953	2958	2960	rBV3	310	267	0.03%	0.003%
74	10.699	3002	3004	3007	rVB2	399	197	0.02%	0.002%
75	10.725	3008	3012	3014	rBV2	488	272	0.03%	0.003%
76	10.930	3072	3076	3079	rVV3	451	334	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031476.D
 Acq On : 09 Jun 2023 02:50
 Operator : SY/MD
 Sample : 03106-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.953	3079	3083	3086	rVV2	483	336	0.03%	0.004%
78	11.101	3127	3129	3131	rBV2	654	330	0.03%	0.004%
79	11.191	3146	3157	3176	rBV	412455	656305	61.99%	7.751%
80	11.474	3242	3245	3247	rBV3	597	423	0.04%	0.005%
81	11.567	3262	3274	3293	rBV	453438	707288	66.80%	8.353%
82	12.287	3496	3498	3503	rVB2	469	294	0.03%	0.003%
83	12.326	3507	3510	3514	rBV3	462	435	0.04%	0.005%
84	12.413	3536	3537	3541	rBV3	401	223	0.02%	0.003%
85	12.477	3555	3557	3558	rBV	380	184	0.02%	0.002%
86	12.593	3589	3593	3596	rVB5	630	462	0.04%	0.005%
87	12.609	3596	3598	3603	rBV3	640	448	0.04%	0.005%
88	12.696	3624	3625	3629	rBV	372	297	0.03%	0.004%
89	12.783	3649	3652	3654	rBV	471	263	0.02%	0.003%
90	12.840	3667	3670	3672	rBV3	443	259	0.02%	0.003%
91	12.889	3680	3685	3692	rBV4	889	1202	0.11%	0.014%
92	12.918	3692	3694	3698	rVV3	448	336	0.03%	0.004%
93	13.065	3735	3740	3741	rBV	649	482	0.05%	0.006%
94	13.197	3779	3781	3782	rBV	330	183	0.02%	0.002%
95	13.274	3803	3805	3807	rBV	407	180	0.02%	0.002%
96	13.387	3836	3840	3843	rBV4	537	568	0.05%	0.007%
97	13.451	3858	3860	3866	rBV2	416	328	0.03%	0.004%
98	13.885	3991	3995	3997	rBV3	694	557	0.05%	0.007%
99	14.490	4181	4183	4186	rBV2	653	524	0.05%	0.006%
100	14.815	4282	4284	4290	rBV5	682	655	0.06%	0.008%




Sum of corrected areas: 8467802

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031476.D
Acq On : 09 Jun 2023 02:50
Operator : SY/MD
Sample : 03106-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FF1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

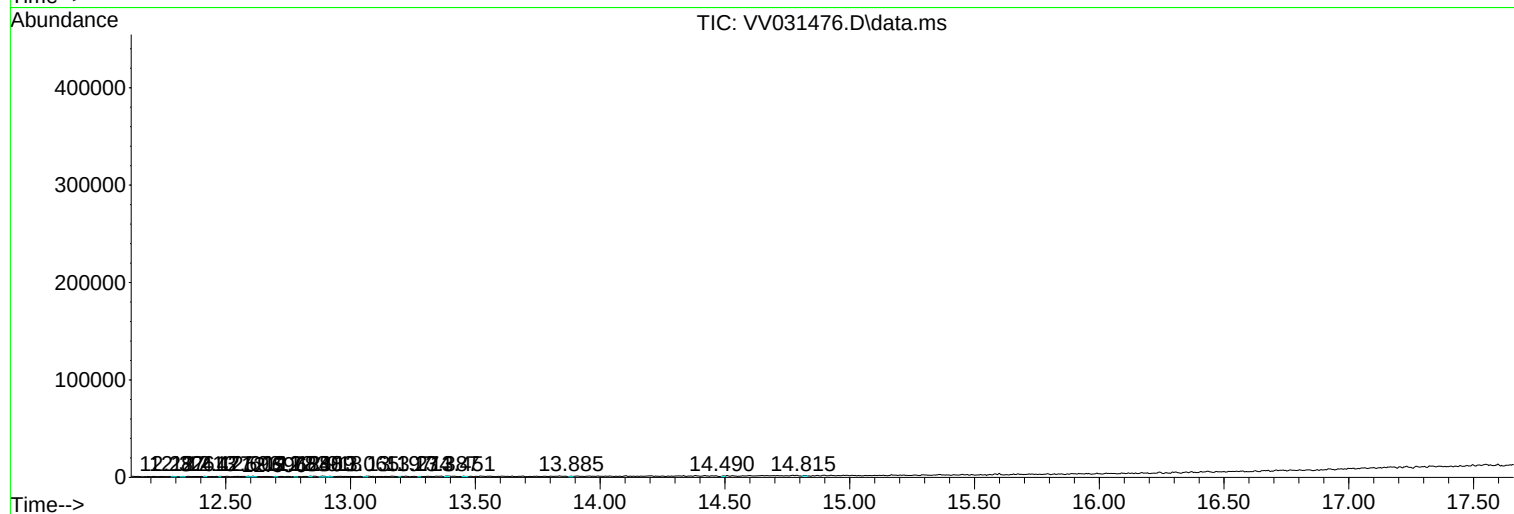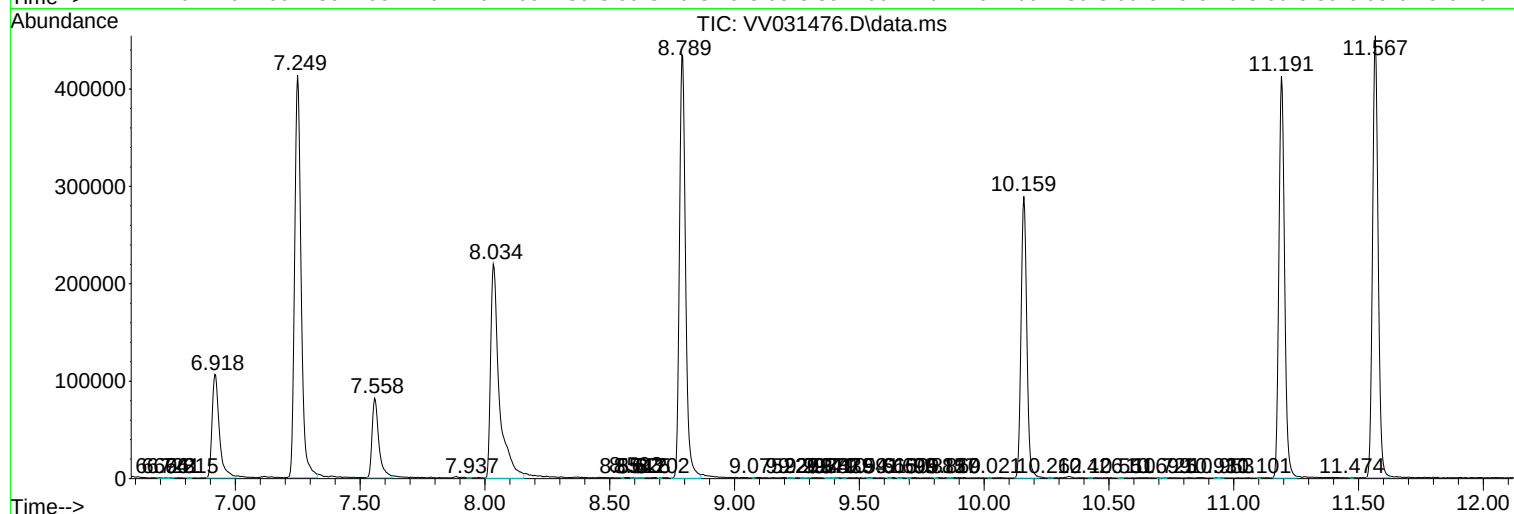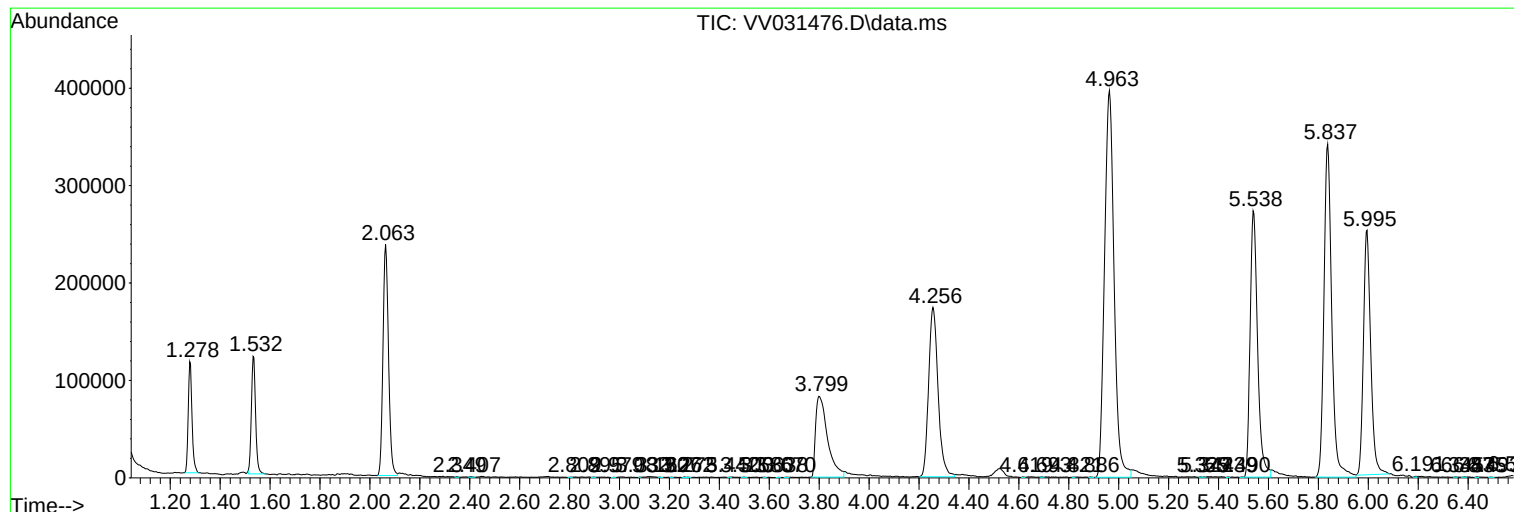

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031476.D
Acq On : 09 Jun 2023 02:50
Operator : SY/MD
Sample : 03106-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FF1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031476.D
Acq On : 09 Jun 2023 02:50
Operator : SY/MD
Sample : 03106-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FF1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------