

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031477.D
 Acq On : 09 Jun 2023 03:14
 Operator : SY/MD
 Sample : 03106-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031477.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	108349	117899	11.89%	1.609%
2	1.532	146	153	170	rVB	109580	130453	13.15%	1.781%
3	2.063	308	318	330	rBV	206787	302248	30.48%	4.126%
4	2.384	416	418	419	rBV	457	174	0.02%	0.002%
5	2.413	425	427	430	rBV2	517	253	0.03%	0.003%
6	2.449	435	438	447	rVB5	1323	1660	0.17%	0.023%
7	2.500	452	454	457	rVB2	379	160	0.02%	0.002%
8	2.651	498	501	503	rBV2	481	317	0.03%	0.004%
9	2.744	526	530	532	rBV3	435	352	0.04%	0.005%
10	2.796	544	546	550	rVB3	465	242	0.02%	0.003%
11	2.870	565	569	571	rBV2	332	230	0.02%	0.003%
12	2.921	583	585	591	rVB	342	269	0.03%	0.004%
13	2.973	599	601	603	rBV2	319	185	0.02%	0.003%
14	2.989	603	606	610	rVB2	436	247	0.02%	0.003%
15	3.034	615	620	622	rBV2	505	343	0.03%	0.005%
16	3.050	623	625	629	rVB3	496	276	0.03%	0.004%
17	3.085	631	636	637	rBV2	238	219	0.02%	0.003%
18	3.137	648	652	653	rBV	300	190	0.02%	0.003%
19	3.195	668	670	674	rVB2	357	168	0.02%	0.002%
20	3.471	750	756	761	rVB3	400	423	0.04%	0.006%
21	3.670	815	818	820	rVB2	521	217	0.02%	0.003%
22	3.693	822	825	829	rBV2	470	346	0.03%	0.005%
23	3.793	845	856	895	rBV	80159	239268	24.13%	3.266%
24	4.256	984	1000	1026	rBV	164757	431045	43.46%	5.884%
25	4.738	1147	1150	1152	rVB3	539	272	0.03%	0.004%
26	4.754	1152	1155	1159	rVB	561	438	0.04%	0.006%
27	4.773	1159	1161	1163	rBV2	519	159	0.02%	0.002%
28	4.863	1183	1189	1191	rBV3	562	649	0.07%	0.009%
29	4.963	1203	1220	1244	rBV2	368578	991746	100.00%	13.539%
30	5.304	1324	1326	1330	rBV2	646	363	0.04%	0.005%
31	5.349	1337	1340	1343	rBV2	479	275	0.03%	0.004%
32	5.420	1359	1362	1363	rBV2	344	193	0.02%	0.003%
33	5.445	1367	1370	1372	rBV2	520	345	0.03%	0.005%
34	5.539	1387	1399	1427	rBV	260240	553240	55.78%	7.552%
35	5.828	1477	1489	1509	rBV3	38065	83967	8.47%	1.146%
36	5.995	1527	1541	1571	rBV	230595	497830	50.20%	6.796%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031477.D
 Acq On : 09 Jun 2023 03:14
 Operator : SY/MD
 Sample : 03106-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	6.214	1606	1609	1612	rBV2	750	542	0.05%	0.007%
38	6.265	1621	1625	1629	rBV4	676	748	0.08%	0.010%
39	6.317	1637	1641	1644	rBV3	479	455	0.05%	0.006%
40	6.522	1702	1705	1707	rBV	436	304	0.03%	0.004%
41	6.564	1712	1718	1719	rBV3	1609	1371	0.14%	0.019%
42	6.792	1786	1789	1792	rBV	371	285	0.03%	0.004%
43	6.837	1800	1803	1804	rBV3	406	196	0.02%	0.003%
44	6.918	1814	1828	1862	rVV	104089	204038	20.57%	2.785%
45	7.249	1920	1931	1961	rBV	375319	671857	67.74%	9.172%
46	7.522	2013	2016	2017	rBV2	536	320	0.03%	0.004%
47	7.558	2018	2027	2054	rVV	76804	143777	14.50%	1.963%
48	7.825	2107	2110	2112	rBV2	398	210	0.02%	0.003%
49	7.889	2127	2130	2133	rBV2	676	370	0.04%	0.005%
50	8.034	2164	2175	2212	rBV2	222048	510765	51.50%	6.973%
51	8.387	2280	2285	2286	rBV2	897	731	0.07%	0.010%
52	8.497	2317	2319	2321	rBV2	383	190	0.02%	0.003%
53	8.532	2327	2330	2331	rBV2	557	302	0.03%	0.004%
54	8.564	2338	2340	2342	rBV	390	160	0.02%	0.002%
55	8.596	2347	2350	2353	rVB2	697	413	0.04%	0.006%
56	8.638	2361	2363	2367	rBV2	425	206	0.02%	0.003%
57	8.789	2398	2410	2435	rBV	412435	702375	70.82%	9.588%
58	8.963	2462	2464	2467	rBV3	626	298	0.03%	0.004%
59	9.021	2480	2482	2485	rBV2	534	294	0.03%	0.004%
60	9.056	2490	2493	2494	rBV	524	263	0.03%	0.004%
61	9.120	2511	2513	2514	rBV	349	164	0.02%	0.002%
62	9.243	2545	2551	2554	rBV3	603	529	0.05%	0.007%
63	9.275	2559	2561	2564	rVV3	383	208	0.02%	0.003%
64	9.333	2574	2579	2582	rBV3	476	417	0.04%	0.006%
65	9.455	2615	2617	2620	rBV2	410	207	0.02%	0.003%
66	9.477	2620	2624	2625	rBV2	367	284	0.03%	0.004%
67	9.635	2672	2673	2675	rBV	437	188	0.02%	0.003%
68	9.818	2727	2730	2733	rBV3	277	207	0.02%	0.003%
69	9.879	2747	2749	2753	rVB3	647	340	0.03%	0.005%
70	9.985	2779	2782	2785	rBV3	434	298	0.03%	0.004%
71	10.014	2789	2791	2793	rBV	367	216	0.02%	0.003%
72	10.159	2824	2836	2858	rBV	274613	438928	44.26%	5.992%
73	10.326	2886	2888	2891	rBV	659	406	0.04%	0.006%
74	10.570	2962	2964	2967	rVB2	396	167	0.02%	0.002%
75	10.641	2982	2986	2991	rVB2	415	359	0.04%	0.005%
76	10.683	2997	2999	3004	rVB2	466	306	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031477.D
 Acq On : 09 Jun 2023 03:14
 Operator : SY/MD
 Sample : 03106-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.786	3029	3031	3034	rBV3	333	216	0.02%	0.003%
78	10.821	3041	3042	3044	rBV	373	177	0.02%	0.002%
79	10.853	3048	3052	3053	rBV2	633	347	0.03%	0.005%
80	10.902	3065	3067	3069	rBV2	428	251	0.03%	0.003%
81	10.927	3072	3075	3078	rVV	523	266	0.03%	0.004%
82	11.008	3098	3100	3107	rVB3	369	377	0.04%	0.005%
83	11.107	3128	3131	3135	rVV3	367	220	0.02%	0.003%
84	11.191	3146	3157	3182	rBV	389964	621511	62.67%	8.484%
85	11.567	3261	3274	3292	rBV	413804	657260	66.27%	8.972%
86	11.750	3329	3331	3334	rBV2	440	170	0.02%	0.002%
87	11.821	3351	3353	3356	rBV2	699	406	0.04%	0.006%
88	11.953	3391	3394	3397	rBV2	539	301	0.03%	0.004%
89	12.098	3435	3439	3441	rBV2	542	367	0.04%	0.005%
90	12.191	3466	3468	3470	rBV2	396	177	0.02%	0.002%
91	12.345	3513	3516	3517	rBV	486	255	0.03%	0.003%
92	12.516	3566	3569	3570	rBV2	371	251	0.03%	0.003%
93	12.551	3576	3580	3581	rBV2	325	181	0.02%	0.002%
94	12.631	3602	3605	3609	rBV3	582	457	0.05%	0.006%
95	13.017	3722	3725	3726	rBV2	358	207	0.02%	0.003%
96	13.557	3890	3893	3895	rBV3	501	404	0.04%	0.006%
97	13.702	3936	3938	3941	rBV3	505	310	0.03%	0.004%
98	13.811	3970	3972	3976	rBV3	581	313	0.03%	0.004%
99	13.934	4008	4010	4012	rBV2	667	313	0.03%	0.004%
100	14.229	4100	4102	4103	rBV2	587	259	0.03%	0.004%




Sum of corrected areas: 7325351

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031477.D
Acq On : 09 Jun 2023 03:14
Operator : SY/MD
Sample : 03106-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

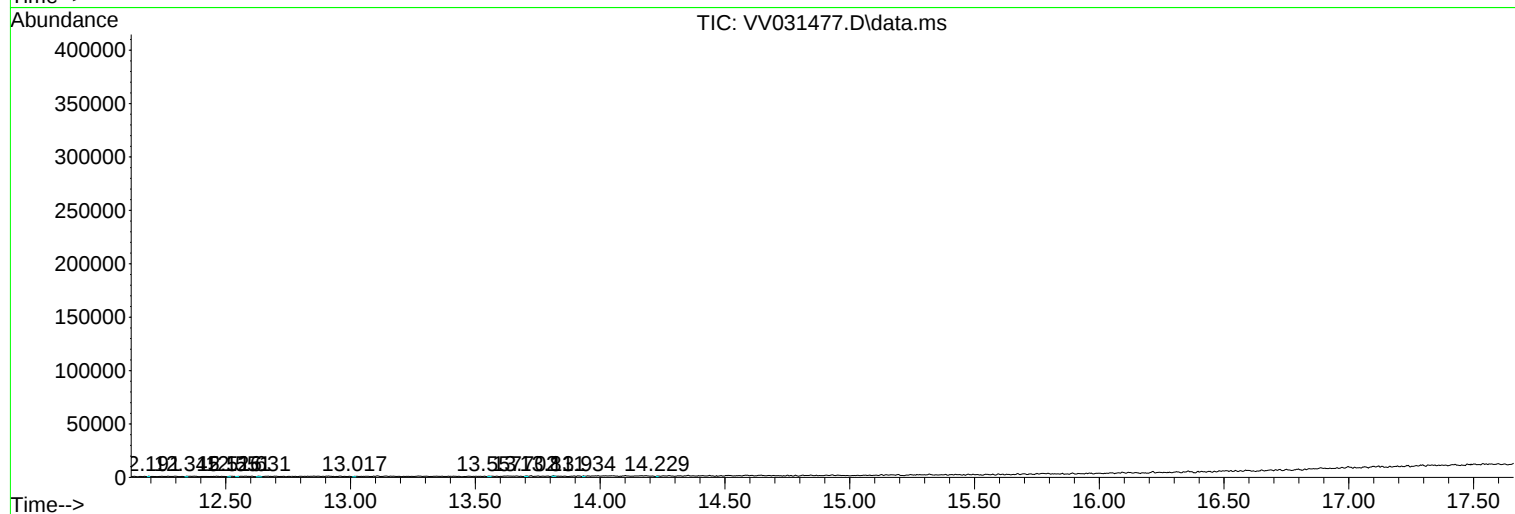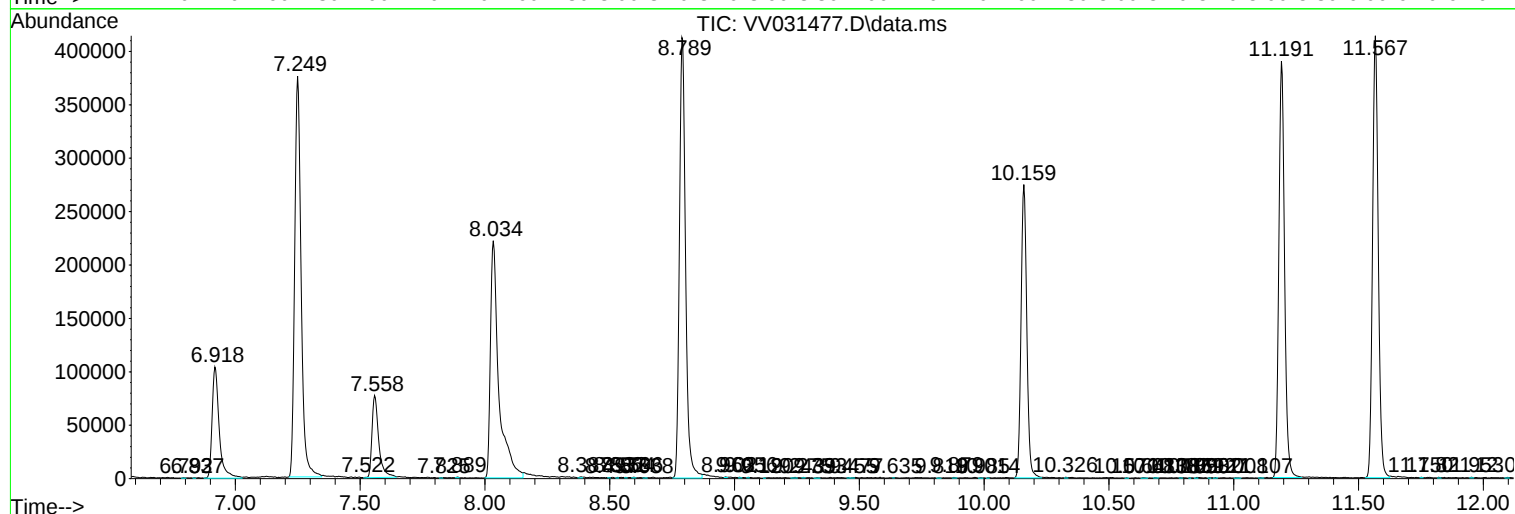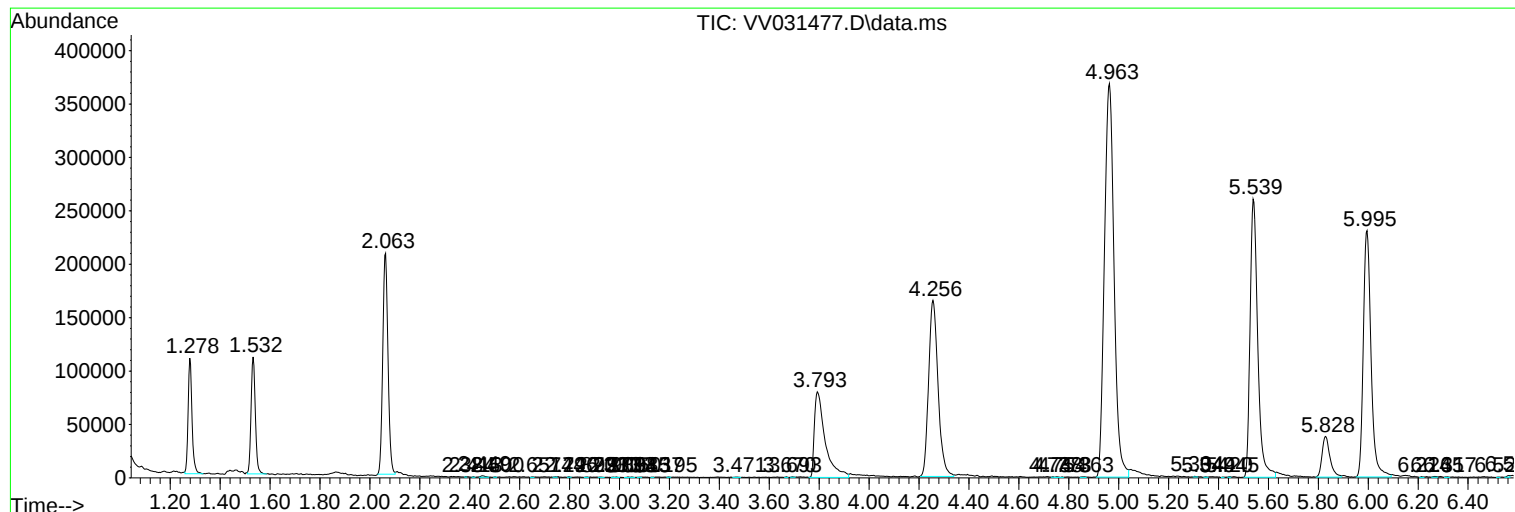

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031477.D
Acq On : 09 Jun 2023 03:14
Operator : SY/MD
Sample : 03106-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031477.D
Acq On : 09 Jun 2023 03:14
Operator : SY/MD
Sample : 03106-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------