

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031478.D
 Acq On : 09 Jun 2023 03:38
 Operator : SY/MD
 Sample : 03106-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FF4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031478.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	93	rVB	111119	121574	11.74%	1.565%
2	1.532	146	153	170	rVB	116253	136125	13.14%	1.752%
3	2.063	308	318	333	rBV	220697	328571	31.72%	4.229%
4	2.317	395	397	398	rBV	492	221	0.02%	0.003%
5	2.381	415	417	422	rVB4	507	345	0.03%	0.004%
6	2.449	435	438	441	rBV3	767	458	0.04%	0.006%
7	2.863	565	567	571	rBV3	506	330	0.03%	0.004%
8	2.925	583	586	588	rBV	421	223	0.02%	0.003%
9	2.941	588	591	595	rVB2	333	254	0.02%	0.003%
10	2.998	606	609	610	rBV2	327	163	0.02%	0.002%
11	3.101	637	641	644	rBV	414	334	0.03%	0.004%
12	3.285	694	698	699	rBV2	356	205	0.02%	0.003%
13	3.355	717	720	722	rBV	304	163	0.02%	0.002%
14	3.394	729	732	737	rBV2	396	329	0.03%	0.004%
15	3.487	758	761	764	rBV	458	360	0.03%	0.005%
16	3.667	813	817	819	rBV2	375	245	0.02%	0.003%
17	3.722	830	834	835	rBV2	502	281	0.03%	0.004%
18	3.796	846	857	891	rBV2	77991	236496	22.83%	3.044%
19	4.256	985	1000	1028	rBV	169094	440582	42.54%	5.670%
20	4.574	1097	1099	1101	rBV	549	223	0.02%	0.003%
21	4.892	1195	1198	1200	rBV3	273	168	0.02%	0.002%
22	4.963	1201	1220	1248	rBV2	386269	1035799	100.00%	13.330%
23	5.371	1345	1347	1350	rBV3	360	238	0.02%	0.003%
24	5.407	1356	1358	1361	rBV3	379	228	0.02%	0.003%
25	5.429	1361	1365	1367	rBV3	483	278	0.03%	0.004%
26	5.539	1387	1399	1433	rBV2	278937	599854	57.91%	7.720%
27	5.834	1475	1491	1521	rBV5	78898	199669	19.28%	2.570%
28	5.995	1528	1541	1576	rBV	238792	514058	49.63%	6.616%
29	6.236	1614	1616	1617	rBV	468	235	0.02%	0.003%
30	6.281	1627	1630	1636	rVB4	399	375	0.04%	0.005%
31	6.313	1636	1640	1643	rVB2	688	491	0.05%	0.006%
32	6.342	1643	1649	1653	rBV3	525	568	0.05%	0.007%
33	6.404	1665	1668	1670	rVB2	624	282	0.03%	0.004%
34	6.452	1679	1683	1687	rVB2	620	511	0.05%	0.007%
35	6.477	1689	1691	1693	rVV	341	173	0.02%	0.002%
36	6.490	1693	1695	1699	rVB2	588	355	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031478.D
 Acq On : 09 Jun 2023 03:38
 Operator : SY/MD
 Sample : 03106-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FF4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	6.532	1704	1708	1710	rVB	374	250	0.02%	0.003%
38	6.580	1710	1723	1726	rBV6	2039	3354	0.32%	0.043%
39	6.696	1757	1759	1761	rBV2	506	256	0.02%	0.003%
40	6.719	1765	1766	1769	rBV3	336	179	0.02%	0.002%
41	6.741	1771	1773	1777	rVB2	389	220	0.02%	0.003%
42	6.867	1809	1812	1813	rBV2	304	165	0.02%	0.002%
43	6.918	1817	1828	1857	rBV	105820	207695	20.05%	2.673%
44	7.249	1917	1931	1957	rBV	397394	727036	70.19%	9.357%
45	7.503	2005	2010	2013	rBV4	715	625	0.06%	0.008%
46	7.558	2018	2027	2051	rVV	77480	144406	13.94%	1.858%
47	7.908	2135	2136	2139	rVB2	773	280	0.03%	0.004%
48	7.947	2146	2148	2153	rVB	322	173	0.02%	0.002%
49	8.034	2165	2175	2209	rBV3	217148	498583	48.14%	6.417%
50	8.378	2280	2282	2283	rBV2	628	245	0.02%	0.003%
51	8.542	2331	2333	2336	rBV3	419	184	0.02%	0.002%
52	8.719	2387	2388	2393	rVB3	577	376	0.04%	0.005%
53	8.747	2393	2397	2398	rBV	439	263	0.03%	0.003%
54	8.789	2399	2410	2434	rBV	444795	752942	72.69%	9.690%
55	9.162	2524	2526	2529	rBV2	305	241	0.02%	0.003%
56	9.175	2529	2530	2533	rVV	576	194	0.02%	0.002%
57	9.191	2533	2535	2539	rVB2	517	343	0.03%	0.004%
58	9.217	2539	2543	2548	rVB3	572	536	0.05%	0.007%
59	9.243	2548	2551	2552	rBV	323	207	0.02%	0.003%
60	9.378	2589	2593	2594	rBV	476	291	0.03%	0.004%
61	9.439	2610	2612	2614	rBV	318	213	0.02%	0.003%
62	9.474	2619	2623	2628	rBV2	354	485	0.05%	0.006%
63	9.600	2659	2662	2665	rBV2	398	341	0.03%	0.004%
64	9.773	2715	2716	2718	rVB	505	177	0.02%	0.002%
65	9.831	2730	2734	2736	rVB2	335	170	0.02%	0.002%
66	9.850	2736	2740	2742	rBV3	571	400	0.04%	0.005%
67	9.870	2742	2746	2749	rBV3	567	523	0.05%	0.007%
68	9.976	2777	2779	2781	rBV2	434	265	0.03%	0.003%
69	10.159	2823	2836	2852	rBV	270577	430522	41.56%	5.541%
70	10.255	2864	2866	2867	rBV	431	201	0.02%	0.003%
71	10.455	2925	2928	2930	rBV	371	277	0.03%	0.004%
72	10.490	2936	2939	2943	rBV2	368	325	0.03%	0.004%
73	10.529	2948	2951	2955	rBV4	340	346	0.03%	0.004%
74	10.603	2972	2974	2978	rBV	413	242	0.02%	0.003%
75	10.693	3000	3002	3005	rBV3	356	236	0.02%	0.003%
76	10.747	3016	3019	3023	rVB2	626	394	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031478.D
 Acq On : 09 Jun 2023 03:38
 Operator : SY/MD
 Sample : 03106-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FF4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.773	3024	3027	3029	rBV	339	179	0.02%	0.002%
78	10.786	3029	3031	3036	rBV2	346	313	0.03%	0.004%
79	10.850	3046	3051	3052	rBV2	506	410	0.04%	0.005%
80	10.892	3062	3064	3066	rBV	413	272	0.03%	0.004%
81	11.017	3101	3103	3105	rBV2	532	252	0.02%	0.003%
82	11.098	3125	3128	3131	rBV2	316	237	0.02%	0.003%
83	11.191	3145	3157	3179	rBV	431228	680944	65.74%	8.764%
84	11.381	3213	3216	3218	rBV2	552	302	0.03%	0.004%
85	11.468	3239	3243	3247	rBV3	443	455	0.04%	0.006%
86	11.567	3261	3274	3290	rBV	432627	687665	66.39%	8.850%
87	11.866	3365	3367	3372	rVB2	508	222	0.02%	0.003%
88	11.934	3385	3388	3389	rBV2	393	222	0.02%	0.003%
89	11.979	3400	3402	3404	rBV2	624	241	0.02%	0.003%
90	12.445	3545	3547	3552	rVB2	553	316	0.03%	0.004%
91	13.001	3717	3720	3722	rBV2	442	345	0.03%	0.004%
92	13.123	3757	3758	3760	rBV	329	182	0.02%	0.002%
93	13.352	3825	3829	3830	rBV3	460	349	0.03%	0.004%
94	13.477	3866	3868	3870	rBV2	498	243	0.02%	0.003%
95	13.513	3877	3879	3884	rVB3	897	511	0.05%	0.007%
96	13.638	3916	3918	3919	rBV2	569	211	0.02%	0.003%
97	13.683	3930	3932	3933	rBV	627	248	0.02%	0.003%
98	14.098	4059	4061	4062	rBV2	461	192	0.02%	0.002%
99	14.178	4084	4086	4092	rVB3	735	699	0.07%	0.009%
100	14.445	4167	4169	4170	rBV2	607	234	0.02%	0.003%




Sum of corrected areas: 7770169

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031478.D
Acq On : 09 Jun 2023 03:38
Operator : SY/MD
Sample : 03106-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FF4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

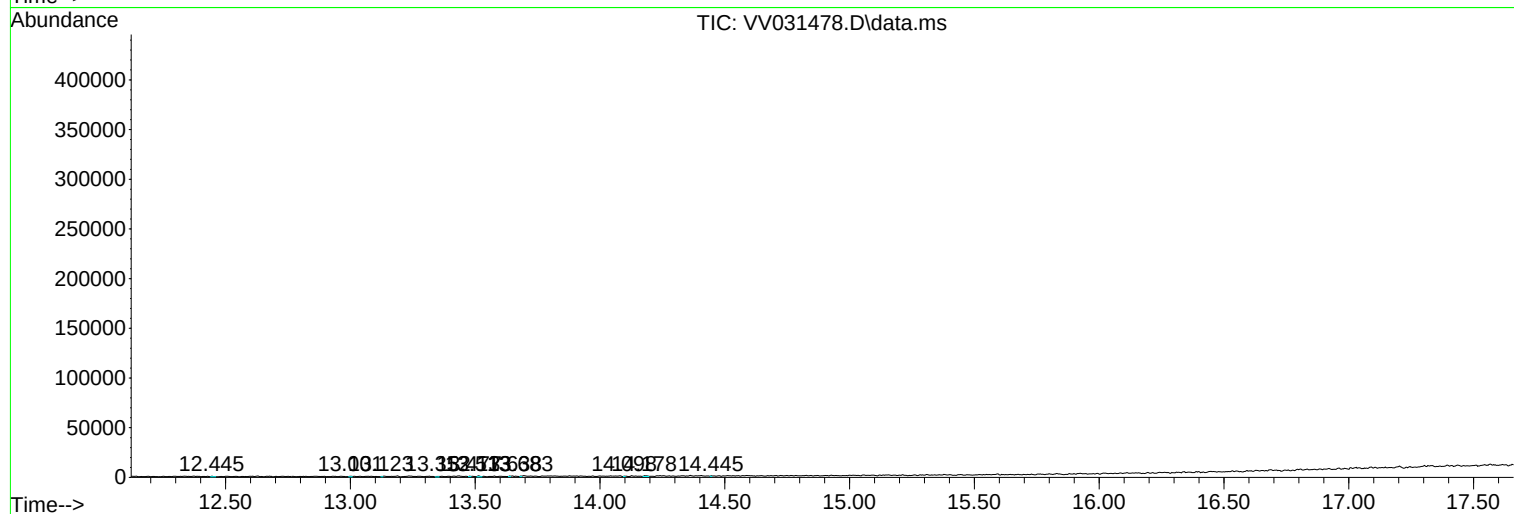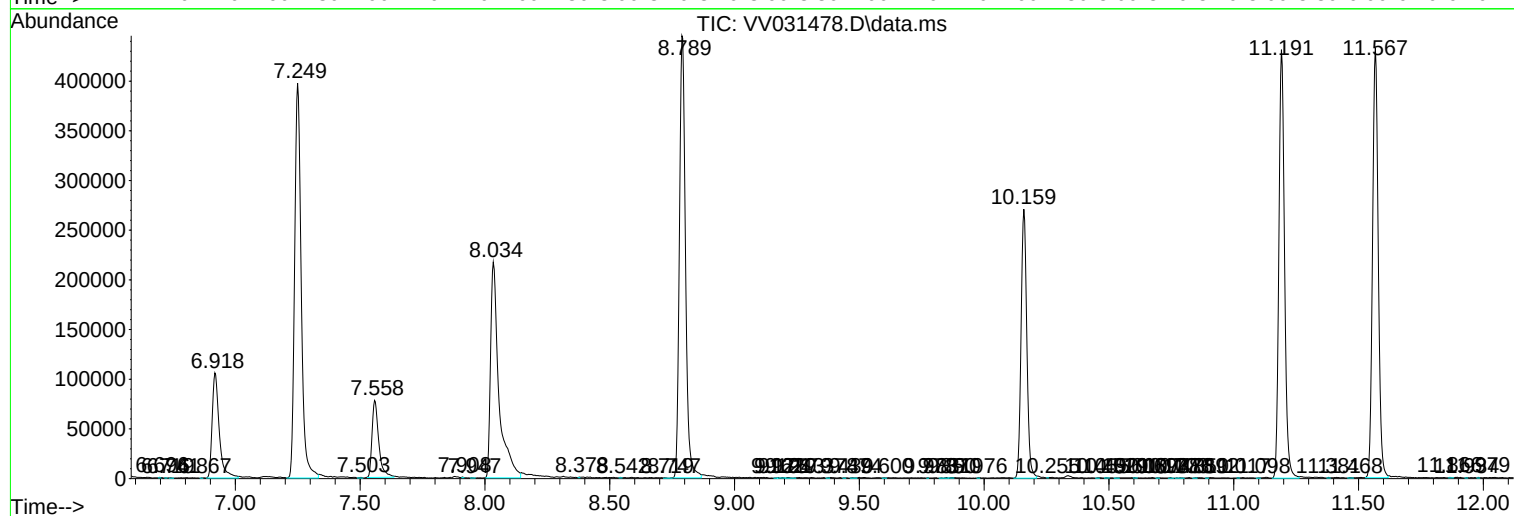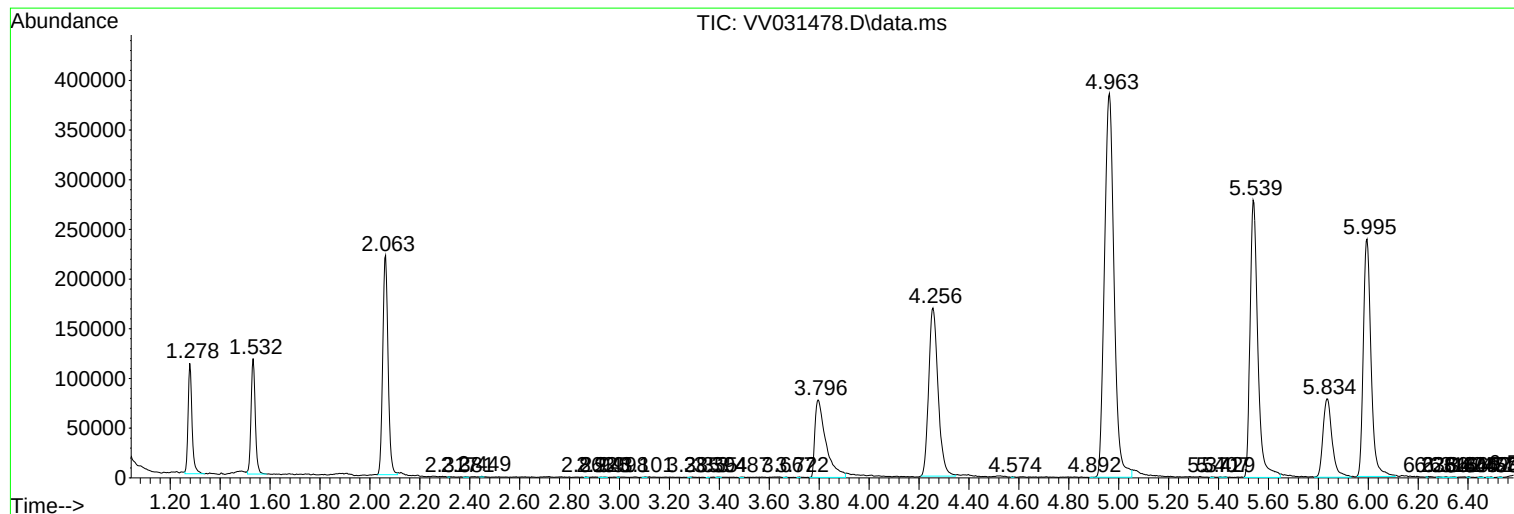

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031478.D
Acq On : 09 Jun 2023 03:38
Operator : SY/MD
Sample : 03106-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FF4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031478.D
Acq On : 09 Jun 2023 03:38
Operator : SY/MD
Sample : 03106-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FF4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------