

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031479.D
 Acq On : 09 Jun 2023 04:01
 Operator : SY/MD
 Sample : 03098-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZEQ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031479.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	84	rVB	117703	121867	11.48%	1.568%
2	1.532	146	153	168	rVB	121028	140126	13.20%	1.803%
3	2.063	308	318	331	rBV	233122	342192	32.24%	4.402%
4	2.275	383	384	387	rBV2	410	173	0.02%	0.002%
5	2.381	414	417	418	rBV2	430	199	0.02%	0.003%
6	2.606	485	487	493	rVB3	430	197	0.02%	0.003%
7	2.754	530	533	536	rBV3	540	327	0.03%	0.004%
8	2.854	562	564	566	rBV	443	236	0.02%	0.003%
9	2.902	576	579	580	rBV2	481	222	0.02%	0.003%
10	2.941	587	591	595	rBV2	231	232	0.02%	0.003%
11	3.015	610	614	617	rBV	445	332	0.03%	0.004%
12	3.060	624	628	631	rBV2	410	344	0.03%	0.004%
13	3.098	637	640	642	rVV	543	269	0.03%	0.003%
14	3.121	642	647	649	rVV2	490	490	0.05%	0.006%
15	3.240	683	684	688	rBV	537	253	0.02%	0.003%
16	3.304	701	704	707	rBV2	305	255	0.02%	0.003%
17	3.343	711	716	720	rBV4	474	475	0.04%	0.006%
18	3.378	723	727	729	rBV	373	262	0.02%	0.003%
19	3.397	729	733	736	rVB2	434	392	0.04%	0.005%
20	3.458	749	752	758	rBV2	322	190	0.02%	0.002%
21	3.494	759	763	765	rBV2	328	179	0.02%	0.002%
22	3.526	770	773	777	rBV	344	338	0.03%	0.004%
23	3.571	785	787	792	rVB2	494	296	0.03%	0.004%
24	3.597	792	795	797	rBV2	292	193	0.02%	0.002%
25	3.642	807	809	813	rVB2	488	296	0.03%	0.004%
26	3.699	823	827	832	rBV2	554	436	0.04%	0.006%
27	3.732	832	837	839	rVB3	457	413	0.04%	0.005%
28	3.748	839	842	845	rBV3	346	244	0.02%	0.003%
29	3.796	847	857	883	rBV	76765	219432	20.67%	2.823%
30	4.256	984	1000	1026	rBV	175071	455178	42.88%	5.856%
31	4.526	1081	1084	1087	rVB3	1361	890	0.08%	0.011%
32	4.542	1087	1089	1091	rBV2	652	391	0.04%	0.005%
33	4.680	1130	1132	1137	rBV2	452	472	0.04%	0.006%
34	4.760	1154	1157	1161	rBV	482	350	0.03%	0.005%
35	4.815	1172	1174	1176	rBV2	374	191	0.02%	0.002%
36	4.963	1202	1220	1245	rBV2	396060	1061431	100.00%	13.655%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031479.D
 Acq On : 09 Jun 2023 04:01
 Operator : SY/MD
 Sample : 03098-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZEQ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	5.465	1373	1376	1378	rBV	348	216	0.02%	0.003%
38	5.539	1387	1399	1433	rBV	275918	589586	55.55%	7.585%
39	5.828	1479	1489	1507	rBV	37687	77353	7.29%	0.995%
40	5.995	1528	1541	1570	rBV	244344	520832	49.07%	6.700%
41	6.249	1616	1620	1622	rBV4	633	588	0.06%	0.008%
42	6.320	1639	1642	1643	rBV	504	264	0.02%	0.003%
43	6.349	1649	1651	1655	rVB3	608	332	0.03%	0.004%
44	6.445	1679	1681	1683	rVB	555	297	0.03%	0.004%
45	6.526	1705	1706	1710	rVB	341	171	0.02%	0.002%
46	6.577	1710	1722	1724	rBV8	1614	2743	0.26%	0.035%
47	6.918	1816	1828	1851	rBV	107778	211286	19.91%	2.718%
48	7.249	1920	1931	1961	rBV	416854	747806	70.45%	9.620%
49	7.558	2018	2027	2052	rBV	82243	151499	14.27%	1.949%
50	7.738	2080	2083	2087	rBV4	522	370	0.03%	0.005%
51	7.873	2121	2125	2126	rBV3	873	554	0.05%	0.007%
52	7.957	2148	2151	2152	rBV	448	226	0.02%	0.003%
53	8.034	2164	2175	2221	rBV2	218264	511271	48.17%	6.577%
54	8.683	2375	2377	2381	rVB3	569	291	0.03%	0.004%
55	8.789	2396	2410	2436	rBV	443543	748756	70.54%	9.632%
56	9.239	2545	2550	2557	rBV3	684	898	0.08%	0.012%
57	9.278	2559	2562	2564	rBV	373	232	0.02%	0.003%
58	9.291	2564	2566	2569	rBV2	397	234	0.02%	0.003%
59	9.432	2605	2610	2614	rVB3	558	578	0.05%	0.007%
60	9.455	2614	2617	2619	rVB2	409	203	0.02%	0.003%
61	9.471	2619	2622	2625	rBV	277	190	0.02%	0.002%
62	9.493	2627	2629	2634	rVV3	496	377	0.04%	0.005%
63	9.651	2675	2678	2679	rBV2	325	208	0.02%	0.003%
64	9.783	2716	2719	2722	rBV2	550	310	0.03%	0.004%
65	9.837	2734	2736	2739	rVB	467	245	0.02%	0.003%
66	9.866	2739	2745	2746	rBV2	701	535	0.05%	0.007%
67	9.927	2761	2764	2766	rBV2	359	224	0.02%	0.003%
68	10.072	2805	2809	2811	rBV2	934	507	0.05%	0.007%
69	10.159	2824	2836	2863	rVV	281093	453314	42.71%	5.832%
70	10.291	2874	2877	2880	rBV	461	295	0.03%	0.004%
71	10.442	2921	2924	2929	rVB	563	373	0.04%	0.005%
72	10.493	2929	2940	2942	rBV5	878	1198	0.11%	0.015%
73	10.513	2942	2946	2947	rBV	423	185	0.02%	0.002%
74	10.616	2975	2978	2981	rVB3	621	468	0.04%	0.006%
75	10.693	2999	3002	3008	rVB2	398	350	0.03%	0.005%
76	10.911	3067	3070	3075	rVB2	382	363	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031479.D
 Acq On : 09 Jun 2023 04:01
 Operator : SY/MD
 Sample : 03098-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZEQ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.944	3078	3080	3083	rVB	388	217	0.02%	0.003%
78	11.091	3123	3126	3129	rBV2	306	217	0.02%	0.003%
79	11.130	3136	3138	3143	rVB	336	173	0.02%	0.002%
80	11.191	3143	3157	3182	rBV	428073	676846	63.77%	8.707%
81	11.358	3207	3209	3212	rVB2	614	260	0.02%	0.003%
82	11.442	3233	3235	3237	rBV2	383	189	0.02%	0.002%
83	11.567	3263	3274	3296	rBV	453355	714726	67.34%	9.195%
84	11.956	3393	3395	3399	rVB3	439	248	0.02%	0.003%
85	12.181	3463	3465	3468	rBV2	368	282	0.03%	0.004%
86	12.230	3478	3480	3484	rVB3	493	269	0.03%	0.003%
87	12.249	3484	3486	3488	rBV	429	228	0.02%	0.003%
88	12.644	3607	3609	3613	rVB2	469	318	0.03%	0.004%
89	12.747	3639	3641	3645	rVB3	332	196	0.02%	0.003%
90	12.776	3645	3650	3651	rBV2	548	406	0.04%	0.005%
91	12.812	3659	3661	3664	rVB	635	319	0.03%	0.004%
92	12.853	3672	3674	3676	rBV2	362	185	0.02%	0.002%
93	13.053	3733	3736	3739	rBV2	509	335	0.03%	0.004%
94	13.223	3786	3789	3792	rVB2	707	401	0.04%	0.005%
95	13.310	3814	3816	3820	rBV2	343	211	0.02%	0.003%
96	13.426	3849	3852	3854	rBV3	638	398	0.04%	0.005%
97	13.734	3945	3948	3951	rBV2	664	398	0.04%	0.005%
98	13.953	4014	4016	4018	rBV	555	250	0.02%	0.003%
99	14.075	4052	4054	4055	rBV2	575	290	0.03%	0.004%
100	14.644	4228	4231	4232	rBV2	780	498	0.05%	0.006%




Sum of corrected areas: 7773351

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031479.D
Acq On : 09 Jun 2023 04:01
Operator : SY/MD
Sample : 03098-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZEQ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

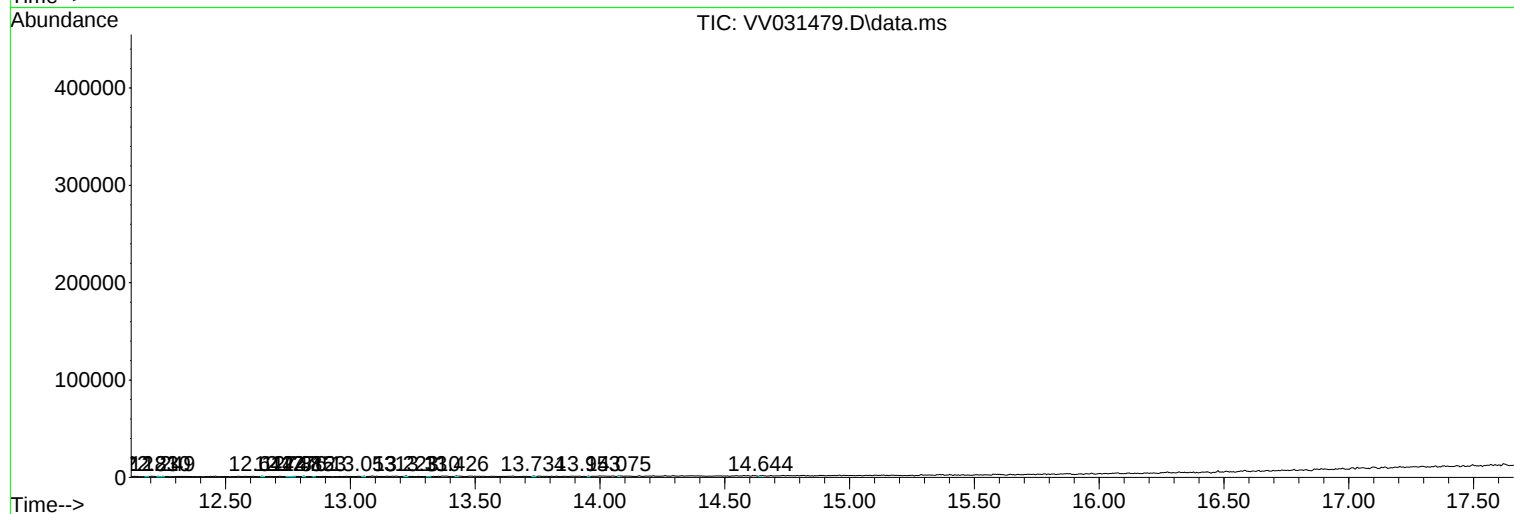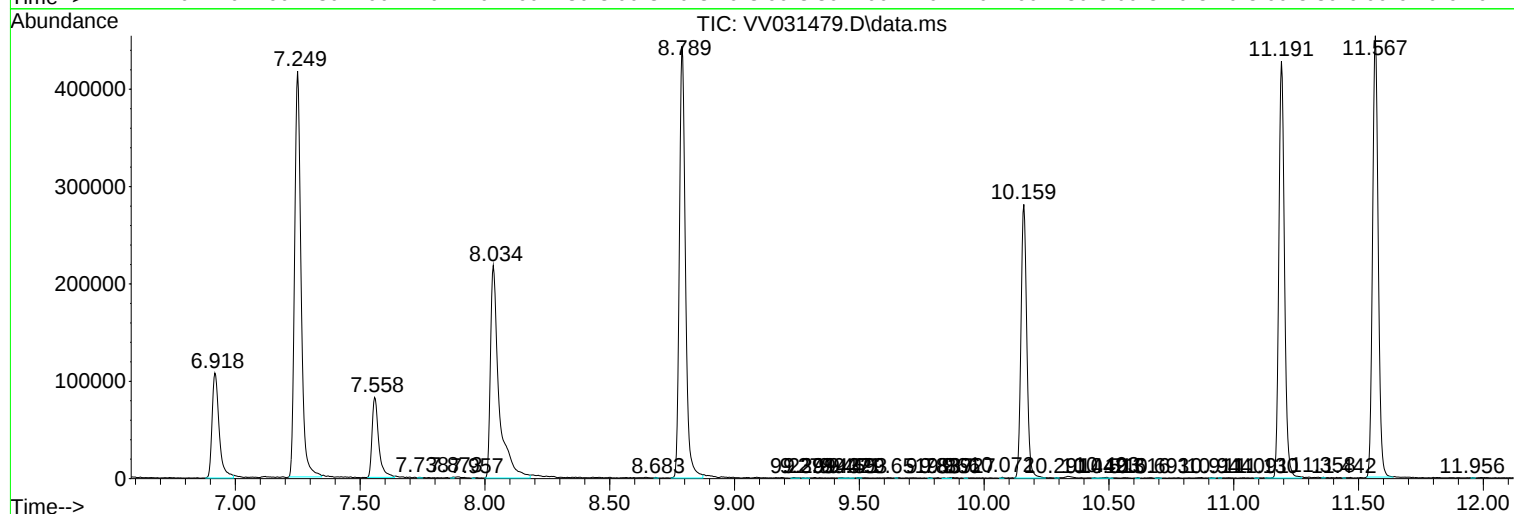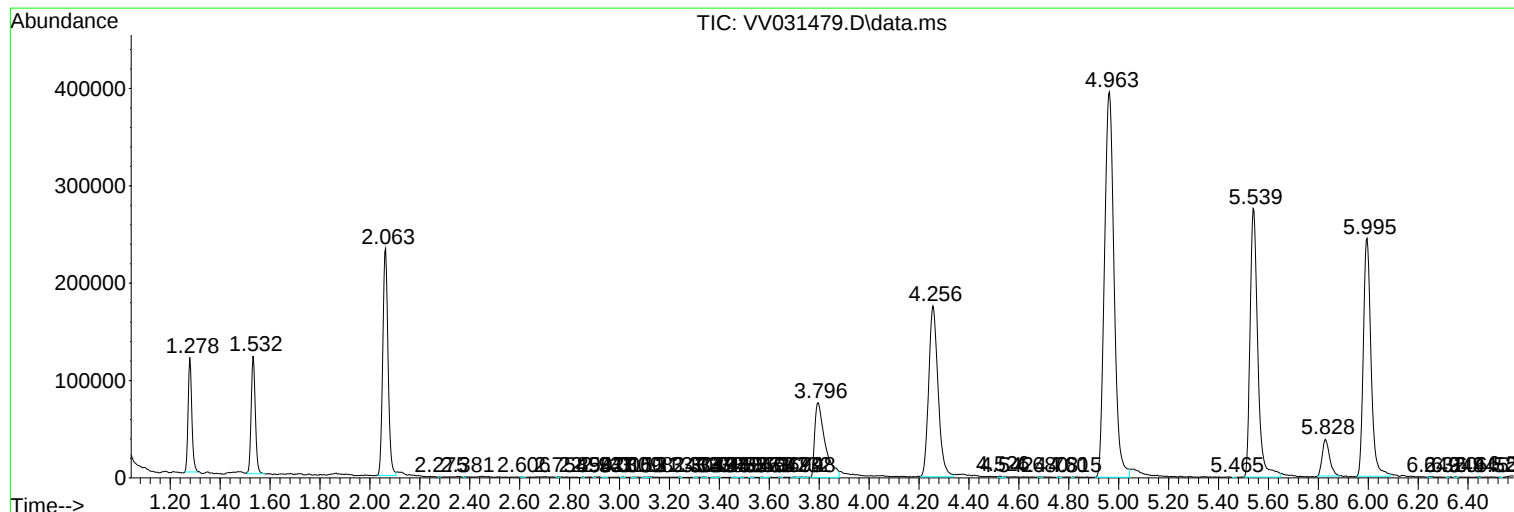

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031479.D
Acq On : 09 Jun 2023 04:01
Operator : SY/MD
Sample : 03098-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZEQ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031479.D
Acq On : 09 Jun 2023 04:01
Operator : SY/MD
Sample : 03098-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZEQ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------