

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031480.D
 Acq On : 09 Jun 2023 04:25
 Operator : SY/MD
 Sample : 03098-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZEP8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031480.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	85	rVB	116875	122449	11.81%	1.600%
2	1.532	146	153	168	rVB	118515	139426	13.45%	1.821%
3	2.063	307	318	332	rBV	225571	336798	32.49%	4.400%
4	2.455	435	440	444	rBV2	1002	961	0.09%	0.013%
5	2.609	486	488	493	rVB3	261	261	0.03%	0.003%
6	2.667	503	506	508	rBV2	482	285	0.03%	0.004%
7	2.786	540	543	549	rBV3	463	347	0.03%	0.005%
8	2.886	572	574	578	rVB4	490	308	0.03%	0.004%
9	3.114	642	645	648	rVB5	398	258	0.02%	0.003%
10	3.133	648	651	654	rBV2	368	225	0.02%	0.003%
11	3.268	689	693	696	rBV3	273	209	0.02%	0.003%
12	3.307	703	705	709	rBV	487	339	0.03%	0.004%
13	3.400	732	734	737	rBV3	386	220	0.02%	0.003%
14	3.468	752	755	757	rVV	315	257	0.02%	0.003%
15	3.500	760	765	767	rBV3	364	210	0.02%	0.003%
16	3.564	780	785	789	rVB3	386	303	0.03%	0.004%
17	3.587	789	792	793	rBV2	545	329	0.03%	0.004%
18	3.690	820	824	828	rBV4	405	295	0.03%	0.004%
19	3.728	832	836	839	rBV3	325	253	0.02%	0.003%
20	3.793	845	856	885	rBV	80703	221202	21.34%	2.890%
21	4.256	983	1000	1030	rBV	172015	450706	43.48%	5.888%
22	4.555	1090	1093	1095	rBV2	472	359	0.03%	0.005%
23	4.793	1165	1167	1170	rBV2	412	239	0.02%	0.003%
24	4.815	1170	1174	1178	rVB4	402	415	0.04%	0.005%
25	4.854	1178	1186	1189	rBV3	781	853	0.08%	0.011%
26	4.963	1202	1220	1242	rBV2	388913	1036554	100.00%	13.541%
27	5.281	1315	1319	1322	rBV3	794	546	0.05%	0.007%
28	5.301	1322	1325	1329	rVB3	822	546	0.05%	0.007%
29	5.384	1349	1351	1354	rBV3	486	240	0.02%	0.003%
30	5.426	1362	1364	1368	rVV2	633	302	0.03%	0.004%
31	5.538	1387	1399	1423	rBV	270321	571707	55.15%	7.469%
32	5.828	1478	1489	1507	rBV2	39323	85759	8.27%	1.120%
33	5.995	1527	1541	1570	rVV	243924	516503	49.83%	6.747%
34	6.201	1603	1605	1606	rBV2	680	231	0.02%	0.003%
35	6.259	1620	1623	1628	rBV5	532	555	0.05%	0.007%
36	6.391	1659	1664	1665	rBV	349	240	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031480.D
 Acq On : 09 Jun 2023 04:25
 Operator : SY/MD
 Sample : 03098-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZEP8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	6.477	1689	1691	1694	rVB2	960	391	0.04%	0.005%
38	6.564	1712	1718	1720	rBV3	1677	1855	0.18%	0.024%
39	6.664	1747	1749	1752	rVV	420	247	0.02%	0.003%
40	6.780	1781	1785	1786	rBV	330	263	0.03%	0.003%
41	6.805	1791	1793	1799	rVB4	462	327	0.03%	0.004%
42	6.918	1816	1828	1850	rBV2	106283	206026	19.88%	2.691%
43	7.249	1919	1931	1966	rBV	411443	740553	71.44%	9.674%
44	7.558	2018	2027	2050	rBV	81635	147052	14.19%	1.921%
45	7.783	2095	2097	2099	rBV2	582	275	0.03%	0.004%
46	7.841	2113	2115	2117	rBV	422	255	0.02%	0.003%
47	7.924	2139	2141	2146	rVB3	628	369	0.04%	0.005%
48	8.030	2162	2174	2213	rBV2	211071	498637	48.11%	6.514%
49	8.500	2315	2320	2321	rBV2	351	312	0.03%	0.004%
50	8.590	2346	2348	2350	rBV2	441	226	0.02%	0.003%
51	8.632	2358	2361	2363	rBV3	593	268	0.03%	0.004%
52	8.664	2368	2371	2372	rBV2	445	212	0.02%	0.003%
53	8.789	2399	2410	2439	rBV	439375	734084	70.82%	9.590%
54	9.024	2478	2483	2487	rVB4	746	616	0.06%	0.008%
55	9.053	2487	2492	2494	rBV	435	399	0.04%	0.005%
56	9.082	2496	2501	2506	rBV5	754	937	0.09%	0.012%
57	9.194	2533	2536	2539	rBV2	376	235	0.02%	0.003%
58	9.220	2539	2544	2546	rBV2	464	367	0.04%	0.005%
59	9.281	2561	2563	2568	rVB4	598	438	0.04%	0.006%
60	9.371	2588	2591	2595	rBV3	707	562	0.05%	0.007%
61	9.500	2628	2631	2634	rVB2	596	391	0.04%	0.005%
62	9.525	2634	2639	2643	rBV2	612	539	0.05%	0.007%
63	9.593	2656	2660	2664	rBV3	584	498	0.05%	0.007%
64	9.625	2667	2670	2671	rBV	341	206	0.02%	0.003%
65	9.677	2682	2686	2688	rBV2	413	363	0.04%	0.005%
66	9.738	2703	2705	2710	rVB2	445	328	0.03%	0.004%
67	9.763	2710	2713	2715	rBV2	326	219	0.02%	0.003%
68	9.850	2736	2740	2741	rBV3	320	254	0.02%	0.003%
69	9.950	2766	2771	2773	rBV3	425	320	0.03%	0.004%
70	10.085	2810	2813	2816	rVB2	398	221	0.02%	0.003%
71	10.107	2816	2820	2821	rBV2	353	239	0.02%	0.003%
72	10.159	2824	2836	2859	rVV	277253	442137	42.65%	5.776%
73	10.336	2885	2891	2895	rVB5	1857	2066	0.20%	0.027%
74	10.487	2933	2938	2946	rVB3	364	497	0.05%	0.006%
75	10.532	2950	2952	2956	rVB2	461	207	0.02%	0.003%
76	10.648	2984	2988	2990	rVB	498	311	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031480.D
 Acq On : 09 Jun 2023 04:25
 Operator : SY/MD
 Sample : 03098-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZEP8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.670	2991	2995	2998	rBV2	428	328	0.03%	0.004%
78	10.715	3008	3009	3014	rVB3	413	267	0.03%	0.003%
79	10.757	3019	3022	3024	rBV3	487	324	0.03%	0.004%
80	10.927	3071	3075	3077	rBV2	348	259	0.02%	0.003%
81	11.011	3099	3101	3104	rVB	653	294	0.03%	0.004%
82	11.062	3114	3117	3118	rBV2	342	218	0.02%	0.003%
83	11.191	3146	3157	3181	rBV	420270	663002	63.96%	8.661%
84	11.471	3241	3244	3245	rBV2	427	250	0.02%	0.003%
85	11.567	3262	3274	3292	rBV	448192	709764	68.47%	9.272%
86	11.763	3333	3335	3341	rBV2	467	330	0.03%	0.004%
87	12.120	3443	3446	3450	rVB3	513	417	0.04%	0.005%
88	12.178	3461	3464	3465	rBV2	334	216	0.02%	0.003%
89	12.564	3581	3584	3586	rBV	556	350	0.03%	0.005%
90	12.606	3594	3597	3599	rBV2	358	249	0.02%	0.003%
91	12.705	3624	3628	3630	rBV2	490	354	0.03%	0.005%
92	12.734	3634	3637	3641	rVB3	786	534	0.05%	0.007%
93	12.821	3661	3664	3670	rBV2	604	488	0.05%	0.006%
94	13.078	3740	3744	3746	rBV3	608	509	0.05%	0.007%
95	13.207	3780	3784	3787	rBV3	802	667	0.06%	0.009%
96	13.609	3904	3909	3911	rBV	518	423	0.04%	0.006%
97	13.702	3936	3938	3942	rVB2	678	395	0.04%	0.005%
98	13.725	3942	3945	3948	rBV3	387	242	0.02%	0.003%
99	13.741	3948	3950	3954	rBV2	553	400	0.04%	0.005%
100	13.760	3954	3956	3958	rBV2	430	223	0.02%	0.003%

Sum of corrected areas: 7654895




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031480.D
Acq On : 09 Jun 2023 04:25
Operator : SY/MD
Sample : 03098-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZEP8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

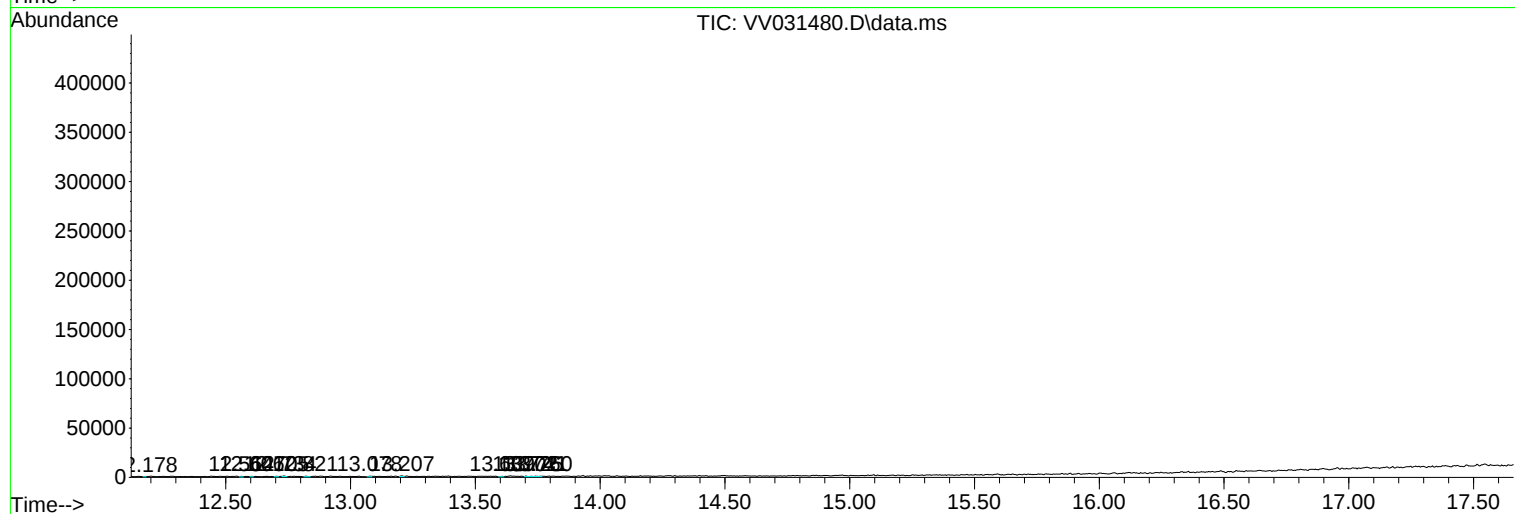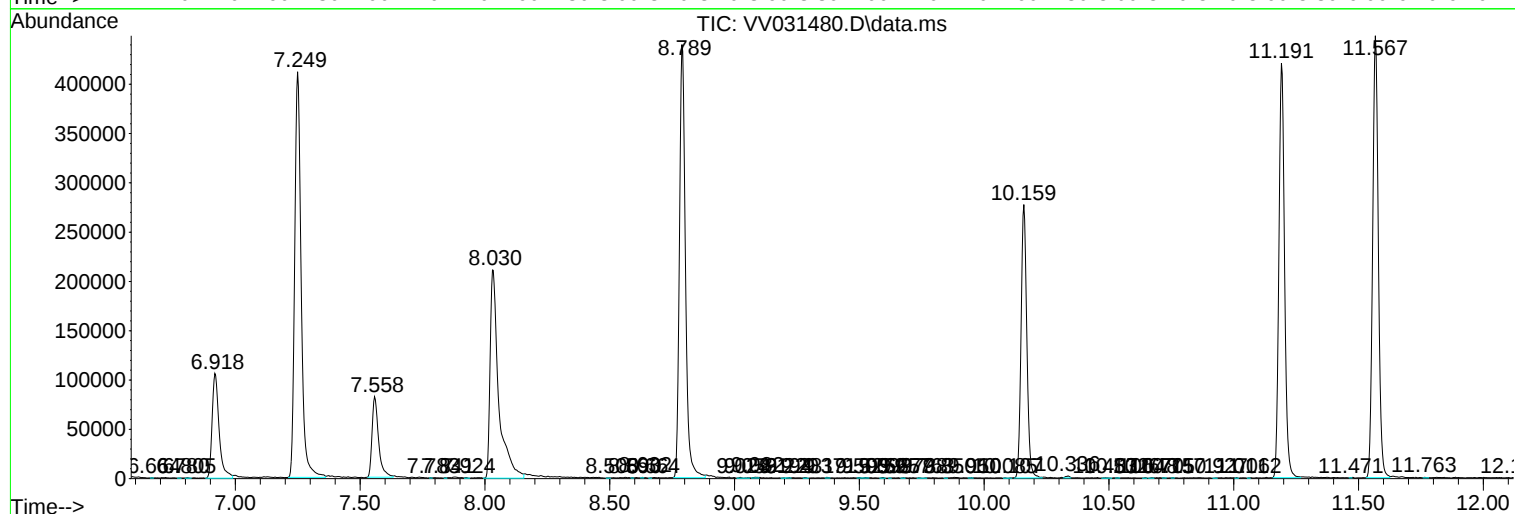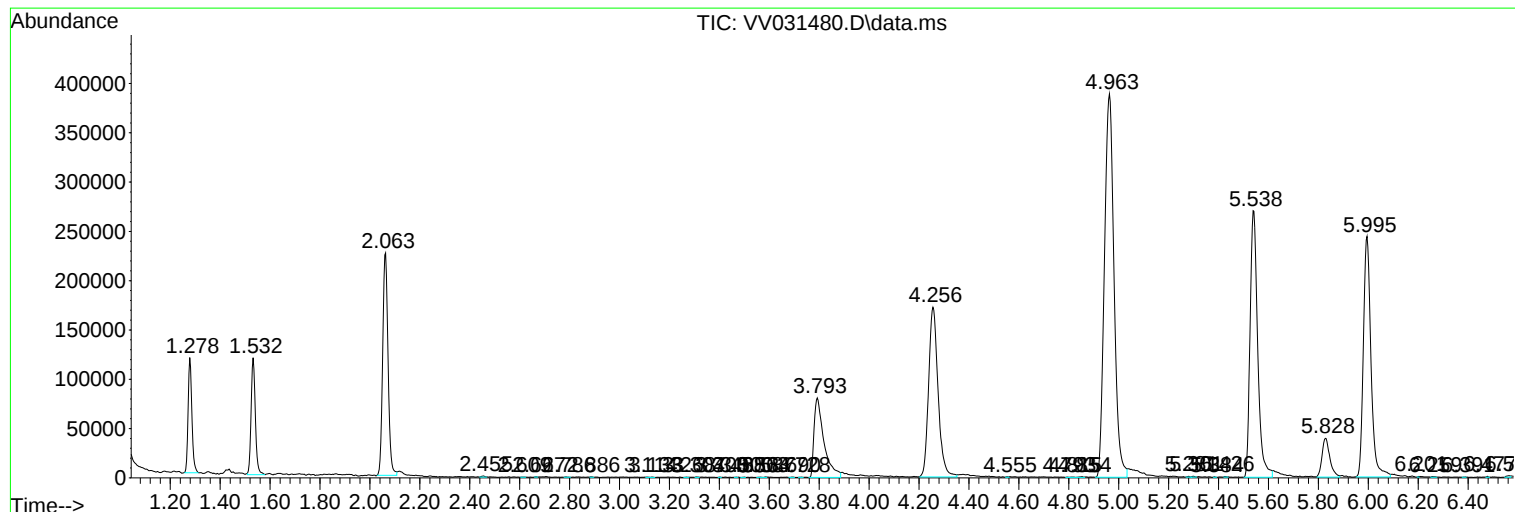

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031480.D
Acq On : 09 Jun 2023 04:25
Operator : SY/MD
Sample : 03098-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZEP8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031480.D
Acq On : 09 Jun 2023 04:25
Operator : SY/MD
Sample : 03098-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZEP8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------