


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031434.D
Acq On : 08 Jun 2023 08:32
Operator : SY/MD
Sample : BFB383
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB383

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Title : VOC Analysis
Last Update : Fri Jun 09 06:27:10 2023

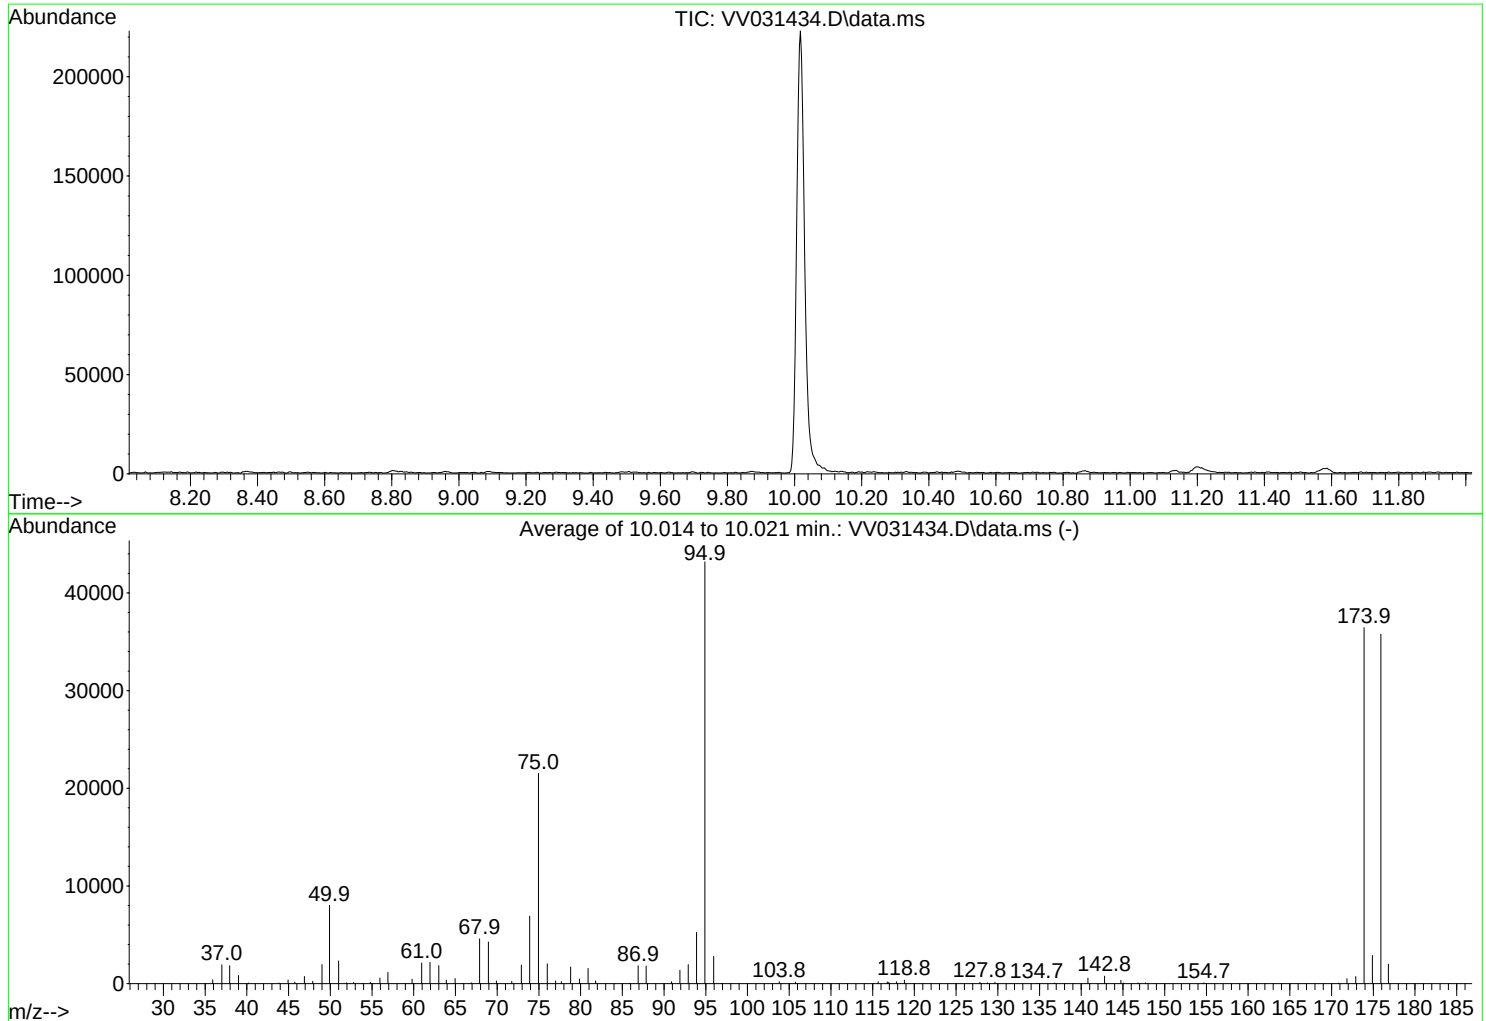

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2780

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.5	8007	PASS
75	95	30	80	49.8	21523	PASS
95	95	100	100	100.0	43184	PASS
96	95	5	9	6.4	2778	PASS
173	174	0.00	2	2.0	718	PASS
174	95	50	120	84.4	36440	PASS
175	174	5	9	7.9	2882	PASS
176	174	95	105	98.2	35781	PASS
177	176	5	10	5.6	2006	PASS

m/z	Abundance
40.00	207.0
43.90	376.0

Instrument :
MSVOA_V
ClientSampleId :
BFB383

m/z	Abundance
35.90	390.0
37.00	1985.0
38.00	1823.0
39.00	819.0
40.20	216.0
43.90	510.0
45.00	363.0
45.80	172.0
46.90	696.0
47.90	212.0
49.00	2002.0
49.90	8097.0
51.00	2342.0
52.80	102.0
54.80	136.0
56.00	611.0
56.90	1199.0
59.80	504.0
60.90	2203.0
62.00	2020.0
63.00	1915.0
63.90	368.0
65.00	566.0
66.90	159.0
67.90	4546.0
68.90	4248.0
69.90	254.0
71.70	216.0
72.90	1869.0
73.90	7048.0
75.00	21344.0
76.00	2201.0
76.90	275.0
77.70	221.0
78.80	1699.0
79.90	426.0
80.90	1481.0
81.80	294.0
86.90	1992.0
87.90	1640.0
90.90	163.0
91.90	1439.0
92.90	1979.0
93.90	5175.0
94.90	43136.0
96.00	2913.0
96.90	107.0
103.80	187.0
105.90	175.0
115.60	172.0
116.70	291.0
117.80	197.0
118.80	378.0
127.80	132.0
128.80	121.0
129.60	128.0
134.70	122.0
140.80	490.0
142.80	796.0
144.80	348.0
154.70	120.0
171.80	492.0
172.90	774.0
173.90	36256.0
174.90	2765.0
175.90	35424.0
176.80	1983.0

Instrument :
MSVOA_V
ClientSampleId :
BFB383

m/z	Abundance
35.90	418.0
37.00	2037.0
38.00	1836.0
39.00	850.0
39.80	204.0
43.80	444.0
44.90	391.0
45.80	164.0
46.90	758.0
47.90	266.0
49.00	2007.0
49.90	8250.0
51.00	2428.0
51.90	116.0
52.80	109.0
54.80	129.0
56.00	567.0
56.90	1195.0
59.80	452.0
61.00	2186.0
62.00	2270.0
63.00	1905.0
63.90	352.0
65.00	548.0
66.90	108.0
67.90	4737.0
68.90	4358.0
69.90	276.0
71.70	243.0
72.90	1952.0
73.90	7085.0
74.90	22200.0
76.00	2089.0
77.00	273.0
77.70	221.0
78.80	1767.0
79.90	471.0
80.90	1596.0
81.80	266.0
86.90	1912.0
87.90	1898.0
90.90	224.0
91.90	1452.0
92.90	1990.0
93.90	5424.0
94.90	44592.0
95.90	2826.0
103.80	201.0
105.70	164.0
115.70	226.0
116.80	234.0
117.00	239.0
117.90	189.0
118.80	389.0
127.80	148.0
129.70	113.0
136.80	108.0
140.80	625.0
142.80	828.0
144.70	380.0
146.80	111.0
147.70	118.0
154.70	114.0
170.80	104.0
171.80	540.0
172.90	768.0
173.90	37528.0
174.90	2961.0
175.90	37048.0
176.80	2055.0

Instrument :
MSVOA_V
ClientSampleId :
BFB383

m/z	Abundance
35.90	393.0
37.00	1765.0
37.90	1846.0
39.00	838.0
39.80	231.0
43.80	351.0
44.90	375.0
45.70	140.0
46.90	754.0
47.90	253.0
49.00	1816.0
49.90	7674.0
51.00	2235.0
52.00	143.0
52.80	115.0
53.80	105.0
54.80	128.0
55.90	528.0
56.90	1045.0
59.80	406.0
61.00	1953.0
61.90	2246.0
63.00	1722.0
63.90	362.0
64.80	484.0
65.80	103.0
67.90	4495.0
69.00	4158.0
69.90	286.0
71.80	233.0
72.90	1903.0
73.90	6599.0
74.90	21024.0
76.00	1799.0
77.10	287.0
77.70	197.0
78.80	1671.0
79.80	509.0
80.90	1581.0
81.80	272.0
85.90	115.0
86.90	1607.0
87.80	1866.0
90.90	221.0
91.90	1263.0
92.90	1908.0
93.90	5136.0
94.90	41824.0
95.90	2594.0
103.80	208.0
105.70	168.0
115.70	204.0
116.90	232.0
117.90	190.0
118.80	314.0
127.90	185.0
128.70	109.0
129.70	139.0
136.80	106.0
140.80	618.0
142.80	714.0
144.70	325.0
145.10	192.0
146.80	129.0
147.70	154.0
170.80	112.0
171.90	487.0
172.90	613.0
173.90	35536.0
174.90	2921.0
175.90	34872.0
176.80	1979.0

Instrument :
MSVOA_V
ClientSampleId :
BFB383