
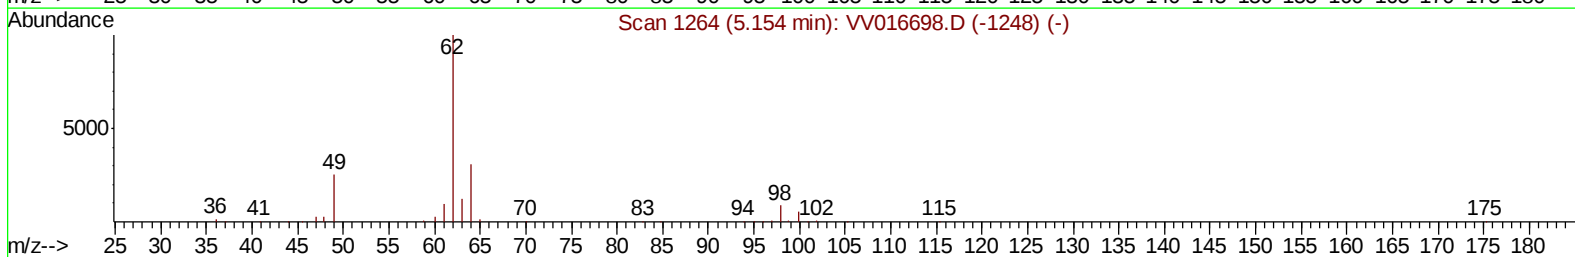
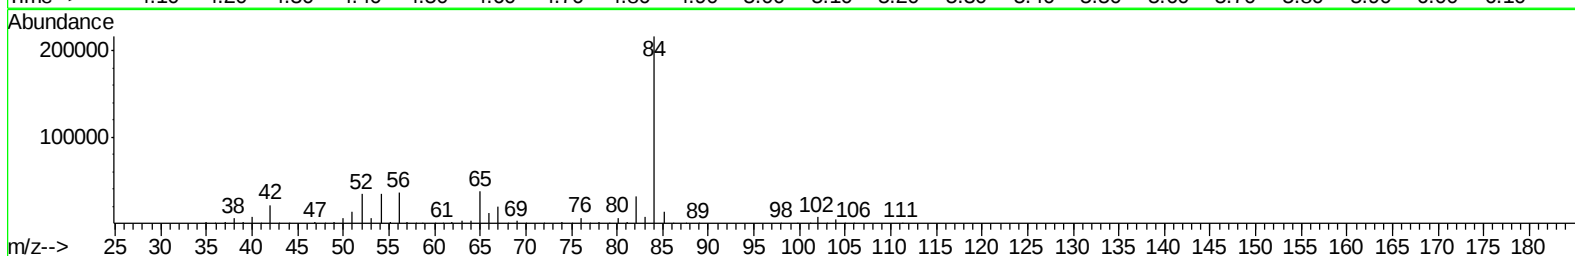


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016700.D
 Acq On : 09 Jun 2020 08:27
 Operator : SY/MD
 Sample : L2862-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jun 10 00:36:40 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jun 10 00:34:30 2020
 Response via : Initial Calibration

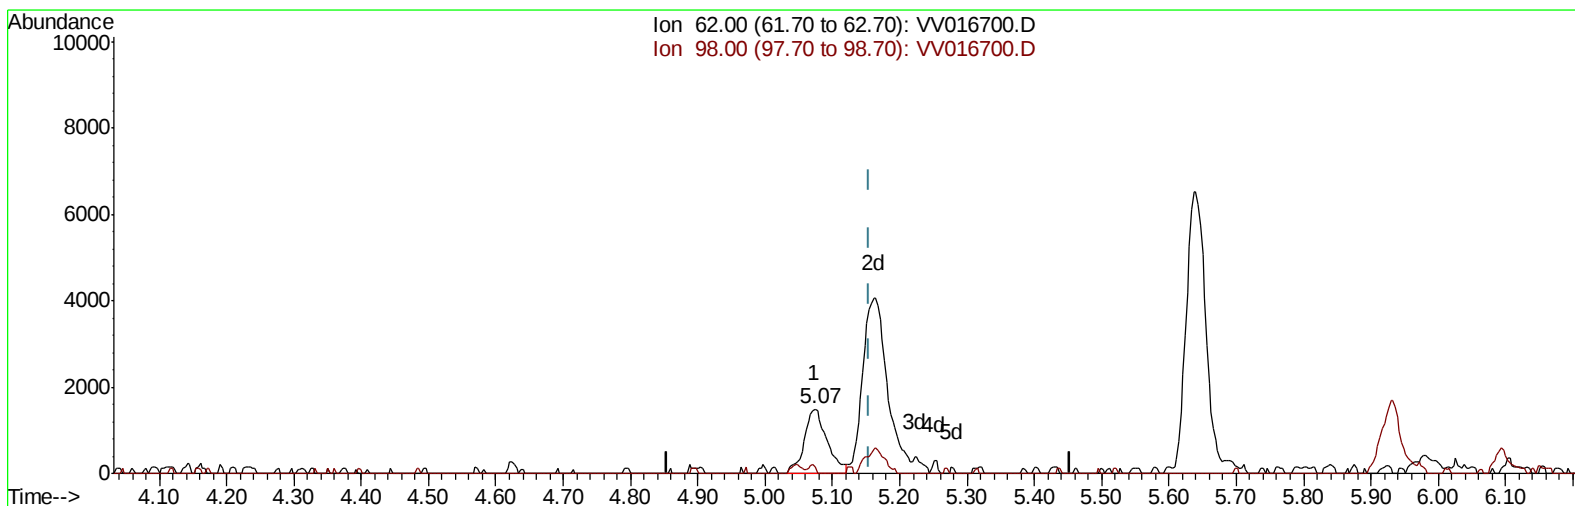

TIC: VV016700.D

(27) 1,2-Dichloroethane (T)

5.074min (-0.080) 0.86ug/L

response 3463

Ion	Exp%	Act%
62.00	100	100
98.00	9.30	10.16
0.00	0.00	0.00
0.00	0.00	0.00