
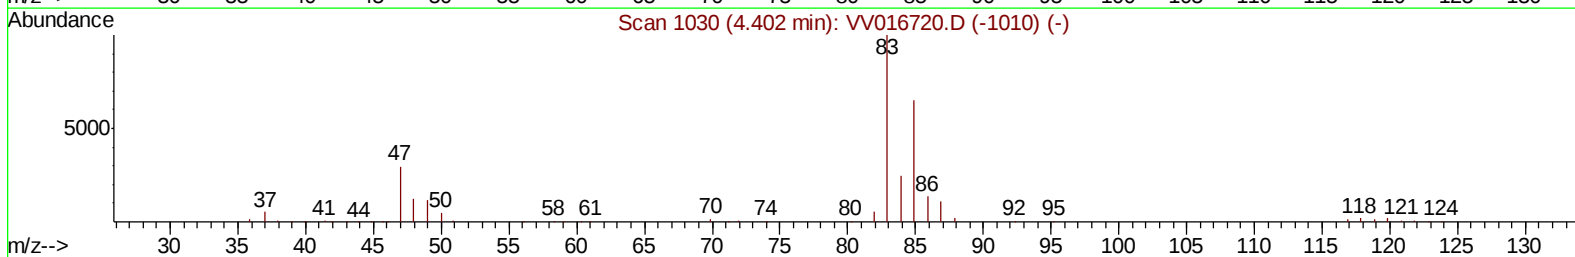
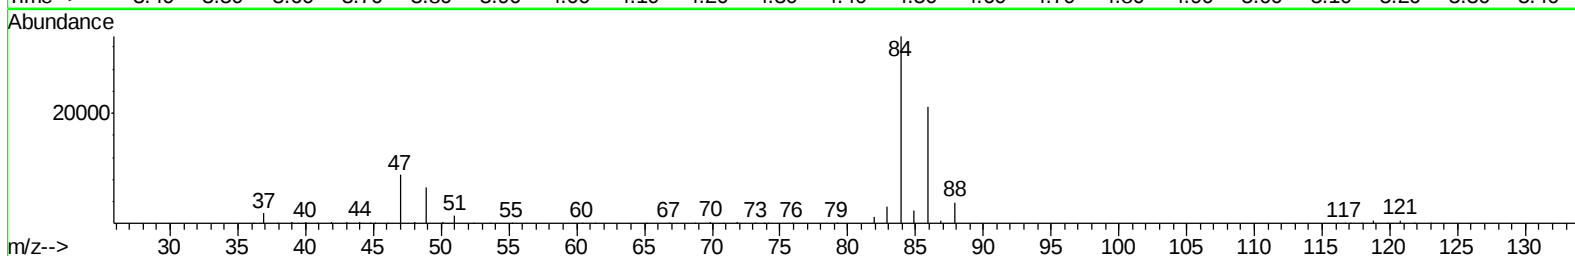


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016742.D
 Acq On : 10 Jun 2020 01:09
 Operator : SY/MD
 Sample : L2914-07 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Quant Time: Jun 10 03:48:23 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jun 10 03:42:58 2020
 Response via : Initial Calibration

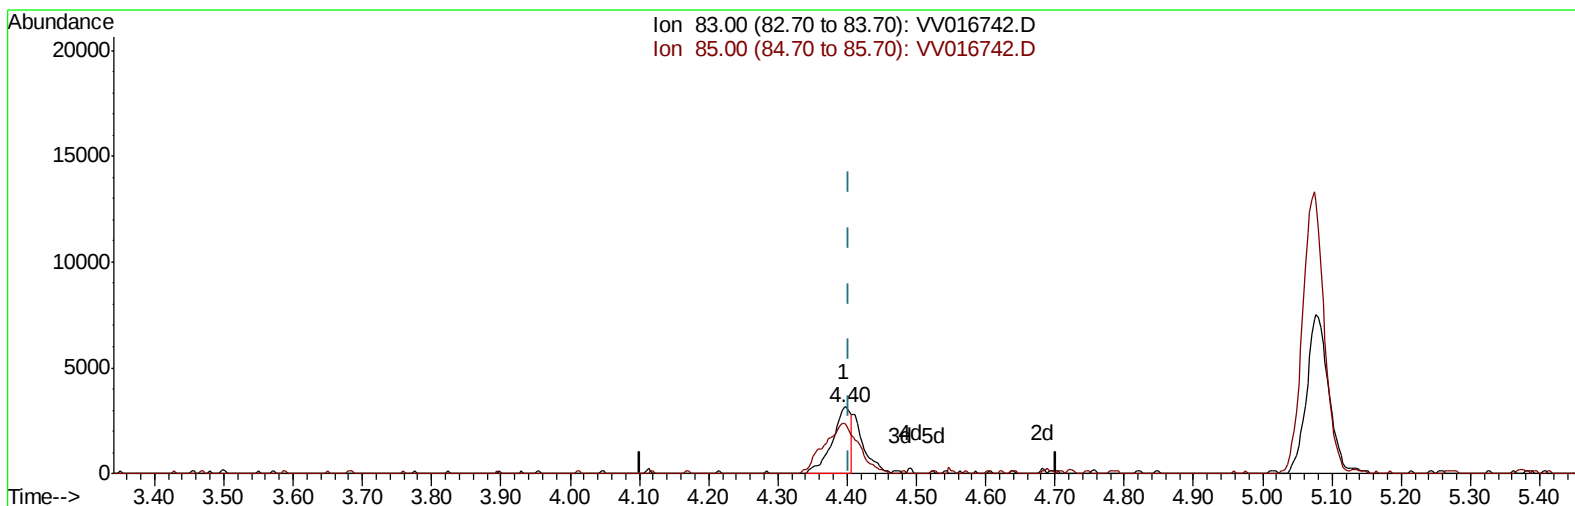

TIC: VV016742.D

(25) Chloroform (T)

4.396min (-0.006) 1.19ug/L

response 5782

Ion	Exp%	Act%
83.00	100	100
85.00	63.00	75.57
0.00	0.00	0.00
0.00	0.00	0.00