
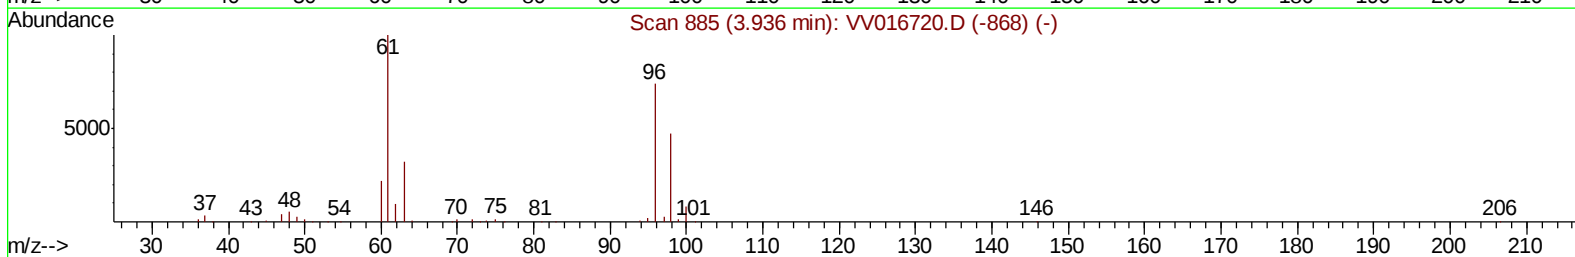
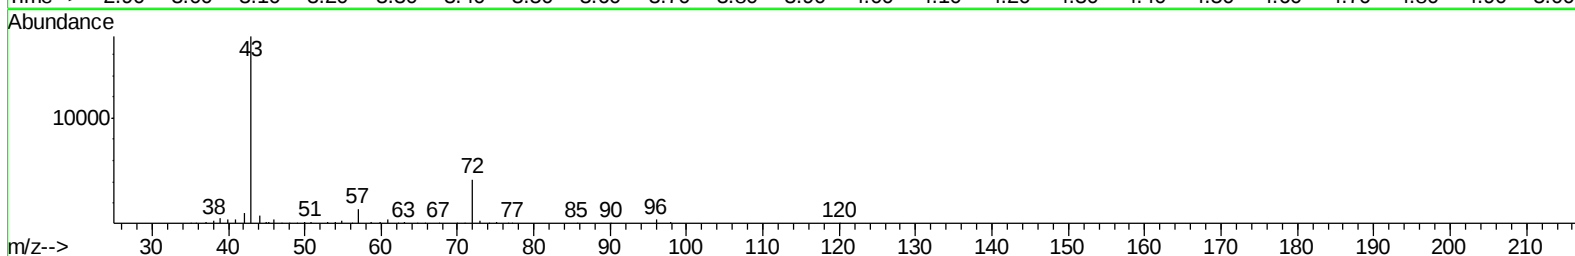


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060920\
Data File : VV016746.D
Acq On : 10 Jun 2020 02:44
Operator : SY/MD
Sample : VSTDCCC050
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 51 Sample Multiplier: 1

Quant Time: Jun 10 03:48:59 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 10 03:42:58 2020
Response via : Initial Calibration

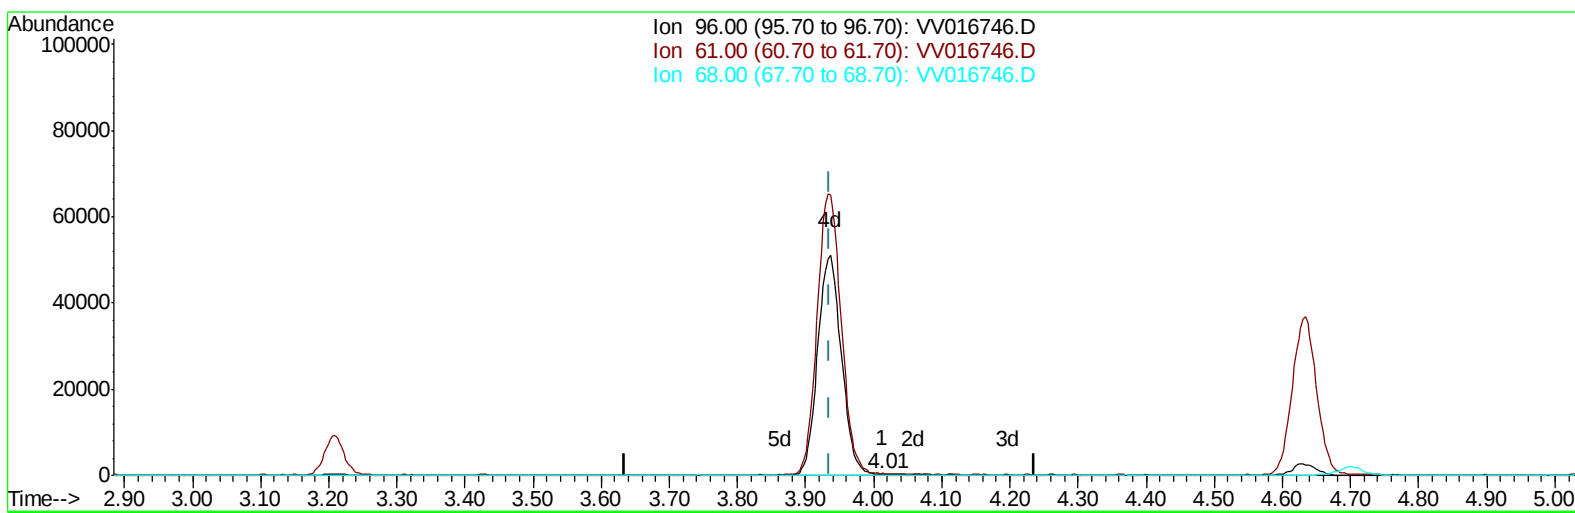

TIC: VV016746.D

(20) cis-1,2-Dichloroethene (T)

4.013min (+0.077) 0.16ug/L

response 401

Ion	Exp%	Act%
96.00	100	100
61.00	133.40	102.69
68.00	0.00	0.00
0.00	0.00	0.00