


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
Data File : VV016700.D
Acq On : 09 Jun 2020 08:27
Operator : SY/MD
Sample : L2862-14
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E28

Manual Integrations
APPROVED

MMDadoda
6/10/2020 3:51:45 PM

Quant Time: Jun 10 00:50:21 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 10 00:34:30 2020
Response via : Initial Calibration

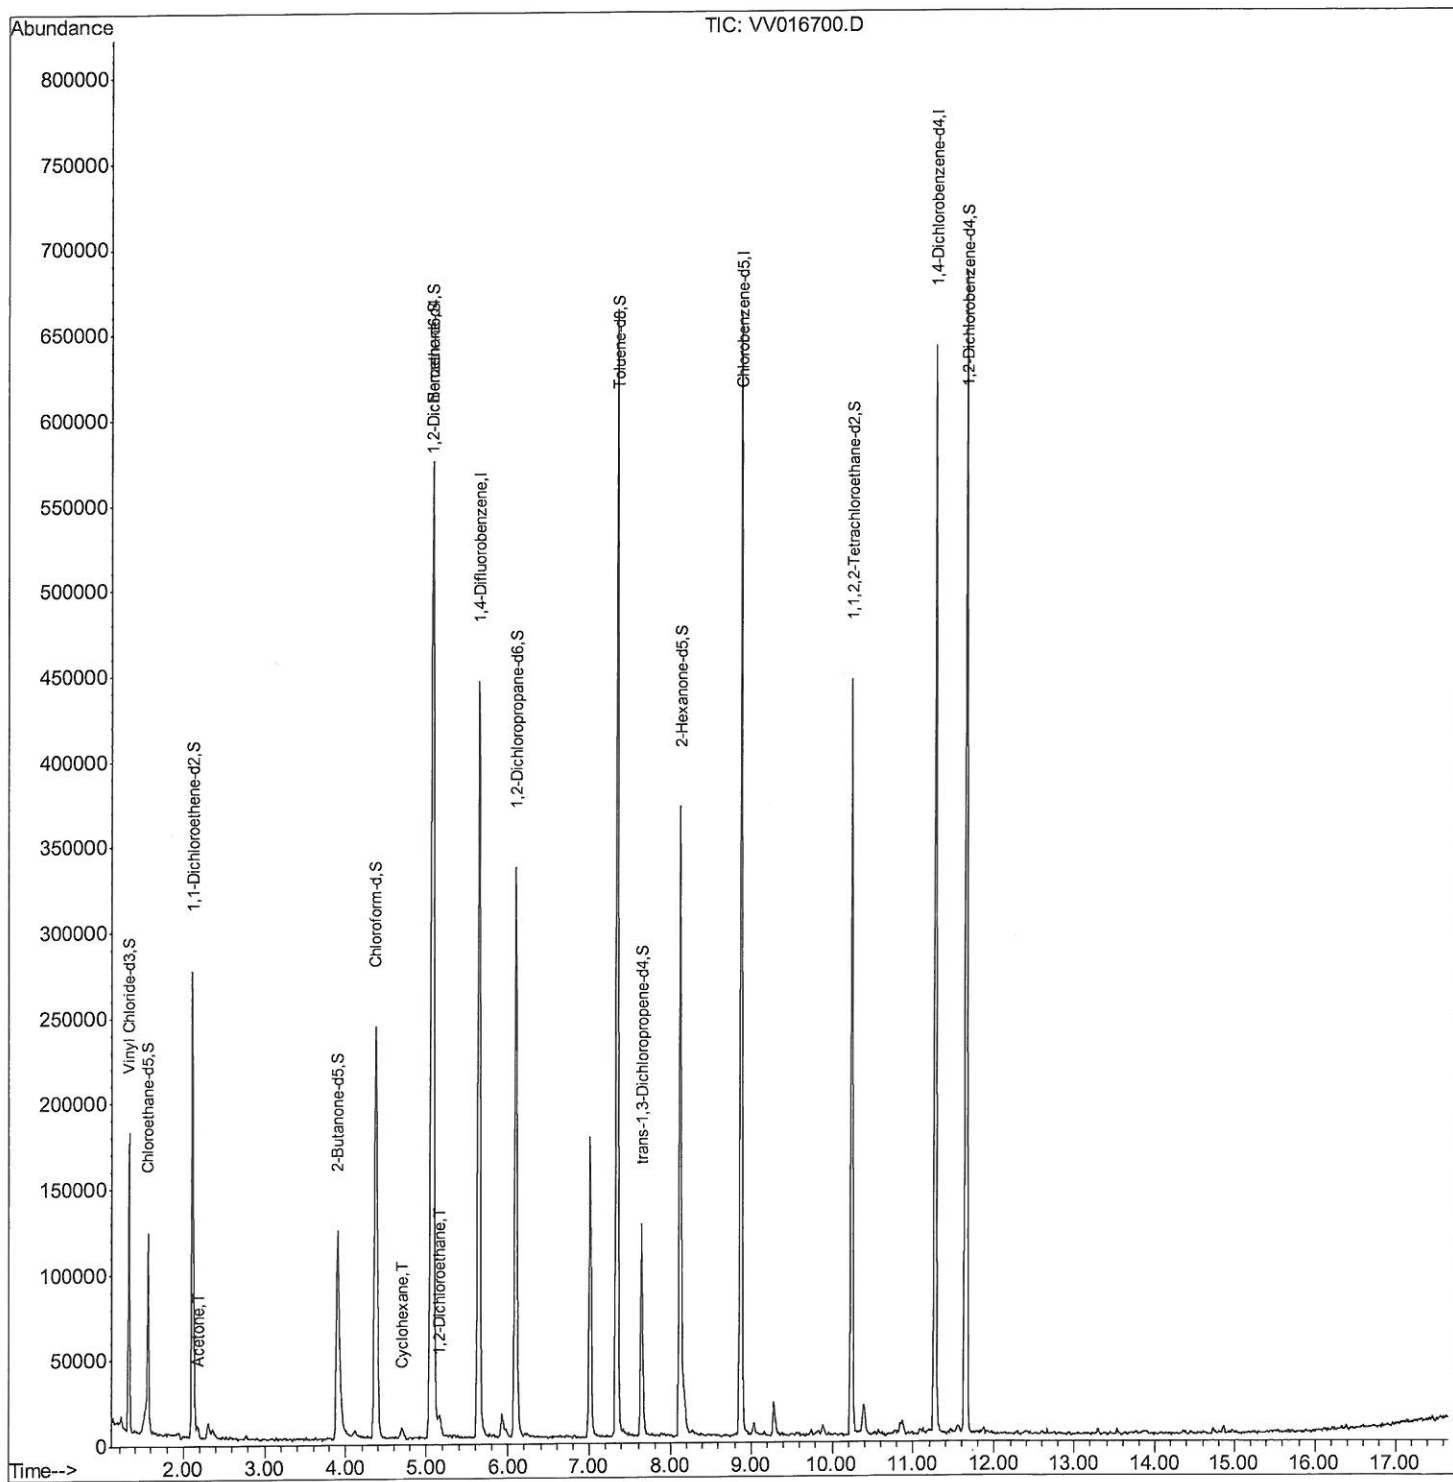

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016700.D
 Acq On : 09 Jun 2020 08:27
 Operator : SY/MD
 Sample : L2862-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E28

Manual Integrations
 APPROVED

MMDadoda
 6/10/2020 3:51:45 PM

Quant Time: Jun 10 00:36:40 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jun 10 00:34:30 2020
 Response via : Initial Calibration

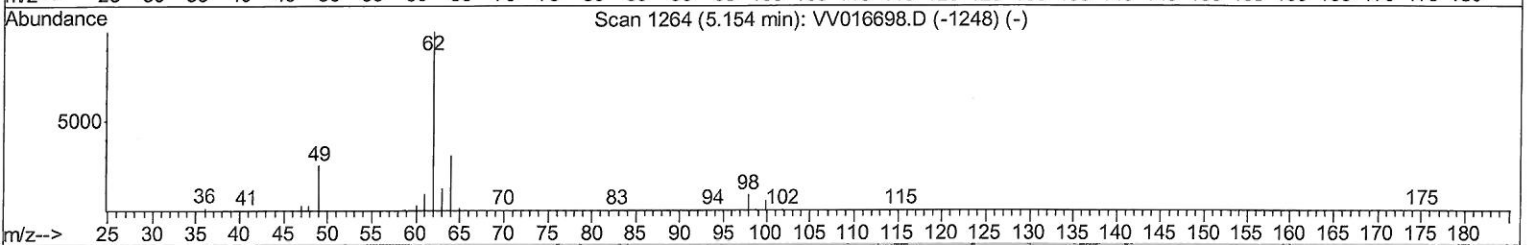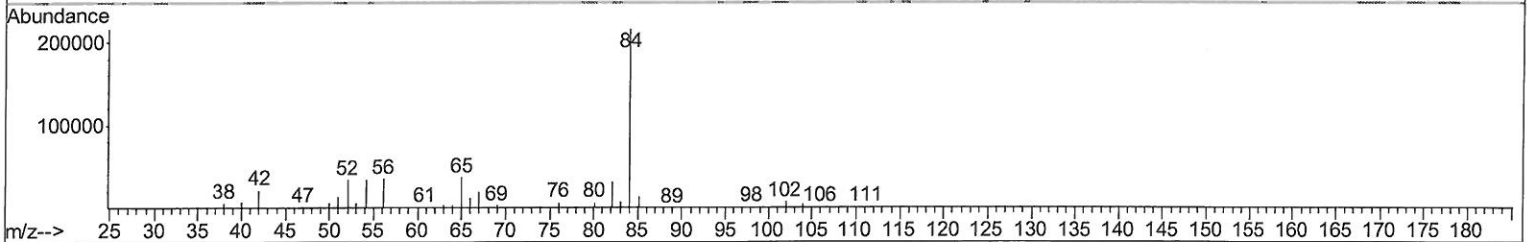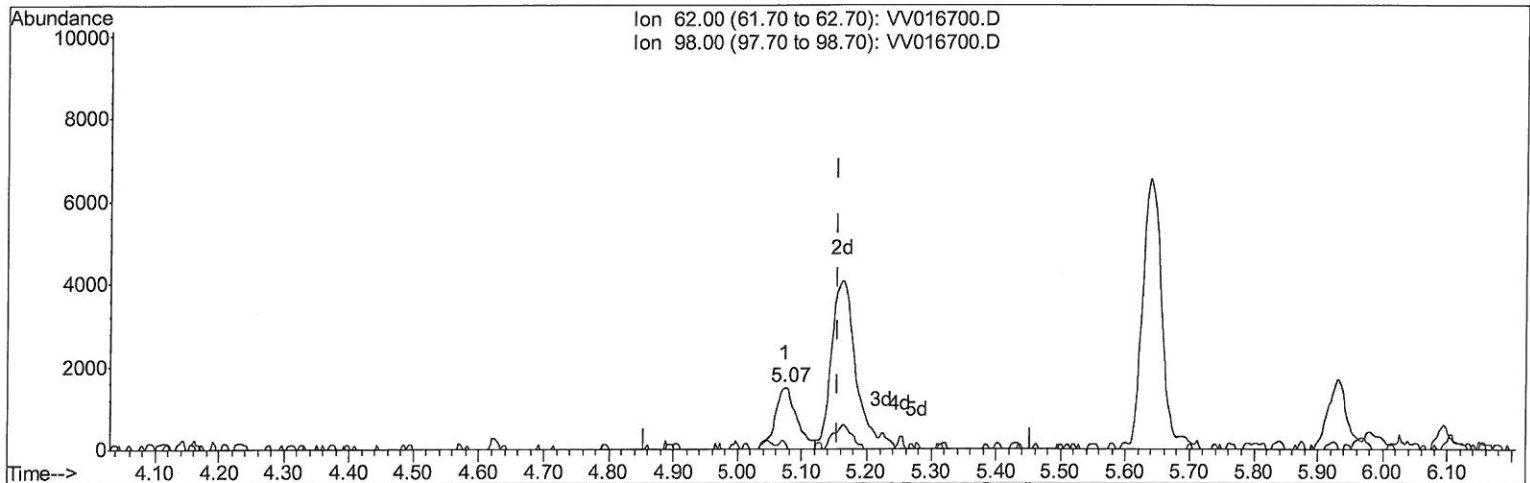

TIC: VV016700.D

(27) 1,2-Dichloroethane (T)

5.074min (-0.080) 0.86ug/L

response 3463

Ion	Exp%	Act%
62.00	100	100
98.00	9.30	10.16
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016700.D
 Acq On : 09 Jun 2020 08:27
 Operator : SY/MD
 Sample : L2862-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E28

Manual Integrations
 APPROVED

MMDadoda
 6/10/2020 3:51:45 PM

Quant Time: Jun 10 00:36:40 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jun 10 00:34:30 2020
 Response via : Initial Calibration

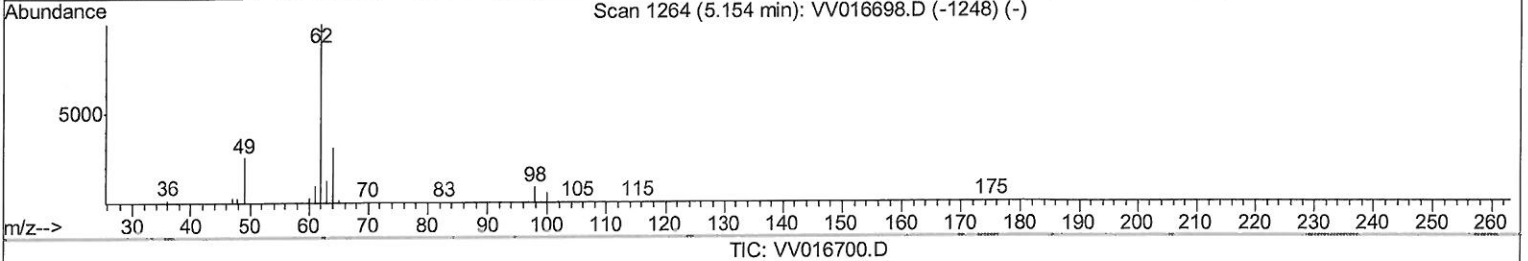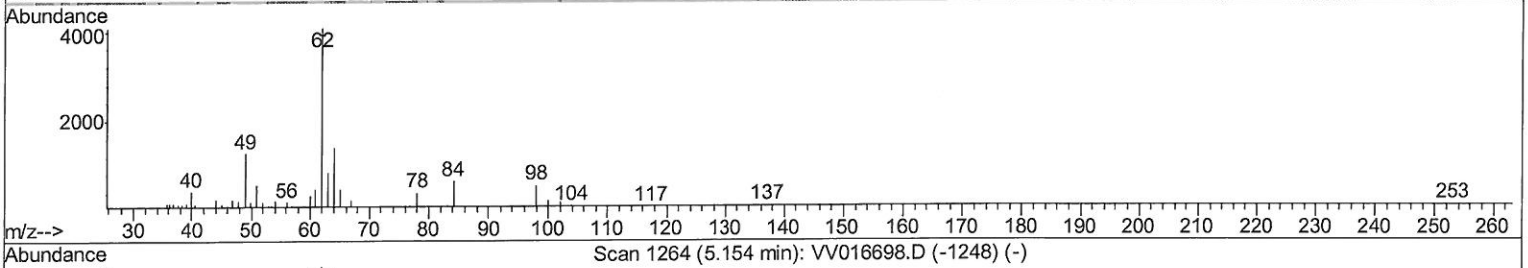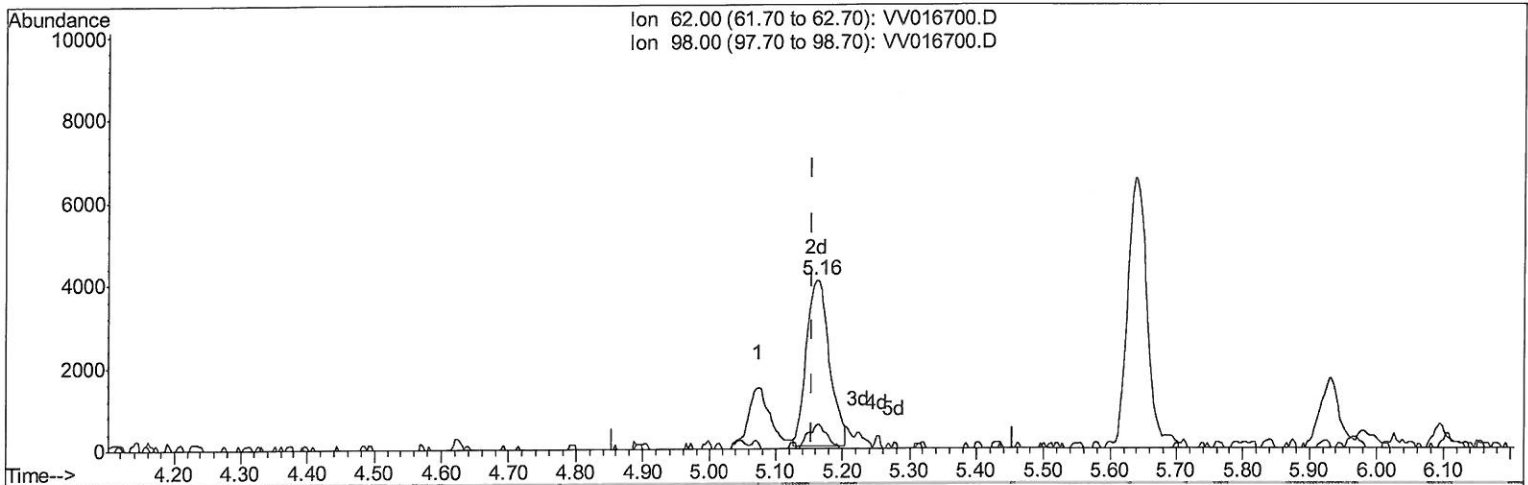

(27) 1,2-Dichloroethane (T)

5.161min (+0.007) 2.42ug/L m

response 9696

Ion	Exp%	Act%
62.00	100	100
98.00	9.30	14.08#
0.00	0.00	0.00
0.00	0.00	0.00

7 MD
6/10/20

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016700.D
 Acq On : 09 Jun 2020 08:27
 Operator : SY/MD
 Sample : L2862-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
ClientSampleId :
 F9E28

Manual Integrations
APPROVED

MMDadoda
 6/10/2020 3:51:45 PM

Quant Time: Jun 10 00:36:40 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jun 10 00:34:30 2020
 Response via : Initial Calibration

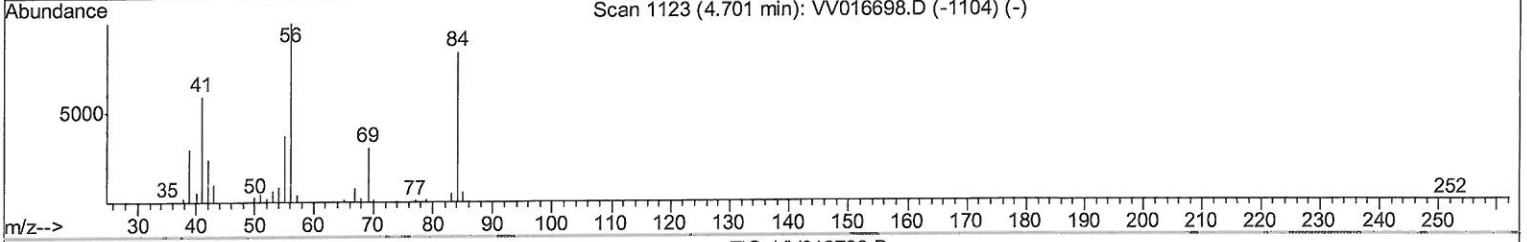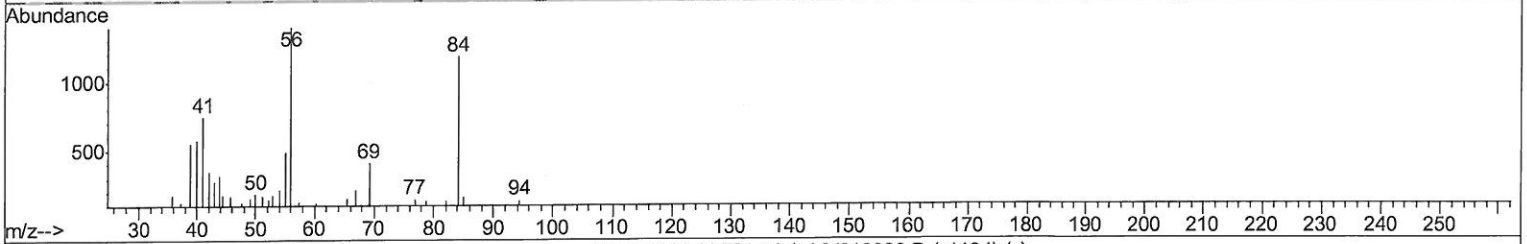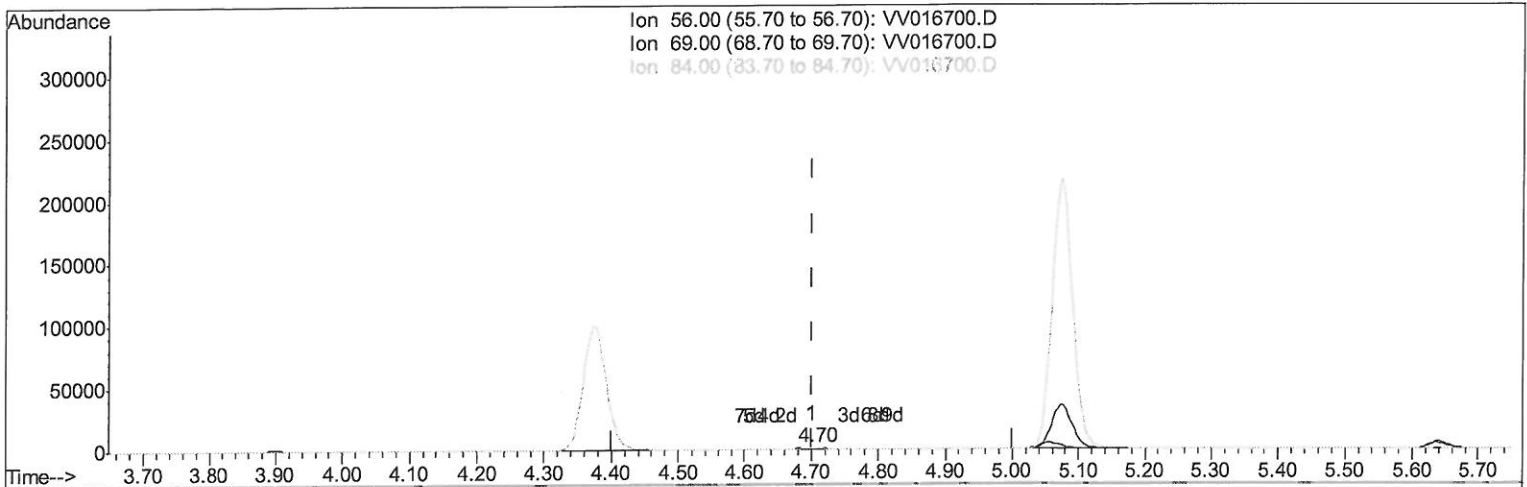

TIC: VV016700.D

(29) Cyclohexane (T)

4.701min (+0.000) 0.57ug/L

response 2413

Ion	Exp%	Act%
56.00	100	100
69.00	31.20	29.34
84.00	86.90	89.35
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016700.D
 Acq On : 09 Jun 2020 08:27
 Operator : SY/MD
 Sample : L2862-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E28

Manual Integrations
 APPROVED

MMDadoda
 6/10/2020 3:51:45 PM

Quant Time: Jun 10 00:36:40 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jun 10 00:34:30 2020
 Response via : Initial Calibration

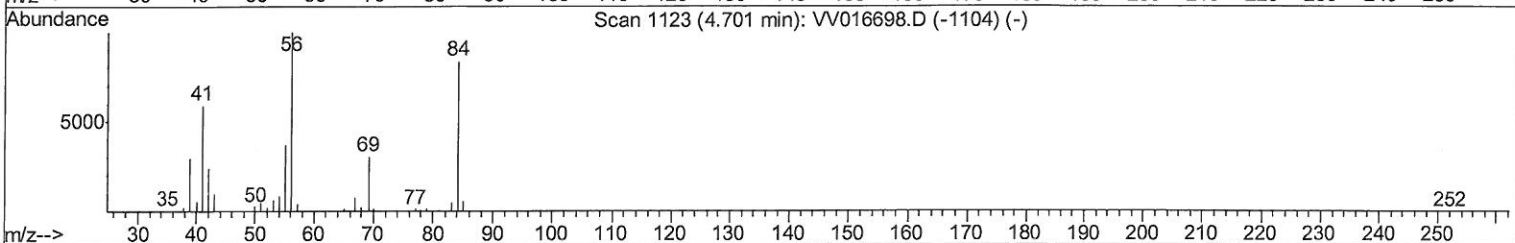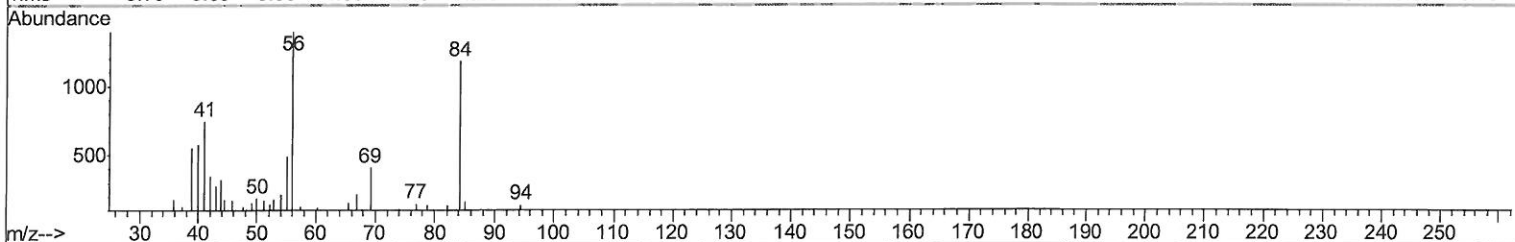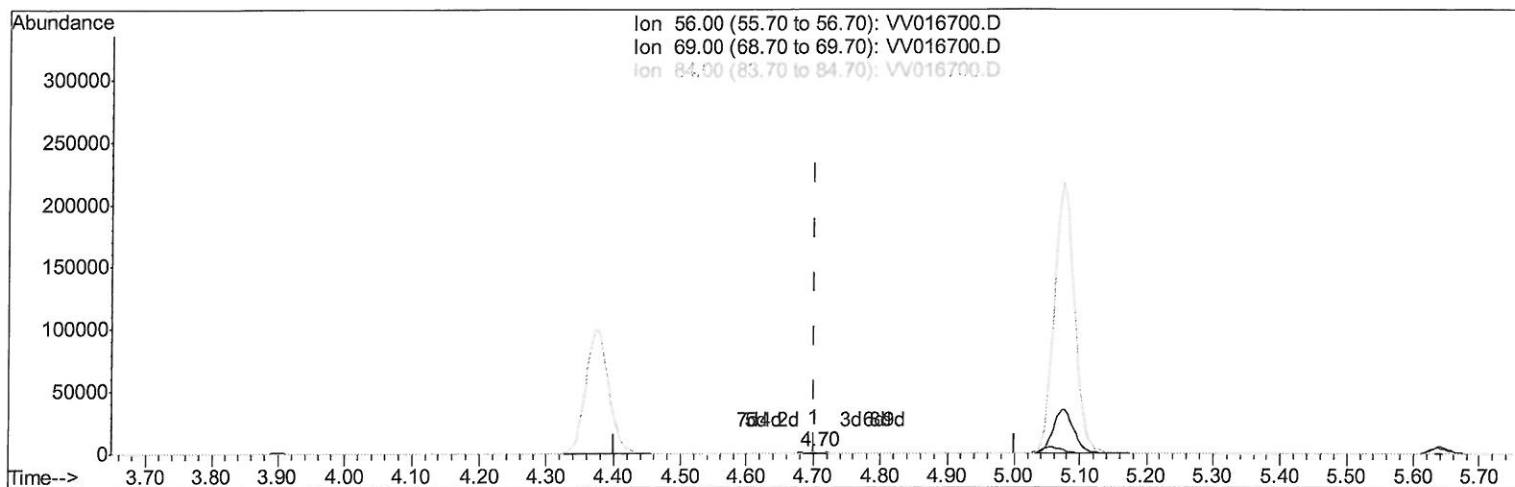

TIC: VV016700.D

(29) Cyclohexane (T)

4.701min (+0.000) 0.83ug/L m

response 3504

Ion	Exp%	Act%
56.00	100	100
69.00	31.20	20.21#
84.00	86.90	61.53#
0.00	0.00	0.00

7 MD
 6/10/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016700.D
 Acq On : 09 Jun 2020 08:27
 Operator : SY/MD
 Sample : L2862-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E28

Manual Integrations
 APPROVED

MMDadoda
 6/10/2020 3:51:45 PM

Quant Time: Jun 10 00:50:21 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jun 10 00:34:30 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	5.64	114	365498	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	341559	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	155507	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	103714	40.21	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	80.42%
7) Chloroethane-d5	1.56	69	60965	39.40	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	78.80%
11) 1,1-Dichloroethene-d2	2.12	63	144057	33.26	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	66.52%
21) 2-Butanone-d5	3.90	46	193115	101.17	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	101.17%
24) Chloroform-d	4.37	84	239064	45.59	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.18%
26) 1,2-Dichloroethane-d4	5.05	65	172858	48.46	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.92%
32) Benzene-d6	5.07	84	470396	47.78	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.56%
36) 1,2-Dichloropropane-d6	6.09	67	148785	48.48	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	96.96%
41) Toluene-d8	7.34	98	416581	46.11	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.22%
43) trans-1,3-Dichloropropene-	7.64	79	66322	41.49	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	82.98%
47) 2-Hexanone-d5	8.11	63	121565	90.85	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	90.85%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	197826	48.69	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	97.38%
64) 1,2-Dichlorobenzene-d4	11.65	152	166055	50.04	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.08%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
13) Acetone	2.18	43	6454	5.132	ug/L	81
27) 1,2-Dichloroethane	5.16	62	9696m	2.417	ug/L	
29) Cyclohexane	4.70	56	3504m	0.826	ug/L	

3 MB
 6/10/20

(#) = qualifier out of range (m) = manual integration (+) = signals summed