


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
Data File : VV016732.D
Acq On : 09 Jun 2020 21:11
Operator : SY/MD
Sample : L2914-16
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E29

Manual Integrations
APPROVED

MMDadoda
6/10/2020 3:52:17 PM

Quant Time: Jun 10 04:56:13 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 10 03:42:58 2020
Response via : Initial Calibration

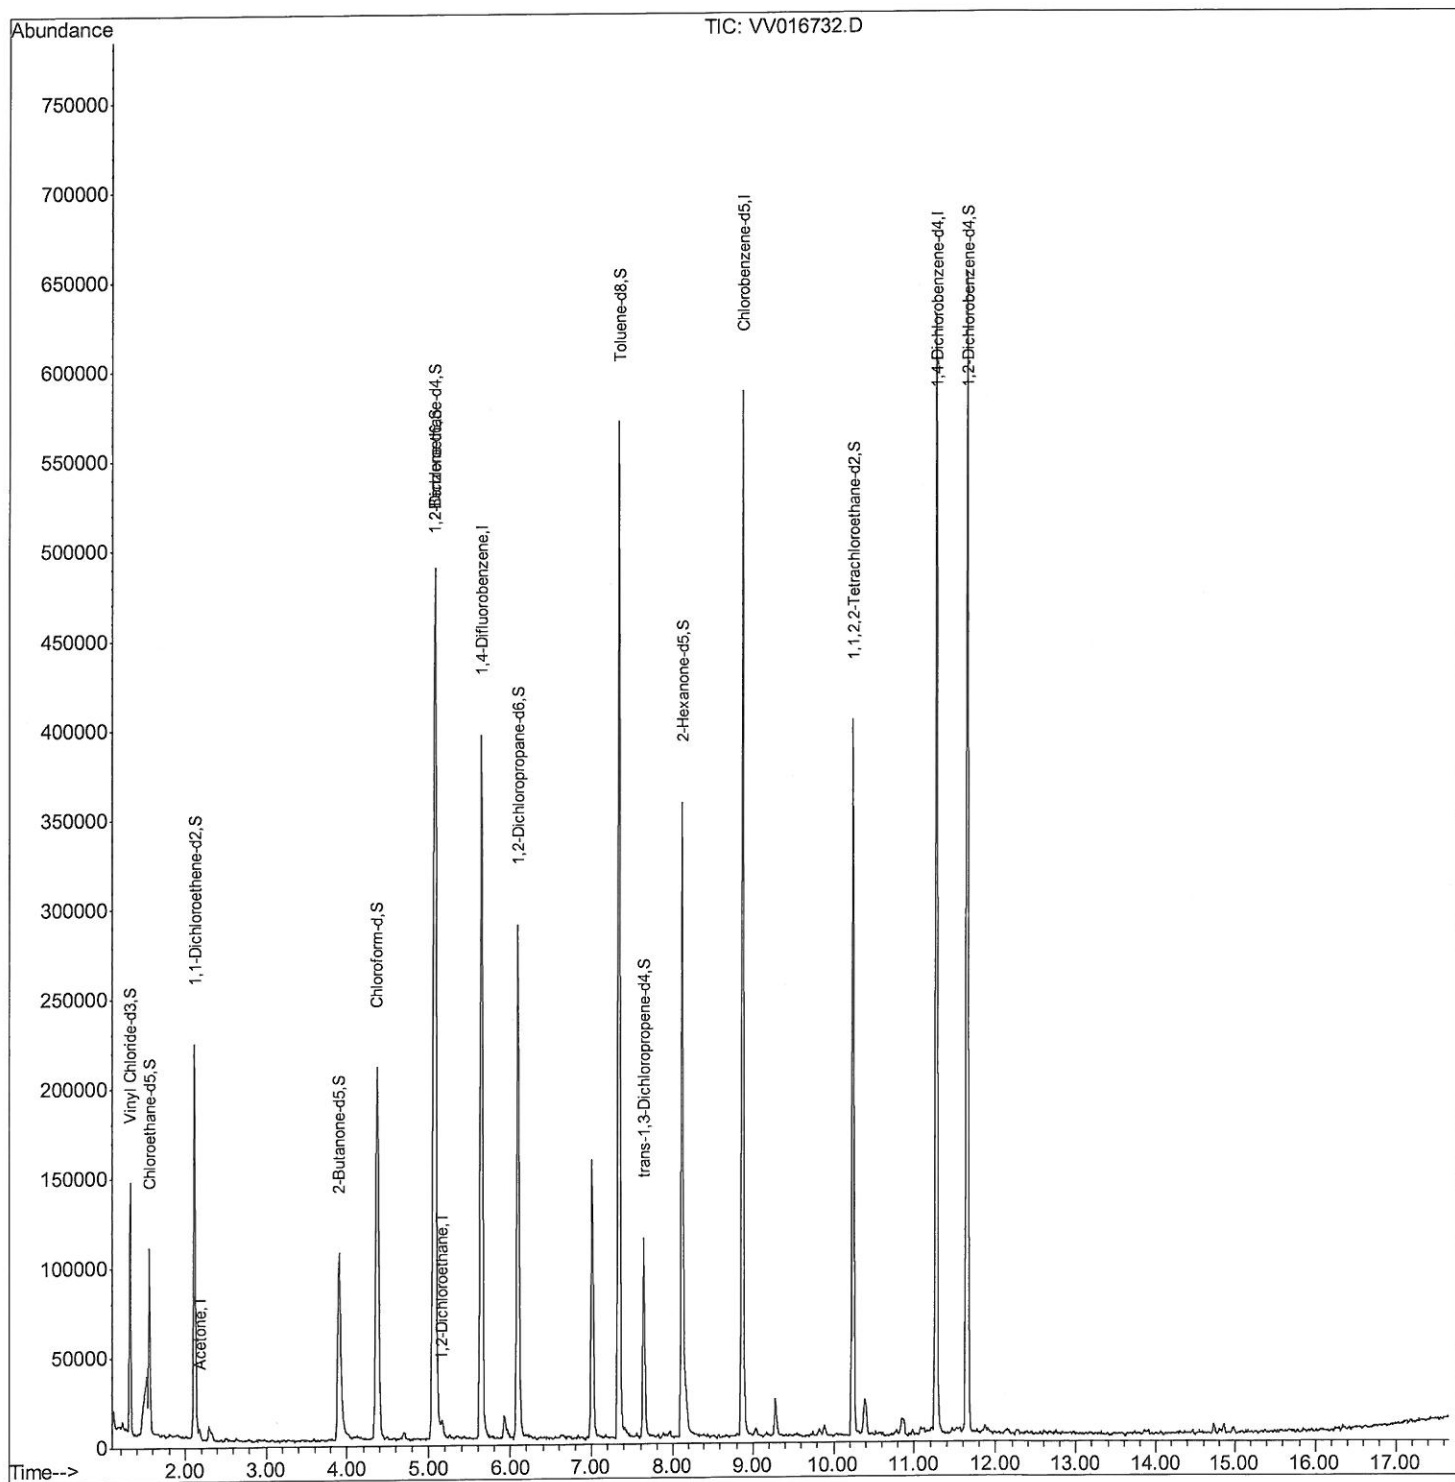

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016732.D
 Acq On : 09 Jun 2020 21:11
 Operator : SY/MD
 Sample : L2914-16
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E29

Manual Integrations
 APPROVED

MMDadoda
 6/10/2020 3:52:17 PM

Quant Time: Jun 10 03:46:40 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jun 10 03:42:58 2020
 Response via : Initial Calibration

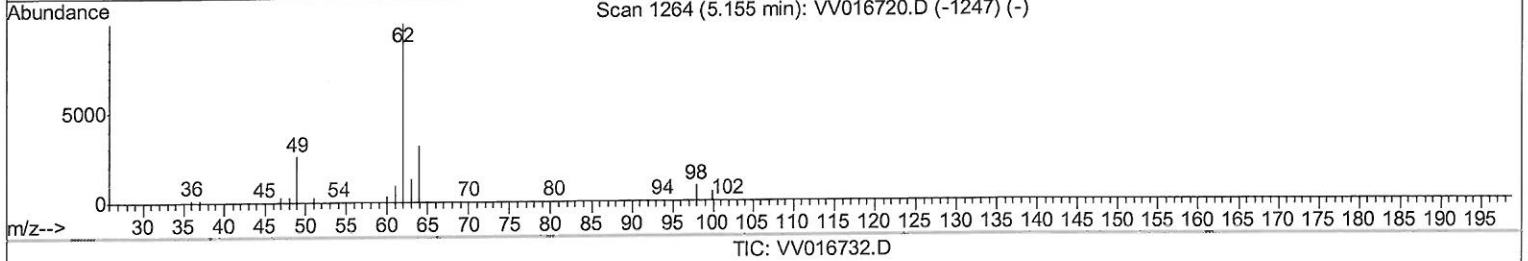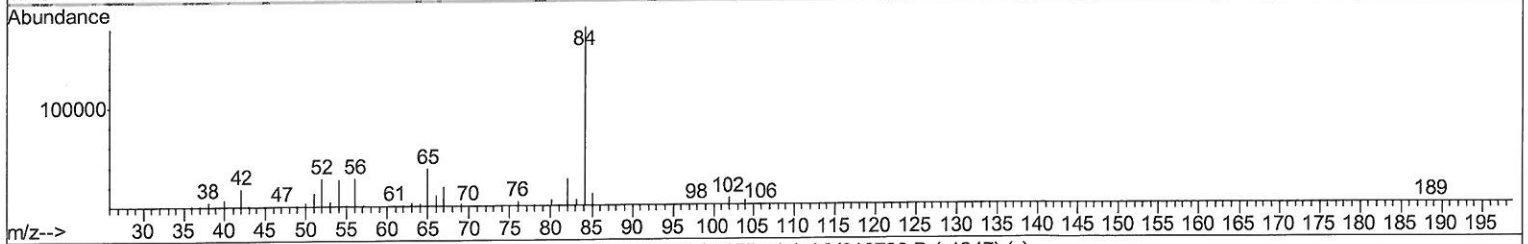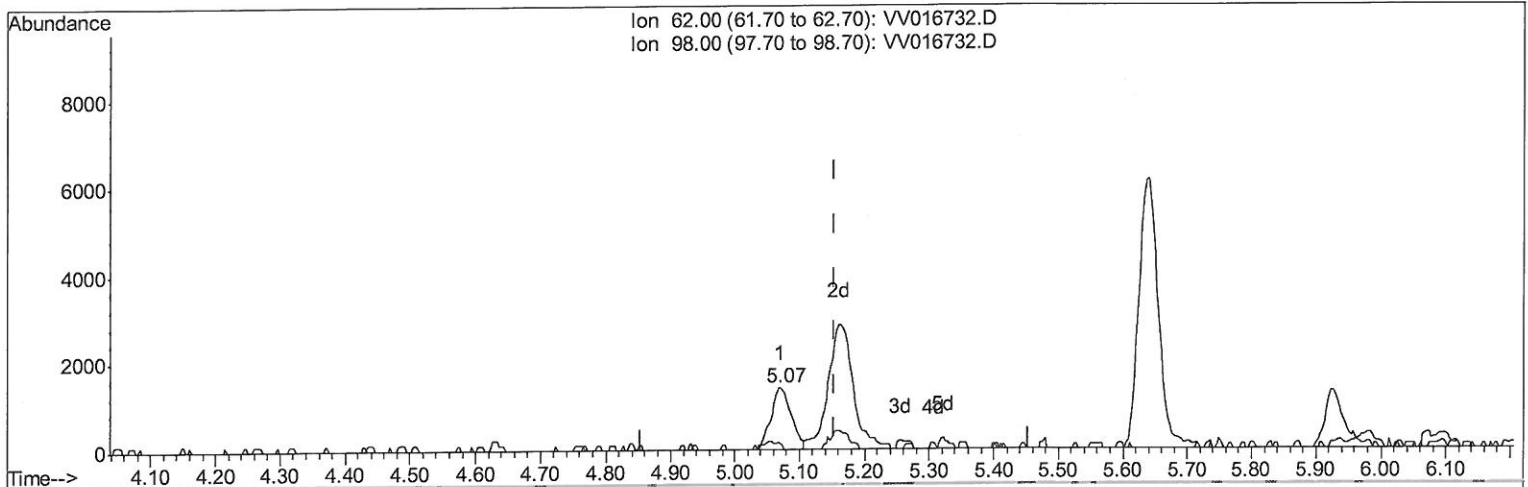

(27) 1,2-Dichloroethane (T)

5.071min (-0.084) 0.86ug/L

response 3073

Ion	Exp%	Act%
62.00	100	100
98.00	9.30	10.69
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016732.D
 Acq On : 09 Jun 2020 21:11
 Operator : SY/MD
 Sample : L2914-16
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampled :
 F9E29

Manual Integrations
 APPROVED

MMDadoda
 6/10/2020 3:52:17 PM

Quant Time: Jun 10 03:46:40 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jun 10 03:42:58 2020
 Response via : Initial Calibration

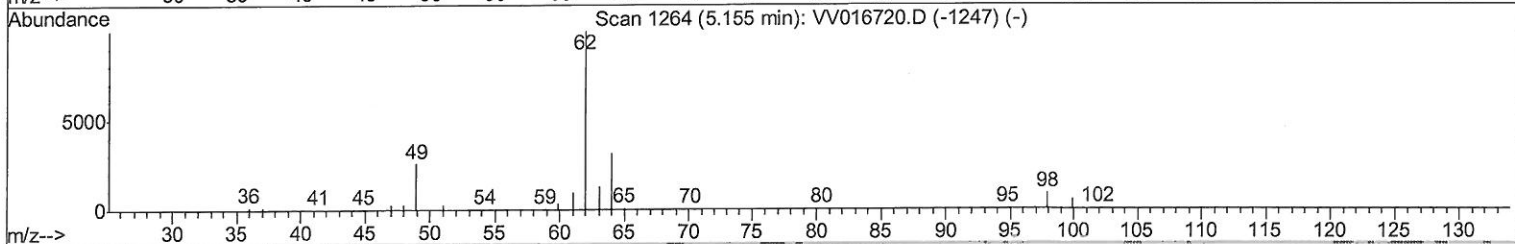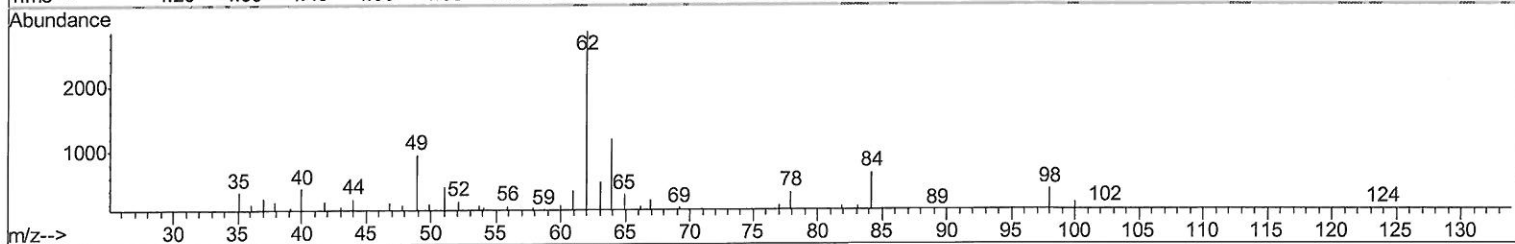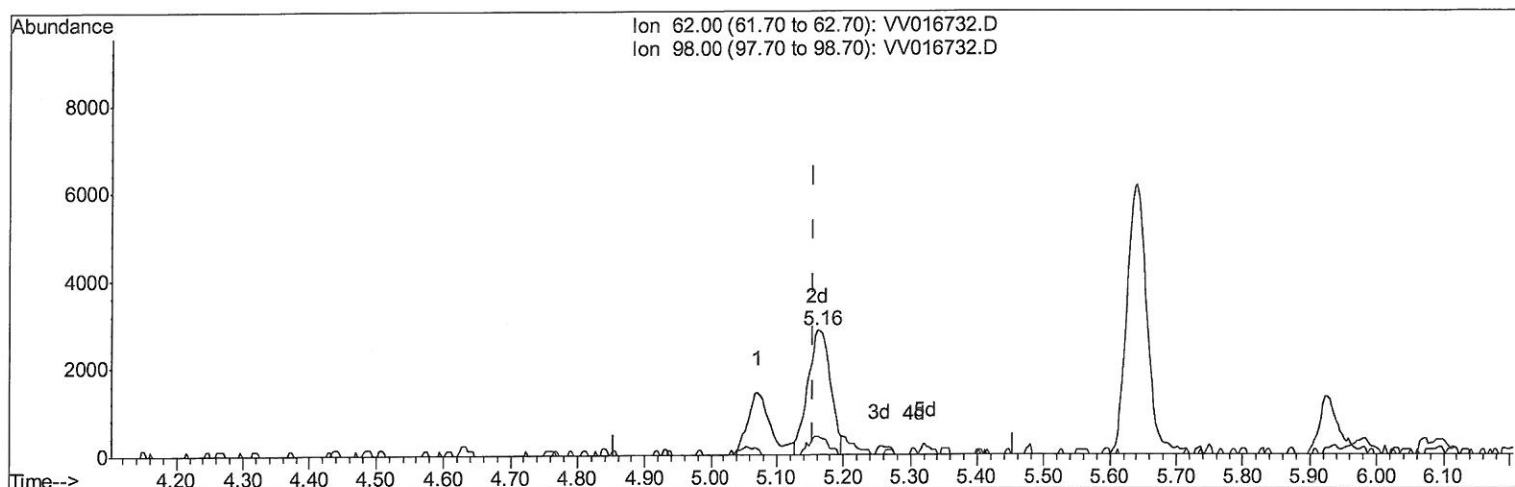

TIC: VV016732.D

(27) 1,2-Dichloroethane (T)

5.161min (+0.006) 1.92ug/L m

response 6832

Ion	Exp%	Act%
62.00	100	100
98.00	9.30	14.59#
0.00	0.00	0.00
0.00	0.00	0.00

MD
 6/10/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016732.D
 Acq On : 09 Jun 2020 21:11
 Operator : SY/MD
 Sample : L2914-16
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E29

Manual Integrations
 APPROVED

MMDadoda
 6/10/2020 3:52:17 PM

Quant Time: Jun 10 04:56:13 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jun 10 03:42:58 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	324723	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	306780	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	153883	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	83214	36.32	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	72.64%
7) Chloroethane-d5	1.55	69	62773	45.66	ug/L	-0.02
Spiked Amount	50.000	Range	70 - 130	Recovery	=	91.32%
11) 1,1-Dichloroethene-d2	2.11	63	115164	29.93	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	59.86%#
21) 2-Butanone-d5	3.90	46	165218	97.42	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	97.42%
24) Chloroform-d	4.37	84	207663	44.57	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.14%
26) 1,2-Dichloroethane-d4	5.05	65	148634	46.90	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.80%
32) Benzene-d6	5.07	84	396539	44.84	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.68%
36) 1,2-Dichloropropane-d6	6.09	67	126623	45.93	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	91.86%
41) Toluene-d8	7.34	98	348072	42.89	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	85.78%
43) trans-1,3-Dichloropropene-	7.64	79	57199	39.84	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	79.68%
47) 2-Hexanone-d5	8.11	63	113386	94.35	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	94.35%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	176095	48.26	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	96.52%
64) 1,2-Dichlorobenzene-d4	11.65	152	157032	47.82	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.64%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
13) Acetone	2.17	43	4753	4.254	ug/L	88
27) 1,2-Dichloroethane	5.16	62	6832m	1.917	ug/L	

7 MD
 6/10/20

(#) = qualifier out of range (m) = manual integration (+) = signals summed