

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016718.D
 Acq On : 09 Jun 2020 15:39
 Operator : SY/MD
 Sample : L2901-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTT3

Quant Time: Jun 10 03:31:52 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jun 10 00:34:30 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	368139	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	349956	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	167171	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	90182	34.72	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	69.44%
7) Chloroethane-d5	1.56	69	68812	44.15	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	88.30%
11) 1,1-Dichloroethene-d2	2.12	63	131937	30.25	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	60.50%
21) 2-Butanone-d5	3.89	46	188189	97.88	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	97.88%
24) Chloroform-d	4.37	84	225841	42.76	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.52%
26) 1,2-Dichloroethane-d4	5.05	65	163460	45.50	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.00%
32) Benzene-d6	5.07	84	436433	43.26	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.52%
36) 1,2-Dichloropropane-d6	6.09	67	139321	44.31	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	88.62%
41) Toluene-d8	7.34	98	392207	42.37	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	84.74%
43) trans-1,3-Dichloropropene-	7.64	79	66536	40.63	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	81.26%
47) 2-Hexanone-d5	8.11	63	123221	89.88	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	89.88%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	190965	45.87	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	91.74%
64) 1,2-Dichlorobenzene-d4	11.65	152	170049	47.67	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.34%


Target Compounds					Ovalue
34) Trichloroethene	5.94	95	6169	2.222 ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
Data File : VV016718.D
Acq On : 09 Jun 2020 15:39
Operator : SY/MD
Sample : L2901-08
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTT3

Quant Time: Jun 10 03:31:52 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 10 00:34:30 2020
Response via : Initial Calibration

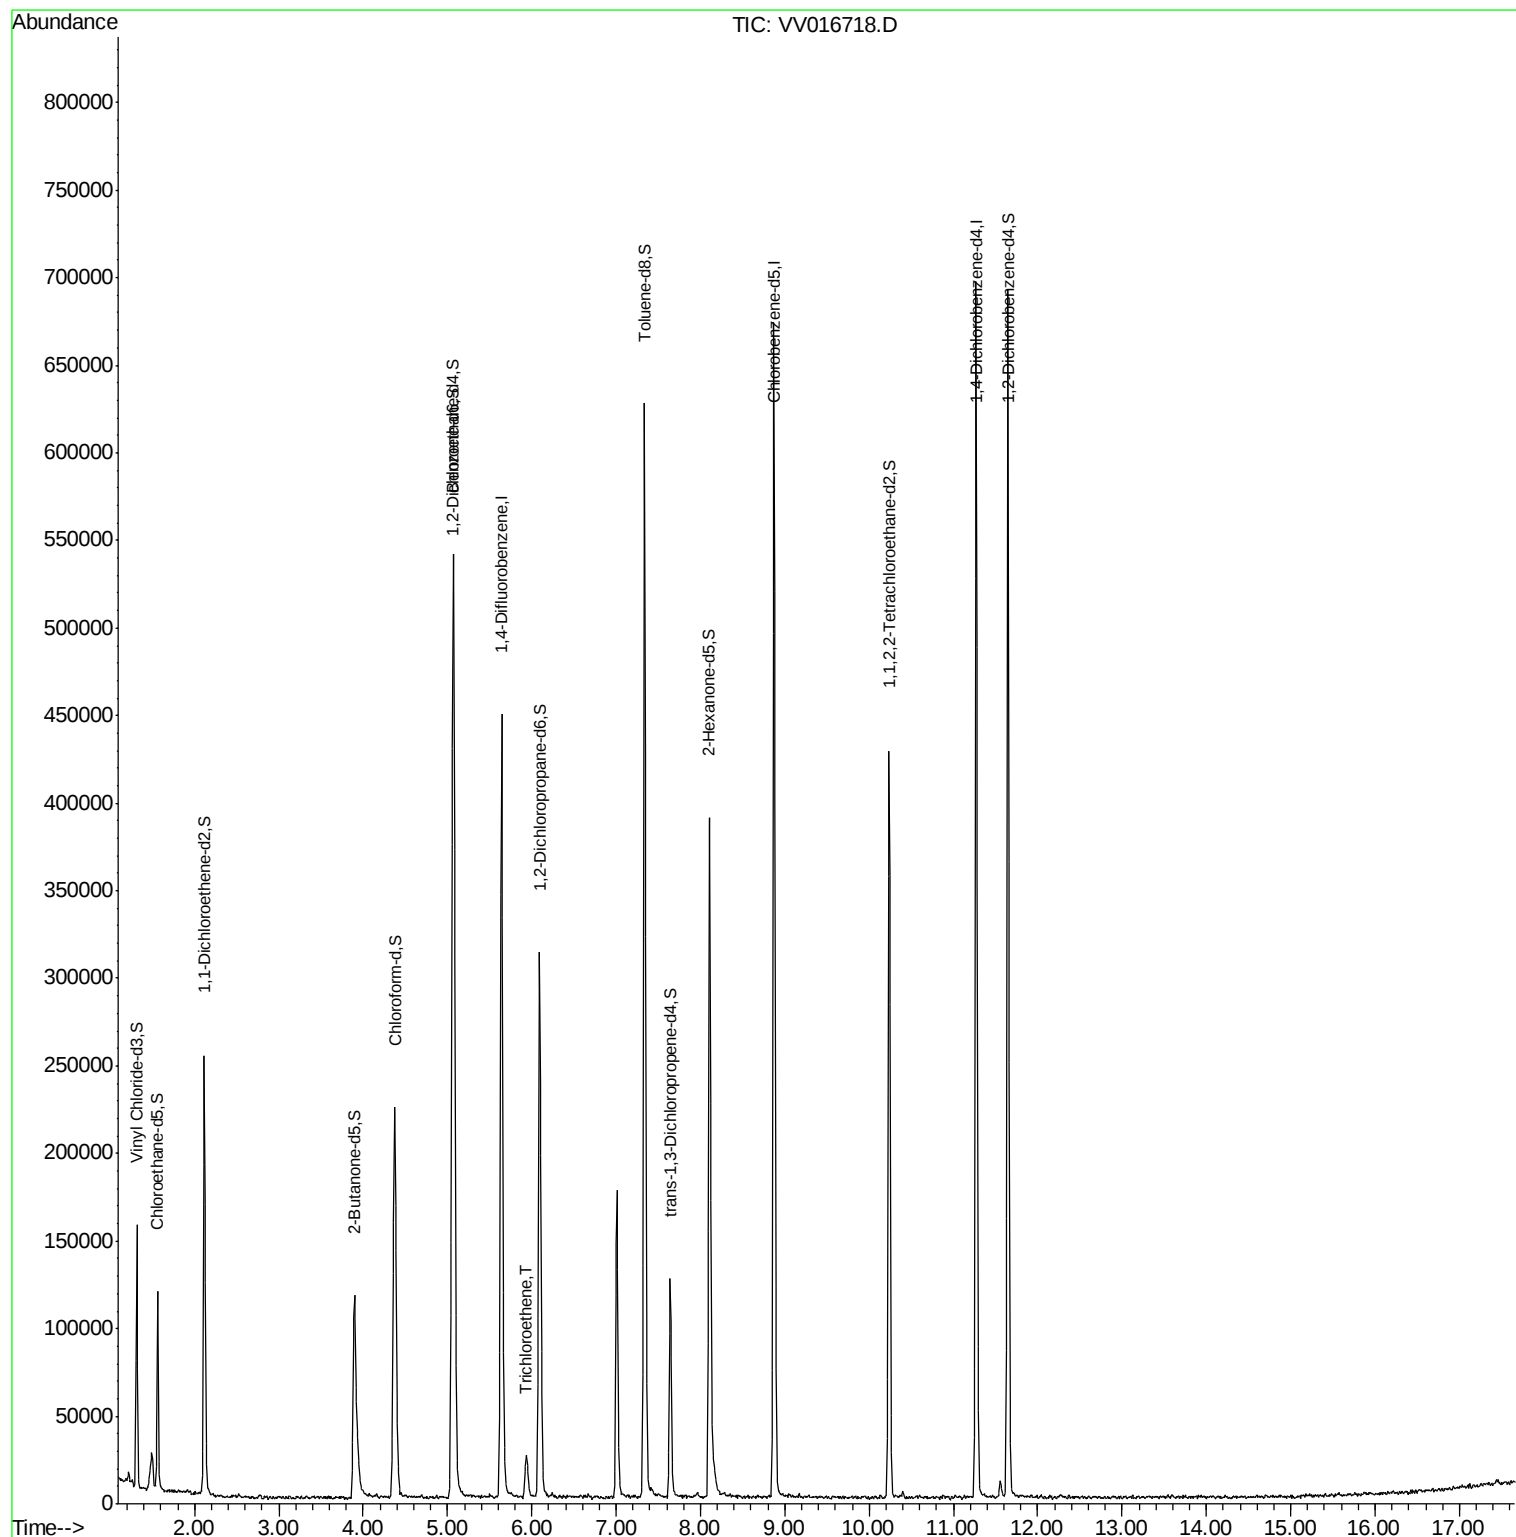

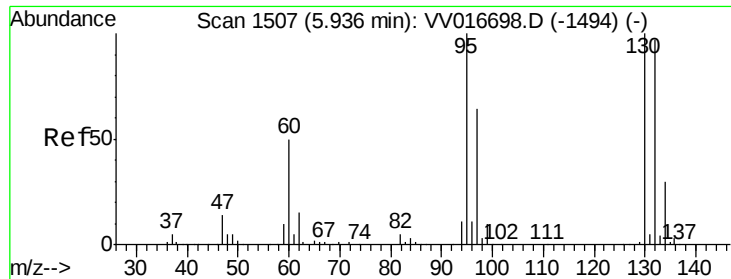

#34
 Trichloroethene
 Concen: 2.222 ug/L
 RT: 5.94 min Scan# 1509
 Delta R.T. 0.01 min
 Lab File: VV016718.D
 Acq: 09 Jun 2020 15:39

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTT3

Tot Ion:	95	Resp:	6169
Ion	Ratio	Lower	Upper
95	100		
97	80.0	44.3	82.3
132	106.1	67.9	126.1
130	102.9	72.2	134.2

