

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016699.D
 Acq On : 09 Jun 2020 08:03
 Operator : SY/MD
 Sample : VV0609WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK75

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	81	rVB	175975	173543	11.69%	1.569%
2	1.563	140	147	157	rVB	124194	146837	9.89%	1.327%
3	2.116	309	319	345	rVB	278938	423775	28.55%	3.831%
4	2.592	465	467	469	rBV3	1313	618	0.04%	0.006%
5	2.704	495	502	504	rBV8	2081	2234	0.15%	0.020%
6	2.769	518	522	523	rBV3	1463	1037	0.07%	0.009%
7	2.846	543	546	548	rBV4	1036	581	0.04%	0.005%
8	2.901	560	563	566	rVB5	1553	870	0.06%	0.008%
9	2.917	566	568	570	rBV	1644	935	0.06%	0.008%
10	3.061	610	613	615	rBV4	998	823	0.06%	0.007%
11	3.155	637	642	644	rBV4	1661	1415	0.10%	0.013%
12	3.203	650	657	659	rBV7	2319	2113	0.14%	0.019%
13	3.322	691	694	695	rBV3	1061	528	0.04%	0.005%
14	3.360	700	706	709	rBV7	2211	2025	0.14%	0.018%
15	3.460	732	737	740	rVB5	1769	1306	0.09%	0.012%
16	3.476	740	742	744	rBV3	1272	753	0.05%	0.007%
17	3.511	750	753	756	rBV5	1343	985	0.07%	0.009%
18	3.598	778	780	785	rBV4	1390	1299	0.09%	0.012%
19	3.698	808	811	814	rBV4	1342	1111	0.07%	0.010%
20	3.733	820	822	826	rBV5	1444	1211	0.08%	0.011%
21	3.769	831	833	836	rBV4	795	545	0.04%	0.005%
22	3.849	854	858	859	rBV3	1564	944	0.06%	0.009%
23	3.897	861	873	902	rVV	117274	331984	22.36%	3.001%
24	4.074	926	928	930	rBV3	1513	720	0.05%	0.007%
25	4.241	979	980	983	rBV3	1328	666	0.04%	0.006%
26	4.373	1006	1021	1043	rBV	238961	584890	39.40%	5.287%
27	4.630	1097	1101	1105	rBV6	1983	1661	0.11%	0.015%
28	4.650	1105	1107	1108	rBV2	1411	647	0.04%	0.006%
29	4.881	1176	1179	1180	rBV2	1196	541	0.04%	0.005%
30	5.071	1219	1238	1263	rBV2	578200	1484518	100.00%	13.419%
31	5.277	1298	1302	1305	rBV4	1499	1587	0.11%	0.014%
32	5.640	1402	1415	1437	rBV	444523	876990	59.08%	7.927%
33	5.891	1487	1493	1494	rBV6	2083	1631	0.11%	0.015%
34	6.093	1544	1556	1576	rBV	334817	669704	45.11%	6.054%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016699.D
 Acq On : 09 Jun 2020 08:03
 Operator : SY/MD
 Sample : VV0609WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK75

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.923	1811	1814	1815	rBV2	1338	824	0.06%	0.007%
36	6.971	1826	1829	1830	rBV2	1954	1075	0.07%	0.010%
37	7.007	1830	1840	1859	rVV	178869	316585	21.33%	2.862%
38	7.167	1888	1890	1893	rBV4	1943	1311	0.09%	0.012%
39	7.235	1908	1911	1912	rBV2	1830	983	0.07%	0.009%
40	7.261	1917	1919	1922	rVV4	1030	599	0.04%	0.005%
41	7.338	1930	1943	1961	rBV	671196	1158471	78.04%	10.472%
42	7.550	2006	2009	2013	rBV4	1982	1930	0.13%	0.017%
43	7.643	2028	2038	2058	rVB2	126681	211745	14.26%	1.914%
44	8.106	2171	2182	2214	rBV	377373	720499	48.53%	6.513%
45	8.605	2335	2337	2342	rVB6	1137	892	0.06%	0.008%
46	8.640	2344	2348	2351	rBV4	1074	990	0.07%	0.009%
47	8.736	2376	2378	2381	rBV4	1510	649	0.04%	0.006%
48	8.875	2409	2421	2443	rBV	642391	1046425	70.49%	9.459%
49	9.138	2500	2503	2506	rBV5	1447	1265	0.09%	0.011%
50	9.270	2542	2544	2545	rBV2	1445	626	0.04%	0.006%
51	9.479	2606	2609	2612	rBV4	1302	1048	0.07%	0.009%
52	9.637	2654	2658	2661	rBV5	1174	950	0.06%	0.009%
53	9.669	2665	2668	2670	rBV4	980	589	0.04%	0.005%
54	9.801	2707	2709	2712	rBV3	1225	738	0.05%	0.007%
55	9.855	2723	2726	2728	rBV3	1551	1069	0.07%	0.010%
56	9.897	2736	2739	2744	rVB6	1716	1120	0.08%	0.010%
57	9.958	2754	2758	2765	rVB7	2416	2466	0.17%	0.022%
58	9.990	2765	2768	2772	rVB5	1675	1091	0.07%	0.010%
59	10.035	2779	2782	2785	rBV4	1780	1343	0.09%	0.012%
60	10.170	2821	2824	2828	rBV6	1389	986	0.07%	0.009%
61	10.238	2834	2845	2862	rVB	435195	676126	45.55%	6.112%
62	10.379	2886	2889	2892	rBV4	1403	1099	0.07%	0.010%
63	10.460	2911	2914	2917	rVB6	1378	1027	0.07%	0.009%
64	10.711	2988	2992	2996	rBV5	1443	1280	0.09%	0.012%
65	10.749	3002	3004	3007	rVB4	1681	801	0.05%	0.007%
66	10.772	3007	3011	3015	rBV7	1702	1919	0.13%	0.017%
67	11.006	3082	3084	3087	rVB3	1643	752	0.05%	0.007%
68	11.103	3112	3114	3118	rVB3	1472	767	0.05%	0.007%
69	11.122	3118	3120	3122	rBV2	1952	1043	0.07%	0.009%
70	11.270	3154	3166	3182	rBV	653682	1010685	68.08%	9.136%
71	11.392	3201	3204	3206	rVB3	1549	741	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016699.D
 Acq On : 09 Jun 2020 08:03
 Operator : SY/MD
 Sample : VV0609WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK75

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.405	3206	3208	3210	rVV3	1105	635	0.04%	0.006%
73	11.434	3212	3217	3220	rBV7	1347	1286	0.09%	0.012%
74	11.505	3237	3239	3241	rBV3	1700	928	0.06%	0.008%
75	11.646	3271	3283	3304	rBV	712500	1136681	76.57%	10.275%
76	11.881	3352	3356	3359	rBV4	1948	1735	0.12%	0.016%
77	11.965	3379	3382	3386	rBV5	1202	1089	0.07%	0.010%
78	12.042	3402	3406	3410	rBV6	1631	1299	0.09%	0.012%
79	12.170	3442	3446	3452	rBV8	2318	2286	0.15%	0.021%
80	12.228	3461	3464	3466	rBV3	1020	773	0.05%	0.007%
81	12.270	3474	3477	3478	rBV3	1246	657	0.04%	0.006%
82	12.408	3514	3520	3521	rBV4	1186	1232	0.08%	0.011%
83	12.444	3528	3531	3534	rVB4	1371	910	0.06%	0.008%
84	12.572	3567	3571	3575	rBV5	1246	1273	0.09%	0.012%
85	12.617	3581	3585	3586	rBV5	1339	667	0.04%	0.006%
86	12.749	3624	3626	3630	rBV4	1410	1030	0.07%	0.009%
87	12.797	3640	3641	3647	rVB5	1294	867	0.06%	0.008%
88	12.849	3652	3657	3659	rBV5	1313	1507	0.10%	0.014%
89	12.913	3674	3677	3679	rBV3	1243	709	0.05%	0.006%
90	13.402	3827	3829	3832	rBV4	938	750	0.05%	0.007%
91	13.678	3912	3915	3919	rVB3	2053	1327	0.09%	0.012%
92	13.701	3919	3922	3924	rBV3	2159	1321	0.09%	0.012%
93	13.865	3968	3973	3977	rBV8	1718	2223	0.15%	0.020%
94	14.222	4080	4084	4086	rBV4	2116	1249	0.08%	0.011%
95	14.273	4097	4100	4104	rBV4	1571	1292	0.09%	0.012%
96	14.627	4208	4210	4213	rBV3	1189	601	0.04%	0.005%
97	14.788	4258	4260	4262	rBV3	1249	685	0.05%	0.006%
98	14.871	4282	4286	4289	rBV6	2216	2207	0.15%	0.020%
99	14.923	4300	4302	4305	rBV4	1851	988	0.07%	0.009%
100	15.395	4448	4449	4453	rBV4	1326	949	0.06%	0.009%


Sum of corrected areas: 11062692

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060920\
Data File : VV016699.D
Acq On : 09 Jun 2020 08:03
Operator : SY/MD
Sample : VV0609WBL01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK75

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

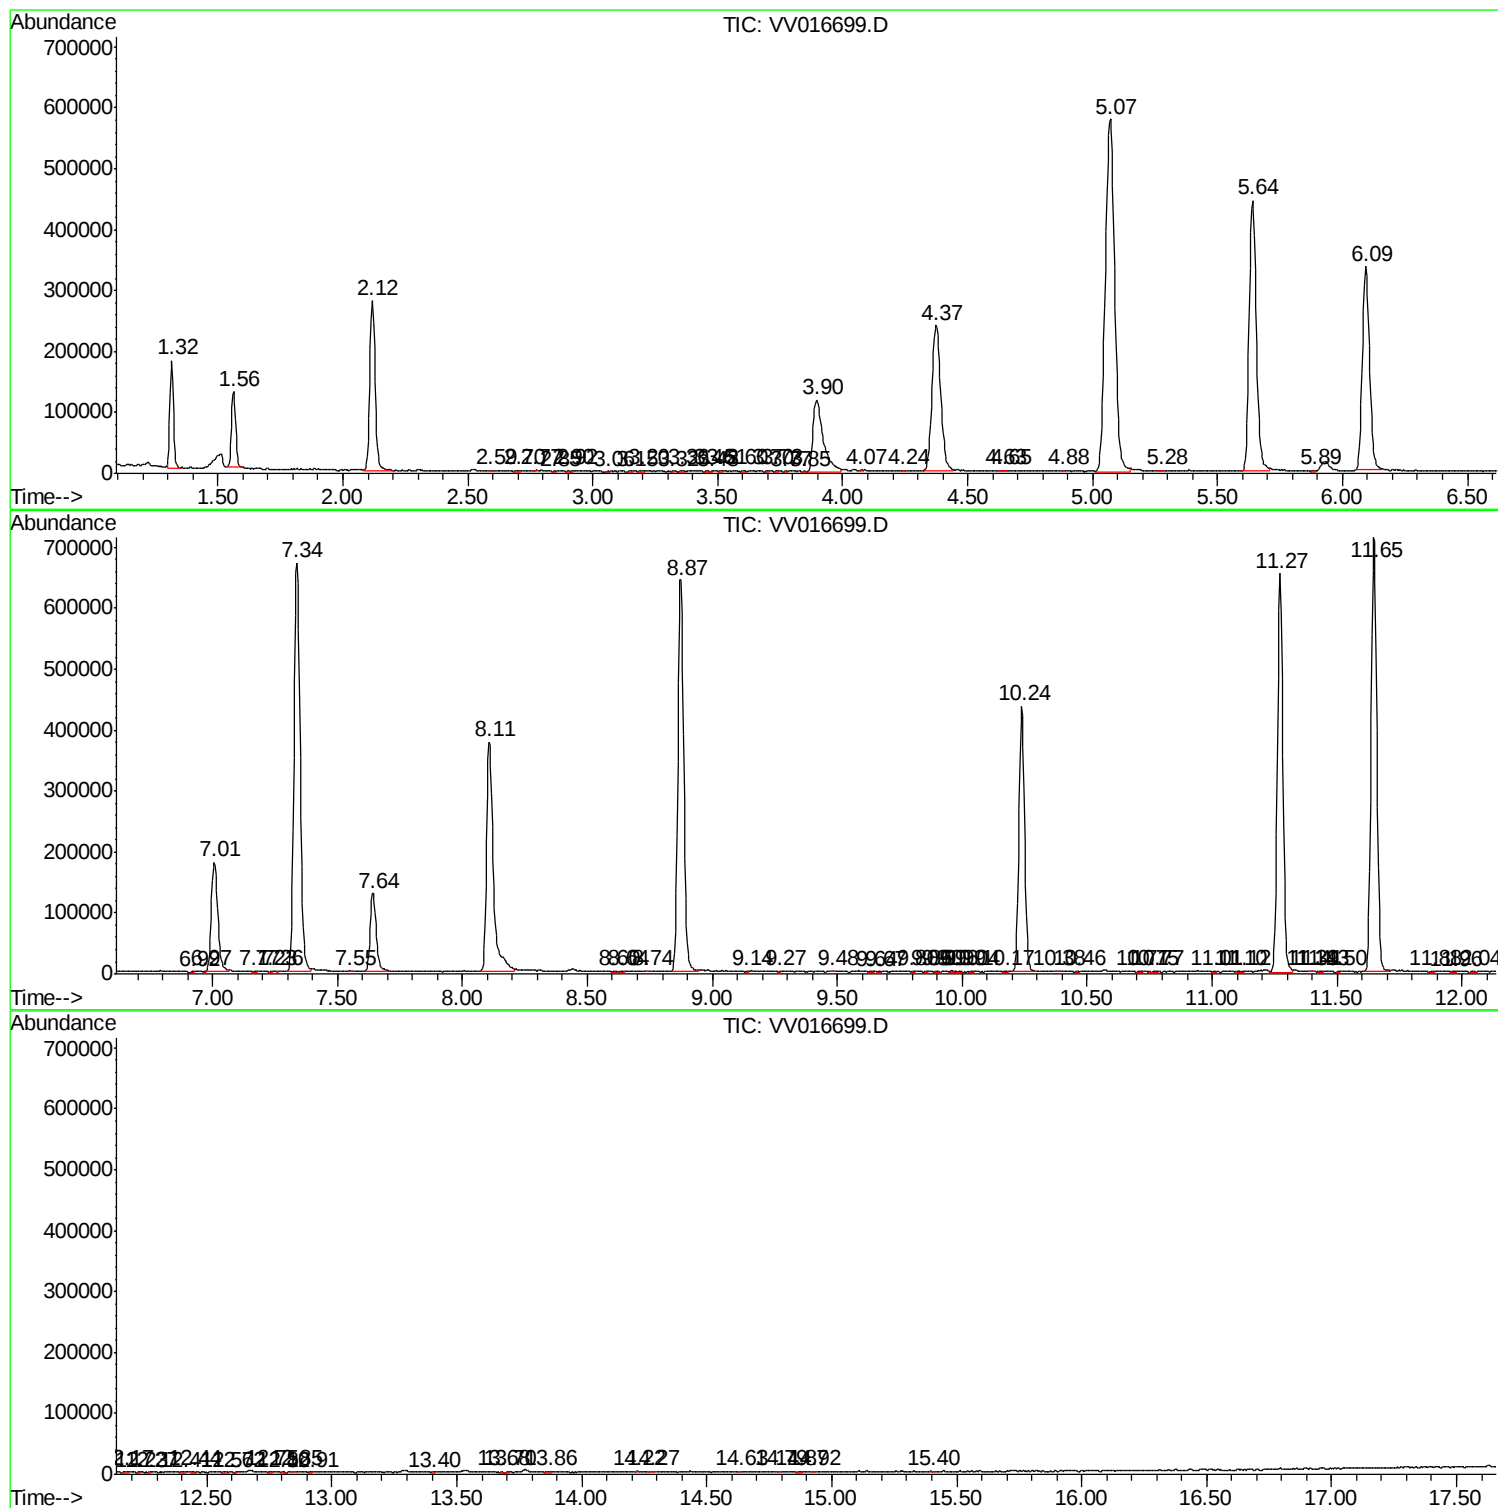

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV060920\
Data File : VV016699.D
Acq On : 09 Jun 2020 08:03
Operator : SY/MD
Sample : VV0609WBL01
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VBLK75

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV060920\
Data File : VV016699.D
Acq On : 09 Jun 2020 08:03
Operator : SY/MD
Sample : VV0609WBL01
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VBLK75

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc