

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016701.D
 Acq On : 09 Jun 2020 08:50
 Operator : SY/MD
 Sample : L2872-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFEP6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	80	rVB	166502	175173	12.07%	1.542%
2	1.563	142	147	157	rVB	123127	135901	9.36%	1.196%
3	2.116	310	319	340	rVB	268952	407327	28.07%	3.585%
4	2.277	363	369	373	rBV9	1333	1628	0.11%	0.014%
5	2.373	396	399	401	rBV3	1673	1115	0.08%	0.010%
6	2.450	421	423	428	rVB4	1701	1392	0.10%	0.012%
7	2.579	461	463	466	rBV3	930	646	0.04%	0.006%
8	2.952	574	579	581	rVB5	1237	894	0.06%	0.008%
9	2.984	586	589	591	rBV4	889	620	0.04%	0.005%
10	3.077	615	618	623	rVB6	1904	1151	0.08%	0.010%
11	3.116	628	630	633	rVB4	2128	1290	0.09%	0.011%
12	3.180	648	650	653	rBV4	1037	749	0.05%	0.007%
13	3.241	666	669	670	rBV3	1369	704	0.05%	0.006%
14	3.479	740	743	748	rVB5	894	860	0.06%	0.008%
15	3.630	789	790	795	rVV3	1975	758	0.05%	0.007%
16	3.682	803	806	809	rBV5	1797	1192	0.08%	0.010%
17	3.759	828	830	833	rVV4	893	672	0.05%	0.006%
18	3.897	863	873	905	rBV2	127354	380353	26.21%	3.348%
19	4.373	1008	1021	1042	rVB	233169	563280	38.81%	4.958%
20	4.997	1210	1215	1218	rBV7	1542	1290	0.09%	0.011%
21	5.071	1220	1238	1261	rBV2	562583	1451323	100.00%	12.774%
22	5.640	1403	1415	1441	rBV	449171	886016	61.05%	7.798%
23	5.778	1456	1458	1462	rBV3	1003	658	0.05%	0.006%
24	6.093	1537	1556	1583	rBV	331482	672893	46.36%	5.922%
25	6.344	1631	1634	1638	rBV6	2062	1662	0.11%	0.015%
26	6.502	1678	1683	1685	rBV3	2291	1851	0.13%	0.016%
27	6.537	1691	1694	1695	rBV3	1426	824	0.06%	0.007%
28	6.768	1764	1766	1769	rBV3	1149	694	0.05%	0.006%
29	6.801	1774	1776	1780	rBV4	1377	751	0.05%	0.007%
30	6.875	1794	1799	1802	rBV7	1302	1265	0.09%	0.011%
31	7.006	1827	1840	1859	rBV2	177519	320370	22.07%	2.820%
32	7.338	1930	1943	1965	rBV	671282	1142414	78.72%	10.055%
33	7.598	2021	2024	2026	rBV4	1969	1116	0.08%	0.010%
34	7.640	2028	2037	2054	rVV	123924	211073	14.54%	1.858%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016701.D
 Acq On : 09 Jun 2020 08:50
 Operator : SY/MD
 Sample : L2872-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFEP6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	7.762	2070	2075	2078	rBV6	2306	1901	0.13%	0.017%
36	7.794	2083	2085	2087	rBV3	1325	760	0.05%	0.007%
37	7.910	2118	2121	2123	rBV4	1656	845	0.06%	0.007%
38	7.997	2138	2148	2169	rVB	219564	379281	26.13%	3.338%
39	8.109	2172	2183	2216	rBV	369836	705680	48.62%	6.211%
40	8.791	2393	2395	2399	rVB5	1940	1186	0.08%	0.010%
41	8.820	2399	2404	2406	rBV4	2412	1579	0.11%	0.014%
42	8.874	2409	2421	2439	rBV	671865	1082020	74.55%	9.523%
43	9.064	2478	2480	2483	rVB4	1241	717	0.05%	0.006%
44	9.083	2483	2486	2487	rBV3	1449	824	0.06%	0.007%
45	9.164	2504	2511	2521	rBV3	2526	4691	0.32%	0.041%
46	9.209	2523	2525	2528	rBV3	1589	1164	0.08%	0.010%
47	9.244	2534	2536	2541	rBV5	1278	1001	0.07%	0.009%
48	9.267	2541	2543	2547	rBV3	2016	1387	0.10%	0.012%
49	9.354	2564	2570	2572	rBV7	1950	1545	0.11%	0.014%
50	9.556	2630	2633	2634	rBV3	1357	786	0.05%	0.007%
51	9.665	2665	2667	2671	rVB4	2556	1529	0.11%	0.013%
52	9.810	2710	2712	2717	rBV6	1502	1081	0.07%	0.010%
53	9.849	2720	2724	2728	rBV7	1034	936	0.06%	0.008%
54	10.173	2822	2825	2827	rBV3	1015	615	0.04%	0.005%
55	10.238	2834	2845	2862	rVB	423652	663520	45.72%	5.840%
56	10.505	2925	2928	2930	rBV2	1939	1044	0.07%	0.009%
57	10.582	2949	2952	2956	rBV3	1601	1072	0.07%	0.009%
58	10.704	2988	2990	2993	rVB3	1162	638	0.04%	0.006%
59	10.759	3006	3007	3010	rBV2	1109	629	0.04%	0.006%
60	10.800	3017	3020	3023	rVB4	2143	1265	0.09%	0.011%
61	10.820	3023	3026	3028	rBV3	1006	615	0.04%	0.005%
62	10.987	3074	3078	3079	rBV3	2118	1177	0.08%	0.010%
63	11.209	3142	3147	3150	rVV6	2385	1860	0.13%	0.016%
64	11.270	3155	3166	3180	rBV	665623	1013973	69.87%	8.924%
65	11.389	3198	3203	3205	rVB5	1459	1343	0.09%	0.012%
66	11.402	3205	3207	3212	rBV5	1225	1046	0.07%	0.009%
67	11.505	3235	3239	3241	rBV4	1259	943	0.06%	0.008%
68	11.649	3268	3284	3302	rBV	678893	1080865	74.47%	9.513%
69	11.916	3363	3367	3370	rBV4	1299	949	0.07%	0.008%
70	11.990	3387	3390	3391	rBV3	1745	825	0.06%	0.007%
71	12.054	3408	3410	3415	rVB6	1101	814	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016701.D
 Acq On : 09 Jun 2020 08:50
 Operator : SY/MD
 Sample : L2872-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFEP6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.083	3417	3419	3425	rVB6	1474	1016	0.07%	0.009%
73	12.119	3425	3430	3433	rBV6	1233	1323	0.09%	0.012%
74	12.157	3438	3442	3443	rBV3	1132	677	0.05%	0.006%
75	12.196	3452	3454	3458	rBV5	953	649	0.04%	0.006%
76	12.299	3483	3486	3488	rBV4	1060	845	0.06%	0.007%
77	12.328	3493	3495	3499	rBV5	1072	948	0.07%	0.008%
78	12.427	3524	3526	3530	rBV6	1231	970	0.07%	0.009%
79	12.469	3536	3539	3542	rBV5	1077	717	0.05%	0.006%
80	12.501	3548	3549	3552	rVB2	1640	899	0.06%	0.008%
81	12.765	3630	3631	3636	rVB5	1748	1130	0.08%	0.010%
82	12.855	3655	3659	3662	rBV4	1812	1569	0.11%	0.014%
83	12.884	3662	3668	3670	rBV6	1555	1454	0.10%	0.013%
84	13.289	3786	3794	3798	rBV6	1783	2750	0.19%	0.024%
85	13.344	3808	3811	3812	rBV2	1743	800	0.06%	0.007%
86	13.415	3830	3833	3835	rBV3	1733	929	0.06%	0.008%
87	13.440	3839	3841	3847	rVB6	2010	1193	0.08%	0.011%
88	13.469	3847	3850	3852	rBV3	1139	892	0.06%	0.008%
89	13.636	3900	3902	3904	rBV2	1583	901	0.06%	0.008%
90	13.916	3985	3989	3990	rBV4	1097	727	0.05%	0.006%
91	13.974	4003	4007	4009	rBV5	1118	863	0.06%	0.008%
92	14.083	4039	4041	4044	rBV3	1450	821	0.06%	0.007%
93	14.132	4054	4056	4061	rBV5	1143	1219	0.08%	0.011%
94	14.177	4068	4070	4072	rBV2	1222	704	0.05%	0.006%
95	14.228	4084	4086	4087	rBV2	1867	828	0.06%	0.007%
96	14.543	4182	4184	4189	rVB5	1028	785	0.05%	0.007%
97	14.591	4196	4199	4201	rBV4	1335	1126	0.08%	0.010%
98	15.045	4336	4340	4341	rBV4	1804	1330	0.09%	0.012%
99	15.086	4351	4353	4354	rBV2	1502	636	0.04%	0.006%
100	15.476	4470	4474	4477	rBV5	1239	1059	0.07%	0.009%


Sum of corrected areas: 11361771

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060920\
Data File : VV016701.D
Acq On : 09 Jun 2020 08:50
Operator : SY/MD
Sample : L2872-14
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFEP6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

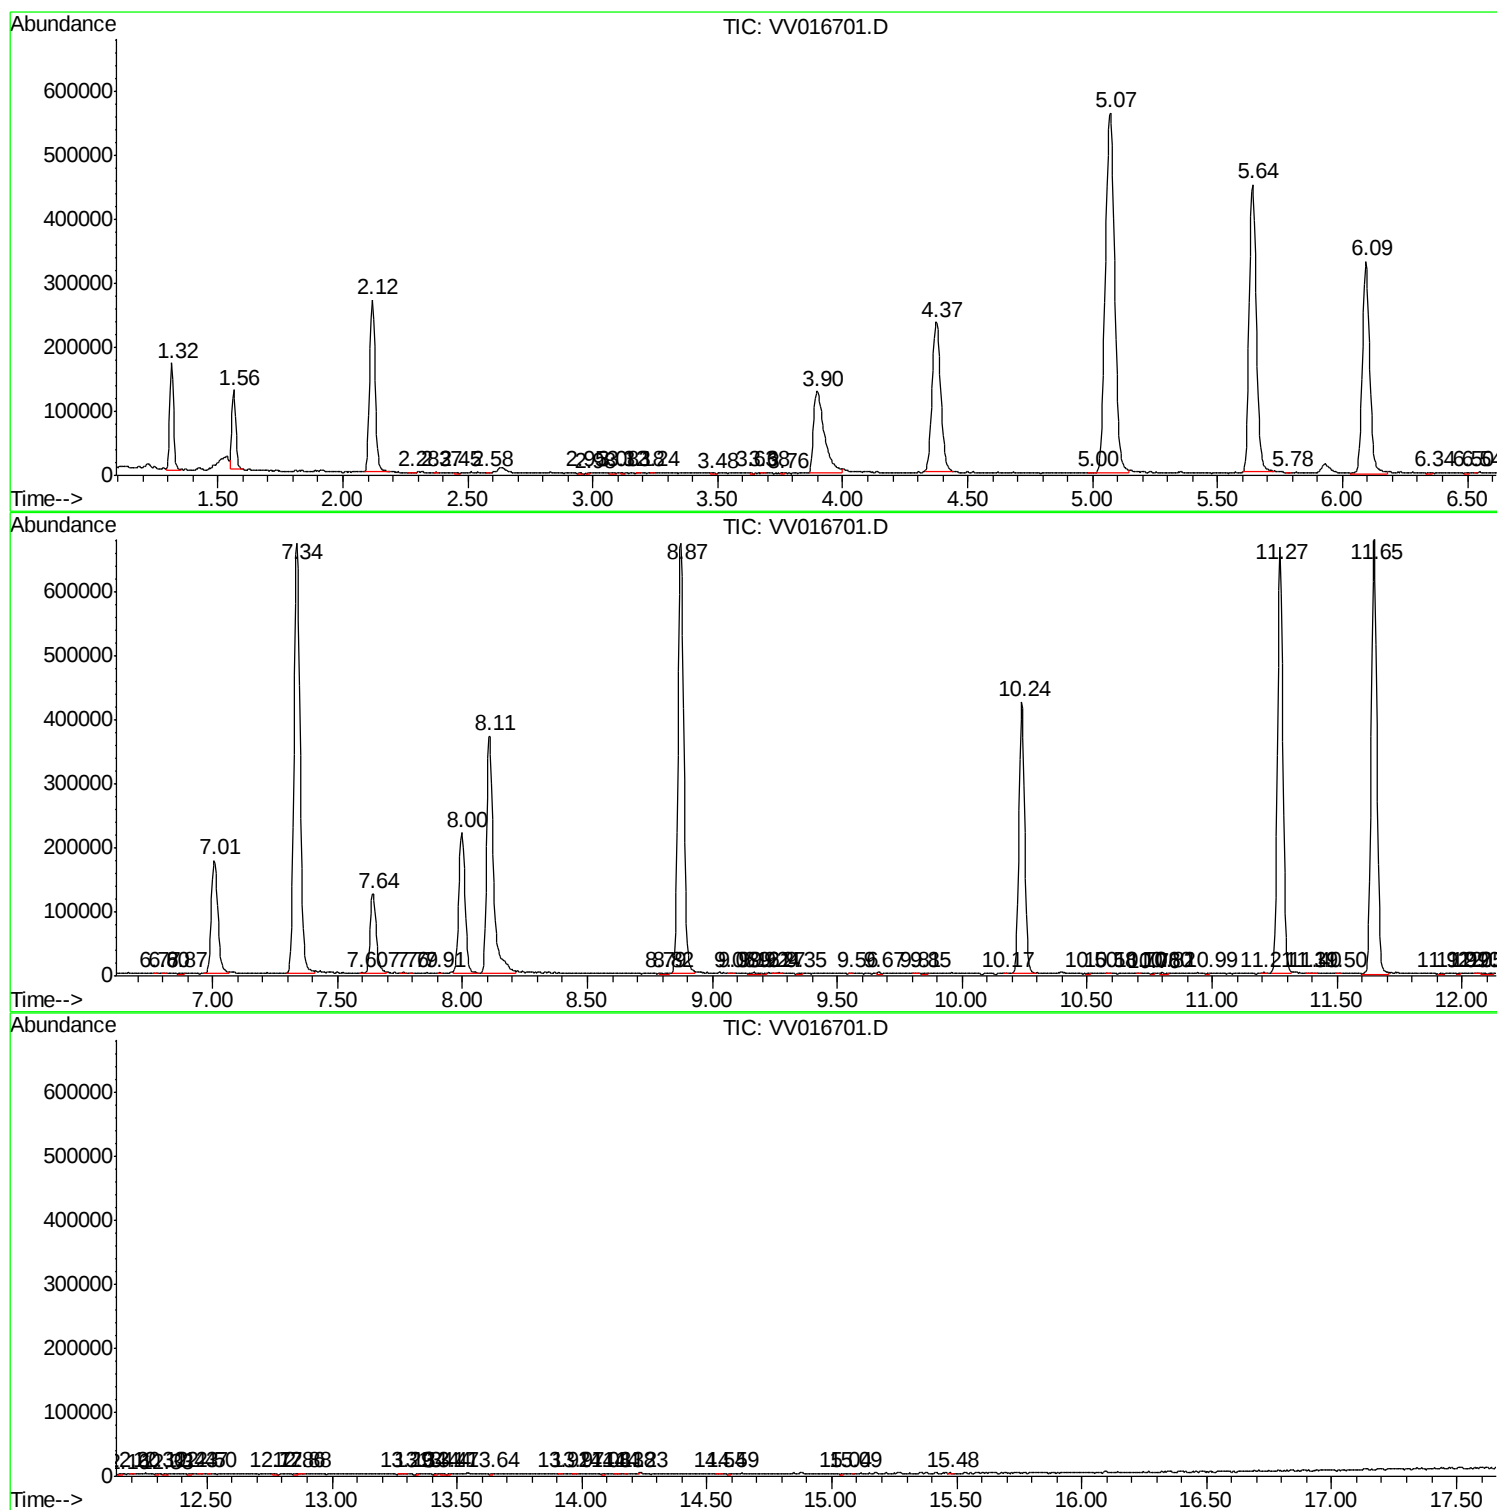

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016701.D
Acq On : 09 Jun 2020 08:50
Operator : SY/MD
Sample : L2872-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFEP6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016701.D
Acq On : 09 Jun 2020 08:50
Operator : SY/MD
Sample : L2872-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFEP6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc