

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016703.D
 Acq On : 09 Jun 2020 09:43
 Operator : SY/MD
 Sample : L2862-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	64	70	81	rVB	178440	189825	13.17%	1.782%
2	2.116	310	319	337	rVB	281087	419984	29.14%	3.943%
3	2.920	568	569	574	rVB4	2463	1409	0.10%	0.013%
4	2.946	574	577	578	rBV3	1218	814	0.06%	0.008%
5	3.042	604	607	609	rVB3	1714	967	0.07%	0.009%
6	3.132	633	635	637	rBV3	1471	772	0.05%	0.007%
7	3.219	660	662	665	rBV4	1744	947	0.07%	0.009%
8	3.258	670	674	676	rVB4	1241	749	0.05%	0.007%
9	3.274	676	679	680	rBV3	1675	857	0.06%	0.008%
10	3.573	767	772	774	rBV5	1518	1295	0.09%	0.012%
11	3.724	817	819	823	rBV4	1433	1210	0.08%	0.011%
12	3.759	828	830	832	rBV3	1077	719	0.05%	0.007%
13	3.807	841	845	849	rVB7	2086	1760	0.12%	0.017%
14	3.827	849	851	855	rBV3	1619	1028	0.07%	0.010%
15	3.856	855	860	861	rBV4	1322	1276	0.09%	0.012%
16	3.897	863	873	903	rBV	110406	306951	21.30%	2.882%
17	4.309	999	1001	1004	rVB3	1600	766	0.05%	0.007%
18	4.373	1004	1021	1044	rBV	234417	575431	39.93%	5.402%
19	4.669	1110	1113	1117	rBV5	1687	1632	0.11%	0.015%
20	4.820	1158	1160	1163	rBV3	1324	935	0.06%	0.009%
21	5.071	1219	1238	1260	rBV2	562453	1441110	100.00%	13.530%
22	5.537	1381	1383	1386	rBV4	1740	1099	0.08%	0.010%
23	5.553	1386	1388	1393	rVB6	1335	963	0.07%	0.009%
24	5.640	1402	1415	1436	rBV	433411	860570	59.72%	8.079%
25	5.878	1487	1489	1490	rBV2	1304	643	0.04%	0.006%
26	6.013	1529	1531	1535	rVB4	1850	1025	0.07%	0.010%
27	6.094	1544	1556	1577	rVB	326291	648585	45.01%	6.089%
28	6.425	1654	1659	1662	rBV7	1793	1785	0.12%	0.017%
29	6.782	1768	1770	1774	rVB4	1562	906	0.06%	0.009%
30	6.868	1795	1797	1802	rVB4	1535	863	0.06%	0.008%
31	6.949	1819	1822	1825	rBV5	1167	996	0.07%	0.009%
32	7.007	1829	1840	1861	rVV	186849	333304	23.13%	3.129%
33	7.338	1931	1943	1960	rBV	650802	1114328	77.32%	10.462%
34	7.640	2027	2037	2053	rBV	130234	223867	15.53%	2.102%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016703.D
 Acq On : 09 Jun 2020 09:43
 Operator : SY/MD
 Sample : L2862-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	8.110	2171	2183	2217	rBV	354007	700315	48.60%	6.575%
36	8.569	2324	2326	2328	rBV3	1549	687	0.05%	0.006%
37	8.582	2328	2330	2332	rVB3	1668	774	0.05%	0.007%
38	8.695	2360	2365	2368	rBV5	1133	1204	0.08%	0.011%
39	8.804	2395	2399	2400	rBV3	1491	949	0.07%	0.009%
40	8.872	2408	2420	2436	rBV	649108	1047230	72.67%	9.832%
41	9.132	2499	2501	2504	rBV4	1463	1073	0.07%	0.010%
42	9.306	2553	2555	2556	rBV	1331	646	0.04%	0.006%
43	9.380	2575	2578	2582	rBV5	1261	1159	0.08%	0.011%
44	9.447	2595	2599	2603	rBV6	1667	1191	0.08%	0.011%
45	9.502	2614	2616	2620	rVB5	1257	653	0.05%	0.006%
46	9.524	2620	2623	2625	rBV4	1785	1336	0.09%	0.013%
47	9.572	2635	2638	2640	rBV3	1724	987	0.07%	0.009%
48	9.592	2640	2644	2647	rBV6	1188	1020	0.07%	0.010%
49	9.630	2654	2656	2661	rBV5	1232	977	0.07%	0.009%
50	9.698	2675	2677	2683	rBV6	1127	961	0.07%	0.009%
51	9.807	2707	2711	2713	rBV5	1435	1260	0.09%	0.012%
52	9.945	2752	2754	2757	rBV3	1389	793	0.06%	0.007%
53	10.080	2793	2796	2798	rBV3	1487	1094	0.08%	0.010%
54	10.145	2813	2816	2819	rBV4	1349	1128	0.08%	0.011%
55	10.180	2825	2827	2829	rBV3	1772	767	0.05%	0.007%
56	10.238	2833	2845	2858	rBV	415076	652142	45.25%	6.123%
57	10.389	2889	2892	2896	rBV5	1527	1353	0.09%	0.013%
58	10.466	2913	2916	2918	rBV3	1817	1191	0.08%	0.011%
59	10.653	2972	2974	2979	rBV4	1660	954	0.07%	0.009%
60	10.743	3000	3002	3005	rVB3	1336	837	0.06%	0.008%
61	10.759	3005	3007	3010	rBV4	1396	924	0.06%	0.009%
62	10.900	3048	3051	3054	rBV4	1170	856	0.06%	0.008%
63	10.974	3069	3074	3077	rBV6	1294	1113	0.08%	0.010%
64	10.994	3077	3080	3082	rVV3	1302	671	0.05%	0.006%
65	11.170	3131	3135	3138	rVB5	1380	1141	0.08%	0.011%
66	11.270	3154	3166	3187	rBV	642135	985862	68.41%	9.256%
67	11.434	3215	3217	3220	rBV4	1194	670	0.05%	0.006%
68	11.550	3251	3253	3255	rBV3	1280	747	0.05%	0.007%
69	11.646	3271	3283	3298	rBV	684543	1065779	73.96%	10.006%
70	11.936	3368	3373	3375	rBV6	1526	864	0.06%	0.008%
71	11.974	3380	3385	3387	rBV5	1415	1233	0.09%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016703.D
 Acq On : 09 Jun 2020 09:43
 Operator : SY/MD
 Sample : L2862-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.000	3390	3393	3394	rBV3	1491	971	0.07%	0.009%
73	12.193	3450	3453	3455	rBV5	1019	675	0.05%	0.006%
74	12.289	3479	3483	3484	rBV4	1016	792	0.05%	0.007%
75	12.354	3500	3503	3507	rVB4	2071	1679	0.12%	0.016%
76	12.373	3507	3509	3511	rBV2	1862	1034	0.07%	0.010%
77	12.476	3539	3541	3547	rVV6	1219	936	0.06%	0.009%
78	12.537	3558	3560	3565	rVB4	1866	1441	0.10%	0.014%
79	12.666	3596	3600	3601	rBV4	1909	1180	0.08%	0.011%
80	12.717	3612	3616	3617	rBV3	1081	805	0.06%	0.008%
81	12.778	3632	3635	3641	rBV8	1298	1309	0.09%	0.012%
82	12.810	3641	3645	3649	rBV7	1628	1654	0.11%	0.016%
83	12.952	3687	3689	3693	rVB5	2065	1339	0.09%	0.013%
84	12.974	3693	3696	3698	rBV3	1614	828	0.06%	0.008%
85	13.000	3702	3704	3708	rBV2	1757	986	0.07%	0.009%
86	13.029	3708	3713	3714	rBV3	1119	834	0.06%	0.008%
87	13.183	3760	3761	3764	rBV3	1189	892	0.06%	0.008%
88	13.222	3771	3773	3777	rBV2	1837	1448	0.10%	0.014%
89	13.424	3834	3836	3838	rBV3	1443	771	0.05%	0.007%
90	13.630	3895	3900	3903	rBV6	2119	1557	0.11%	0.015%
91	13.711	3923	3925	3928	rBV4	1107	686	0.05%	0.006%
92	13.884	3975	3979	3984	rBV7	731	779	0.05%	0.007%
93	14.048	4028	4030	4032	rBV2	1413	824	0.06%	0.008%
94	14.096	4043	4045	4048	rBV3	1623	864	0.06%	0.008%
95	14.302	4107	4109	4112	rBV4	1182	738	0.05%	0.007%
96	14.402	4137	4140	4142	rBV4	1133	768	0.05%	0.007%
97	14.437	4149	4151	4154	rBV4	1245	644	0.04%	0.006%
98	14.730	4240	4242	4244	rBV3	1374	686	0.05%	0.006%
99	15.000	4322	4326	4329	rBV4	1878	1470	0.10%	0.014%
100	15.492	4476	4479	4481	rBV3	1839	939	0.07%	0.009%


Sum of corrected areas: 10651441

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060920\
Data File : VV016703.D
Acq On : 09 Jun 2020 09:43
Operator : SY/MD
Sample : L2862-02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

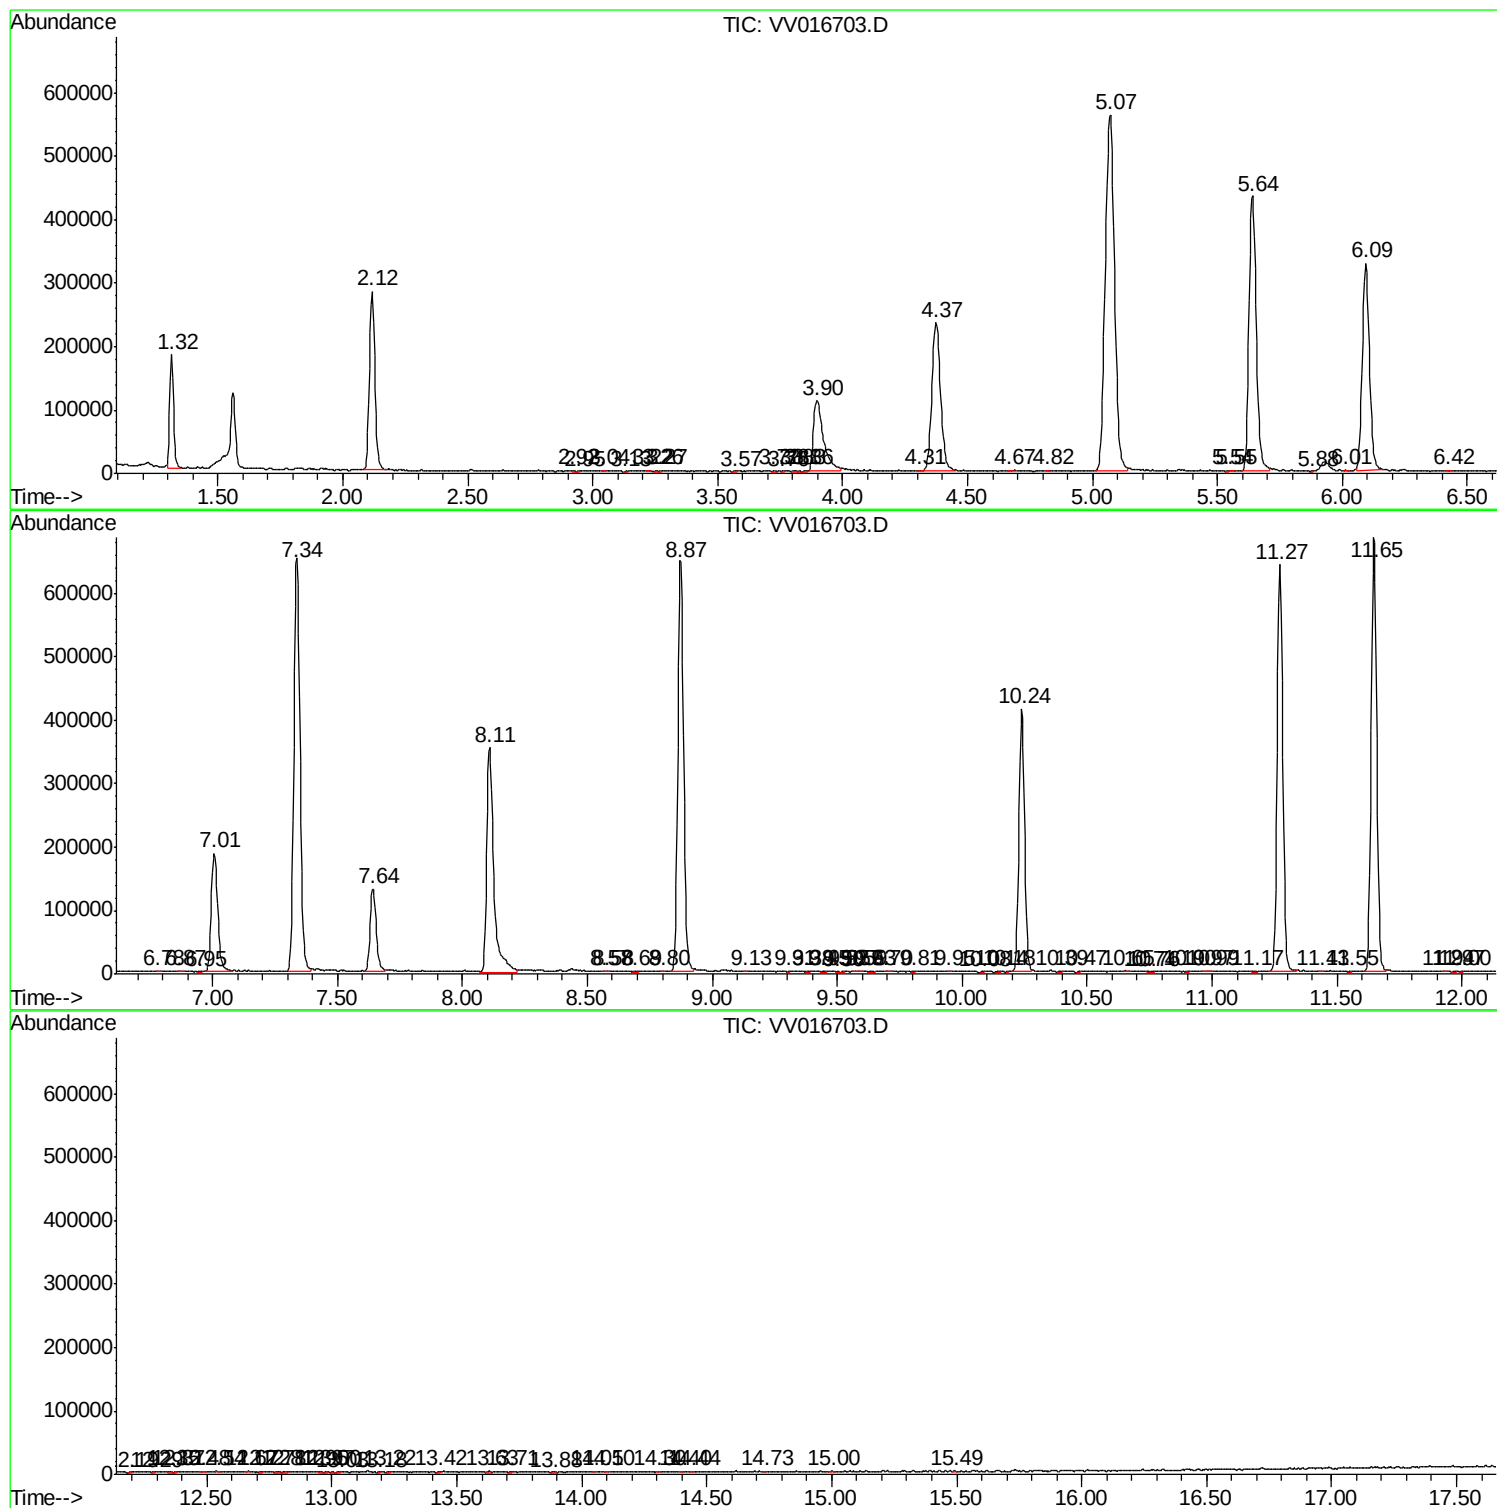

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016703.D
Acq On : 09 Jun 2020 09:43
Operator : SY/MD
Sample : L2862-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016703.D
Acq On : 09 Jun 2020 09:43
Operator : SY/MD
Sample : L2862-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc