

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016705.D
 Acq On : 09 Jun 2020 10:30
 Operator : SY/MD
 Sample : L2875-16
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTT8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	82	rVB2	265051	284163	22.45%	2.857%
2	1.553	138	144	159	rVB	103464	129637	10.24%	1.304%
3	2.116	309	319	332	rBV	235836	351428	27.76%	3.534%
4	2.286	370	372	373	rBV3	1407	508	0.04%	0.005%
5	2.868	550	553	557	rBV5	1541	1378	0.11%	0.014%
6	3.113	627	629	632	rBV3	1663	1007	0.08%	0.010%
7	3.190	651	653	654	rVB2	962	289	0.02%	0.003%
8	3.206	654	658	659	rBV5	686	421	0.03%	0.004%
9	3.257	673	674	675	rBV	1139	387	0.03%	0.004%
10	3.299	685	687	688	rBV3	653	289	0.02%	0.003%
11	3.312	689	691	692	rVV2	997	363	0.03%	0.004%
12	3.338	697	699	702	rVV4	1342	632	0.05%	0.006%
13	3.367	705	708	712	rBV5	1463	1333	0.11%	0.013%
14	3.482	742	744	746	rBV3	881	506	0.04%	0.005%
15	3.540	761	762	764	rVB	1373	345	0.03%	0.003%
16	3.553	764	766	767	rBV2	1034	403	0.03%	0.004%
17	3.595	774	779	784	rBV7	1825	1991	0.16%	0.020%
18	3.630	786	790	792	rBV4	1608	1232	0.10%	0.012%
19	3.646	792	795	797	rBV3	1449	755	0.06%	0.008%
20	3.691	805	809	811	rBV5	1651	1234	0.10%	0.012%
21	3.704	811	813	816	rVB3	1523	703	0.06%	0.007%
22	3.724	816	819	821	rBV3	868	497	0.04%	0.005%
23	3.746	821	826	828	rBV4	1463	1108	0.09%	0.011%
24	3.894	862	872	909	rBV	118524	374693	29.60%	3.768%
25	4.116	939	941	942	rBV2	1352	598	0.05%	0.006%
26	4.241	978	980	982	rBV3	1287	878	0.07%	0.009%
27	4.277	990	991	995	rVB3	1387	735	0.06%	0.007%
28	4.373	1000	1021	1048	rBV	207235	514625	40.65%	5.175%
29	4.531	1067	1070	1073	rBV5	1375	1176	0.09%	0.012%
30	4.643	1103	1105	1107	rBV3	1803	759	0.06%	0.008%
31	4.810	1152	1157	1159	rBV4	1875	1811	0.14%	0.018%
32	4.936	1195	1196	1197	rBV	755	270	0.02%	0.003%
33	4.971	1206	1207	1210	rVB2	1189	478	0.04%	0.005%
34	5.068	1221	1237	1261	rBV2	493759	1266026	100.00%	12.730%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016705.D
 Acq On : 09 Jun 2020 10:30
 Operator : SY/MD
 Sample : L2875-16
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTT8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	5.421	1345	1347	1351	rBV3	1720	976	0.08%	0.010%
36	5.460	1357	1359	1360	rBV2	1353	524	0.04%	0.005%
37	5.505	1370	1373	1376	rBV4	1668	1277	0.10%	0.013%
38	5.547	1383	1386	1388	rBV4	1701	1022	0.08%	0.010%
39	5.640	1402	1415	1435	rBV	344514	693526	54.78%	6.974%
40	5.862	1481	1484	1485	rBV3	1724	844	0.07%	0.008%
41	6.093	1543	1556	1578	rBV	284239	578472	45.69%	5.817%
42	6.476	1672	1675	1679	rBV5	1237	1229	0.10%	0.012%
43	6.768	1764	1766	1768	rBV3	943	422	0.03%	0.004%
44	6.823	1780	1783	1784	rBV2	1208	594	0.05%	0.006%
45	6.862	1793	1795	1797	rBV2	684	310	0.02%	0.003%
46	6.887	1801	1803	1805	rBV3	1511	659	0.05%	0.007%
47	6.916	1810	1812	1817	rBV6	1303	1014	0.08%	0.010%
48	7.006	1829	1840	1855	rBV	167544	295351	23.33%	2.970%
49	7.129	1876	1878	1880	rVB3	1970	863	0.07%	0.009%
50	7.338	1931	1943	1961	rBV	584596	990980	78.27%	9.965%
51	7.640	2028	2037	2054	rBV	120339	197860	15.63%	1.990%
52	7.897	2115	2117	2119	rBV3	1871	925	0.07%	0.009%
53	8.106	2172	2182	2214	rBV	400176	754703	59.61%	7.589%
54	8.344	2253	2256	2258	rBV3	2094	1336	0.11%	0.013%
55	8.524	2310	2312	2314	rBV2	1158	519	0.04%	0.005%
56	8.630	2342	2345	2346	rBV3	1385	811	0.06%	0.008%
57	8.665	2354	2356	2361	rBV5	1323	1067	0.08%	0.011%
58	8.874	2410	2421	2440	rVB	518372	840327	66.38%	8.450%
59	9.289	2548	2550	2554	rVB3	2030	1258	0.10%	0.013%
60	9.309	2554	2556	2559	rBV4	1270	642	0.05%	0.006%
61	9.553	2631	2632	2634	rBV2	1148	481	0.04%	0.005%
62	9.582	2639	2641	2644	rVV3	1492	726	0.06%	0.007%
63	9.768	2697	2699	2701	rBV3	1229	562	0.04%	0.006%
64	10.170	2822	2824	2828	rBV5	1654	946	0.07%	0.010%
65	10.238	2833	2845	2863	rVV	415167	651497	51.46%	6.551%
66	10.447	2907	2910	2911	rBV2	1559	949	0.07%	0.010%
67	10.518	2928	2932	2933	rBV4	2091	1518	0.12%	0.015%
68	10.919	3052	3057	3059	rBV6	1490	1251	0.10%	0.013%
69	11.026	3088	3090	3092	rBV3	1392	641	0.05%	0.006%
70	11.128	3120	3122	3124	rBV3	1843	687	0.05%	0.007%
71	11.270	3155	3166	3185	rBV	566391	875550	69.16%	8.804%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016705.D
 Acq On : 09 Jun 2020 10:30
 Operator : SY/MD
 Sample : L2875-16
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTT8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.553	3245	3254	3265	rBV3	15626	29338	2.32%	0.295%
73	11.646	3272	3283	3308	rVB	664154	1050317	82.96%	10.561%
74	11.897	3358	3361	3362	rBV3	1309	683	0.05%	0.007%
75	12.096	3419	3423	3424	rBV4	1346	955	0.08%	0.010%
76	12.257	3470	3473	3475	rBV4	1275	667	0.05%	0.007%
77	12.328	3492	3495	3496	rBV3	1653	870	0.07%	0.009%
78	12.533	3556	3559	3562	rBV6	1621	1225	0.10%	0.012%
79	12.624	3585	3587	3589	rBV4	1439	676	0.05%	0.007%
80	12.697	3608	3610	3614	rVB4	1200	821	0.06%	0.008%
81	12.865	3658	3662	3663	rBV4	2372	1481	0.12%	0.015%
82	12.945	3683	3687	3688	rBV4	2028	1200	0.09%	0.012%
83	13.096	3731	3734	3736	rBV2	1762	905	0.07%	0.009%
84	13.244	3777	3780	3782	rBV2	1038	748	0.06%	0.008%
85	13.482	3852	3854	3856	rBV3	1519	547	0.04%	0.006%
86	13.813	3956	3957	3958	rBV	1255	457	0.04%	0.005%
87	13.836	3963	3964	3965	rBV	912	279	0.02%	0.003%
88	13.861	3969	3972	3975	rBV5	1686	1095	0.09%	0.011%
89	14.225	4083	4085	4088	rVB3	1790	775	0.06%	0.008%
90	14.241	4088	4090	4092	rBV3	1816	926	0.07%	0.009%
91	14.649	4214	4217	4219	rBV3	1524	916	0.07%	0.009%
92	14.951	4305	4311	4313	rBV5	1680	1617	0.13%	0.016%
93	15.109	4356	4360	4362	rBV4	1783	1488	0.12%	0.015%
94	15.389	4442	4447	4449	rBV6	2115	1874	0.15%	0.019%


Sum of corrected areas: 9944837

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060920\
Data File : VV016705.D
Acq On : 09 Jun 2020 10:30
Operator : SY/MD
Sample : L2875-16
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
ETTT8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

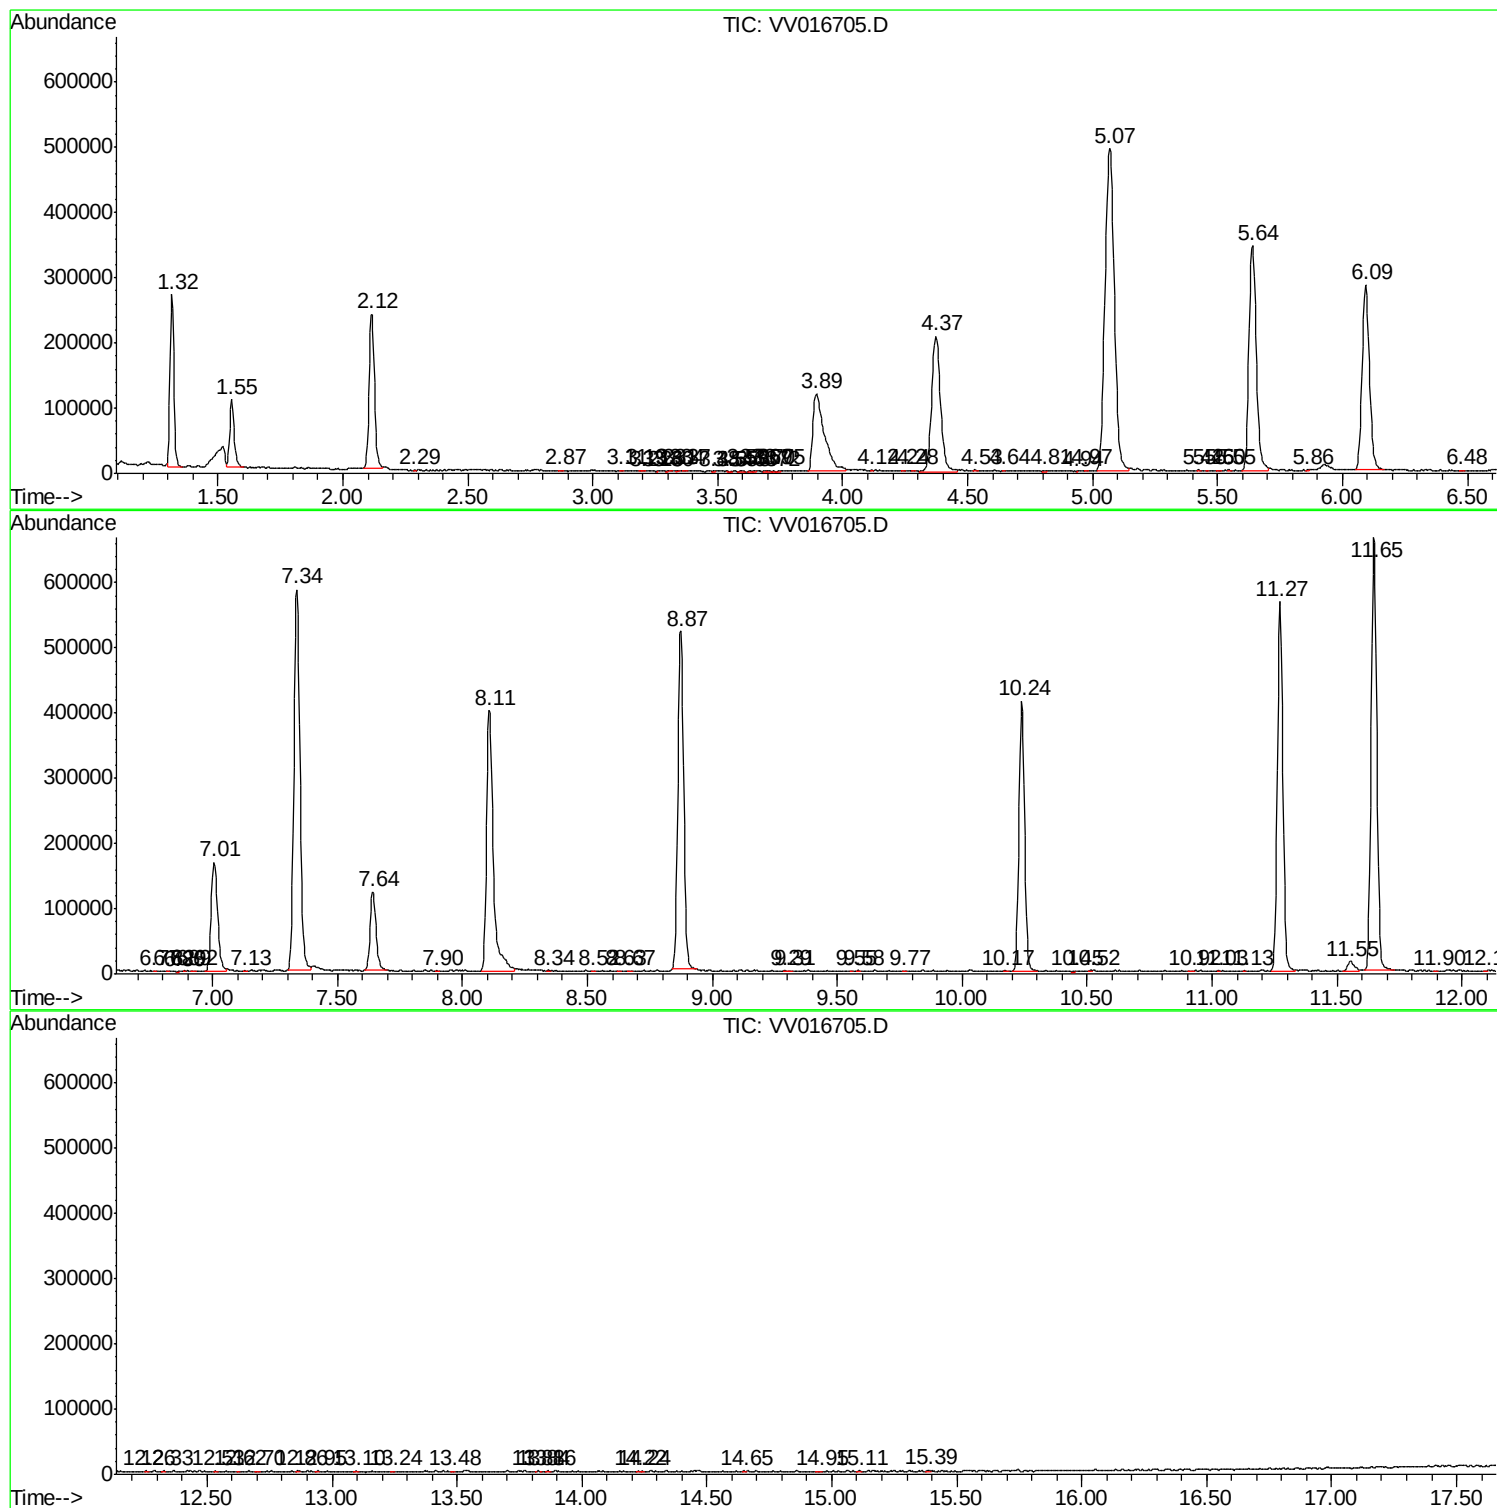

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016705.D
Acq On : 09 Jun 2020 10:30
Operator : SY/MD
Sample : L2875-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTT8

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016705.D
Acq On : 09 Jun 2020 10:30
Operator : SY/MD
Sample : L2875-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTT8

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc