

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016706.D
 Acq On : 09 Jun 2020 10:54
 Operator : SY/MD
 Sample : L2861-10DL 200X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E42DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	79	rVB	170280	174881	13.28%	1.536%
2	1.560	140	146	158	rVB	117463	141376	10.73%	1.242%
3	2.116	310	319	332	rBV	260973	380354	28.88%	3.342%
4	2.299	374	376	378	rBV3	1321	555	0.04%	0.005%
5	2.868	551	553	556	rBV4	1163	623	0.05%	0.005%
6	2.942	573	576	578	rBV4	1377	1121	0.09%	0.010%
7	3.045	606	608	610	rBV3	1204	623	0.05%	0.005%
8	3.174	647	648	650	rBV2	1119	530	0.04%	0.005%
9	3.225	658	664	665	rBV4	1617	1571	0.12%	0.014%
10	3.286	680	683	687	rBV5	1761	1510	0.11%	0.013%
11	3.306	687	689	693	rBV4	1071	826	0.06%	0.007%
12	3.351	701	703	707	rVB3	1632	763	0.06%	0.007%
13	3.425	721	726	727	rBV5	1212	827	0.06%	0.007%
14	3.749	826	827	829	rBV2	1072	568	0.04%	0.005%
15	3.894	857	872	903	rBV	118330	335771	25.49%	2.950%
16	4.302	995	999	1002	rBV5	1276	1238	0.09%	0.011%
17	4.373	1007	1021	1042	rVV2	227219	552725	41.97%	4.856%
18	4.630	1097	1101	1104	rBV5	1634	1281	0.10%	0.011%
19	4.804	1152	1155	1158	rBV5	1658	1292	0.10%	0.011%
20	4.855	1169	1171	1175	rVB5	1725	1084	0.08%	0.010%
21	4.978	1204	1209	1212	rVB6	1714	1426	0.11%	0.013%
22	5.071	1219	1238	1244	rBV2	557016	1317046	100.00%	11.571%
23	5.566	1390	1392	1395	rBV3	1294	743	0.06%	0.007%
24	5.640	1401	1415	1438	rBV	430688	862930	65.52%	7.582%
25	6.093	1543	1556	1577	rBV	319609	639848	48.58%	5.622%
26	6.280	1612	1614	1617	rBV3	1864	1154	0.09%	0.010%
27	6.351	1634	1636	1639	rBV4	1324	698	0.05%	0.006%
28	6.540	1693	1695	1698	rVB4	1639	586	0.04%	0.005%
29	6.762	1761	1764	1766	rBV3	1998	1191	0.09%	0.010%
30	6.884	1797	1802	1803	rBV4	1346	1070	0.08%	0.009%
31	6.939	1817	1819	1822	rBV4	1091	894	0.07%	0.008%
32	7.006	1829	1840	1858	rBV2	183063	329091	24.99%	2.891%
33	7.338	1931	1943	1956	rBV	636188	1095797	83.20%	9.627%
34	7.412	1958	1966	1980	rVB	134570	229829	17.45%	2.019%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016706.D
 Acq On : 09 Jun 2020 10:54
 Operator : SY/MD
 Sample : L2861-10DL 200X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E42DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	7.640	2029	2037	2055	rVB	129875	215019	16.33%	1.889%
36	7.897	2115	2117	2118	rBV2	1237	551	0.04%	0.005%
37	7.920	2121	2124	2128	rVB6	1670	1264	0.10%	0.011%
38	8.106	2172	2182	2210	rBV	380424	700695	53.20%	6.156%
39	8.354	2257	2259	2263	rBV5	1478	693	0.05%	0.006%
40	8.547	2317	2319	2323	rVV5	1207	505	0.04%	0.004%
41	8.788	2391	2394	2398	rBV5	2052	1522	0.12%	0.013%
42	8.875	2409	2421	2434	rBV	647005	1053338	79.98%	9.254%
43	9.032	2461	2470	2484	rBV	173945	273956	20.80%	2.407%
44	9.283	2540	2548	2553	rBV10	5178	8360	0.63%	0.073%
45	9.386	2578	2580	2581	rBV2	1930	893	0.07%	0.008%
46	9.566	2629	2636	2650	rVB2	57899	90101	6.84%	0.792%
47	10.167	2820	2823	2827	rBV5	1671	1718	0.13%	0.015%
48	10.238	2833	2845	2864	rVB	429413	673124	51.11%	5.914%
49	10.682	2981	2983	2987	rBV4	1587	1063	0.08%	0.009%
50	10.759	3000	3007	3016	rBV3	10207	17598	1.34%	0.155%
51	10.939	3055	3063	3071	rBV3	10963	17700	1.34%	0.156%
52	11.074	3103	3105	3110	rBV5	1494	896	0.07%	0.008%
53	11.270	3155	3166	3182	rBV	697271	1058429	80.36%	9.299%
54	11.550	3246	3253	3261	rBV9	7388	12656	0.96%	0.111%
55	11.646	3272	3283	3298	rBV	711278	1106209	83.99%	9.719%
56	11.936	3366	3373	3375	rBV8	2036	2301	0.17%	0.020%
57	12.006	3391	3395	3398	rBV4	2157	1639	0.12%	0.014%
58	12.045	3401	3407	3410	rBV7	2130	2683	0.20%	0.024%
59	12.186	3448	3451	3453	rBV4	1044	719	0.05%	0.006%
60	12.318	3489	3492	3494	rBV3	1697	951	0.07%	0.008%
61	12.366	3504	3507	3511	rBV5	1269	1343	0.10%	0.012%
62	12.489	3541	3545	3547	rBV4	1781	1245	0.09%	0.011%
63	12.601	3579	3580	3584	rBV3	858	671	0.05%	0.006%
64	12.643	3591	3593	3597	rBV3	1339	953	0.07%	0.008%
65	12.662	3597	3599	3602	rBV4	1308	944	0.07%	0.008%
66	12.720	3613	3617	3620	rBV6	1114	1104	0.08%	0.010%
67	12.807	3641	3644	3645	rBV3	1153	603	0.05%	0.005%
68	12.826	3645	3650	3655	rVV9	1327	1542	0.12%	0.014%
69	12.907	3669	3675	3678	rBV7	2868	3370	0.26%	0.030%
70	12.974	3692	3696	3697	rBV4	1059	825	0.06%	0.007%
71	13.032	3711	3714	3716	rBV4	1253	1001	0.08%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016706.D
 Acq On : 09 Jun 2020 10:54
 Operator : SY/MD
 Sample : L2861-10DL 200X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E42DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	13.054	3719	3721	3723	rBV3	1072	512	0.04%	0.004%
73	13.112	3736	3739	3742	rBV5	1545	947	0.07%	0.008%
74	13.167	3754	3756	3758	rBV4	1090	730	0.06%	0.006%
75	13.289	3792	3794	3797	rBV2	1067	784	0.06%	0.007%
76	13.344	3809	3811	3813	rBV3	1463	974	0.07%	0.009%
77	13.415	3832	3833	3835	rBV2	1283	539	0.04%	0.005%
78	13.530	3863	3869	3876	rBV2	7902	11610	0.88%	0.102%
79	13.598	3887	3890	3894	rBV6	2202	2038	0.15%	0.018%
80	13.653	3899	3907	3909	rBV9	2619	3583	0.27%	0.031%
81	13.714	3923	3926	3930	rVB5	1204	788	0.06%	0.007%
82	13.736	3930	3933	3935	rBV4	1144	728	0.06%	0.006%
83	13.820	3957	3959	3961	rBV3	889	571	0.04%	0.005%
84	13.948	3997	3999	4002	rBV4	1443	1009	0.08%	0.009%
85	14.000	4011	4015	4018	rBV4	1546	1317	0.10%	0.012%
86	14.231	4084	4087	4088	rBV2	1293	658	0.05%	0.006%
87	14.286	4102	4104	4107	rBV3	1449	1095	0.08%	0.010%
88	14.366	4127	4129	4134	rVB5	1299	990	0.08%	0.009%
89	14.392	4135	4137	4141	rVB5	1073	486	0.04%	0.004%
90	14.527	4175	4179	4180	rBV3	1486	973	0.07%	0.009%
91	14.579	4193	4195	4198	rVB4	1745	721	0.05%	0.006%
92	14.598	4198	4201	4203	rBV3	1825	1267	0.10%	0.011%
93	14.649	4215	4217	4220	rBV4	1193	811	0.06%	0.007%
94	14.743	4244	4246	4247	rBV2	1170	468	0.04%	0.004%
95	14.816	4267	4269	4272	rBV3	1786	969	0.07%	0.009%
96	14.858	4278	4282	4287	rVB8	2145	1798	0.14%	0.016%
97	14.929	4302	4304	4306	rBV3	2030	868	0.07%	0.008%
98	15.029	4332	4335	4339	rVB6	1909	1431	0.11%	0.013%
99	15.051	4339	4342	4346	rBV5	2069	1955	0.15%	0.017%
100	15.440	4459	4463	4464	rBV4	2070	1395	0.11%	0.012%


Sum of corrected areas: 11382021

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060920\
Data File : VV016706.D
Acq On : 09 Jun 2020 10:54
Operator : SY/MD
Sample : L2861-10DL 200X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E42DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

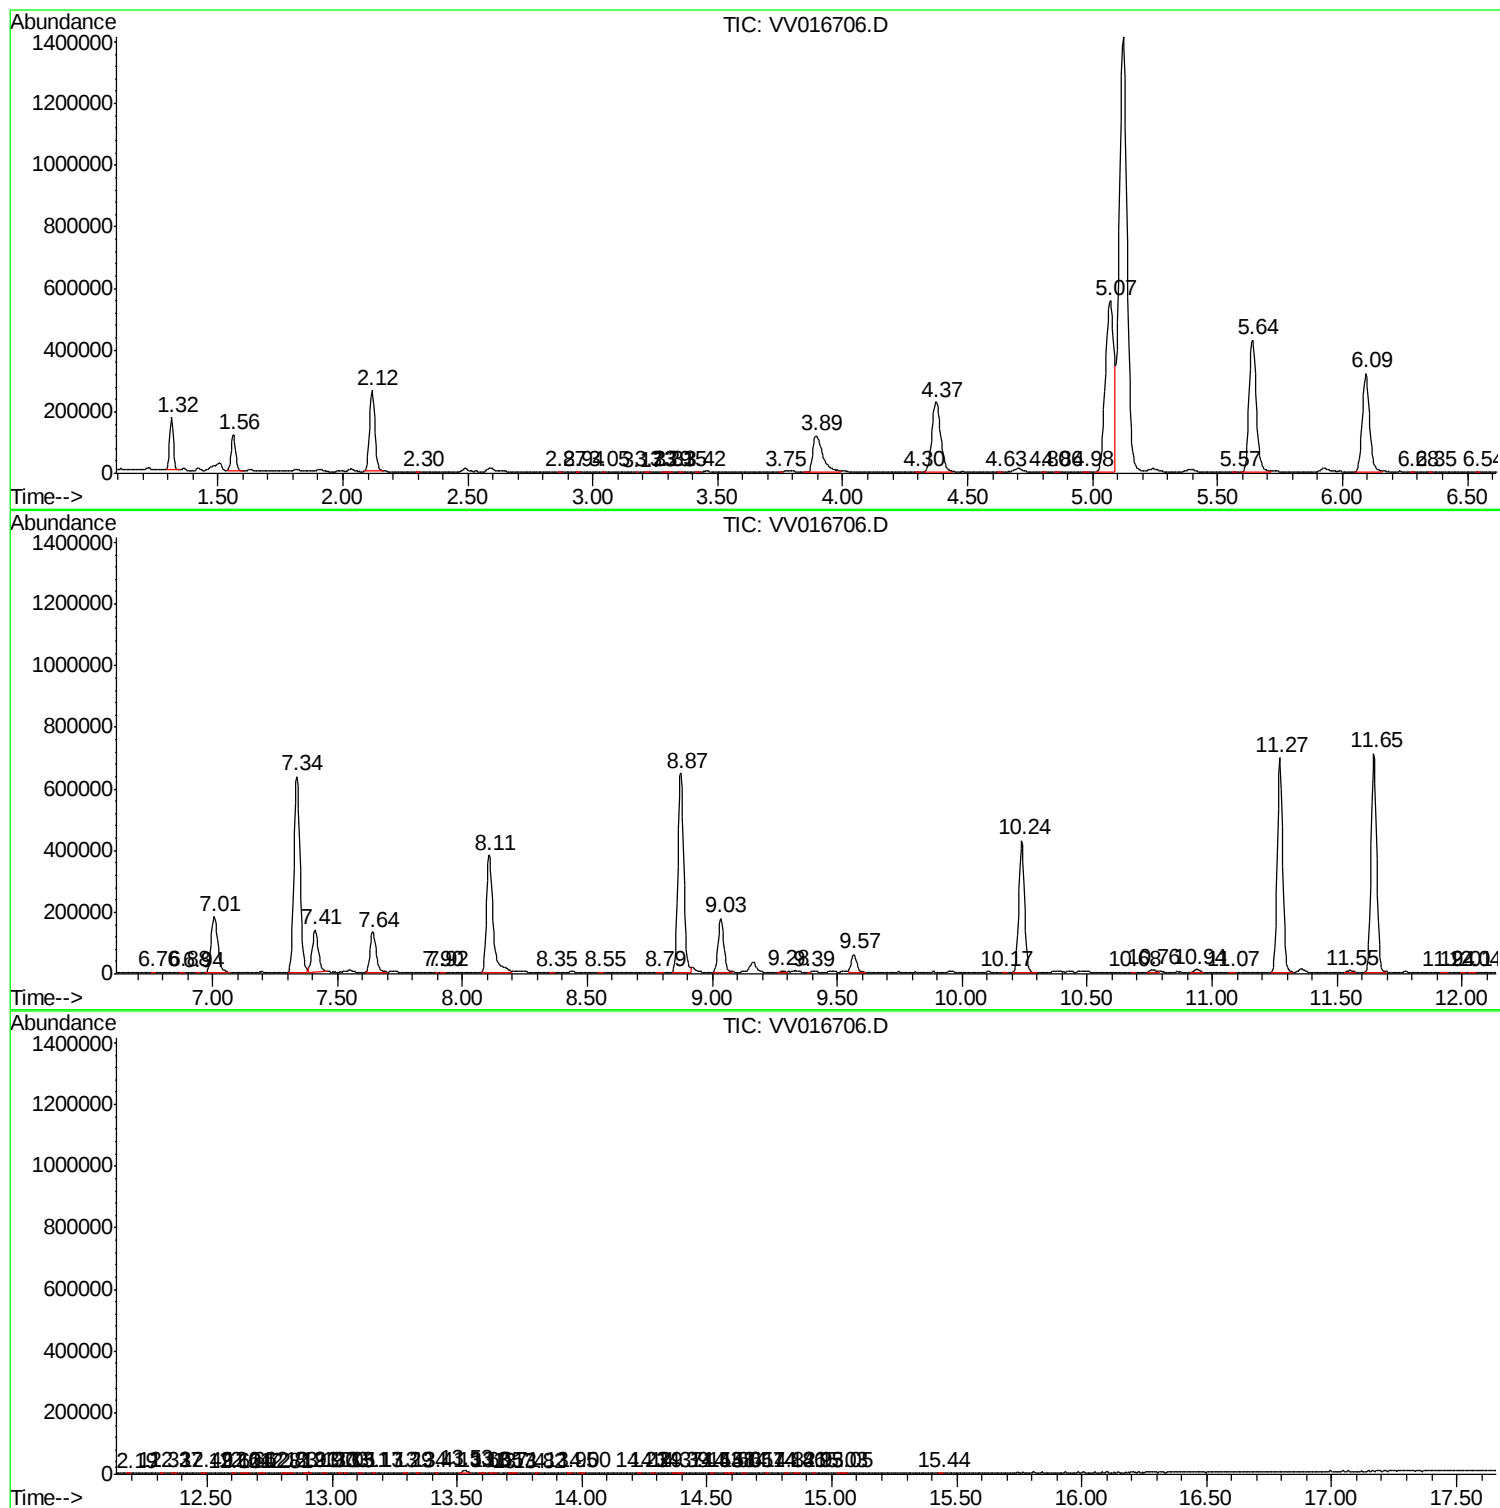

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016706.D
Acq On : 09 Jun 2020 10:54
Operator : SY/MD
Sample : L2861-10DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E42DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016706.D
Acq On : 09 Jun 2020 10:54
Operator : SY/MD
Sample : L2861-10DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E42DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc