

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016707.D
 Acq On : 09 Jun 2020 11:18
 Operator : SY/MD
 Sample : L2875-15
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	84	rVB	177669	181413	12.46%	1.659%
2	1.556	139	145	159	rVB	123988	145376	9.98%	1.329%
3	2.116	310	319	337	rVB	276643	408885	28.07%	3.738%
4	2.396	404	406	410	rBV3	1526	987	0.07%	0.009%
5	2.447	420	422	426	rVB4	1892	1134	0.08%	0.010%
6	2.482	431	433	438	rVV4	1177	871	0.06%	0.008%
7	2.740	510	513	519	rVB7	1659	1353	0.09%	0.012%
8	2.765	519	521	524	rBV4	1314	934	0.06%	0.009%
9	2.817	532	537	540	rBV7	1644	1850	0.13%	0.017%
10	2.920	566	569	574	rBV6	2051	1753	0.12%	0.016%
11	2.958	577	581	586	rBV8	1506	1910	0.13%	0.017%
12	3.190	650	653	658	rVV7	1312	1453	0.10%	0.013%
13	3.331	693	697	698	rBV4	1457	979	0.07%	0.009%
14	3.392	714	716	720	rVB3	2134	1217	0.08%	0.011%
15	3.428	725	727	730	rVB2	1726	1041	0.07%	0.010%
16	3.453	730	735	736	rBV5	1488	1309	0.09%	0.012%
17	3.505	747	751	754	rVB4	1925	1272	0.09%	0.012%
18	3.598	777	780	784	rVB6	1629	1092	0.07%	0.010%
19	3.659	796	799	803	rVB4	2033	1535	0.11%	0.014%
20	3.752	825	828	831	rBV4	1453	1230	0.08%	0.011%
21	3.820	846	849	854	rVB7	1531	887	0.06%	0.008%
22	3.894	862	872	904	rBV	119360	325183	22.33%	2.973%
23	4.119	939	942	944	rBV4	1704	804	0.06%	0.007%
24	4.215	968	972	976	rBV6	1590	1526	0.10%	0.014%
25	4.280	990	992	995	rVB3	1713	794	0.05%	0.007%
26	4.302	996	999	1001	rBV5	1439	904	0.06%	0.008%
27	4.373	1006	1021	1047	rVB	234505	579193	39.77%	5.295%
28	4.640	1102	1104	1107	rBV4	1387	848	0.06%	0.008%
29	4.707	1123	1125	1131	rVV6	1754	1113	0.08%	0.010%
30	4.781	1142	1148	1149	rBV4	1266	1275	0.09%	0.012%
31	4.846	1166	1168	1172	rVB4	1965	1066	0.07%	0.010%
32	4.958	1198	1203	1204	rBV5	1631	1410	0.10%	0.013%
33	4.997	1213	1215	1220	rVB5	1669	945	0.06%	0.009%
34	5.068	1220	1237	1265	rBV2	566194	1456418	100.00%	13.316%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016707.D
 Acq On : 09 Jun 2020 11:18
 Operator : SY/MD
 Sample : L2875-15
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	5.357	1324	1327	1332	rBV7	1804	1544	0.11%	0.014%
36	5.476	1362	1364	1368	rBV4	1465	1342	0.09%	0.012%
37	5.576	1393	1395	1399	rVB4	2220	1134	0.08%	0.010%
38	5.640	1401	1415	1440	rBV	417522	843177	57.89%	7.709%
39	5.788	1459	1461	1466	rBV4	2187	1921	0.13%	0.018%
40	6.093	1543	1556	1574	rBV	325217	653741	44.89%	5.977%
41	6.341	1631	1633	1636	rBV3	1295	883	0.06%	0.008%
42	6.457	1667	1669	1671	rBV2	1745	894	0.06%	0.008%
43	6.633	1720	1724	1727	rBV5	2022	1992	0.14%	0.018%
44	6.875	1796	1799	1805	rBV6	1595	1476	0.10%	0.013%
45	6.900	1805	1807	1814	rVB7	1188	1053	0.07%	0.010%
46	7.006	1828	1840	1860	rBV	188450	332509	22.83%	3.040%
47	7.338	1931	1943	1960	rBV	656206	1120663	76.95%	10.246%
48	7.640	2028	2037	2055	rBV	132608	218644	15.01%	1.999%
49	7.855	2101	2104	2107	rBV4	1134	943	0.06%	0.009%
50	7.874	2109	2110	2112	rBV2	1530	856	0.06%	0.008%
51	8.106	2171	2182	2210	rBV	387409	743472	51.05%	6.797%
52	8.752	2379	2383	2387	rVB6	1436	1195	0.08%	0.011%
53	8.874	2409	2421	2438	rBV	625588	1015554	69.73%	9.285%
54	9.157	2505	2509	2512	rBV6	1340	1125	0.08%	0.010%
55	9.276	2545	2546	2551	rBV4	1391	1144	0.08%	0.010%
56	9.331	2560	2563	2566	rBV4	1797	1097	0.08%	0.010%
57	9.363	2570	2573	2576	rBV4	1742	1093	0.08%	0.010%
58	9.479	2606	2609	2611	rBV5	1763	1223	0.08%	0.011%
59	9.546	2625	2630	2632	rBV5	1405	1019	0.07%	0.009%
60	9.765	2693	2698	2699	rBV4	1182	1045	0.07%	0.010%
61	9.935	2748	2751	2753	rBV4	1244	812	0.06%	0.007%
62	10.083	2794	2797	2799	rBV4	1375	813	0.06%	0.007%
63	10.238	2829	2845	2859	rBV	440053	687180	47.18%	6.283%
64	10.524	2931	2934	2941	rVB8	1645	1256	0.09%	0.011%
65	10.559	2941	2945	2946	rBV4	1723	1303	0.09%	0.012%
66	10.746	3002	3003	3006	rBV3	1108	775	0.05%	0.007%
67	10.939	3060	3063	3066	rBV5	2092	1447	0.10%	0.013%
68	11.273	3154	3167	3182	rBV	637119	993180	68.19%	9.080%
69	11.646	3271	3283	3302	rBV	721135	1130907	77.65%	10.340%
70	11.955	3377	3379	3382	rBV3	1480	858	0.06%	0.008%
71	12.054	3406	3410	3417	rVB9	1446	1472	0.10%	0.013%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016707.D
 Acq On : 09 Jun 2020 11:18
 Operator : SY/MD
 Sample : L2875-15
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.135	3432	3435	3440	rVB5	1018	928	0.06%	0.008%
73	12.164	3440	3444	3451	rBV8	2154	2179	0.15%	0.020%
74	12.206	3451	3457	3460	rBV6	2120	2177	0.15%	0.020%
75	12.289	3481	3483	3487	rVB3	1645	897	0.06%	0.008%
76	12.318	3487	3492	3499	rBV9	1643	2119	0.15%	0.019%
77	12.521	3551	3555	3559	rVB6	1109	902	0.06%	0.008%
78	12.659	3592	3598	3602	rBV8	2102	2259	0.16%	0.021%
79	12.939	3682	3685	3689	rVB4	1611	1129	0.08%	0.010%
80	12.977	3696	3697	3701	rVB4	1410	963	0.07%	0.009%
81	13.009	3704	3707	3712	rBV6	1587	1485	0.10%	0.014%
82	13.032	3712	3714	3718	rVB4	1482	791	0.05%	0.007%
83	13.054	3718	3721	3723	rBV4	1157	815	0.06%	0.007%
84	13.138	3744	3747	3750	rBV4	1150	807	0.06%	0.007%
85	13.289	3790	3794	3795	rBV3	1258	866	0.06%	0.008%
86	13.620	3894	3897	3899	rBV3	1774	1393	0.10%	0.013%
87	13.662	3908	3910	3914	rBV4	1226	1060	0.07%	0.010%
88	13.984	4006	4010	4015	rVB7	1915	1639	0.11%	0.015%
89	14.016	4015	4020	4022	rBV5	1352	1175	0.08%	0.011%
90	14.045	4025	4029	4030	rBV4	1239	891	0.06%	0.008%
91	14.135	4055	4057	4064	rVB8	1961	1699	0.12%	0.016%
92	14.247	4089	4092	4094	rBV3	1112	899	0.06%	0.008%
93	14.501	4168	4171	4173	rVB3	1499	864	0.06%	0.008%
94	14.537	4180	4182	4186	rBV3	1175	866	0.06%	0.008%
95	14.656	4216	4219	4223	rBV5	2106	1779	0.12%	0.016%
96	14.707	4231	4235	4238	rBV5	2378	1981	0.14%	0.018%
97	14.832	4272	4274	4276	rBV3	1714	934	0.06%	0.009%
98	15.241	4399	4401	4405	rVB4	1466	984	0.07%	0.009%
99	15.472	4471	4473	4476	rBV3	1819	1012	0.07%	0.009%
100	15.614	4514	4517	4521	rBV6	1683	1490	0.10%	0.014%


Sum of corrected areas: 10937685

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060920\
Data File : VV016707.D
Acq On : 09 Jun 2020 11:18
Operator : SY/MD
Sample : L2875-15
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

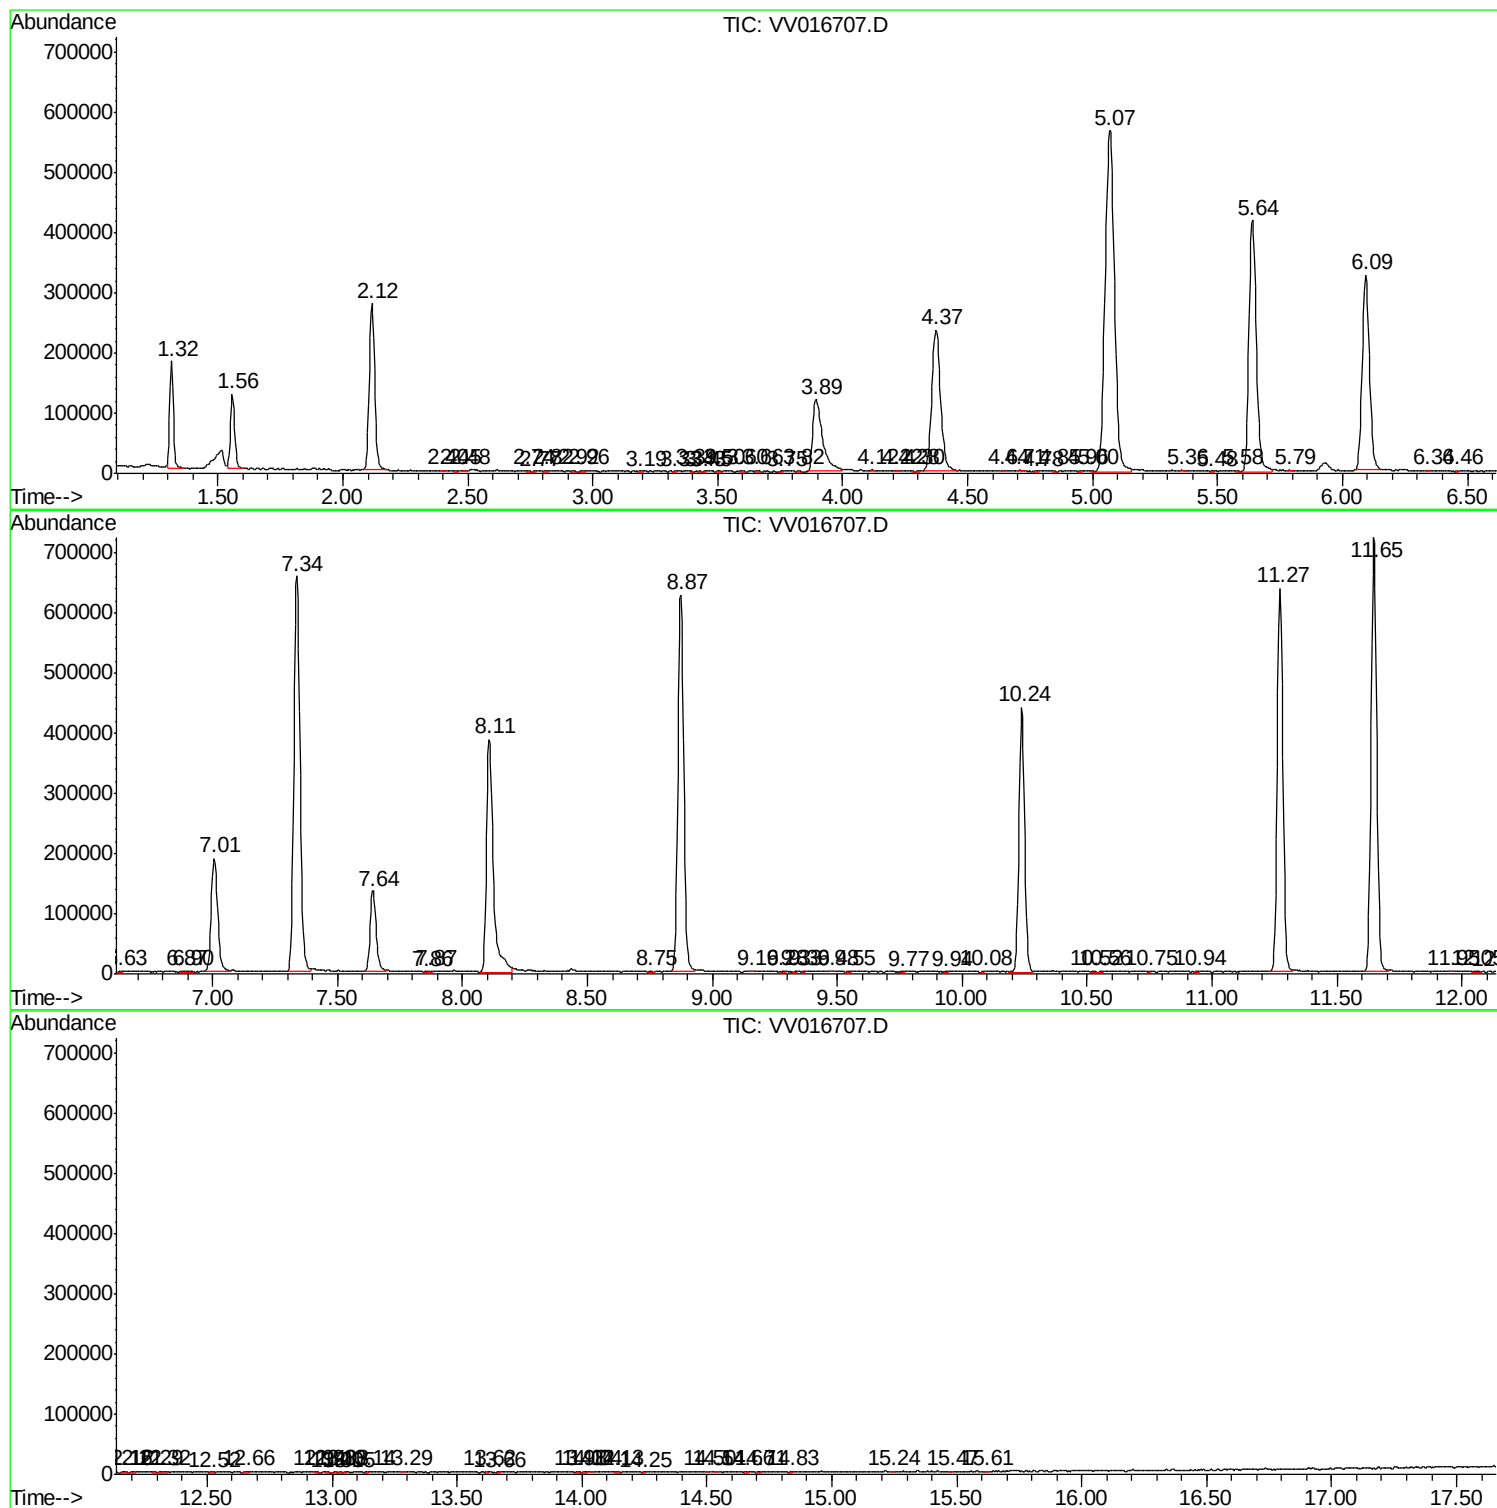

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016707.D
Acq On : 09 Jun 2020 11:18
Operator : SY/MD
Sample : L2875-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016707.D
Acq On : 09 Jun 2020 11:18
Operator : SY/MD
Sample : L2875-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc