

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016709.D
 Acq On : 09 Jun 2020 12:05
 Operator : SY/MD
 Sample : L2861-15DL2 250X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E48DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	79	rVB	165167	168050	12.11%	1.532%
2	1.560	139	146	156	rVB	105176	127904	9.22%	1.166%
3	2.116	310	319	332	rVB	246491	358972	25.88%	3.272%
4	2.357	390	394	396	rBV4	1360	1004	0.07%	0.009%
5	2.367	396	397	402	rVB4	1718	1005	0.07%	0.009%
6	2.412	407	411	413	rBV4	2019	1800	0.13%	0.016%
7	2.746	511	515	517	rVB4	1245	856	0.06%	0.008%
8	2.872	551	554	556	rBV3	1280	772	0.06%	0.007%
9	2.962	579	582	585	rBV3	1548	1380	0.10%	0.013%
10	3.013	596	598	600	rVB3	2047	793	0.06%	0.007%
11	3.109	626	628	631	rBV4	1378	697	0.05%	0.006%
12	3.158	638	643	645	rBV5	1118	1065	0.08%	0.010%
13	3.267	676	677	680	rVB3	2073	815	0.06%	0.007%
14	3.569	770	771	776	rVB3	1251	765	0.06%	0.007%
15	3.595	776	779	780	rVV3	1509	874	0.06%	0.008%
16	3.621	784	787	796	rVV8	1537	2055	0.15%	0.019%
17	3.656	796	798	802	rVV3	1343	963	0.07%	0.009%
18	3.682	802	806	809	rVV5	1595	1472	0.11%	0.013%
19	3.708	812	814	819	rVB4	1068	871	0.06%	0.008%
20	3.775	830	835	838	rBV4	2140	1770	0.13%	0.016%
21	3.830	847	852	857	rVB7	1023	1075	0.08%	0.010%
22	3.894	862	872	900	rVV	114268	301318	21.72%	2.746%
23	4.254	981	984	987	rVB4	1569	864	0.06%	0.008%
24	4.299	995	998	999	rBV3	866	497	0.04%	0.005%
25	4.373	1006	1021	1045	rBV	224479	547984	39.50%	4.994%
26	4.524	1065	1068	1069	rBV2	2304	1383	0.10%	0.013%
27	4.859	1168	1172	1174	rBV4	1616	1194	0.09%	0.011%
28	4.888	1179	1181	1184	rBV4	1018	666	0.05%	0.006%
29	4.939	1194	1197	1199	rVB4	1026	553	0.04%	0.005%
30	4.952	1199	1201	1205	rBV4	1100	726	0.05%	0.007%
31	5.071	1220	1238	1247	rBV2	534241	1387177	100.00%	12.643%
32	5.341	1317	1322	1327	rBV7	2401	3468	0.25%	0.032%
33	5.585	1395	1398	1401	rBV5	2052	1123	0.08%	0.010%
34	5.640	1401	1415	1434	rBV	465411	928739	66.95%	8.465%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016709.D
 Acq On : 09 Jun 2020 12:05
 Operator : SY/MD
 Sample : L2861-15DL2 250X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E48DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.093	1541	1556	1575	rBV	314875	636505	45.88%	5.801%
36	6.389	1646	1648	1651	rBV4	1221	840	0.06%	0.008%
37	6.482	1675	1677	1679	rBV3	1368	503	0.04%	0.005%
38	6.723	1748	1752	1754	rBV5	1989	1830	0.13%	0.017%
39	6.759	1761	1763	1766	rBV3	1081	604	0.04%	0.006%
40	6.785	1769	1771	1775	rBV5	1473	708	0.05%	0.006%
41	6.859	1788	1794	1799	rBV8	1566	1454	0.10%	0.013%
42	6.887	1799	1803	1805	rBV4	1374	1052	0.08%	0.010%
43	6.916	1810	1812	1813	rBV2	1571	764	0.06%	0.007%
44	7.006	1829	1840	1862	rBV	182059	321989	23.21%	2.935%
45	7.338	1931	1943	1959	rBV	625870	1072230	77.30%	9.773%
46	7.540	2004	2006	2007	rBV2	1954	852	0.06%	0.008%
47	7.643	2027	2038	2056	rBV	129920	225928	16.29%	2.059%
48	8.106	2172	2182	2216	rBV	375470	712827	51.39%	6.497%
49	8.373	2263	2265	2270	rVB4	1737	1486	0.11%	0.014%
50	8.444	2279	2287	2291	rBV8	4591	6294	0.45%	0.057%
51	8.627	2339	2344	2345	rBV4	1392	868	0.06%	0.008%
52	8.637	2345	2347	2350	rVB3	1046	552	0.04%	0.005%
53	8.656	2350	2353	2355	rBV4	1920	1272	0.09%	0.012%
54	8.756	2380	2384	2388	rBV7	1729	1549	0.11%	0.014%
55	8.875	2409	2421	2445	rBV	694690	1145540	82.58%	10.441%
56	9.035	2464	2471	2485	rVB	30018	49754	3.59%	0.453%
57	9.235	2530	2533	2536	rBV4	1336	802	0.06%	0.007%
58	9.399	2579	2584	2585	rBV5	2713	1940	0.14%	0.018%
59	9.476	2596	2608	2615	rBV5	4272	9523	0.69%	0.087%
60	10.238	2830	2845	2863	rBV	435260	678097	48.88%	6.180%
61	10.341	2874	2877	2880	rBV5	1658	1045	0.08%	0.010%
62	10.653	2971	2974	2975	rBV3	844	534	0.04%	0.005%
63	10.688	2981	2985	2986	rBV3	1555	1030	0.07%	0.009%
64	10.942	3053	3064	3072	rBV3	4108	8628	0.62%	0.079%
65	11.013	3084	3086	3089	rVB4	1604	949	0.07%	0.009%
66	11.035	3089	3093	3095	rBV4	1046	847	0.06%	0.008%
67	11.071	3102	3104	3110	rBV6	1506	1053	0.08%	0.010%
68	11.100	3110	3113	3114	rBV3	1404	696	0.05%	0.006%
69	11.190	3137	3141	3144	rBV4	1365	1388	0.10%	0.013%
70	11.222	3148	3151	3152	rBV3	1210	795	0.06%	0.007%
71	11.270	3155	3166	3180	rBV	722561	1105875	79.72%	10.079%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016709.D
 Acq On : 09 Jun 2020 12:05
 Operator : SY/MD
 Sample : L2861-15DL2 250X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E48DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.460	3222	3225	3231	rBV8	2191	1689	0.12%	0.015%
73	11.646	3272	3283	3298	rBV	689137	1091571	78.69%	9.949%
74	11.874	3352	3354	3356	rBV4	1196	617	0.04%	0.006%
75	11.929	3369	3371	3374	rBV4	1193	573	0.04%	0.005%
76	11.952	3374	3378	3379	rBV4	1320	808	0.06%	0.007%
77	12.135	3431	3435	3441	rVB9	2186	2403	0.17%	0.022%
78	12.199	3453	3455	3458	rBV4	1305	696	0.05%	0.006%
79	12.302	3484	3487	3490	rBV4	1900	1567	0.11%	0.014%
80	12.353	3500	3503	3504	rBV2	1324	584	0.04%	0.005%
81	12.646	3591	3594	3598	rVB5	1529	1182	0.09%	0.011%
82	12.675	3598	3603	3607	rBV7	1749	2259	0.16%	0.021%
83	12.990	3699	3701	3703	rBV3	1018	511	0.04%	0.005%
84	13.061	3721	3723	3725	rBV3	814	495	0.04%	0.005%
85	13.112	3737	3739	3741	rBV3	1124	691	0.05%	0.006%
86	13.196	3763	3765	3767	rBV3	1173	597	0.04%	0.005%
87	13.222	3772	3773	3775	rBV2	1434	558	0.04%	0.005%
88	13.325	3803	3805	3807	rBV2	1123	622	0.04%	0.006%
89	13.424	3833	3836	3837	rBV3	956	543	0.04%	0.005%
90	13.434	3837	3839	3841	rVV3	1222	633	0.05%	0.006%
91	13.582	3882	3885	3892	rVB9	1785	1706	0.12%	0.016%
92	13.717	3924	3927	3930	rBV5	1787	923	0.07%	0.008%
93	14.225	4081	4085	4088	rBV5	1758	1601	0.12%	0.015%
94	14.456	4154	4157	4160	rBV4	1620	1517	0.11%	0.014%
95	14.517	4173	4176	4181	rBV6	1206	1066	0.08%	0.010%
96	14.540	4181	4183	4185	rBV2	1479	553	0.04%	0.005%
97	14.726	4239	4241	4246	rBV5	1654	1135	0.08%	0.010%
98	15.096	4350	4356	4358	rBV7	1492	1508	0.11%	0.014%
99	15.144	4367	4371	4375	rBV7	1928	2197	0.16%	0.020%
100	15.485	4472	4477	4479	rBV5	2230	1706	0.12%	0.016%


Sum of corrected areas: 10971764

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060920\
Data File : VV016709.D
Acq On : 09 Jun 2020 12:05
Operator : SY/MD
Sample : L2861-15DL2 250X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E48DL2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

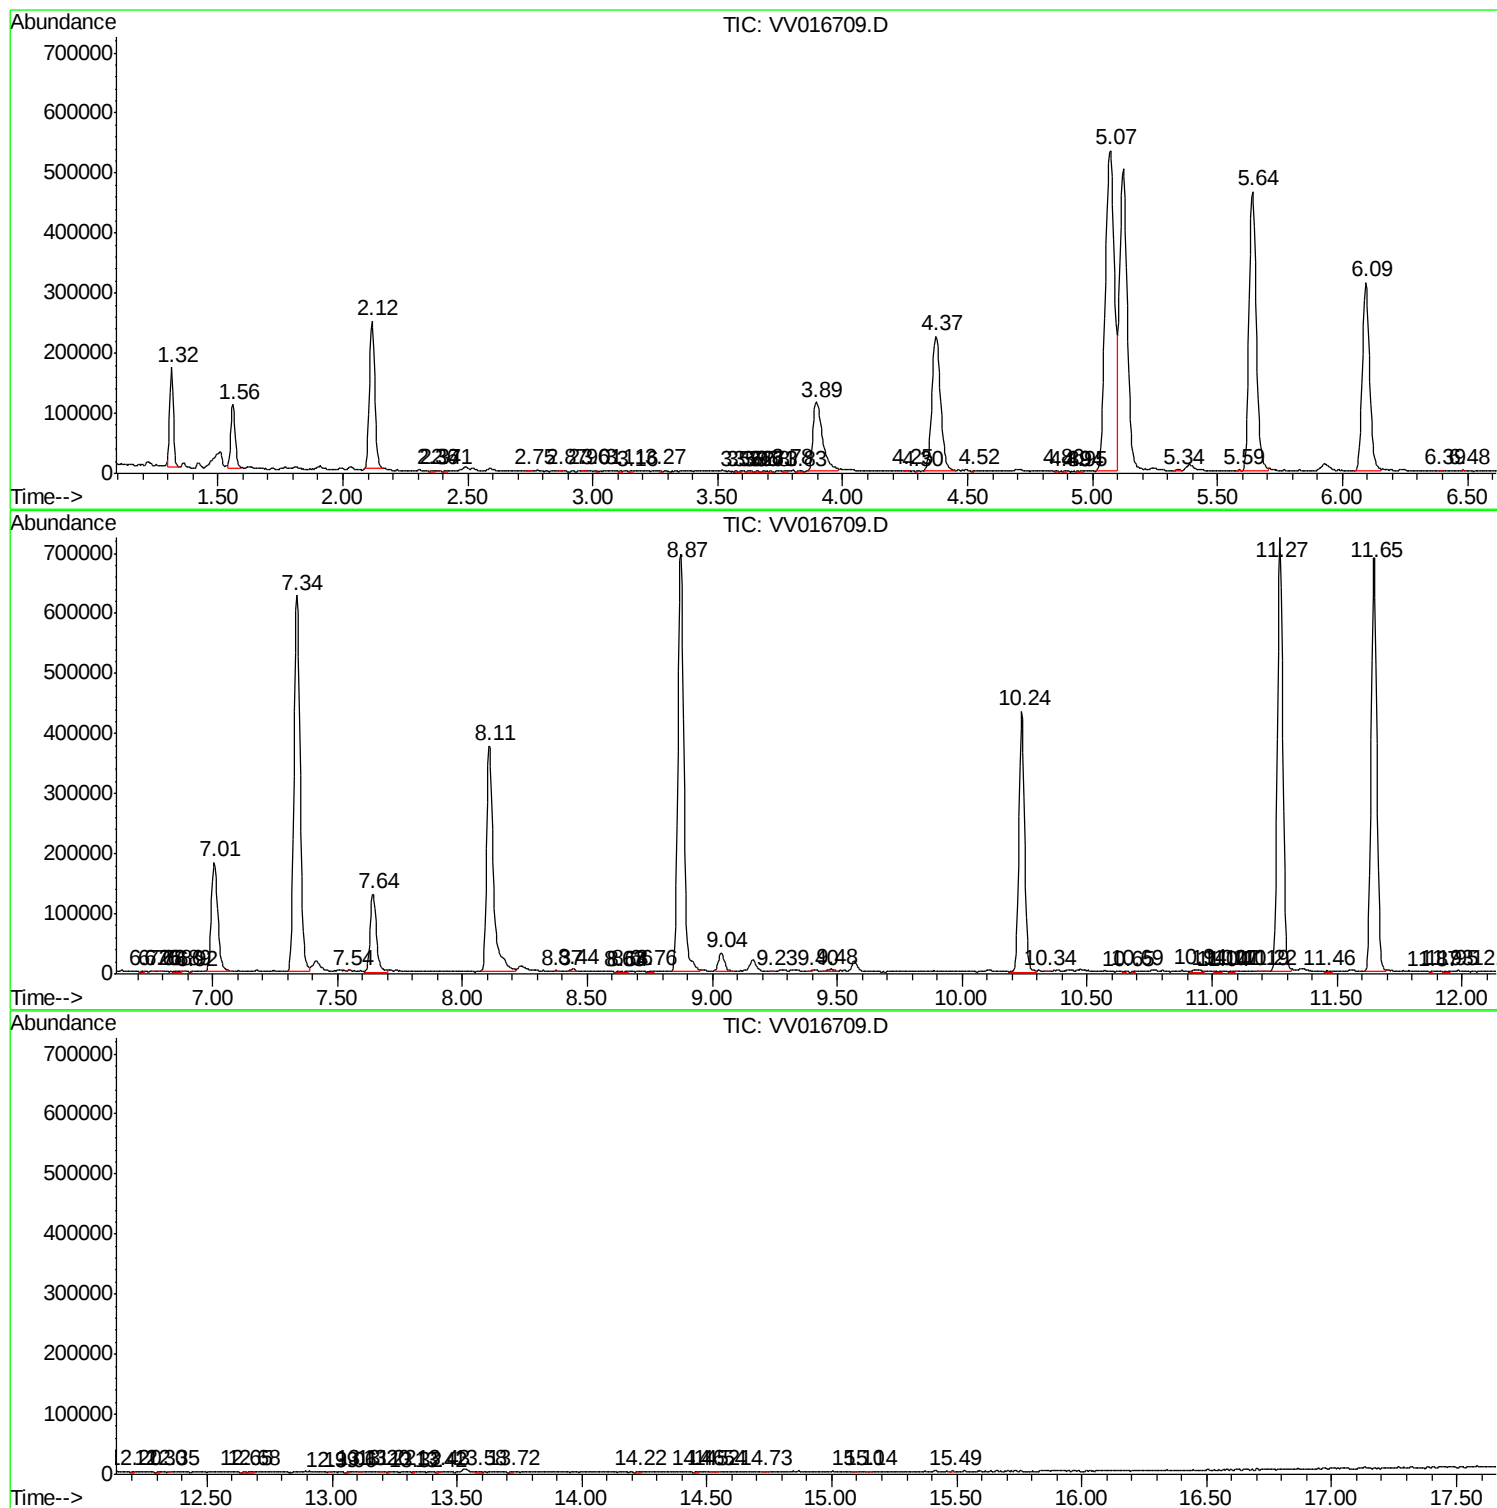

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016709.D
Acq On : 09 Jun 2020 12:05
Operator : SY/MD
Sample : L2861-15DL2 250X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E48DL2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016709.D
Acq On : 09 Jun 2020 12:05
Operator : SY/MD
Sample : L2861-15DL2 250X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E48DL2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc