

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016710.D
 Acq On : 09 Jun 2020 12:29
 Operator : SY/MD
 Sample : L2861-19DL2 500X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E67DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	83	rVB	151704	152736	11.07%	1.393%
2	1.566	141	148	160	rVB	107452	131046	9.50%	1.195%
3	2.116	310	319	335	rBV	244452	367284	26.62%	3.349%
4	2.360	392	395	397	rBV4	1883	1251	0.09%	0.011%
5	2.399	405	407	411	rBV4	2489	1828	0.13%	0.017%
6	2.476	428	431	433	rBV3	1980	1525	0.11%	0.014%
7	2.672	489	492	495	rBV5	1029	709	0.05%	0.006%
8	2.688	495	497	502	rVV5	1153	848	0.06%	0.008%
9	2.727	507	509	511	rBV3	1121	564	0.04%	0.005%
10	2.785	525	527	533	rBV6	1246	1180	0.09%	0.011%
11	3.019	598	600	601	rBV2	975	525	0.04%	0.005%
12	3.106	622	627	628	rBV4	1511	1246	0.09%	0.011%
13	3.135	633	636	638	rBV4	1119	820	0.06%	0.007%
14	3.145	638	639	642	rVB3	1484	493	0.04%	0.004%
15	3.171	642	647	653	rBV9	1483	1833	0.13%	0.017%
16	3.293	682	685	686	rBV3	936	509	0.04%	0.005%
17	3.357	701	705	707	rBV5	1201	879	0.06%	0.008%
18	3.392	714	716	720	rVB3	1600	661	0.05%	0.006%
19	3.441	728	731	735	rBV4	2031	2006	0.15%	0.018%
20	3.547	762	764	767	rBV4	1401	742	0.05%	0.007%
21	3.643	791	794	796	rBV4	982	627	0.05%	0.006%
22	3.675	801	804	806	rBV3	1098	672	0.05%	0.006%
23	3.701	810	812	815	rVB3	1306	785	0.06%	0.007%
24	3.724	815	819	820	rBV2	1025	725	0.05%	0.007%
25	3.733	820	822	825	rVB3	1293	621	0.05%	0.006%
26	3.753	825	828	830	rBV4	2099	1423	0.10%	0.013%
27	3.836	848	854	855	rBV5	869	760	0.06%	0.007%
28	3.894	861	872	901	rBV	116903	314400	22.79%	2.867%
29	4.245	980	981	985	rBV4	1010	606	0.04%	0.006%
30	4.373	1008	1021	1049	rVB	225041	544848	39.49%	4.968%
31	4.608	1091	1094	1096	rVV3	1274	702	0.05%	0.006%
32	4.640	1102	1104	1105	rBV2	2001	785	0.06%	0.007%
33	4.698	1120	1122	1126	rBV3	1553	1075	0.08%	0.010%
34	4.836	1163	1165	1166	rBV2	1433	666	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016710.D
 Acq On : 09 Jun 2020 12:29
 Operator : SY/MD
 Sample : L2861-19DL2 500X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E67DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	4.875	1171	1177	1178	rBV4	2012	1806	0.13%	0.016%
36	4.955	1200	1202	1205	rBV3	1205	639	0.05%	0.006%
37	4.994	1212	1214	1215	rBV2	1364	652	0.05%	0.006%
38	5.071	1220	1238	1247	rBV2	540002	1379548	100.00%	12.579%
39	5.569	1390	1393	1396	rBV4	1449	1008	0.07%	0.009%
40	5.640	1401	1415	1439	rBV	473685	942012	68.28%	8.590%
41	5.929	1494	1505	1516	rBV9	13466	29943	2.17%	0.273%
42	6.093	1543	1556	1579	rBV	309982	624810	45.29%	5.697%
43	6.347	1633	1635	1638	rBV4	1490	1212	0.09%	0.011%
44	6.701	1742	1745	1747	rBV3	1595	844	0.06%	0.008%
45	6.791	1771	1773	1776	rBV5	944	586	0.04%	0.005%
46	6.833	1783	1786	1787	rBV3	1182	570	0.04%	0.005%
47	6.926	1811	1815	1818	rBV5	1487	1237	0.09%	0.011%
48	7.006	1828	1840	1858	rBV	180651	320264	23.22%	2.920%
49	7.241	1909	1913	1914	rBV4	1831	1043	0.08%	0.010%
50	7.338	1930	1943	1957	rBV	629737	1080938	78.35%	9.857%
51	7.643	2027	2038	2051	rBV	127938	212100	15.37%	1.934%
52	7.887	2112	2114	2122	rVB9	1331	1067	0.08%	0.010%
53	7.939	2127	2130	2135	rBV6	1779	1282	0.09%	0.012%
54	8.035	2155	2160	2162	rBV5	1523	1630	0.12%	0.015%
55	8.106	2172	2182	2211	rBV	386263	708749	51.38%	6.463%
56	8.592	2331	2333	2335	rBV4	1503	699	0.05%	0.006%
57	8.707	2364	2369	2370	rBV4	1259	1056	0.08%	0.010%
58	8.875	2409	2421	2448	rVB	712701	1156105	83.80%	10.542%
59	9.527	2621	2624	2627	rBV5	2148	1470	0.11%	0.013%
60	9.884	2729	2735	2738	rBV8	2810	3623	0.26%	0.033%
61	9.929	2747	2749	2751	rBV3	1014	649	0.05%	0.006%
62	10.006	2771	2773	2775	rBV3	1063	510	0.04%	0.005%
63	10.238	2834	2845	2859	rBV	436689	671726	48.69%	6.125%
64	10.518	2931	2932	2933	rBV	1710	650	0.05%	0.006%
65	10.759	3004	3007	3008	rBV3	1660	863	0.06%	0.008%
66	10.929	3056	3060	3063	rBV6	4072	4013	0.29%	0.037%
67	11.090	3108	3110	3111	rBV2	1317	574	0.04%	0.005%
68	11.270	3154	3166	3188	rVV	753116	1146574	83.11%	10.455%
69	11.646	3271	3283	3299	rBV	693784	1099350	79.69%	10.024%
70	11.884	3354	3357	3362	rVB7	1424	1187	0.09%	0.011%
71	11.919	3366	3368	3369	rBV2	1439	725	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016710.D
 Acq On : 09 Jun 2020 12:29
 Operator : SY/MD
 Sample : L2861-19DL2 500X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E67DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.048	3406	3408	3410	rBV3	1319	554	0.04%	0.005%
73	12.064	3410	3413	3414	rBV2	1749	966	0.07%	0.009%
74	12.106	3421	3426	3427	rBV5	1832	1320	0.10%	0.012%
75	12.273	3475	3478	3486	rBV8	998	1318	0.10%	0.012%
76	12.495	3543	3547	3550	rBV4	1472	1103	0.08%	0.010%
77	12.598	3576	3579	3583	rBV8	1491	1092	0.08%	0.010%
78	12.620	3584	3586	3589	rVB4	1616	807	0.06%	0.007%
79	12.640	3589	3592	3595	rBV4	1453	1140	0.08%	0.010%
80	12.675	3599	3603	3605	rBV4	1350	878	0.06%	0.008%
81	12.919	3677	3679	3681	rBV2	1409	687	0.05%	0.006%
82	12.968	3692	3694	3698	rBV5	1565	984	0.07%	0.009%
83	13.167	3754	3756	3759	rVB3	1372	776	0.06%	0.007%
84	13.218	3768	3772	3775	rBV5	1107	1080	0.08%	0.010%
85	13.447	3841	3843	3845	rBV3	1556	752	0.05%	0.007%
86	13.562	3876	3879	3880	rBV3	1022	664	0.05%	0.006%
87	13.681	3915	3916	3920	rVB2	1125	681	0.05%	0.006%
88	13.726	3926	3930	3932	rBV4	1050	881	0.06%	0.008%
89	13.746	3932	3936	3937	rBV3	761	500	0.04%	0.005%
90	13.781	3944	3947	3949	rBV3	1642	962	0.07%	0.009%
91	13.916	3987	3989	3992	rBV3	1315	1112	0.08%	0.010%
92	14.032	4023	4025	4027	rBV3	1455	788	0.06%	0.007%
93	14.161	4063	4065	4067	rBV2	1107	657	0.05%	0.006%
94	14.186	4070	4073	4076	rBV4	1951	1089	0.08%	0.010%
95	14.472	4160	4162	4164	rBV2	1942	1129	0.08%	0.010%
96	14.514	4170	4175	4177	rBV5	1690	1430	0.10%	0.013%
97	14.588	4193	4198	4201	rBV6	1603	1669	0.12%	0.015%
98	14.620	4206	4208	4211	rVV4	1193	612	0.04%	0.006%
99	14.717	4232	4238	4240	rBV6	1131	1302	0.09%	0.012%
100	15.167	4377	4378	4380	rBV2	1590	715	0.05%	0.007%


Sum of corrected areas: 10966742

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060920\
Data File : VV016710.D
Acq On : 09 Jun 2020 12:29
Operator : SY/MD
Sample : L2861-19DL2 500X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E67DL2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

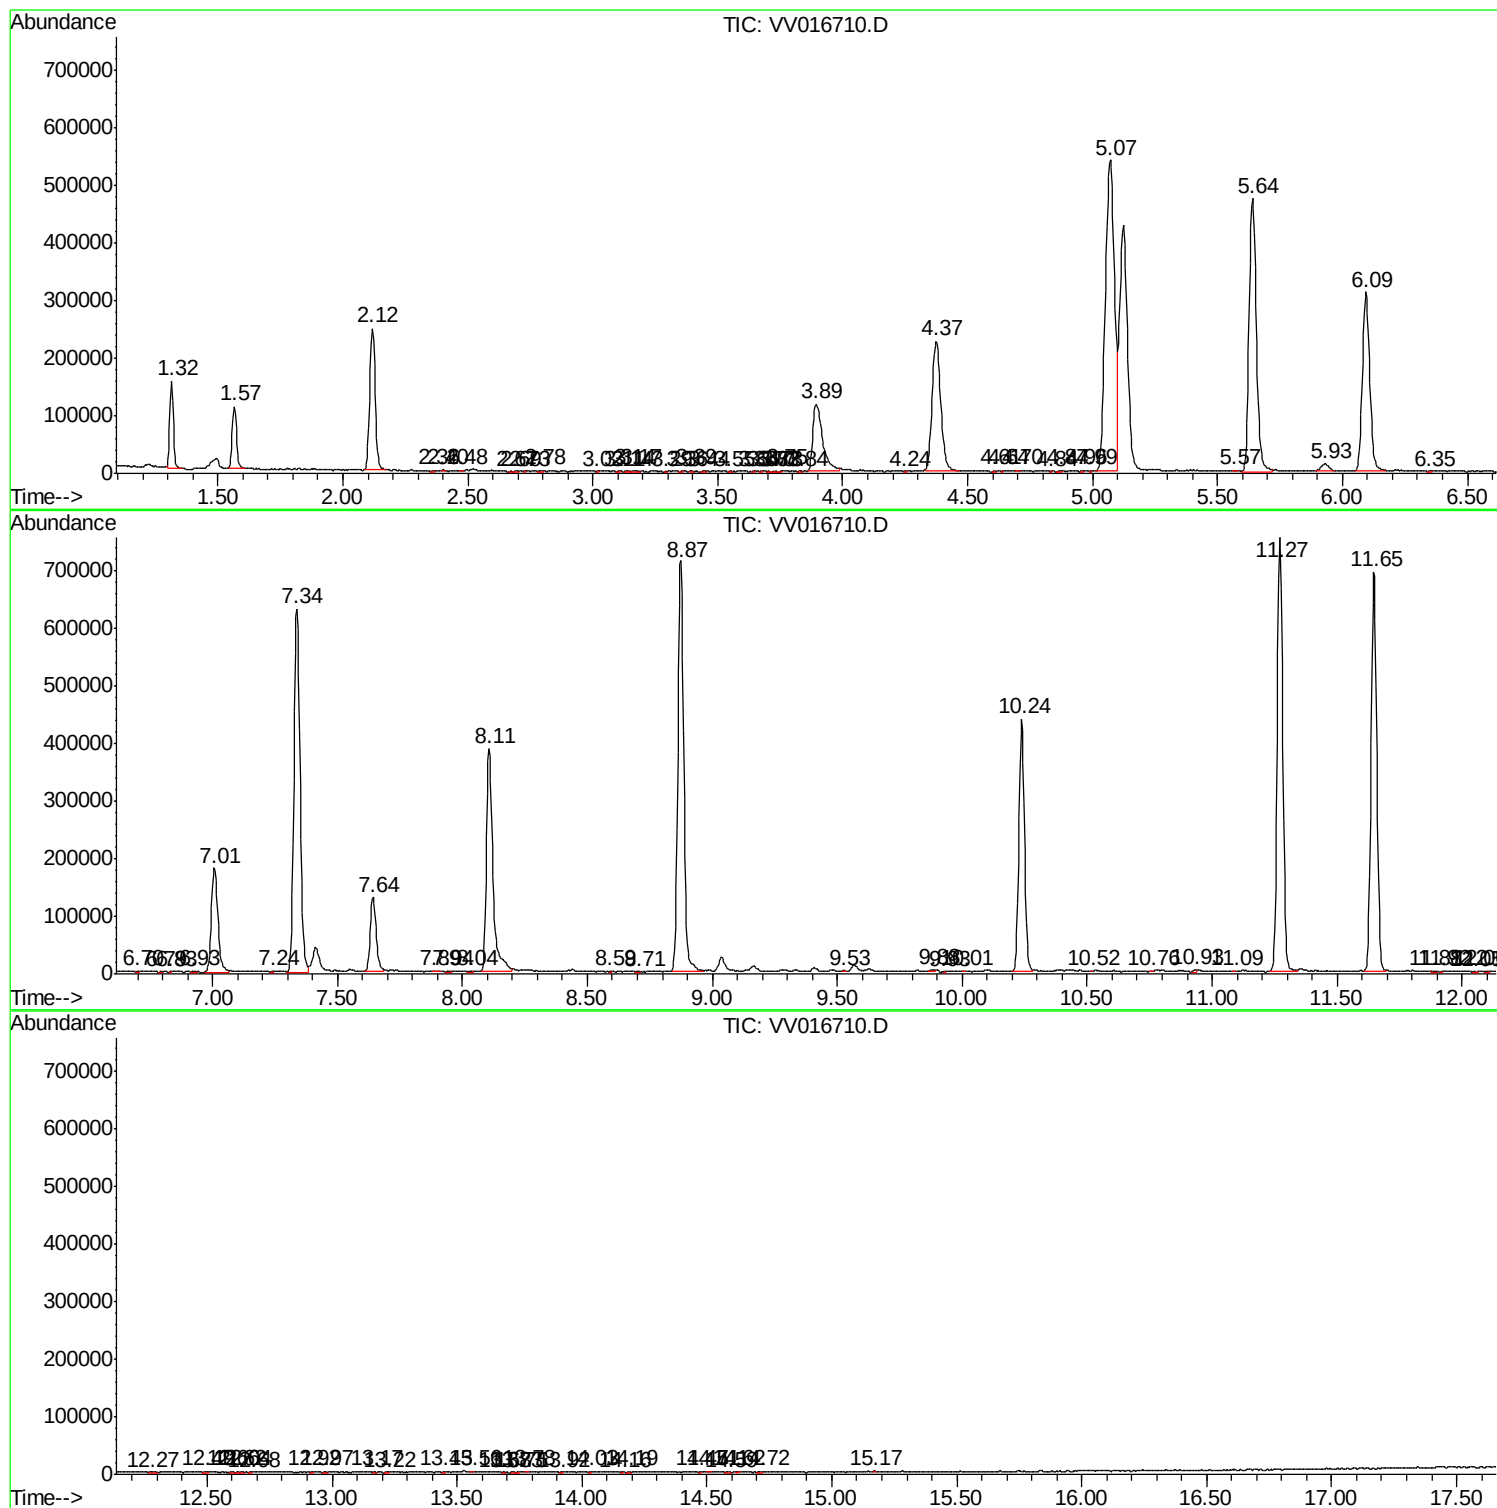

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016710.D
Acq On : 09 Jun 2020 12:29
Operator : SY/MD
Sample : L2861-19DL2 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E67DL2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016710.D
Acq On : 09 Jun 2020 12:29
Operator : SY/MD
Sample : L2861-19DL2 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E67DL2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc