

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016712.D
 Acq On : 09 Jun 2020 13:17
 Operator : SY/MD
 Sample : L2901-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTY7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.222	37	41	51	rVB	27738	26686	2.03%	0.255%
2	1.312	64	69	81	rVB	150439	153161	11.63%	1.466%
3	1.557	139	145	158	rVB	105826	126433	9.60%	1.210%
4	2.116	310	319	338	rVB	233324	345150	26.20%	3.304%
5	2.499	435	438	440	rBV4	1148	619	0.05%	0.006%
6	2.511	440	442	444	rBV2	1595	914	0.07%	0.009%
7	2.608	470	472	475	rBV3	1267	793	0.06%	0.008%
8	2.920	566	569	572	rVB5	1557	899	0.07%	0.009%
9	3.090	617	622	625	rBV8	1415	996	0.08%	0.010%
10	3.177	647	649	651	rBV2	1698	728	0.06%	0.007%
11	3.521	755	756	759	rVB3	1713	694	0.05%	0.007%
12	3.547	761	764	767	rVB5	1031	548	0.04%	0.005%
13	3.576	767	773	774	rBV4	888	617	0.05%	0.006%
14	3.598	777	780	781	rBV3	1517	888	0.07%	0.008%
15	3.769	831	833	835	rBV3	1238	559	0.04%	0.005%
16	3.894	859	872	901	rBV	110179	295567	22.44%	2.829%
17	4.151	947	952	953	rBV5	2105	1656	0.13%	0.016%
18	4.183	959	962	967	rBV6	1530	1684	0.13%	0.016%
19	4.373	1006	1021	1045	rBV	215386	526006	39.93%	5.035%
20	4.688	1117	1119	1121	rBV3	1278	749	0.06%	0.007%
21	4.788	1148	1150	1154	rBV5	1545	1058	0.08%	0.010%
22	4.817	1157	1159	1162	rBV3	1332	854	0.06%	0.008%
23	4.981	1207	1210	1211	rBV3	1182	805	0.06%	0.008%
24	5.068	1221	1237	1261	rBV2	510153	1317395	100.00%	12.610%
25	5.508	1370	1374	1376	rBV4	1788	1346	0.10%	0.013%
26	5.640	1400	1415	1440	rBV	447107	901611	68.44%	8.630%
27	6.093	1544	1556	1583	rVB	300636	605097	45.93%	5.792%
28	6.412	1653	1655	1658	rBV3	1213	665	0.05%	0.006%
29	6.482	1674	1677	1681	rVB5	1925	1136	0.09%	0.011%
30	6.534	1690	1693	1695	rBV3	1412	1012	0.08%	0.010%
31	6.849	1788	1791	1793	rBV4	1003	555	0.04%	0.005%
32	6.887	1801	1803	1806	rBV3	1647	927	0.07%	0.009%
33	7.006	1830	1840	1863	rVB	170538	302333	22.95%	2.894%
34	7.338	1929	1943	1961	rBV	602826	1041736	79.08%	9.971%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016712.D
 Acq On : 09 Jun 2020 13:17
 Operator : SY/MD
 Sample : L2901-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTY7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	7.640	2027	2037	2056	rBV	123418	213714	16.22%	2.046%
36	7.833	2095	2097	2099	rBV3	1307	550	0.04%	0.005%
37	7.887	2111	2114	2116	rBV3	916	638	0.05%	0.006%
38	8.032	2156	2159	2160	rBV2	1329	694	0.05%	0.007%
39	8.071	2168	2171	2172	rBV3	1578	936	0.07%	0.009%
40	8.109	2172	2183	2212	rVV	341218	676086	51.32%	6.471%
41	8.386	2266	2269	2275	rVB7	2468	2349	0.18%	0.022%
42	8.415	2275	2278	2280	rBV3	1446	993	0.08%	0.010%
43	8.450	2287	2289	2293	rBV4	1625	1098	0.08%	0.011%
44	8.701	2365	2367	2373	rVV6	1163	752	0.06%	0.007%
45	8.746	2377	2381	2384	rBV5	2110	2005	0.15%	0.019%
46	8.875	2408	2421	2443	rBV	684556	1092079	82.90%	10.453%
47	9.074	2480	2483	2484	rBV3	1245	794	0.06%	0.008%
48	9.096	2488	2490	2492	rVV2	1894	960	0.07%	0.009%
49	9.132	2496	2501	2503	rBV4	1553	1205	0.09%	0.012%
50	9.228	2528	2531	2534	rBV5	1543	957	0.07%	0.009%
51	9.254	2537	2539	2543	rBV5	1479	1046	0.08%	0.010%
52	9.357	2568	2571	2574	rBV3	1598	1326	0.10%	0.013%
53	9.402	2583	2585	2587	rBV3	1217	657	0.05%	0.006%
54	9.489	2605	2612	2616	rBV9	1863	1816	0.14%	0.017%
55	9.514	2616	2620	2622	rBV4	1502	1065	0.08%	0.010%
56	9.653	2660	2663	2668	rBV7	2299	1564	0.12%	0.015%
57	9.868	2728	2730	2733	rBV3	958	566	0.04%	0.005%
58	9.958	2755	2758	2762	rBV5	1901	1342	0.10%	0.013%
59	9.987	2763	2767	2769	rBV4	1761	1170	0.09%	0.011%
60	10.167	2817	2823	2827	rBV9	1547	1738	0.13%	0.017%
61	10.238	2834	2845	2861	rBV	394525	608477	46.19%	5.824%
62	10.437	2905	2907	2909	rBV3	907	628	0.05%	0.006%
63	10.508	2927	2929	2935	rBV7	1127	905	0.07%	0.009%
64	10.746	3001	3003	3006	rVB4	1654	1067	0.08%	0.010%
65	10.768	3006	3010	3013	rVB5	1680	1067	0.08%	0.010%
66	10.942	3057	3064	3065	rBV7	3025	2787	0.21%	0.027%
67	11.077	3103	3106	3107	rBV3	1135	646	0.05%	0.006%
68	11.119	3117	3119	3126	rVB7	1223	1160	0.09%	0.011%
69	11.270	3153	3166	3180	rBV	697534	1069608	81.19%	10.238%
70	11.646	3272	3283	3304	rVB	672029	1058885	80.38%	10.136%
71	11.800	3328	3331	3333	rBV4	1897	1287	0.10%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016712.D
 Acq On : 09 Jun 2020 13:17
 Operator : SY/MD
 Sample : L2901-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTY7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.923	3367	3369	3373	rBV5	1652	1288	0.10%	0.012%
73	11.945	3374	3376	3378	rBV3	1175	735	0.06%	0.007%
74	11.990	3388	3390	3393	rBV4	1287	853	0.06%	0.008%
75	12.042	3404	3406	3410	rVV4	1116	793	0.06%	0.008%
76	12.064	3411	3413	3420	rVV8	1481	924	0.07%	0.009%
77	12.469	3533	3539	3542	rBV7	1625	1807	0.14%	0.017%
78	12.485	3542	3544	3547	rVV4	1294	884	0.07%	0.008%
79	12.524	3550	3556	3560	rBV6	1671	2180	0.17%	0.021%
80	12.546	3560	3563	3564	rBV3	1122	616	0.05%	0.006%
81	12.630	3587	3589	3592	rBV2	1514	678	0.05%	0.006%
82	12.762	3628	3630	3633	rVB3	1253	697	0.05%	0.007%
83	12.800	3637	3642	3643	rBV4	1511	1325	0.10%	0.013%
84	12.842	3654	3655	3658	rBV3	1322	894	0.07%	0.009%
85	12.945	3683	3687	3688	rBV4	1141	759	0.06%	0.007%
86	13.032	3710	3714	3718	rVV7	1427	1014	0.08%	0.010%
87	13.183	3759	3761	3765	rBV3	1012	701	0.05%	0.007%
88	13.260	3779	3785	3789	rBV8	2564	2582	0.20%	0.025%
89	13.331	3803	3807	3811	rBV8	1487	1116	0.08%	0.011%
90	13.495	3856	3858	3865	rBV8	1587	1425	0.11%	0.014%
91	13.527	3865	3868	3870	rBV3	1579	996	0.08%	0.010%
92	13.591	3885	3888	3890	rBV3	1025	674	0.05%	0.006%
93	13.730	3927	3931	3933	rBV4	942	573	0.04%	0.005%
94	14.009	4016	4018	4022	rVB4	1390	983	0.07%	0.009%
95	14.453	4153	4156	4158	rBV3	1261	737	0.06%	0.007%
96	14.466	4158	4160	4163	rVB3	1712	1050	0.08%	0.010%
97	14.485	4163	4166	4168	rBV2	2033	1453	0.11%	0.014%
98	14.566	4188	4191	4192	rBV2	1212	626	0.05%	0.006%
99	14.759	4248	4251	4253	rBV4	1522	915	0.07%	0.009%
100	14.916	4298	4300	4307	rVB8	1866	1445	0.11%	0.014%


Sum of corrected areas: 10447217

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060920\
Data File : VV016712.D
Acq On : 09 Jun 2020 13:17
Operator : SY/MD
Sample : L2901-14
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTY7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

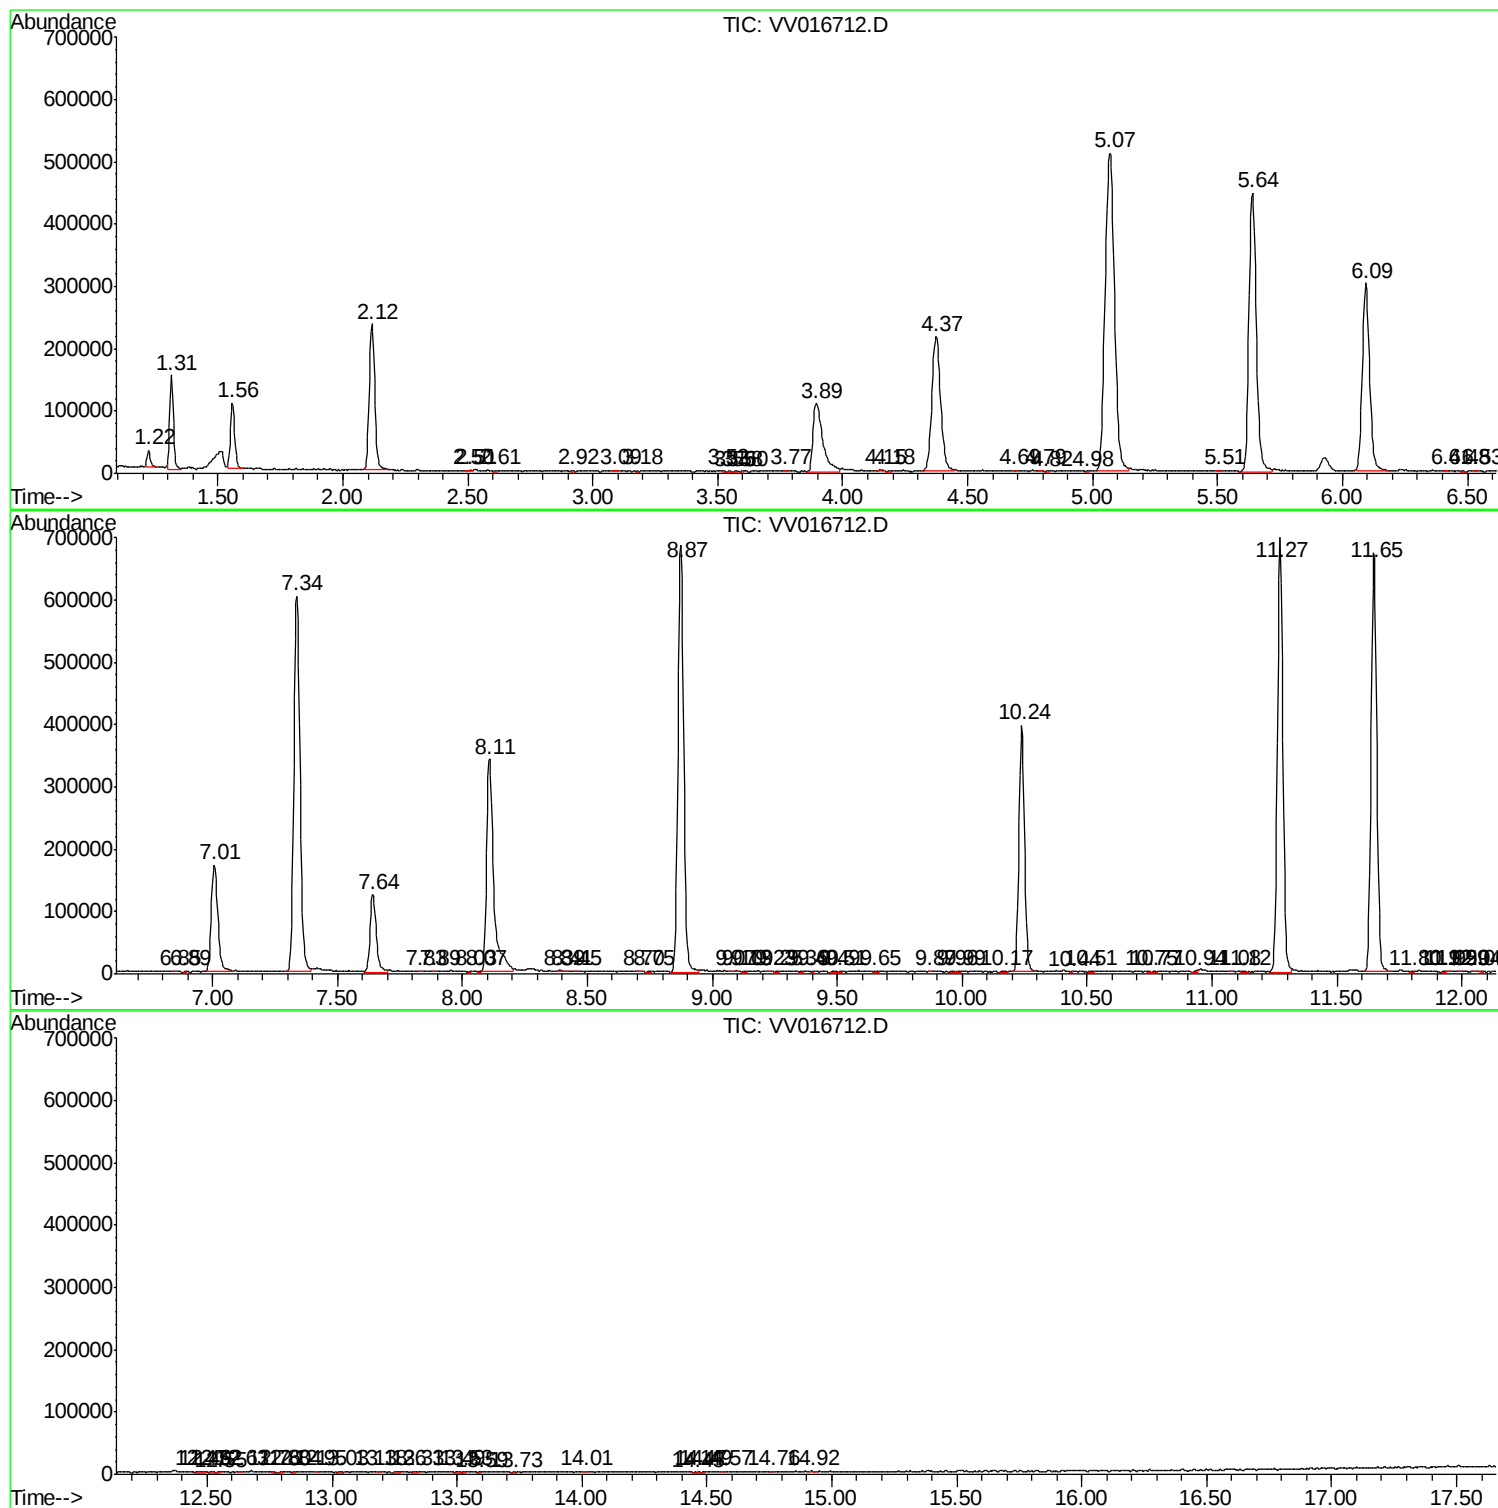

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016712.D
Acq On : 09 Jun 2020 13:17
Operator : SY/MD
Sample : L2901-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTY7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016712.D
Acq On : 09 Jun 2020 13:17
Operator : SY/MD
Sample : L2901-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTY7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc