

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016713.D
 Acq On : 09 Jun 2020 13:41
 Operator : SY/MD
 Sample : L2901-15
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTZ0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	79	rVB	158428	154428	11.27%	1.572%
2	1.563	140	147	161	rVB	112038	137633	10.04%	1.401%
3	2.116	310	319	335	rVB	248371	363138	26.49%	3.697%
4	2.354	390	393	394	rBV3	1709	1021	0.07%	0.010%
5	2.634	469	480	487	rBV3	3162	6607	0.48%	0.067%
6	2.923	568	570	575	rVB5	1488	1104	0.08%	0.011%
7	2.971	584	585	588	rBV3	1115	582	0.04%	0.006%
8	3.241	666	669	670	rBV3	1044	609	0.04%	0.006%
9	3.257	670	674	678	rVB6	1319	951	0.07%	0.010%
10	3.283	678	682	685	rBV5	1572	1428	0.10%	0.015%
11	3.373	707	710	713	rBV4	2119	1521	0.11%	0.015%
12	3.457	733	736	738	rBV4	1637	947	0.07%	0.010%
13	3.675	800	804	806	rBV4	1538	950	0.07%	0.010%
14	3.730	817	821	823	rBV5	924	672	0.05%	0.007%
15	3.894	858	872	905	rBV	111308	314526	22.95%	3.202%
16	4.251	977	983	988	rBV10	2070	2939	0.21%	0.030%
17	4.273	988	990	996	rVB6	1606	1156	0.08%	0.012%
18	4.373	1005	1021	1047	rVV	224968	549853	40.12%	5.598%
19	4.515	1063	1065	1067	rVB2	1795	632	0.05%	0.006%
20	4.666	1110	1112	1114	rBV2	1569	730	0.05%	0.007%
21	4.720	1127	1129	1133	rVB4	1560	679	0.05%	0.007%
22	4.920	1188	1191	1192	rBV3	1142	626	0.05%	0.006%
23	5.071	1219	1238	1266	rBV2	530544	1370610	100.00%	13.954%
24	5.640	1403	1415	1440	rBV	340462	677831	49.45%	6.901%
25	5.997	1524	1526	1530	rVB5	2123	1298	0.09%	0.013%
26	6.023	1530	1534	1535	rBV4	1536	1042	0.08%	0.011%
27	6.093	1542	1556	1580	rBV	306144	623755	45.51%	6.350%
28	6.338	1631	1632	1635	rBV2	1231	738	0.05%	0.008%
29	6.482	1674	1677	1682	rBV8	1511	1473	0.11%	0.015%
30	6.595	1710	1712	1717	rVB4	1255	1052	0.08%	0.011%
31	6.643	1723	1727	1729	rBV5	1542	1064	0.08%	0.011%
32	6.746	1757	1759	1761	rBV3	1598	851	0.06%	0.009%
33	7.006	1829	1840	1862	rBV	177813	310837	22.68%	3.165%
34	7.241	1910	1913	1917	rVB5	829	576	0.04%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016713.D
 Acq On : 09 Jun 2020 13:41
 Operator : SY/MD
 Sample : L2901-15
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTZ0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	7.338	1931	1943	1960	rBV	619386	1052053	76.76%	10.711%
36	7.643	2028	2038	2054	rBV2	121981	207503	15.14%	2.113%
37	7.842	2097	2100	2104	rBV4	1780	1252	0.09%	0.013%
38	8.106	2172	2182	2215	rVV2	340527	679080	49.55%	6.914%
39	8.434	2281	2284	2286	rBV3	2059	1424	0.10%	0.014%
40	8.498	2302	2304	2306	rBV2	1008	640	0.05%	0.007%
41	8.617	2338	2341	2343	rBV3	1016	631	0.05%	0.006%
42	8.685	2359	2362	2366	rBV4	1489	1013	0.07%	0.010%
43	8.730	2374	2376	2377	rBV2	1278	676	0.05%	0.007%
44	8.794	2393	2396	2400	rBV5	1236	1247	0.09%	0.013%
45	8.874	2409	2421	2437	rBV	509763	826655	60.31%	8.416%
46	9.083	2484	2486	2490	rBV5	1592	942	0.07%	0.010%
47	9.328	2560	2562	2565	rBV4	1457	889	0.06%	0.009%
48	9.350	2565	2569	2571	rBV5	1254	667	0.05%	0.007%
49	9.363	2571	2573	2577	rVV4	1092	619	0.05%	0.006%
50	9.434	2592	2595	2599	rBV4	2144	1680	0.12%	0.017%
51	9.546	2628	2630	2632	rBV3	988	591	0.04%	0.006%
52	9.714	2678	2682	2685	rBV5	1398	1033	0.08%	0.011%
53	9.794	2705	2707	2710	rBV4	1721	995	0.07%	0.010%
54	9.862	2725	2728	2732	rBV6	1899	1162	0.08%	0.012%
55	9.952	2752	2756	2760	rVV6	1406	1232	0.09%	0.013%
56	10.038	2780	2783	2784	rBV2	1144	664	0.05%	0.007%
57	10.116	2803	2807	2808	rBV4	1507	866	0.06%	0.009%
58	10.190	2827	2830	2831	rVV3	1726	1021	0.07%	0.010%
59	10.238	2835	2845	2862	rVB	396558	619952	45.23%	6.312%
60	10.350	2878	2880	2883	rVB4	1452	758	0.06%	0.008%
61	10.868	3037	3041	3047	rBV8	1948	2370	0.17%	0.024%
62	11.029	3086	3091	3095	rVB7	1438	1266	0.09%	0.013%
63	11.099	3111	3113	3115	rBV	1118	642	0.05%	0.007%
64	11.122	3115	3120	3123	rVB6	2340	1945	0.14%	0.020%
65	11.270	3155	3166	3187	rBV	514334	797178	58.16%	8.116%
66	11.427	3213	3215	3217	rBV3	1309	680	0.05%	0.007%
67	11.646	3272	3283	3300	rVB	665578	1047942	76.46%	10.669%
68	11.874	3352	3354	3357	rBV2	1272	814	0.06%	0.008%
69	12.251	3468	3471	3474	rBV4	1631	876	0.06%	0.009%
70	12.273	3476	3478	3482	rVB5	1451	878	0.06%	0.009%
71	12.524	3553	3556	3558	rBV4	1681	1033	0.08%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016713.D
 Acq On : 09 Jun 2020 13:41
 Operator : SY/MD
 Sample : L2901-15
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTZ0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.598	3577	3579	3582	rVB4	1290	718	0.05%	0.007%
73	12.627	3582	3588	3589	rBV4	1310	1273	0.09%	0.013%
74	12.858	3654	3660	3662	rBV6	1807	1779	0.13%	0.018%
75	12.939	3682	3685	3686	rBV2	1621	855	0.06%	0.009%
76	13.164	3752	3755	3756	rBV2	976	649	0.05%	0.007%
77	13.222	3769	3773	3774	rBV3	989	672	0.05%	0.007%
78	13.392	3823	3826	3830	rVV6	1547	1611	0.12%	0.016%
79	13.427	3834	3837	3839	rBV3	1194	586	0.04%	0.006%
80	13.524	3865	3867	3870	rVB4	1359	687	0.05%	0.007%
81	13.543	3870	3873	3875	rBV3	1471	859	0.06%	0.009%
82	13.652	3905	3907	3910	rVB3	1564	859	0.06%	0.009%
83	13.669	3910	3912	3915	rVB3	1307	601	0.04%	0.006%
84	13.685	3915	3917	3918	rBV2	1608	677	0.05%	0.007%
85	13.762	3938	3941	3943	rBV3	1124	885	0.06%	0.009%
86	13.807	3951	3955	3959	rBV5	1358	1239	0.09%	0.013%
87	13.836	3960	3964	3966	rBV4	1050	808	0.06%	0.008%
88	13.881	3975	3978	3979	rBV3	2041	1067	0.08%	0.011%
89	13.968	4003	4005	4007	rBV3	1594	973	0.07%	0.010%
90	14.003	4014	4016	4018	rBV3	1305	673	0.05%	0.007%
91	14.305	4106	4110	4111	rBV2	1790	926	0.07%	0.009%
92	14.424	4144	4147	4150	rBV4	1087	903	0.07%	0.009%
93	14.469	4156	4161	4163	rBV5	1733	1210	0.09%	0.012%
94	14.492	4166	4168	4170	rBV2	1513	681	0.05%	0.007%
95	14.504	4170	4172	4174	rBV3	1191	674	0.05%	0.007%
96	14.540	4179	4183	4184	rBV3	1275	890	0.06%	0.009%
97	14.984	4316	4321	4325	rBV7	1789	2012	0.15%	0.020%
98	15.238	4398	4400	4402	rBV3	1900	1117	0.08%	0.011%
99	15.321	4423	4426	4427	rBV3	2027	1131	0.08%	0.012%
100	15.575	4503	4505	4506	rBV2	1643	746	0.05%	0.008%


Sum of corrected areas: 9822489

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060920\
Data File : VV016713.D
Acq On : 09 Jun 2020 13:41
Operator : SY/MD
Sample : L2901-15
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETT20

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

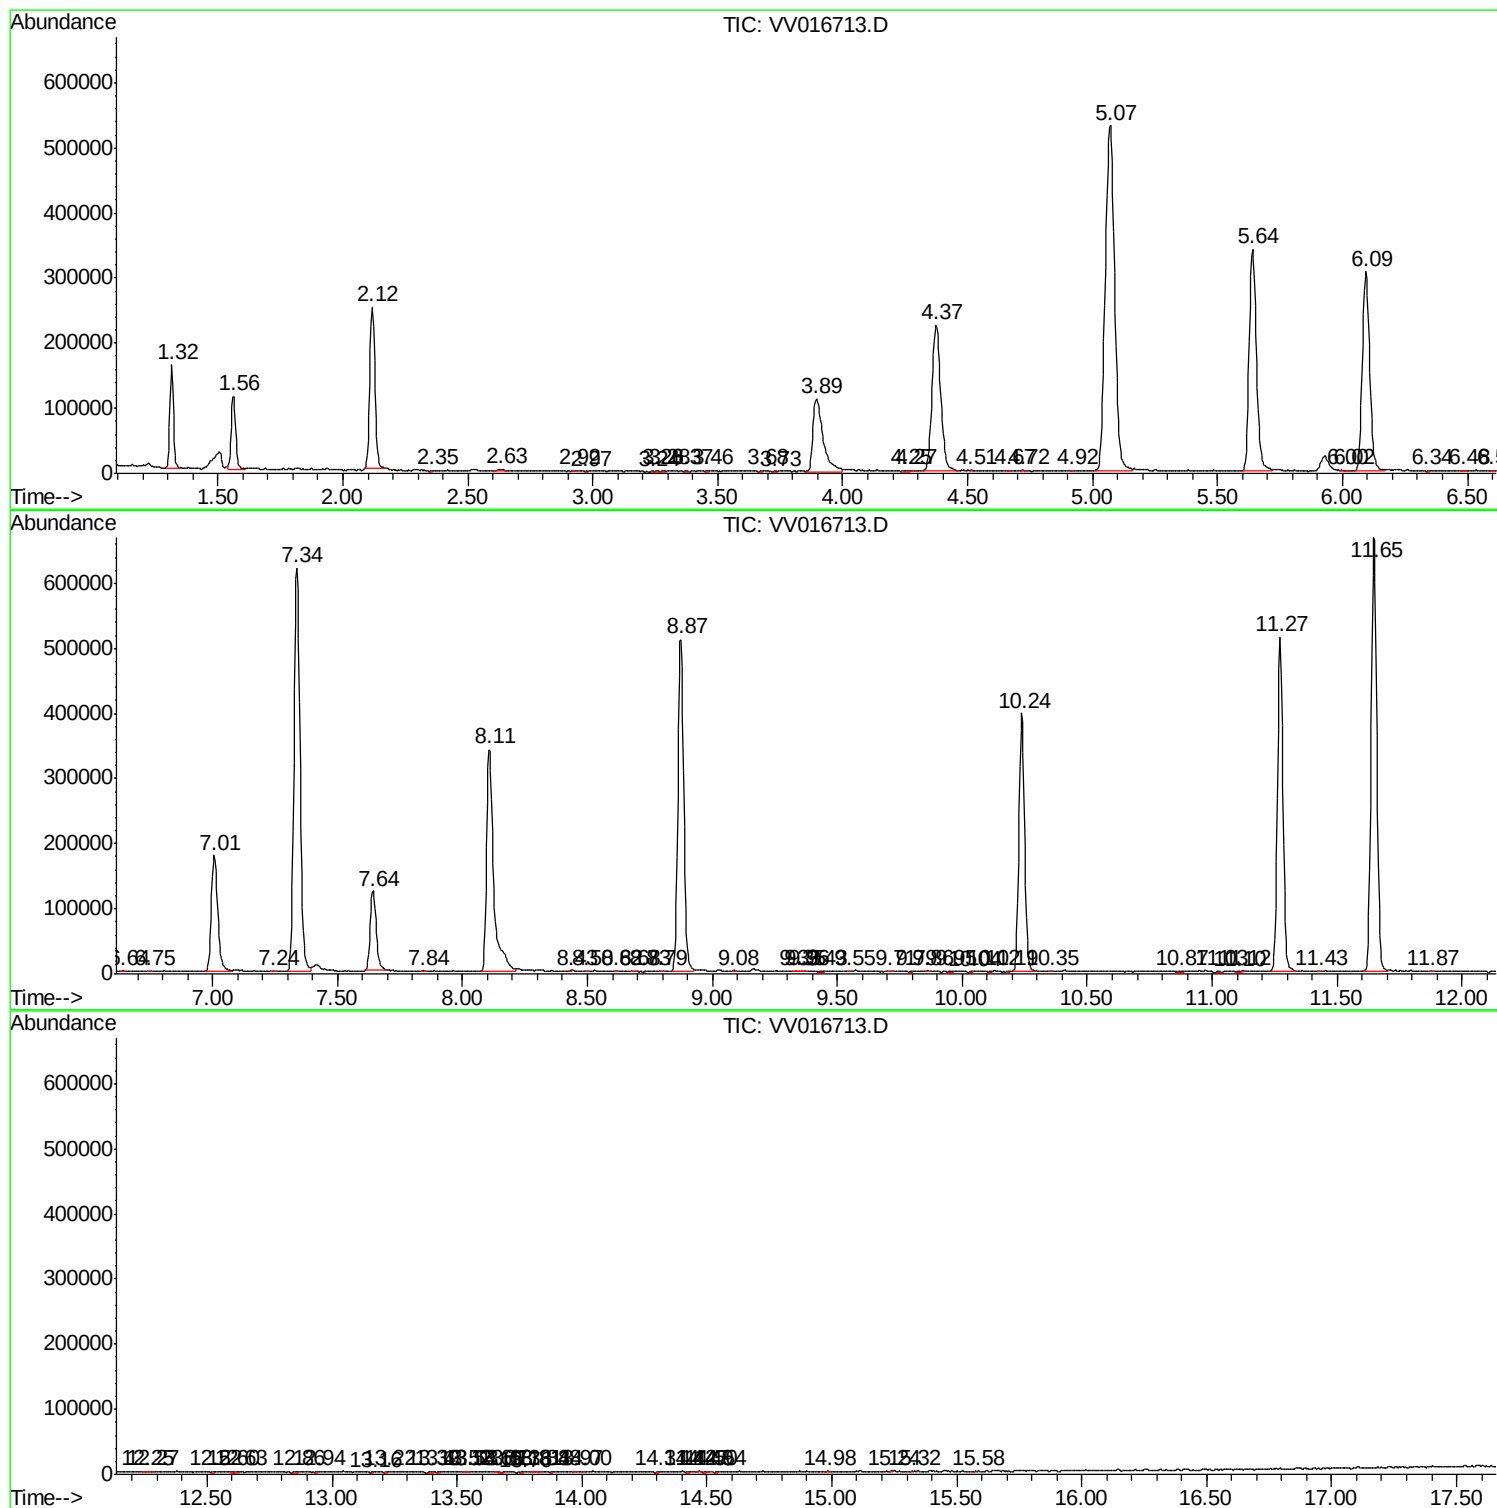

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016713.D
Acq On : 09 Jun 2020 13:41
Operator : SY/MD
Sample : L2901-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTZO

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016713.D
Acq On : 09 Jun 2020 13:41
Operator : SY/MD
Sample : L2901-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETT20

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc