

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016714.D
 Acq On : 09 Jun 2020 14:04
 Operator : SY/MD
 Sample : L2901-19
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTR2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	64	70	81	rVB	158028	157702	11.21%	1.476%
2	1.566	141	148	158	rVB	117270	137438	9.77%	1.287%
3	2.119	310	320	333	rBV	253766	377194	26.82%	3.531%
4	2.479	428	432	433	rBV3	2048	1589	0.11%	0.015%
5	2.627	475	478	480	rBV2	1577	1071	0.08%	0.010%
6	2.721	504	507	510	rBV3	1468	1266	0.09%	0.012%
7	2.910	563	566	570	rBV4	1305	960	0.07%	0.009%
8	3.020	597	600	602	rBV4	1685	1029	0.07%	0.010%
9	3.155	639	642	645	rBV5	1851	1185	0.08%	0.011%
10	3.203	653	657	661	rBV7	1918	1826	0.13%	0.017%
11	3.338	694	699	701	rBV6	1941	1476	0.10%	0.014%
12	3.399	715	718	720	rBV4	1321	714	0.05%	0.007%
13	3.415	720	723	725	rBV3	1365	848	0.06%	0.008%
14	3.450	731	734	737	rBV5	1469	955	0.07%	0.009%
15	3.502	748	750	754	rVB4	1455	941	0.07%	0.009%
16	3.582	771	775	778	rBV5	1012	947	0.07%	0.009%
17	3.634	788	791	797	rBV6	1203	1404	0.10%	0.013%
18	3.711	811	815	817	rBV4	1097	849	0.06%	0.008%
19	3.724	817	819	822	rVV4	1072	777	0.06%	0.007%
20	3.795	837	841	843	rBV4	1623	1255	0.09%	0.012%
21	3.894	862	872	901	rBV	117688	311752	22.17%	2.918%
22	4.222	971	974	976	rBV4	1334	717	0.05%	0.007%
23	4.267	986	988	991	rBV3	1521	1036	0.07%	0.010%
24	4.373	1006	1021	1042	rBV	229965	558874	39.74%	5.231%
25	4.537	1068	1072	1075	rBV6	1954	1669	0.12%	0.016%
26	4.659	1106	1110	1111	rBV3	1555	1171	0.08%	0.011%
27	4.827	1159	1162	1165	rBV5	1819	1559	0.11%	0.015%
28	4.913	1183	1189	1193	rVB7	1707	1691	0.12%	0.016%
29	4.955	1200	1202	1205	rBV4	1379	1017	0.07%	0.010%
30	5.071	1219	1238	1260	rBV2	543958	1406175	100.00%	13.163%
31	5.640	1402	1415	1434	rBV	414167	824699	58.65%	7.720%
32	5.930	1492	1505	1522	rBV	10938	26790	1.91%	0.251%
33	6.093	1543	1556	1578	rBV2	316467	641207	45.60%	6.002%
34	6.405	1651	1653	1655	rBV4	1348	821	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016714.D
 Acq On : 09 Jun 2020 14:04
 Operator : SY/MD
 Sample : L2901-19
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTR2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.466	1670	1672	1676	rBV4	1228	839	0.06%	0.008%
36	6.492	1678	1680	1684	rVB5	1503	815	0.06%	0.008%
37	6.611	1714	1717	1720	rBV5	1198	1171	0.08%	0.011%
38	6.653	1728	1730	1733	rBV3	1889	1158	0.08%	0.011%
39	6.743	1755	1758	1763	rBV7	905	861	0.06%	0.008%
40	6.917	1809	1812	1813	rBV2	1662	929	0.07%	0.009%
41	7.007	1829	1840	1862	rBV	184527	325708	23.16%	3.049%
42	7.338	1929	1943	1964	rBV	642398	1104487	78.55%	10.339%
43	7.598	2021	2024	2026	rBV4	1108	811	0.06%	0.008%
44	7.640	2027	2037	2055	rVV	124643	215573	15.33%	2.018%
45	7.923	2120	2125	2130	rBV7	1952	1919	0.14%	0.018%
46	8.106	2172	2182	2217	rBV	380453	714691	50.83%	6.690%
47	8.772	2385	2389	2391	rBV4	1826	1344	0.10%	0.013%
48	8.785	2391	2393	2397	rBV5	1683	1215	0.09%	0.011%
49	8.875	2407	2421	2443	rBV	623664	1023035	72.75%	9.576%
50	9.203	2520	2523	2526	rBV6	1562	1520	0.11%	0.014%
51	9.309	2554	2556	2560	rVB4	1266	738	0.05%	0.007%
52	9.457	2600	2602	2608	rVB7	1932	1280	0.09%	0.012%
53	9.495	2608	2614	2615	rBV4	962	802	0.06%	0.008%
54	9.778	2699	2702	2703	rBV3	1454	889	0.06%	0.008%
55	9.904	2738	2741	2745	rBV3	1185	1050	0.07%	0.010%
56	9.997	2766	2770	2773	rBV5	1069	958	0.07%	0.009%
57	10.161	2817	2821	2823	rVB4	1111	753	0.05%	0.007%
58	10.238	2834	2845	2863	rVB	438632	684436	48.67%	6.407%
59	10.460	2911	2914	2916	rBV3	1520	1012	0.07%	0.009%
60	10.537	2933	2938	2940	rBV6	1435	1354	0.10%	0.013%
61	10.592	2953	2955	2960	rVB6	1415	919	0.07%	0.009%
62	10.714	2991	2993	2996	rBV3	1533	1066	0.08%	0.010%
63	10.936	3059	3062	3065	rBV4	1395	1014	0.07%	0.009%
64	10.978	3074	3075	3081	rVB3	1758	1535	0.11%	0.014%
65	11.006	3081	3084	3085	rBV3	1216	826	0.06%	0.008%
66	11.071	3100	3104	3108	rBV7	1276	1291	0.09%	0.012%
67	11.113	3114	3117	3120	rBV3	1698	1076	0.08%	0.010%
68	11.270	3155	3166	3185	rBV	631238	973061	69.20%	9.109%
69	11.556	3247	3255	3263	rBV8	7896	13162	0.94%	0.123%
70	11.646	3272	3283	3299	rBV	713297	1093739	77.78%	10.238%
71	11.865	3349	3351	3354	rBV4	1114	802	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016714.D
 Acq On : 09 Jun 2020 14:04
 Operator : SY/MD
 Sample : L2901-19
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTR2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.932	3369	3372	3374	rBV4	1302	781	0.06%	0.007%
73	12.003	3390	3394	3395	rBV4	1910	1170	0.08%	0.011%
74	12.042	3402	3406	3407	rBV4	1375	985	0.07%	0.009%
75	12.109	3425	3427	3432	rBV6	1870	1338	0.10%	0.013%
76	12.232	3462	3465	3467	rBV4	1916	1012	0.07%	0.009%
77	12.370	3506	3508	3514	rVB7	1734	1282	0.09%	0.012%
78	12.598	3576	3579	3584	rBV7	1622	1302	0.09%	0.012%
79	12.810	3642	3645	3647	rBV4	1786	968	0.07%	0.009%
80	12.920	3677	3679	3682	rVB4	1674	972	0.07%	0.009%
81	12.939	3682	3685	3687	rBV3	1693	930	0.07%	0.009%
82	13.013	3706	3708	3713	rVB4	1989	1351	0.10%	0.013%
83	13.051	3714	3720	3723	rBV6	2071	2548	0.18%	0.024%
84	13.180	3754	3760	3762	rBV7	1648	1723	0.12%	0.016%
85	13.228	3772	3775	3777	rVB3	1500	923	0.07%	0.009%
86	13.254	3781	3783	3787	rBV5	1232	688	0.05%	0.006%
87	13.289	3792	3794	3797	rVB3	2288	1087	0.08%	0.010%
88	13.318	3801	3803	3806	rBV3	1557	1146	0.08%	0.011%
89	13.370	3816	3819	3821	rBV3	1143	731	0.05%	0.007%
90	13.839	3961	3965	3970	rBV8	1954	2283	0.16%	0.021%
91	13.920	3986	3990	3994	rBV5	1199	808	0.06%	0.008%
92	14.212	4077	4081	4085	rBV7	1536	1381	0.10%	0.013%
93	14.248	4088	4092	4094	rBV5	1437	1311	0.09%	0.012%
94	14.354	4123	4125	4127	rBV4	1551	800	0.06%	0.007%
95	14.466	4155	4160	4161	rBV4	1515	1295	0.09%	0.012%
96	14.511	4172	4174	4176	rBV3	1088	717	0.05%	0.007%
97	14.945	4306	4309	4311	rBV3	1427	736	0.05%	0.007%
98	15.000	4322	4326	4327	rBV3	1851	1165	0.08%	0.011%
99	15.260	4404	4407	4408	rBV2	1781	967	0.07%	0.009%
100	15.884	4598	4601	4606	rBV6	2099	2074	0.15%	0.019%


Sum of corrected areas: 10682917

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060920\
Data File : VV016714.D
Acq On : 09 Jun 2020 14:04
Operator : SY/MD
Sample : L2901-19
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTR2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

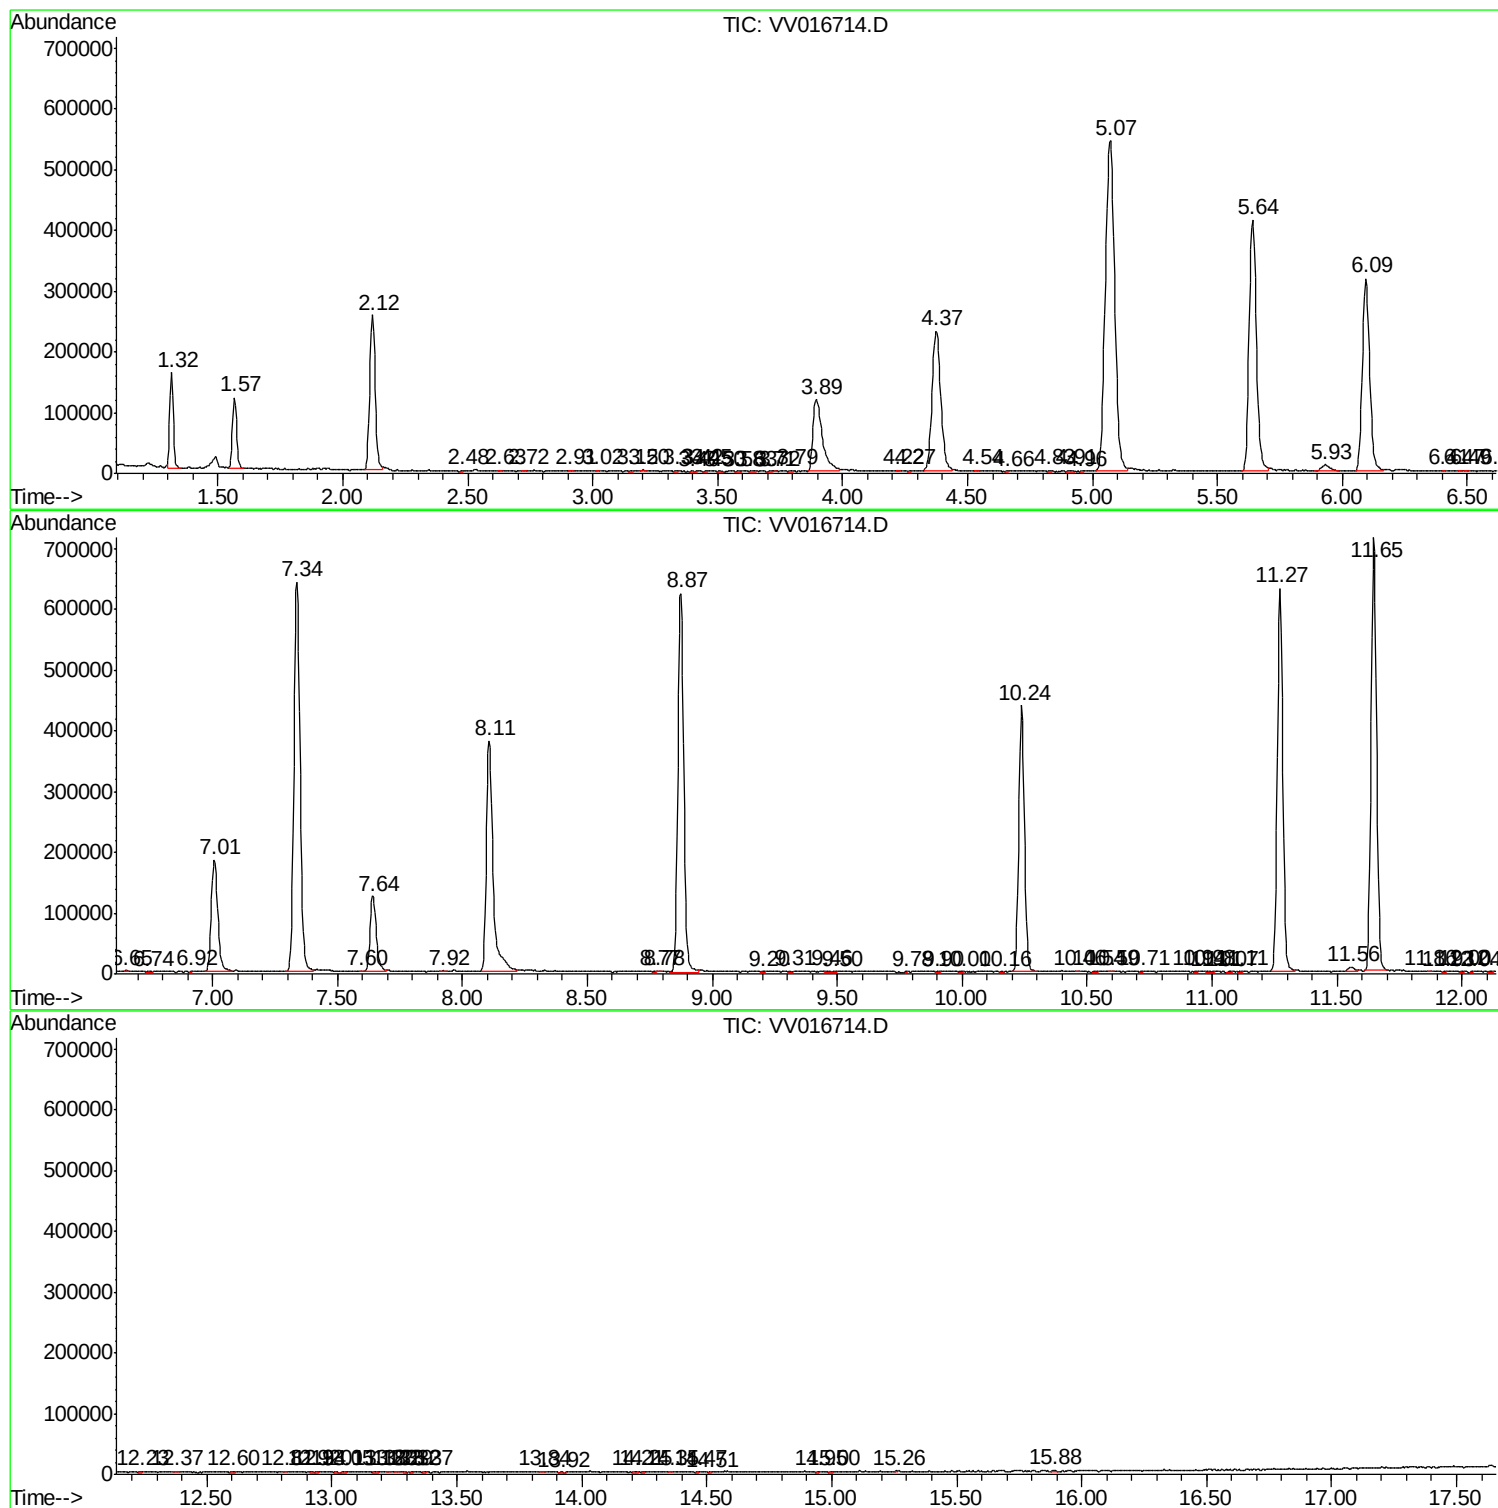

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016714.D
Acq On : 09 Jun 2020 14:04
Operator : SY/MD
Sample : L2901-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTR2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016714.D
Acq On : 09 Jun 2020 14:04
Operator : SY/MD
Sample : L2901-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTR2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc