

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016717.D
 Acq On : 09 Jun 2020 15:15
 Operator : SY/MD
 Sample : L2849-11DL 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTR6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	83	rVB2	293057	312767	23.24%	2.684%
2	1.556	139	145	157	rVB	110274	131909	9.80%	1.132%
3	2.116	310	319	335	rVB	246757	360174	26.76%	3.090%
4	2.280	367	370	372	rBV3	1970	1267	0.09%	0.011%
5	2.627	474	478	480	rBV4	3025	2461	0.18%	0.021%
6	2.730	508	510	513	rVB2	1459	613	0.05%	0.005%
7	2.865	550	552	556	rVB3	1641	879	0.07%	0.008%
8	2.904	561	564	565	rBV3	1044	545	0.04%	0.005%
9	3.032	602	604	606	rBV3	1270	599	0.04%	0.005%
10	3.058	609	612	615	rVV5	952	666	0.05%	0.006%
11	3.180	648	650	651	rBV2	1122	570	0.04%	0.005%
12	3.212	658	660	666	rVB6	2289	2167	0.16%	0.019%
13	3.251	666	672	673	rBV3	1730	1277	0.09%	0.011%
14	3.354	703	704	708	rVB4	1543	700	0.05%	0.006%
15	3.421	722	725	726	rBV3	1485	617	0.05%	0.005%
16	3.431	726	728	732	rVV4	1274	795	0.06%	0.007%
17	3.550	761	765	770	rBV8	1795	1443	0.11%	0.012%
18	3.614	783	785	787	rBV2	1009	535	0.04%	0.005%
19	3.640	790	793	797	rVB4	1715	1213	0.09%	0.010%
20	3.662	797	800	808	rVB9	2019	2576	0.19%	0.022%
21	3.701	808	812	813	rBV4	1405	884	0.07%	0.008%
22	3.740	818	824	829	rBV9	1527	1824	0.14%	0.016%
23	3.798	838	842	844	rBV5	1333	734	0.05%	0.006%
24	3.830	849	852	853	rBV2	1068	641	0.05%	0.005%
25	3.933	862	884	912	rBV3	298397	999635	74.27%	8.577%
26	4.232	975	977	979	rBV2	1520	646	0.05%	0.006%
27	4.244	979	981	986	rVB5	1620	1089	0.08%	0.009%
28	4.373	1001	1021	1048	rBV	223925	548354	40.74%	4.705%
29	4.569	1076	1082	1087	rBV9	1782	2711	0.20%	0.023%
30	4.601	1090	1092	1094	rBV3	1678	1042	0.08%	0.009%
31	4.942	1195	1198	1202	rVV4	1483	800	0.06%	0.007%
32	4.997	1212	1215	1219	rBV5	1515	1423	0.11%	0.012%
33	5.071	1219	1238	1262	rVV3	519870	1345873	100.00%	11.548%
34	5.299	1306	1309	1310	rBV3	1777	929	0.07%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016717.D
 Acq On : 09 Jun 2020 15:15
 Operator : SY/MD
 Sample : L2849-11DL 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTR6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	5.640	1401	1415	1437	rBV	449027	890146	66.14%	7.637%
36	6.093	1540	1556	1579	rBV2	306673	624115	46.37%	5.355%
37	6.341	1628	1633	1636	rBV6	1910	1689	0.13%	0.014%
38	6.502	1678	1683	1685	rBV5	1520	1340	0.10%	0.011%
39	6.572	1703	1705	1706	rBV2	1476	616	0.05%	0.005%
40	6.891	1800	1804	1806	rVB5	1399	930	0.07%	0.008%
41	6.907	1806	1809	1816	rBV7	1805	2307	0.17%	0.020%
42	7.006	1829	1840	1858	rBV	167922	303707	22.57%	2.606%
43	7.338	1931	1943	1962	rBV	614420	1044114	77.58%	8.959%
44	7.559	2009	2012	2015	rBV6	1883	1474	0.11%	0.013%
45	7.640	2028	2037	2052	rBV	123015	204087	15.16%	1.751%
46	7.823	2092	2094	2097	rBV3	2108	1389	0.10%	0.012%
47	7.903	2117	2119	2122	rBV3	951	751	0.06%	0.006%
48	8.106	2172	2182	2220	rBV	433874	807961	60.03%	6.932%
49	8.553	2317	2321	2323	rBV5	1775	1355	0.10%	0.012%
50	8.813	2399	2402	2404	rBV3	1484	684	0.05%	0.006%
51	8.874	2409	2421	2439	rVV	672381	1090861	81.05%	9.360%
52	9.093	2487	2489	2492	rVB4	2091	1079	0.08%	0.009%
53	9.289	2546	2550	2554	rBV7	1457	1362	0.10%	0.012%
54	9.328	2560	2562	2566	rBV6	1489	1121	0.08%	0.010%
55	9.418	2587	2590	2592	rBV4	1326	949	0.07%	0.008%
56	9.460	2599	2603	2606	rBV5	1044	1015	0.08%	0.009%
57	9.598	2644	2646	2649	rBV3	1331	800	0.06%	0.007%
58	9.743	2685	2691	2695	rBV9	2185	2725	0.20%	0.023%
59	9.772	2698	2700	2702	rBV3	1134	592	0.04%	0.005%
60	9.804	2706	2710	2712	rBV4	1467	1210	0.09%	0.010%
61	9.900	2738	2740	2741	rBV2	2084	905	0.07%	0.008%
62	9.981	2763	2765	2771	rBV7	1060	836	0.06%	0.007%
63	10.238	2834	2845	2859	rBV	432640	666002	49.48%	5.714%
64	10.402	2892	2896	2898	rBV4	2434	2059	0.15%	0.018%
65	10.511	2926	2930	2934	rBV7	1703	1641	0.12%	0.014%
66	10.659	2973	2976	2977	rBV3	1169	833	0.06%	0.007%
67	10.733	2997	2999	3002	rBV3	1283	780	0.06%	0.007%
68	11.170	3133	3135	3138	rBV3	1586	1150	0.09%	0.010%
69	11.270	3155	3166	3184	rBV	723326	1113298	82.72%	9.552%
70	11.379	3196	3200	3205	rBV8	1622	1712	0.13%	0.015%
71	11.466	3224	3227	3231	rVB6	1744	1416	0.11%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016717.D
 Acq On : 09 Jun 2020 15:15
 Operator : SY/MD
 Sample : L2849-11DL 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTR6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.646	3271	3283	3299	rBV	722444	1119249	83.16%	9.603%
73	11.913	3362	3366	3368	rBV4	1405	1448	0.11%	0.012%
74	11.958	3379	3380	3383	rVB3	1607	732	0.05%	0.006%
75	12.148	3437	3439	3444	rVB5	1571	933	0.07%	0.008%
76	12.177	3444	3448	3450	rBV5	1192	1113	0.08%	0.010%
77	12.453	3531	3534	3535	rBV3	1758	1069	0.08%	0.009%
78	12.508	3549	3551	3555	rVB3	1517	917	0.07%	0.008%
79	12.537	3555	3560	3563	rBV5	2080	1895	0.14%	0.016%
80	12.566	3567	3569	3571	rVB3	1921	908	0.07%	0.008%
81	12.598	3571	3579	3581	rBV9	1469	2020	0.15%	0.017%
82	12.643	3591	3593	3595	rBV3	1174	774	0.06%	0.007%
83	12.736	3619	3622	3623	rBV2	1125	582	0.04%	0.005%
84	12.987	3696	3700	3701	rBV4	1321	673	0.05%	0.006%
85	13.045	3716	3718	3722	rBV5	1181	976	0.07%	0.008%
86	13.064	3722	3724	3726	rVV3	1194	703	0.05%	0.006%
87	13.093	3730	3733	3734	rBV3	1330	714	0.05%	0.006%
88	13.151	3749	3751	3755	rVB3	1609	847	0.06%	0.007%
89	13.173	3755	3758	3759	rBV3	869	542	0.04%	0.005%
90	13.273	3787	3789	3790	rBV2	1152	600	0.04%	0.005%
91	13.591	3885	3888	3890	rBV3	1934	1062	0.08%	0.009%
92	13.659	3907	3909	3910	rBV2	1655	565	0.04%	0.005%
93	13.775	3943	3945	3948	rBV3	1480	1110	0.08%	0.010%
94	13.813	3955	3957	3960	rBV3	1346	819	0.06%	0.007%
95	13.861	3969	3972	3975	rBV5	1620	938	0.07%	0.008%
96	13.894	3979	3982	3984	rBV2	1191	798	0.06%	0.007%
97	13.916	3984	3989	3991	rBV5	1790	1232	0.09%	0.011%
98	14.369	4127	4130	4133	rBV4	1421	964	0.07%	0.008%
99	14.656	4216	4219	4221	rBV4	1291	840	0.06%	0.007%
100	14.849	4276	4279	4280	rBV2	1280	568	0.04%	0.005%


Sum of corrected areas: 11654960

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060920\
Data File : VV016717.D
Acq On : 09 Jun 2020 15:15
Operator : SY/MD
Sample : L2849-11DL 20X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTR6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

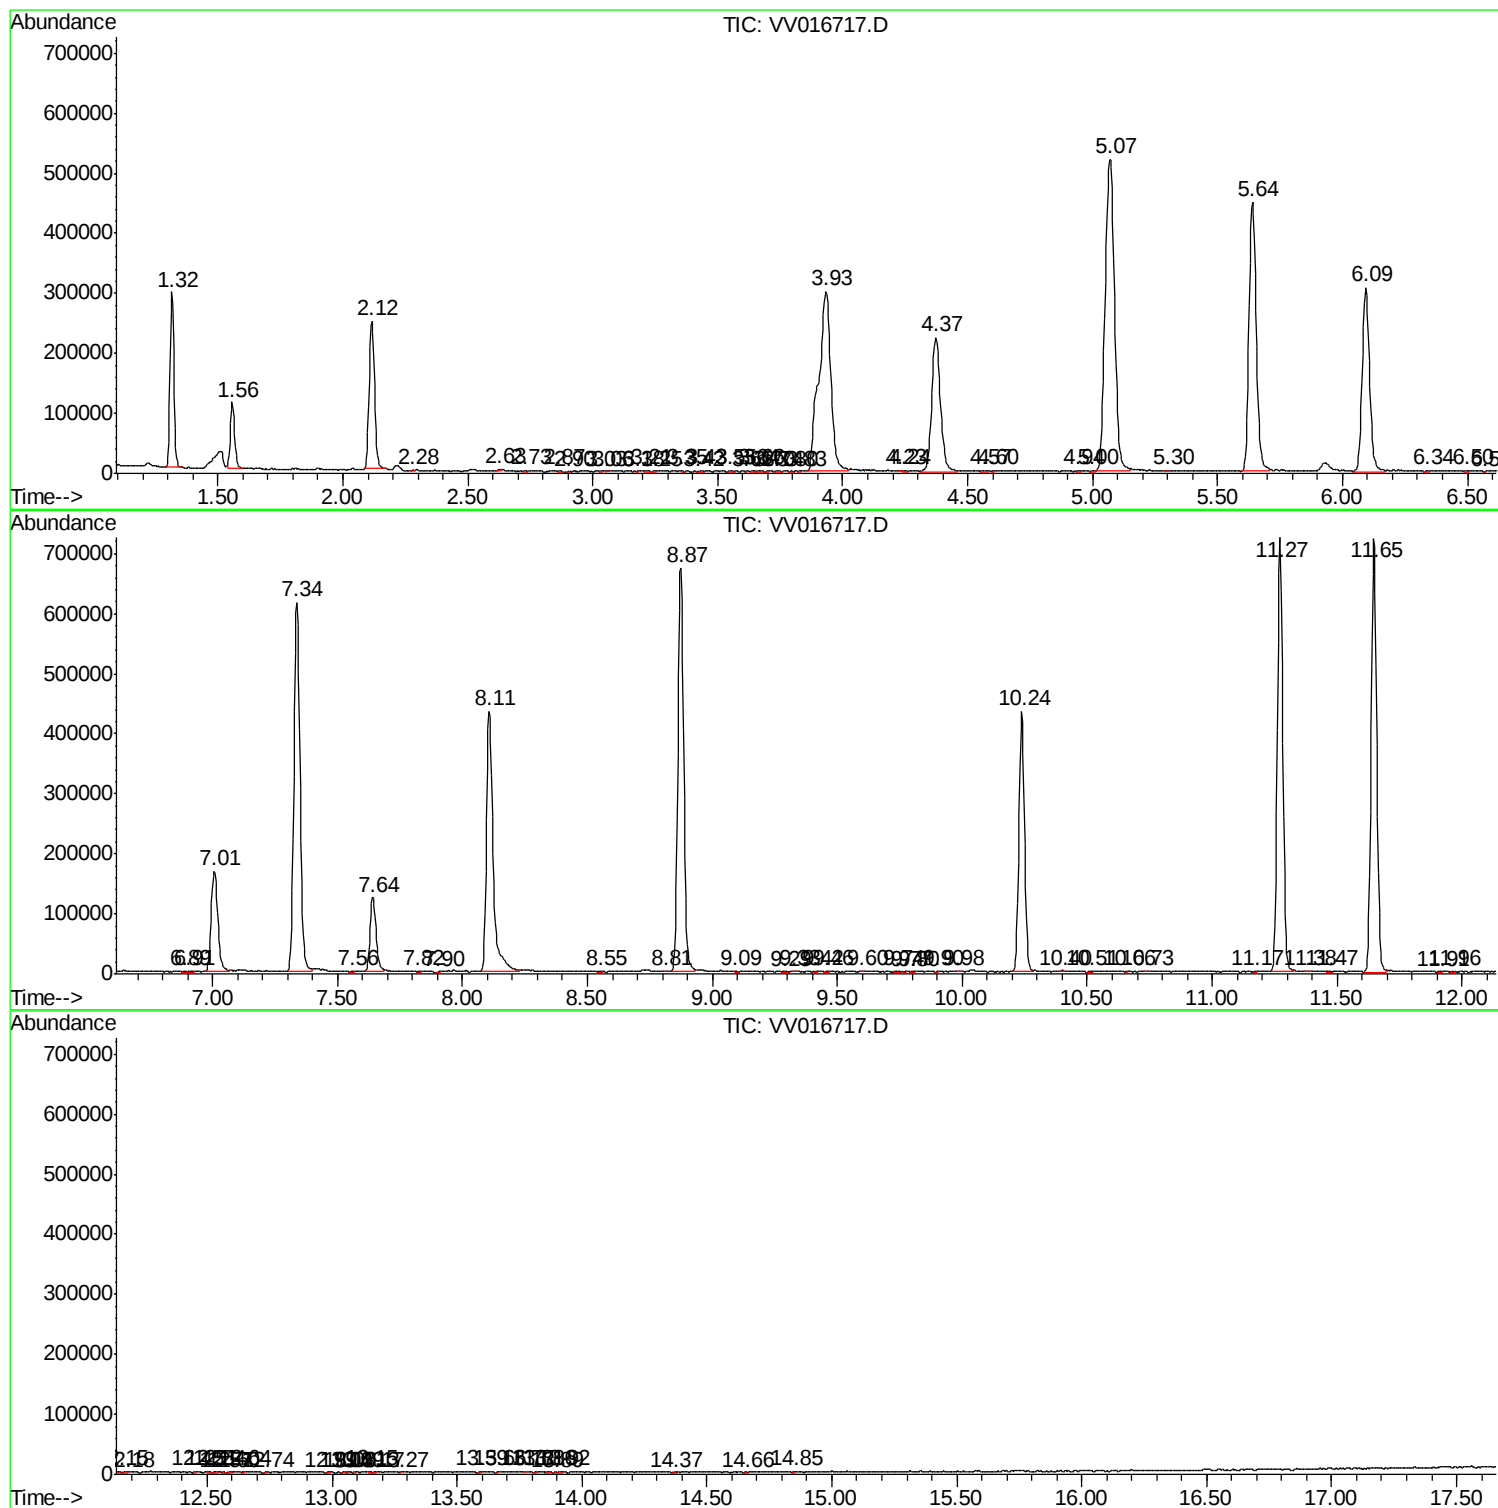

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016717.D
Acq On : 09 Jun 2020 15:15
Operator : SY/MD
Sample : L2849-11DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTR6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016717.D
Acq On : 09 Jun 2020 15:15
Operator : SY/MD
Sample : L2849-11DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTR6DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc