

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016718.D
 Acq On : 09 Jun 2020 15:39
 Operator : SY/MD
 Sample : L2901-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTT3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	81	rVB	150406	152967	11.08%	1.422%
2	1.563	140	147	160	rVB	112483	133903	9.70%	1.244%
3	2.116	310	319	331	rVB	247640	359026	26.00%	3.337%
4	2.675	491	493	496	rBV4	1500	1014	0.07%	0.009%
5	2.759	515	519	520	rBV4	1563	1135	0.08%	0.011%
6	2.888	554	559	560	rBV5	1533	1283	0.09%	0.012%
7	2.933	571	573	576	rVB3	1827	962	0.07%	0.009%
8	3.116	628	630	633	rBV4	1347	879	0.06%	0.008%
9	3.206	655	658	662	rBV3	1452	1313	0.10%	0.012%
10	3.261	672	675	681	rBV6	1870	2001	0.14%	0.019%
11	3.415	721	723	727	rVB4	1863	1276	0.09%	0.012%
12	3.531	755	759	761	rBV4	1317	870	0.06%	0.008%
13	3.553	764	766	770	rVB5	1520	860	0.06%	0.008%
14	3.618	784	786	790	rVB4	1790	1142	0.08%	0.011%
15	3.675	801	804	805	rBV2	1506	635	0.05%	0.006%
16	3.782	835	837	841	rBV3	1287	1018	0.07%	0.009%
17	3.823	847	850	851	rBV3	1090	755	0.05%	0.007%
18	3.894	862	872	900	rBV	115756	326874	23.67%	3.038%
19	4.200	965	967	970	rBV3	1488	974	0.07%	0.009%
20	4.322	1001	1005	1006	rBV3	1598	1086	0.08%	0.010%
21	4.373	1006	1021	1042	rVV	222629	548275	39.70%	5.096%
22	5.071	1218	1238	1267	rBV2	539119	1381132	100.00%	12.836%
23	5.402	1339	1341	1343	rBV3	1608	649	0.05%	0.006%
24	5.640	1402	1415	1440	rBV	446502	888710	64.35%	8.260%
25	5.936	1492	1507	1525	rBV8	24624	64277	4.65%	0.597%
26	6.093	1544	1556	1577	rVB	308599	618466	44.78%	5.748%
27	6.727	1748	1753	1756	rBV6	1609	2008	0.15%	0.019%
28	6.910	1809	1810	1813	rBV2	1618	731	0.05%	0.007%
29	7.006	1829	1840	1858	rBV	175602	313734	22.72%	2.916%
30	7.260	1916	1919	1922	rBV3	1584	1139	0.08%	0.011%
31	7.338	1931	1943	1962	rBV	623209	1065201	77.13%	9.900%
32	7.640	2028	2037	2056	rBV2	125333	218537	15.82%	2.031%
33	7.794	2083	2085	2089	rBV5	2093	1591	0.12%	0.015%
34	7.846	2099	2101	2103	rBV3	1500	842	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016718.D
 Acq On : 09 Jun 2020 15:39
 Operator : SY/MD
 Sample : L2901-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTT3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	8.045	2159	2163	2165	rBV4	1023	714	0.05%	0.007%
36	8.106	2172	2182	2217	rVV	387454	710929	51.47%	6.607%
37	8.424	2279	2281	2285	rVB3	1737	995	0.07%	0.009%
38	8.447	2285	2288	2290	rBV4	2008	1522	0.11%	0.014%
39	8.518	2304	2310	2313	rBV6	1687	1711	0.12%	0.016%
40	8.617	2338	2341	2342	rBV2	1341	671	0.05%	0.006%
41	8.669	2354	2357	2358	rBV2	1262	711	0.05%	0.007%
42	8.871	2409	2420	2438	rBV	670404	1087023	78.71%	10.103%
43	9.167	2510	2512	2516	rVB5	2129	1060	0.08%	0.010%
44	9.566	2630	2636	2639	rBV7	1568	1452	0.11%	0.013%
45	9.624	2652	2654	2657	rBV4	1097	626	0.05%	0.006%
46	9.688	2669	2674	2676	rBV5	1123	898	0.07%	0.008%
47	9.714	2679	2682	2684	rBV4	1187	761	0.06%	0.007%
48	9.746	2690	2692	2696	rBV3	1200	870	0.06%	0.008%
49	9.772	2696	2700	2701	rBV4	917	653	0.05%	0.006%
50	10.003	2770	2772	2774	rBV2	1447	810	0.06%	0.008%
51	10.132	2809	2812	2815	rBV4	1917	1384	0.10%	0.013%
52	10.193	2826	2831	2833	rBV5	1354	1287	0.09%	0.012%
53	10.238	2833	2845	2859	rVV	426251	673693	48.78%	6.261%
54	10.537	2934	2938	2940	rBV4	1520	1351	0.10%	0.013%
55	10.598	2950	2957	2960	rBV8	2160	2404	0.17%	0.022%
56	10.659	2972	2976	2978	rBV4	1583	1227	0.09%	0.011%
57	10.694	2984	2987	2990	rBV2	1211	694	0.05%	0.006%
58	10.839	3030	3032	3034	rBV3	1584	1028	0.07%	0.010%
59	10.874	3041	3043	3045	rBV3	1347	723	0.05%	0.007%
60	10.913	3052	3055	3057	rBV3	1720	1243	0.09%	0.012%
61	10.981	3070	3076	3080	rBV7	2036	2456	0.18%	0.023%
62	11.112	3113	3117	3118	rBV4	1353	1017	0.07%	0.009%
63	11.128	3120	3122	3127	rVB5	2000	1425	0.10%	0.013%
64	11.270	3154	3166	3182	rBV	693980	1058143	76.61%	9.834%
65	11.646	3272	3283	3300	rVB	687641	1067659	77.30%	9.923%
66	12.038	3403	3405	3410	rVB4	1872	1316	0.10%	0.012%
67	12.183	3447	3450	3451	rBV3	1727	965	0.07%	0.009%
68	12.228	3462	3464	3465	rBV2	1344	641	0.05%	0.006%
69	12.447	3529	3532	3533	rBV3	1282	734	0.05%	0.007%
70	12.556	3563	3566	3571	rVB6	1503	1161	0.08%	0.011%
71	12.598	3577	3579	3583	rBV5	1262	1039	0.08%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016718.D
 Acq On : 09 Jun 2020 15:39
 Operator : SY/MD
 Sample : L2901-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTT3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.656	3591	3597	3600	rBV5	1492	1641	0.12%	0.015%
73	12.720	3615	3617	3619	rBV3	1507	800	0.06%	0.007%
74	12.752	3625	3627	3630	rBV3	1383	891	0.06%	0.008%
75	12.794	3634	3640	3644	rBV5	1305	1510	0.11%	0.014%
76	12.817	3644	3647	3649	rBV4	1120	720	0.05%	0.007%
77	12.845	3653	3656	3658	rBV3	1166	756	0.05%	0.007%
78	12.977	3694	3697	3702	rBV7	1501	1481	0.11%	0.014%
79	13.125	3738	3743	3747	rVB7	2203	2072	0.15%	0.019%
80	13.173	3754	3758	3760	rBV4	1860	1243	0.09%	0.012%
81	13.222	3770	3773	3776	rBV3	1253	1033	0.07%	0.010%
82	13.447	3840	3843	3847	rBV5	1506	1266	0.09%	0.012%
83	13.534	3868	3870	3873	rBV3	1777	1238	0.09%	0.012%
84	13.585	3884	3886	3889	rBV4	1774	1370	0.10%	0.013%
85	13.665	3909	3911	3917	rVB6	1529	1427	0.10%	0.013%
86	13.723	3927	3929	3930	rBV2	1680	638	0.05%	0.006%
87	13.849	3965	3968	3969	rBV3	1627	893	0.06%	0.008%
88	13.903	3982	3985	3988	rBV4	1699	936	0.07%	0.009%
89	13.939	3994	3996	3998	rBV3	1422	667	0.05%	0.006%
90	14.009	4014	4018	4020	rBV5	1070	705	0.05%	0.007%
91	14.170	4065	4068	4071	rVB4	1469	856	0.06%	0.008%
92	14.312	4110	4112	4117	rBV5	1329	1282	0.09%	0.012%
93	14.366	4126	4129	4132	rBV3	1534	995	0.07%	0.009%
94	14.701	4231	4233	4237	rBV4	1445	1233	0.09%	0.011%
95	14.791	4259	4261	4265	rBV4	1469	901	0.07%	0.008%
96	15.096	4353	4356	4357	rBV3	1349	639	0.05%	0.006%
97	15.125	4361	4365	4367	rBV2	2256	1789	0.13%	0.017%
98	15.177	4378	4381	4383	rBV4	1623	704	0.05%	0.007%
99	15.482	4474	4476	4478	rBV3	1724	797	0.06%	0.007%
100	15.514	4484	4486	4489	rBV3	1410	1053	0.08%	0.010%


Sum of corrected areas: 10759797

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060920\
Data File : VV016718.D
Acq On : 09 Jun 2020 15:39
Operator : SY/MD
Sample : L2901-08
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTT3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

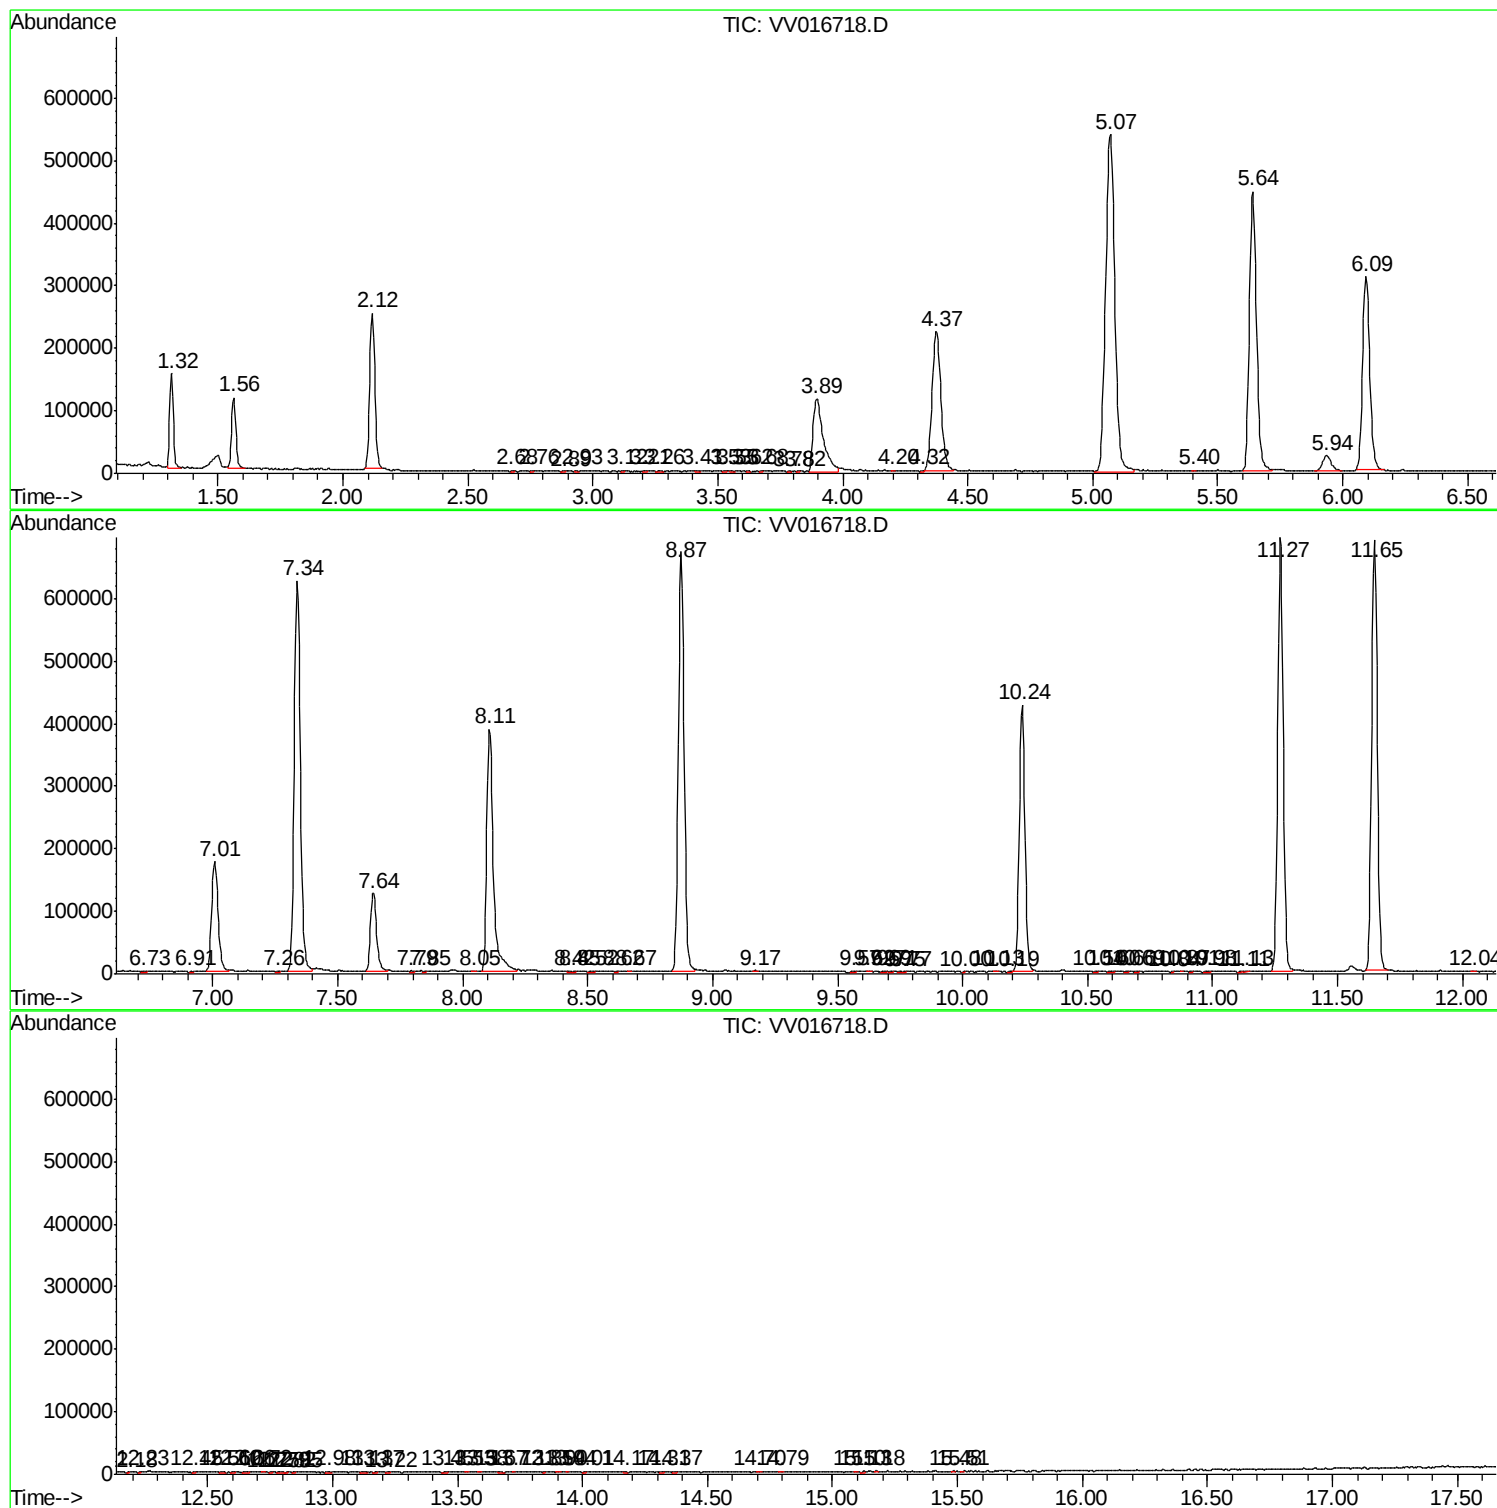

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016718.D
Acq On : 09 Jun 2020 15:39
Operator : SY/MD
Sample : L2901-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTT3

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016718.D
Acq On : 09 Jun 2020 15:39
Operator : SY/MD
Sample : L2901-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTT3

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc