

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016721.D
 Acq On : 09 Jun 2020 16:49
 Operator : SY/MD
 Sample : VV0609WBL02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK76

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	78	rVB	157612	154841	11.08%	1.423%
2	1.573	144	150	165	rVB	121613	140452	10.05%	1.291%
3	2.119	311	320	335	rVB	263169	386383	27.65%	3.550%
4	2.499	436	438	439	rBV2	1594	697	0.05%	0.006%
5	2.746	510	515	516	rBV5	1454	1246	0.09%	0.011%
6	2.946	572	577	581	rBV6	1322	1434	0.10%	0.013%
7	3.032	599	604	607	rBV6	1371	982	0.07%	0.009%
8	3.065	610	614	618	rBV6	2318	2036	0.15%	0.019%
9	3.119	627	631	633	rBV4	1860	1285	0.09%	0.012%
10	3.203	652	657	658	rBV5	1487	1100	0.08%	0.010%
11	3.264	672	676	679	rVV5	1764	1123	0.08%	0.010%
12	3.389	712	715	717	rBV4	1418	808	0.06%	0.007%
13	3.495	744	748	753	rBV7	2150	2276	0.16%	0.021%
14	3.704	809	813	817	rVB	13121	7525	0.54%	0.069%
15	3.849	856	858	862	rBV4	1540	1093	0.08%	0.010%
16	3.894	862	872	898	rBV	121092	320343	22.92%	2.944%
17	4.171	955	958	960	rBV4	1577	983	0.07%	0.009%
18	4.248	978	982	983	rBV3	1109	750	0.05%	0.007%
19	4.312	1000	1002	1005	rBV4	1794	1027	0.07%	0.009%
20	4.373	1005	1021	1052	rVV	226409	561598	40.19%	5.161%
21	4.621	1094	1098	1099	rBV3	1421	1196	0.09%	0.011%
22	4.782	1146	1148	1152	rBV5	1678	1030	0.07%	0.009%
23	4.884	1178	1180	1182	rBV3	1290	694	0.05%	0.006%
24	4.917	1188	1190	1193	rBV3	1073	717	0.05%	0.007%
25	5.071	1218	1238	1264	rVV2	542418	1397365	100.00%	12.840%
26	5.640	1402	1415	1443	rBV	439070	880405	63.00%	8.090%
27	5.929	1497	1505	1518	rVB7	12658	26890	1.92%	0.247%
28	6.093	1541	1556	1577	rBV	315439	646579	46.27%	5.941%
29	6.399	1646	1651	1656	rBV7	1420	1655	0.12%	0.015%
30	6.486	1675	1678	1679	rBV3	1416	964	0.07%	0.009%
31	6.910	1807	1810	1814	rBV4	1569	1145	0.08%	0.011%
32	6.945	1818	1821	1826	rBV6	2074	1325	0.09%	0.012%
33	7.007	1828	1840	1856	rBV2	180231	319446	22.86%	2.935%
34	7.338	1931	1943	1961	rVV	641924	1092265	78.17%	10.037%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016721.D
 Acq On : 09 Jun 2020 16:49
 Operator : SY/MD
 Sample : VV0609WBL02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK76

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	7.643	2025	2038	2053	rBV	127454	219042	15.68%	2.013%
36	7.807	2085	2089	2092	rBV5	1999	1614	0.12%	0.015%
37	7.965	2134	2138	2140	rBV4	1493	1177	0.08%	0.011%
38	7.994	2143	2147	2149	rBV5	2361	1759	0.13%	0.016%
39	8.106	2170	2182	2211	rBV	391461	716380	51.27%	6.583%
40	8.547	2317	2319	2321	rBV3	1827	868	0.06%	0.008%
41	8.605	2330	2337	2339	rBV7	1488	1333	0.10%	0.012%
42	8.707	2367	2369	2374	rVB6	1590	1238	0.09%	0.011%
43	8.733	2374	2377	2380	rBV5	1475	788	0.06%	0.007%
44	8.801	2394	2398	2401	rBV6	1258	1278	0.09%	0.012%
45	8.875	2409	2421	2440	rBV	665228	1071489	76.68%	9.846%
46	9.100	2488	2491	2493	rBV3	1532	929	0.07%	0.009%
47	9.232	2528	2532	2536	rVB6	1311	1084	0.08%	0.010%
48	9.283	2546	2548	2552	rBV4	2271	1286	0.09%	0.012%
49	9.482	2606	2610	2611	rBV4	1510	1234	0.09%	0.011%
50	9.691	2672	2675	2676	rBV3	1764	858	0.06%	0.008%
51	9.936	2747	2751	2752	rBV3	1731	1082	0.08%	0.010%
52	10.067	2790	2792	2797	rVB5	1343	1095	0.08%	0.010%
53	10.135	2811	2813	2815	rBV3	1421	881	0.06%	0.008%
54	10.238	2834	2845	2862	rVV	432024	668432	47.84%	6.142%
55	10.421	2899	2902	2907	rVB7	2051	1697	0.12%	0.016%
56	10.559	2941	2945	2948	rBV4	1898	2042	0.15%	0.019%
57	10.656	2972	2975	2977	rBV3	1127	813	0.06%	0.007%
58	10.707	2987	2991	2998	rBV8	1887	2407	0.17%	0.022%
59	10.801	3017	3020	3024	rVB5	1924	1448	0.10%	0.013%
60	10.823	3024	3027	3029	rBV4	2118	1113	0.08%	0.010%
61	10.923	3055	3058	3060	rBV4	1934	1338	0.10%	0.012%
62	11.019	3086	3088	3093	rVB5	1843	1440	0.10%	0.013%
63	11.045	3093	3096	3099	rBV5	1226	968	0.07%	0.009%
64	11.096	3109	3112	3114	rBV4	1438	1018	0.07%	0.009%
65	11.270	3156	3166	3187	rVB	683911	1053494	75.39%	9.681%
66	11.495	3232	3236	3243	rVB8	1902	2092	0.15%	0.019%
67	11.524	3243	3245	3251	rBV7	1663	1626	0.12%	0.015%
68	11.646	3272	3283	3302	rVB	697161	1087001	77.79%	9.988%
69	11.801	3327	3331	3333	rBV4	1353	1147	0.08%	0.011%
70	12.167	3442	3445	3447	rBV4	1051	761	0.05%	0.007%
71	12.270	3472	3477	3478	rBV5	1471	898	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016721.D
 Acq On : 09 Jun 2020 16:49
 Operator : SY/MD
 Sample : VV0609WBL02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK76

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.296	3482	3485	3487	rBV3	1337	803	0.06%	0.007%
73	12.321	3489	3493	3495	rBV5	1360	916	0.07%	0.008%
74	12.421	3516	3524	3526	rBV8	1403	1867	0.13%	0.017%
75	12.521	3554	3555	3560	rVB5	1361	812	0.06%	0.007%
76	12.669	3595	3601	3602	rBV5	6620	5826	0.42%	0.054%
77	12.762	3627	3630	3635	rVV5	1310	1460	0.10%	0.013%
78	12.784	3635	3637	3640	rVV3	1390	907	0.06%	0.008%
79	12.820	3644	3648	3650	rBV5	1022	832	0.06%	0.008%
80	12.887	3667	3669	3671	rBV2	1202	706	0.05%	0.006%
81	12.900	3671	3673	3677	rBV5	1331	997	0.07%	0.009%
82	13.289	3785	3794	3802	rBV6	8728	14068	1.01%	0.129%
83	13.415	3827	3833	3834	rVB5	880	712	0.05%	0.007%
84	13.530	3861	3869	3879	rVB2	11355	19350	1.38%	0.178%
85	13.890	3975	3981	3983	rBV6	2042	1688	0.12%	0.016%
86	13.935	3991	3995	3996	rBV4	1208	688	0.05%	0.006%
87	14.138	4056	4058	4062	rBV4	1134	808	0.06%	0.007%
88	14.190	4071	4074	4075	rBV3	1841	1188	0.09%	0.011%
89	14.238	4086	4089	4096	rVB9	2136	2311	0.17%	0.021%
90	14.273	4096	4100	4103	rBV4	1152	975	0.07%	0.009%
91	14.347	4120	4123	4126	rBV3	988	706	0.05%	0.006%
92	14.370	4126	4130	4132	rBV5	1181	956	0.07%	0.009%
93	14.418	4141	4145	4148	rBV5	1498	1321	0.09%	0.012%
94	14.440	4150	4152	4157	rVV5	1334	889	0.06%	0.008%
95	14.678	4224	4226	4230	rBV4	1260	919	0.07%	0.008%
96	14.971	4313	4317	4320	rVB5	1966	1499	0.11%	0.014%
97	15.148	4370	4372	4375	rBV3	1404	953	0.07%	0.009%
98	15.189	4383	4385	4387	rBV3	2039	1074	0.08%	0.010%
99	15.402	4448	4451	4453	rBV3	1390	925	0.07%	0.008%
100	15.836	4581	4586	4588	rBV4	1730	1619	0.12%	0.015%


Sum of corrected areas: 10882583

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060920\
Data File : VV016721.D
Acq On : 09 Jun 2020 16:49
Operator : SY/MD
Sample : VV0609WBL02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK76

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

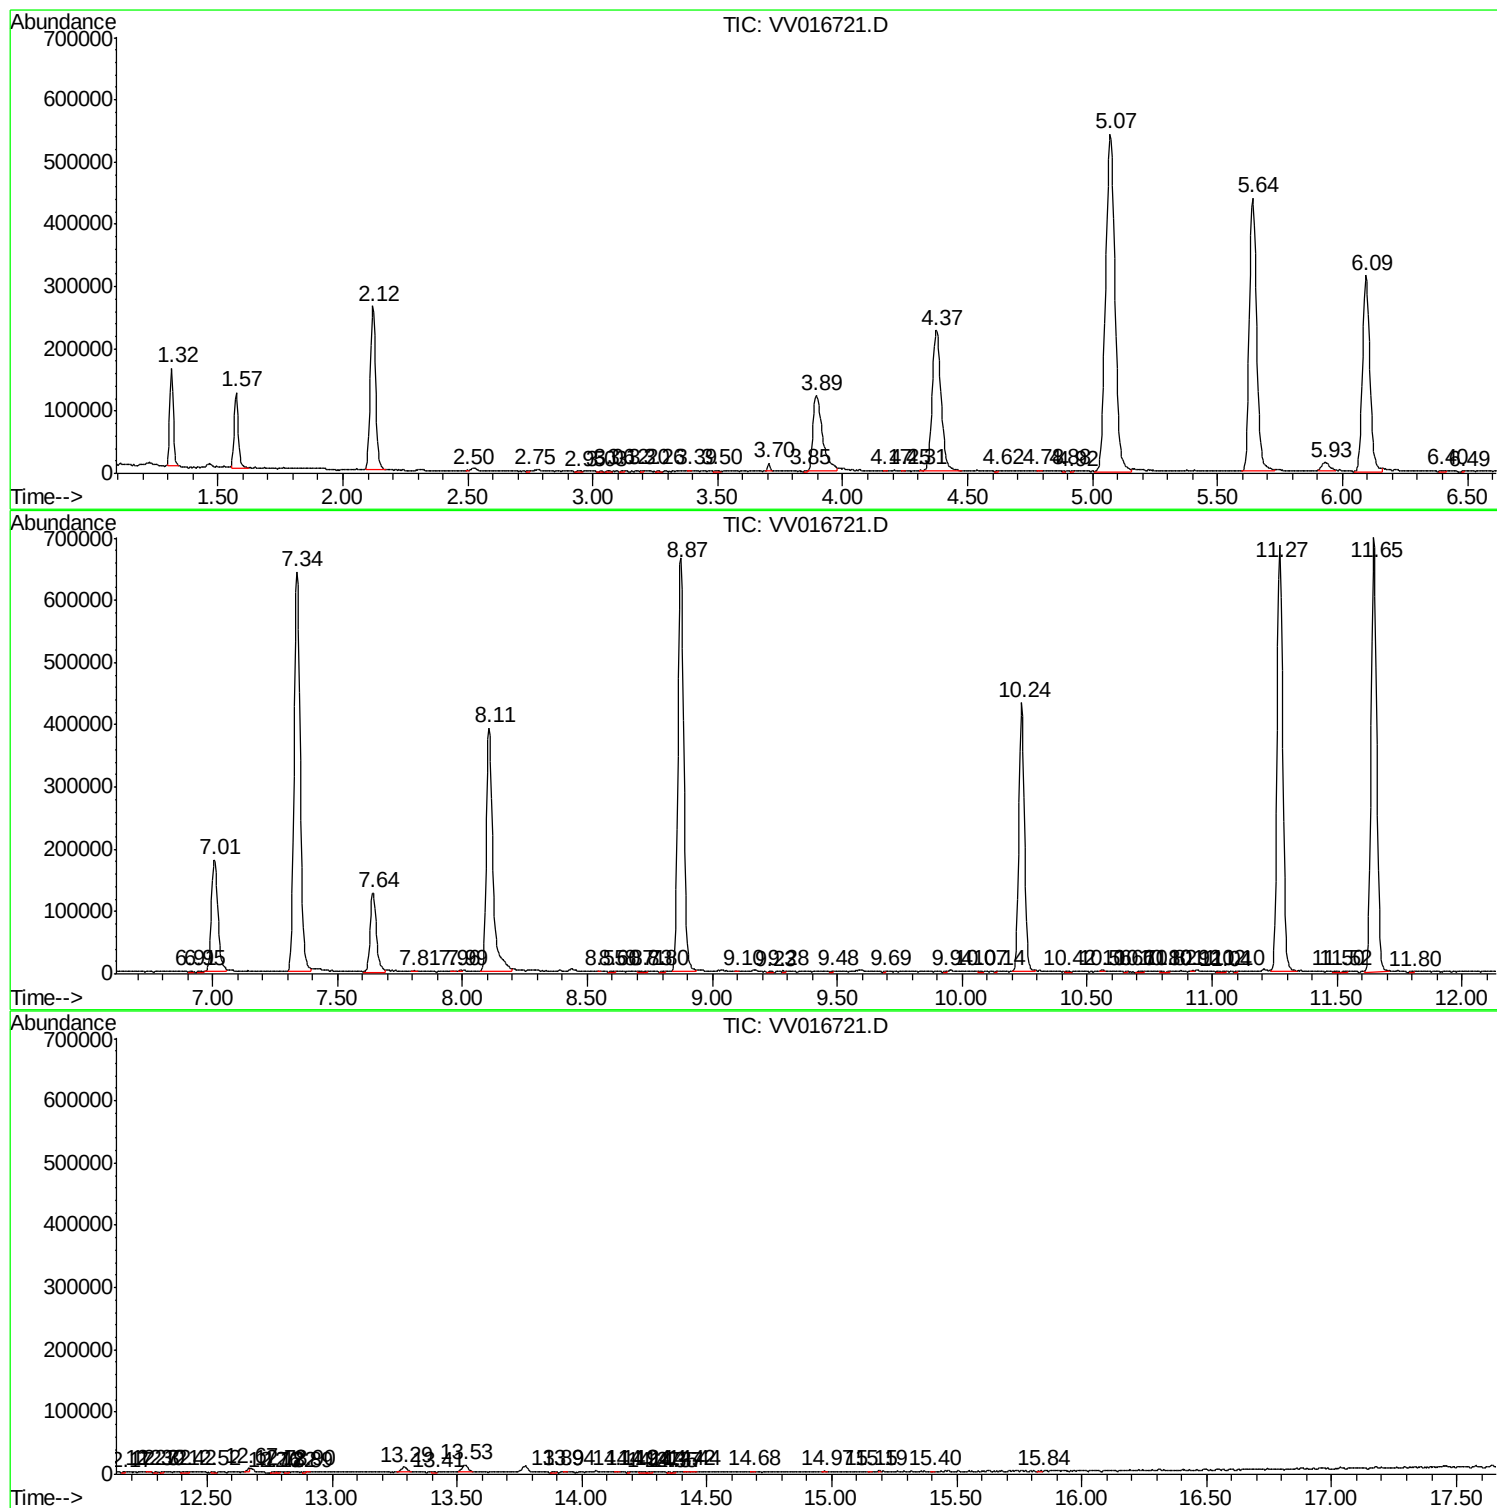

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016721.D
Acq On : 09 Jun 2020 16:49
Operator : SY/MD
Sample : VV0609WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK76

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV060920\
Data File : VV016721.D
Acq On : 09 Jun 2020 16:49
Operator : SY/MD
Sample : VV0609WBL02
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VBLK76

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc