

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016722.D
 Acq On : 09 Jun 2020 17:13
 Operator : SY/MD
 Sample : L2901-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTS6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	79	rVB	145243	139204	10.88%	1.423%
2	1.560	140	146	158	rVB	101033	118580	9.26%	1.212%
3	2.116	309	319	339	rVB	227778	339299	26.51%	3.469%
4	2.570	457	460	461	rBV3	1562	813	0.06%	0.008%
5	2.692	495	498	501	rBV4	1529	1114	0.09%	0.011%
6	2.708	501	503	505	rBV2	1393	774	0.06%	0.008%
7	2.836	540	543	545	rBV3	1409	723	0.06%	0.007%
8	2.914	564	567	574	rBV9	1805	1885	0.15%	0.019%
9	3.042	603	607	612	rBV7	2086	1605	0.13%	0.016%
10	3.103	623	626	631	rBV6	2486	1744	0.14%	0.018%
11	3.229	661	665	668	rBV5	1352	1302	0.10%	0.013%
12	3.258	672	674	677	rBV4	1384	726	0.06%	0.007%
13	3.283	680	682	686	rVB4	1580	701	0.05%	0.007%
14	3.309	686	690	694	rBV5	1350	1318	0.10%	0.013%
15	3.386	710	714	719	rBV6	1327	1310	0.10%	0.013%
16	3.444	728	732	734	rVB5	1054	697	0.05%	0.007%
17	3.473	738	741	744	rBV4	1556	902	0.07%	0.009%
18	3.512	750	753	754	rBV3	1532	1023	0.08%	0.010%
19	3.615	783	785	788	rBV4	1016	745	0.06%	0.008%
20	3.679	801	805	809	rVB6	1891	1643	0.13%	0.017%
21	3.894	862	872	902	rBV2	105330	277357	21.67%	2.836%
22	4.164	954	956	962	rBV7	1673	1453	0.11%	0.015%
23	4.373	1008	1021	1044	rVB	207170	497298	38.85%	5.085%
24	4.685	1116	1118	1121	rVB2	1518	779	0.06%	0.008%
25	4.704	1121	1124	1125	rBV2	1929	1169	0.09%	0.012%
26	4.814	1156	1158	1161	rVB3	1709	713	0.06%	0.007%
27	4.856	1166	1171	1174	rBV7	2144	1893	0.15%	0.019%
28	4.926	1190	1193	1197	rBV5	1236	984	0.08%	0.010%
29	4.991	1210	1213	1216	rBV5	1154	909	0.07%	0.009%
30	5.068	1221	1237	1268	rVV2	496839	1280009	100.00%	13.088%
31	5.251	1292	1294	1299	rBV5	2011	1764	0.14%	0.018%
32	5.322	1312	1316	1320	rBV5	1715	1759	0.14%	0.018%
33	5.547	1380	1386	1389	rBV7	1910	1813	0.14%	0.019%
34	5.640	1400	1415	1437	rBV	381181	770327	60.18%	7.876%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016722.D
 Acq On : 09 Jun 2020 17:13
 Operator : SY/MD
 Sample : L2901-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTS6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.093	1543	1556	1576	rBV	290136	583467	45.58%	5.966%
36	6.598	1711	1713	1717	rBV2	1607	1250	0.10%	0.013%
37	6.788	1769	1772	1775	rBV5	1370	700	0.05%	0.007%
38	7.007	1829	1840	1857	rVV	166488	294998	23.05%	3.016%
39	7.338	1931	1943	1962	rVV	578728	1001130	78.21%	10.236%
40	7.550	2006	2009	2014	rBV8	1729	1553	0.12%	0.016%
41	7.640	2027	2037	2055	rBV	118554	202501	15.82%	2.071%
42	7.753	2069	2072	2074	rBV4	1248	952	0.07%	0.010%
43	8.106	2172	2182	2211	rBV	361862	673483	52.62%	6.886%
44	8.437	2282	2285	2288	rVB5	1983	1206	0.09%	0.012%
45	8.534	2313	2315	2320	rVB6	1131	805	0.06%	0.008%
46	8.740	2374	2379	2382	rBV7	1161	1231	0.10%	0.013%
47	8.804	2394	2399	2401	rBV5	2574	2306	0.18%	0.024%
48	8.817	2401	2403	2406	rVB3	1893	1020	0.08%	0.010%
49	8.875	2406	2421	2442	rBV	578098	943752	73.73%	9.650%
50	9.081	2481	2485	2486	rBV4	1273	730	0.06%	0.007%
51	9.434	2592	2595	2598	rBV5	1137	847	0.07%	0.009%
52	9.495	2609	2614	2619	rBV8	1649	2004	0.16%	0.020%
53	9.518	2619	2621	2624	rVV3	974	707	0.06%	0.007%
54	9.566	2634	2636	2640	rBV4	1362	1284	0.10%	0.013%
55	9.646	2659	2661	2665	rBV5	1414	1278	0.10%	0.013%
56	9.823	2713	2716	2721	rBV6	1484	1113	0.09%	0.011%
57	9.926	2745	2748	2751	rBV4	1540	1094	0.09%	0.011%
58	10.084	2795	2797	2801	rBV5	1757	1229	0.10%	0.013%
59	10.238	2830	2845	2860	rBV	412935	640422	50.03%	6.548%
60	10.363	2881	2884	2886	rBV3	1249	873	0.07%	0.009%
61	10.521	2927	2933	2934	rBV5	1452	1457	0.11%	0.015%
62	10.720	2992	2995	2999	rBV4	1103	914	0.07%	0.009%
63	10.769	3006	3010	3013	rVB4	1598	1201	0.09%	0.012%
64	10.884	3042	3046	3050	rBV6	1828	1530	0.12%	0.016%
65	10.923	3053	3058	3059	rBV4	2169	1513	0.12%	0.015%
66	11.029	3087	3091	3093	rBV4	2012	1476	0.12%	0.015%
67	11.177	3135	3137	3139	rBV3	2348	1123	0.09%	0.011%
68	11.270	3155	3166	3182	rBV	589325	912637	71.30%	9.332%
69	11.386	3199	3202	3205	rBV4	1238	924	0.07%	0.009%
70	11.479	3227	3231	3236	rVB8	1388	1361	0.11%	0.014%
71	11.505	3236	3239	3242	rBV4	843	719	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016722.D
 Acq On : 09 Jun 2020 17:13
 Operator : SY/MD
 Sample : L2901-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTS6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.550	3246	3253	3255	rBV6	3739	3681	0.29%	0.038%
73	11.646	3272	3283	3299	rBV	632958	1003979	78.44%	10.266%
74	11.862	3349	3350	3355	rVB4	1461	823	0.06%	0.008%
75	11.884	3355	3357	3360	rVB4	1701	1064	0.08%	0.011%
76	12.032	3400	3403	3407	rBV3	1857	1388	0.11%	0.014%
77	12.376	3506	3510	3512	rBV3	1882	1321	0.10%	0.014%
78	12.408	3516	3520	3522	rBV4	1139	899	0.07%	0.009%
79	12.444	3528	3531	3533	rBV4	1247	909	0.07%	0.009%
80	12.566	3566	3569	3571	rBV3	1475	962	0.08%	0.010%
81	12.633	3585	3590	3593	rBV6	1368	1245	0.10%	0.013%
82	12.752	3625	3627	3632	rVB5	1500	888	0.07%	0.009%
83	12.942	3683	3686	3691	rBV7	961	739	0.06%	0.008%
84	13.138	3743	3747	3753	rVB8	1608	1551	0.12%	0.016%
85	13.299	3791	3797	3799	rBV5	2347	2443	0.19%	0.025%
86	13.592	3885	3888	3890	rBV4	1255	952	0.07%	0.010%
87	13.621	3893	3897	3898	rBV3	1962	1464	0.11%	0.015%
88	13.662	3902	3910	3912	rBV8	1380	1617	0.13%	0.017%
89	13.749	3934	3937	3938	rBV3	1424	785	0.06%	0.008%
90	13.855	3965	3970	3973	rBV5	1358	1423	0.11%	0.015%
91	13.903	3981	3985	3988	rBV4	1326	1141	0.09%	0.012%
92	14.196	4073	4076	4079	rBV4	1180	979	0.08%	0.010%
93	14.257	4091	4095	4096	rBV3	1161	854	0.07%	0.009%
94	14.370	4128	4130	4135	rBV5	1495	1102	0.09%	0.011%
95	14.389	4135	4136	4140	rBV4	1345	1001	0.08%	0.010%
96	14.485	4162	4166	4168	rVB4	1460	901	0.07%	0.009%
97	14.592	4196	4199	4200	rBV3	1847	1037	0.08%	0.011%
98	14.907	4295	4297	4303	rBV6	2345	1579	0.12%	0.016%
99	15.292	4414	4417	4420	rBV5	1785	1163	0.09%	0.012%
100	15.903	4605	4607	4608	rBV2	2157	1061	0.08%	0.011%


Sum of corrected areas: 9780076

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060920\
Data File : VV016722.D
Acq On : 09 Jun 2020 17:13
Operator : SY/MD
Sample : L2901-05
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTS6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

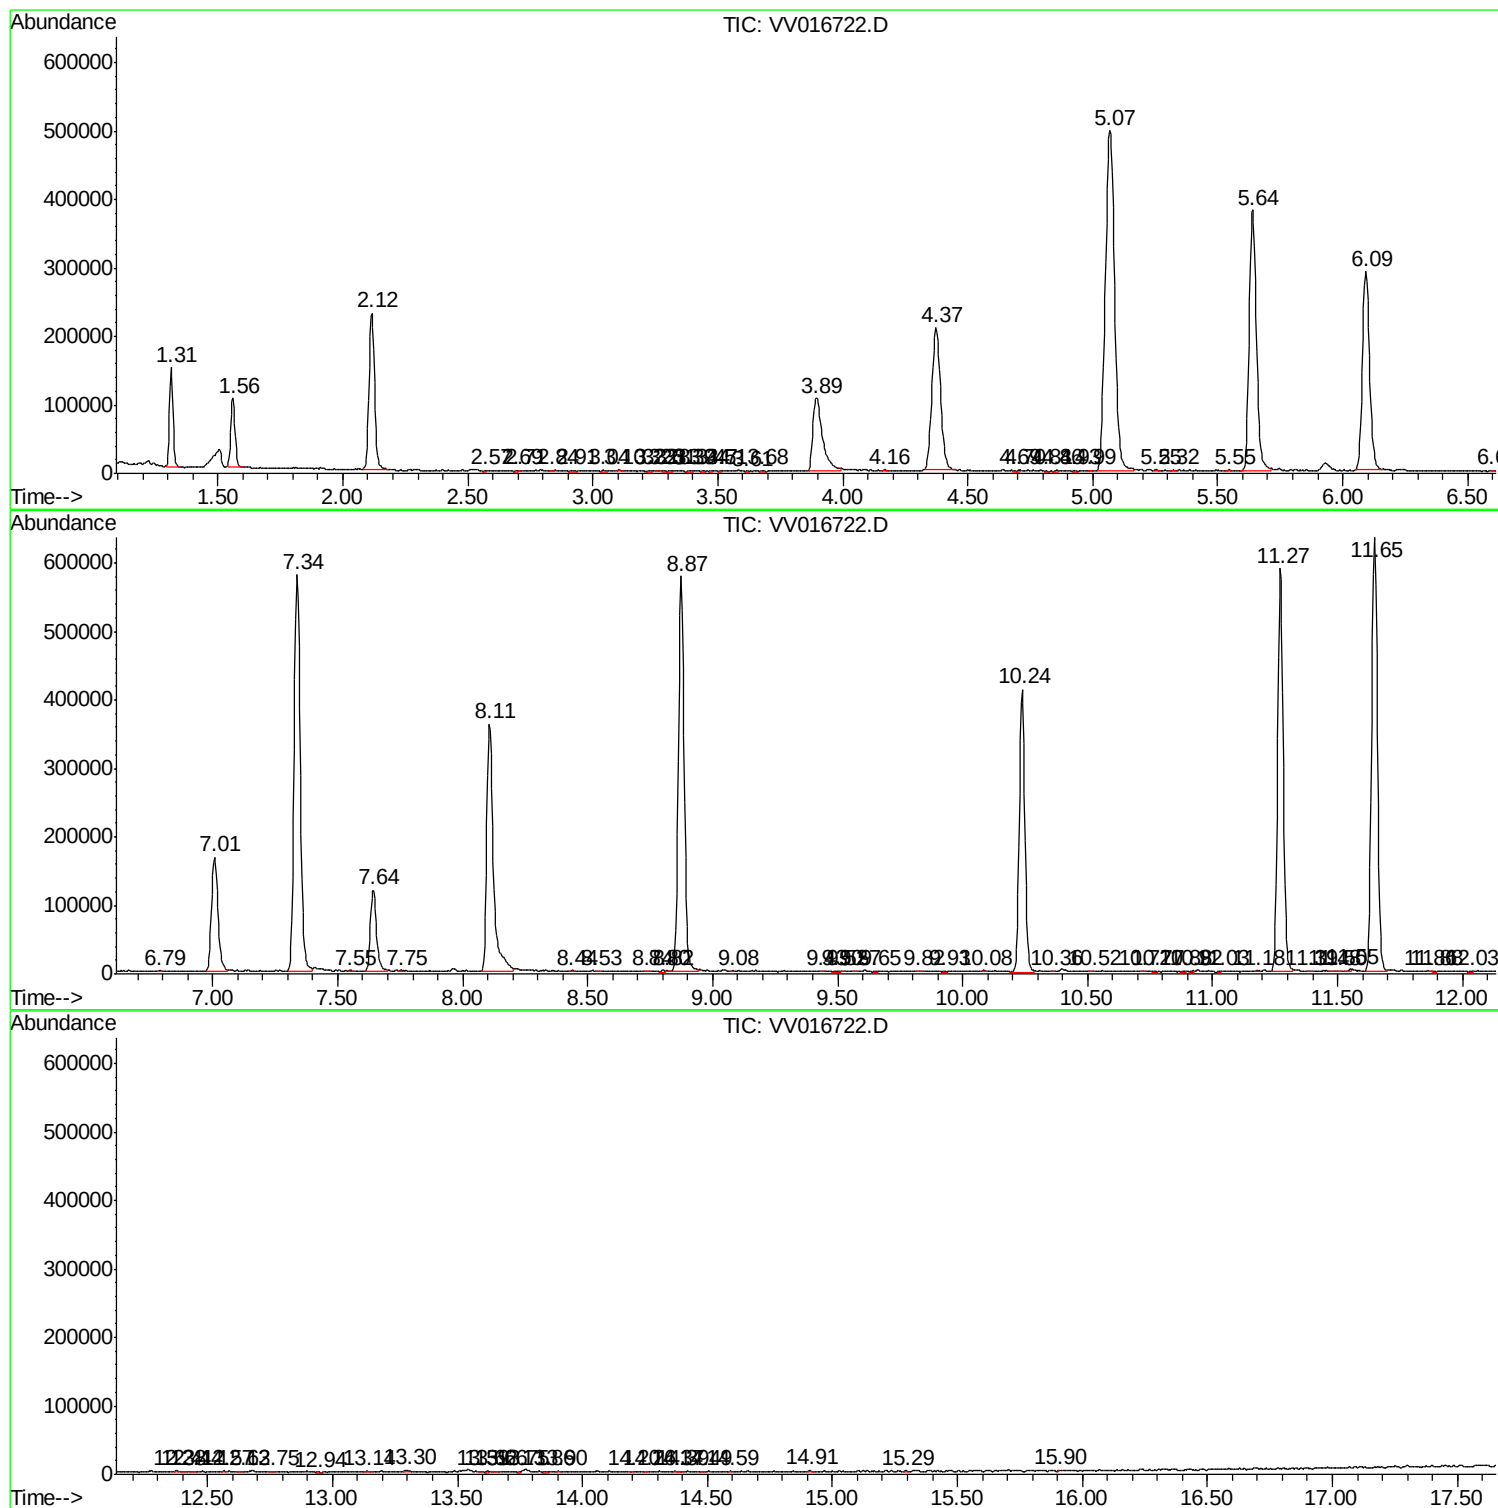

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV060920\
Data File : VV016722.D
Acq On : 09 Jun 2020 17:13
Operator : SY/MD
Sample : L2901-05
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
ETTS6

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016722.D
Acq On : 09 Jun 2020 17:13
Operator : SY/MD
Sample : L2901-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTS6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc