

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016723.D
 Acq On : 09 Jun 2020 17:37
 Operator : SY/MD
 Sample : L2901-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTX6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	64	69	82	rVB	137818	142516	11.31%	1.460%
2	1.556	139	145	160	rVB	101693	122011	9.68%	1.250%
3	2.116	309	319	332	rBV	221893	329895	26.18%	3.379%
4	2.470	426	429	430	rBV3	1193	595	0.05%	0.006%
5	2.569	455	460	462	rBV5	1218	1267	0.10%	0.013%
6	2.926	570	571	575	rVB4	1174	690	0.05%	0.007%
7	3.045	606	608	609	rBV2	1475	522	0.04%	0.005%
8	3.261	670	675	678	rBV4	1655	1695	0.13%	0.017%
9	3.351	702	703	707	rVB4	1278	713	0.06%	0.007%
10	3.409	719	721	727	rVB7	1700	1456	0.12%	0.015%
11	3.454	733	735	739	rBV3	1090	893	0.07%	0.009%
12	3.566	768	770	773	rBV3	790	529	0.04%	0.005%
13	3.582	773	775	782	rVB7	2303	1708	0.14%	0.017%
14	3.624	785	788	792	rVB4	1608	1167	0.09%	0.012%
15	3.653	794	797	802	rBV7	2134	1481	0.12%	0.015%
16	3.791	835	840	843	rBV6	1390	1273	0.10%	0.013%
17	3.894	862	872	897	rBV	106929	280425	22.26%	2.872%
18	4.286	992	994	998	rBV6	1568	905	0.07%	0.009%
19	4.322	1003	1005	1006	rBV2	1267	481	0.04%	0.005%
20	4.373	1006	1021	1042	rVV	207791	507951	40.32%	5.203%
21	4.752	1135	1139	1142	rBV6	1266	1311	0.10%	0.013%
22	4.772	1142	1145	1146	rBV3	1307	679	0.05%	0.007%
23	4.839	1163	1166	1170	rVB5	1427	832	0.07%	0.009%
24	4.945	1197	1199	1202	rBV4	1099	559	0.04%	0.006%
25	5.068	1221	1237	1264	rBV2	492013	1259928	100.00%	12.905%
26	5.547	1383	1386	1388	rBV4	1067	653	0.05%	0.007%
27	5.640	1402	1415	1437	rBV	385326	774569	61.48%	7.934%
28	5.929	1493	1505	1521	rBV9	12577	29221	2.32%	0.299%
29	6.093	1543	1556	1574	rBV	288842	580690	46.09%	5.948%
30	6.434	1660	1662	1664	rBV3	1677	879	0.07%	0.009%
31	6.576	1704	1706	1707	rBV2	1639	626	0.05%	0.006%
32	6.814	1776	1780	1782	rBV4	1780	1314	0.10%	0.013%
33	6.849	1789	1791	1793	rBV3	1331	683	0.05%	0.007%
34	6.913	1808	1811	1812	rBV3	1498	910	0.07%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016723.D
 Acq On : 09 Jun 2020 17:37
 Operator : SY/MD
 Sample : L2901-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTX6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.942	1818	1820	1823	rVB4	934	524	0.04%	0.005%
36	7.006	1830	1840	1859	rBV	168906	293098	23.26%	3.002%
37	7.174	1888	1892	1896	rBV8	1253	1017	0.08%	0.010%
38	7.338	1930	1943	1959	rBV	571382	979947	77.78%	10.037%
39	7.534	2002	2004	2005	rBV2	1362	649	0.05%	0.007%
40	7.640	2028	2037	2051	rBV	117584	195571	15.52%	2.003%
41	7.772	2076	2078	2079	rBV2	1670	764	0.06%	0.008%
42	8.006	2149	2151	2153	rVB2	2681	1096	0.09%	0.011%
43	8.109	2173	2183	2199	rBV	351683	644495	51.15%	6.601%
44	8.588	2328	2332	2335	rBV5	1581	1616	0.13%	0.017%
45	8.788	2392	2394	2397	rBV4	1214	780	0.06%	0.008%
46	8.875	2410	2421	2446	rVB	587768	947537	75.21%	9.705%
47	9.161	2505	2510	2514	rBV8	2320	2538	0.20%	0.026%
48	9.273	2543	2545	2549	rVB4	2179	1324	0.11%	0.014%
49	9.315	2557	2558	2560	rBV2	927	514	0.04%	0.005%
50	9.685	2669	2673	2675	rBV4	1136	1064	0.08%	0.011%
51	9.714	2680	2682	2684	rBV3	1174	608	0.05%	0.006%
52	9.762	2695	2697	2703	rVB7	1488	1220	0.10%	0.012%
53	10.064	2789	2791	2796	rBV4	1348	1165	0.09%	0.012%
54	10.161	2819	2821	2823	rBV3	1827	1037	0.08%	0.011%
55	10.196	2828	2832	2833	rBV3	1452	1040	0.08%	0.011%
56	10.238	2833	2845	2861	rVV	412617	639768	50.78%	6.553%
57	10.363	2880	2884	2888	rVB4	2180	1759	0.14%	0.018%
58	10.402	2890	2896	2905	rVB8	4056	6664	0.53%	0.068%
59	10.456	2909	2913	2916	rBV4	1789	1599	0.13%	0.016%
60	10.518	2929	2932	2934	rBV3	1158	818	0.06%	0.008%
61	10.640	2967	2970	2973	rBV5	1123	878	0.07%	0.009%
62	10.688	2982	2985	2991	rVB8	1964	1770	0.14%	0.018%
63	10.717	2991	2994	2998	rVB5	1760	1415	0.11%	0.014%
64	10.820	3024	3026	3029	rBV3	1038	796	0.06%	0.008%
65	10.984	3075	3077	3079	rBV3	1196	798	0.06%	0.008%
66	11.270	3155	3166	3187	rBV	596766	923697	73.31%	9.461%
67	11.447	3219	3221	3225	rVB5	1397	754	0.06%	0.008%
68	11.479	3227	3231	3233	rBV5	1479	1009	0.08%	0.010%
69	11.514	3240	3242	3247	rBV6	1670	1421	0.11%	0.015%
70	11.646	3270	3283	3301	rBV	645344	1023397	81.23%	10.482%
71	12.013	3393	3397	3399	rBV4	1315	896	0.07%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016723.D
 Acq On : 09 Jun 2020 17:37
 Operator : SY/MD
 Sample : L2901-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTX6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.096	3418	3423	3427	rBV6	2021	2320	0.18%	0.024%
73	12.183	3448	3450	3455	rVB5	1371	1074	0.09%	0.011%
74	12.215	3455	3460	3463	rBV5	1737	1345	0.11%	0.014%
75	12.231	3463	3465	3466	rBV2	910	460	0.04%	0.005%
76	12.325	3489	3494	3495	rBV3	1424	1282	0.10%	0.013%
77	12.431	3524	3527	3529	rVB4	1396	710	0.06%	0.007%
78	12.444	3529	3531	3534	rBV3	1142	501	0.04%	0.005%
79	12.521	3552	3555	3558	rBV6	1525	1059	0.08%	0.011%
80	12.546	3558	3563	3566	rVB6	1623	1481	0.12%	0.015%
81	12.640	3589	3592	3595	rBV4	1720	1119	0.09%	0.011%
82	12.662	3595	3599	3601	rBV5	1324	1219	0.10%	0.012%
83	12.726	3616	3619	3622	rBV4	1556	932	0.07%	0.010%
84	12.952	3687	3689	3691	rBV3	1162	764	0.06%	0.008%
85	13.025	3707	3712	3715	rVB7	1488	1175	0.09%	0.012%
86	13.042	3715	3717	3718	rBV2	1375	610	0.05%	0.006%
87	13.070	3723	3726	3729	rVB4	1767	1047	0.08%	0.011%
88	13.096	3731	3734	3736	rBV2	1615	911	0.07%	0.009%
89	13.109	3736	3738	3742	rBV4	1325	1136	0.09%	0.012%
90	13.196	3764	3765	3768	rBV2	1191	664	0.05%	0.007%
91	13.267	3784	3787	3788	rBV3	1017	548	0.04%	0.006%
92	13.443	3840	3842	3845	rBV3	1407	947	0.08%	0.010%
93	13.485	3853	3855	3857	rBV3	991	522	0.04%	0.005%
94	13.633	3899	3901	3904	rVB3	1088	497	0.04%	0.005%
95	14.096	4043	4045	4048	rBV3	1128	696	0.06%	0.007%
96	14.347	4120	4123	4127	rBV4	1619	1692	0.13%	0.017%
97	14.460	4154	4158	4161	rBV4	751	743	0.06%	0.008%
98	14.511	4171	4174	4176	rBV4	1325	639	0.05%	0.007%
99	14.723	4238	4240	4241	rBV2	1525	506	0.04%	0.005%
100	14.832	4272	4274	4276	rBV3	1197	556	0.04%	0.006%


Sum of corrected areas: 9763225

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060920\
Data File : VV016723.D
Acq On : 09 Jun 2020 17:37
Operator : SY/MD
Sample : L2901-11
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTX6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

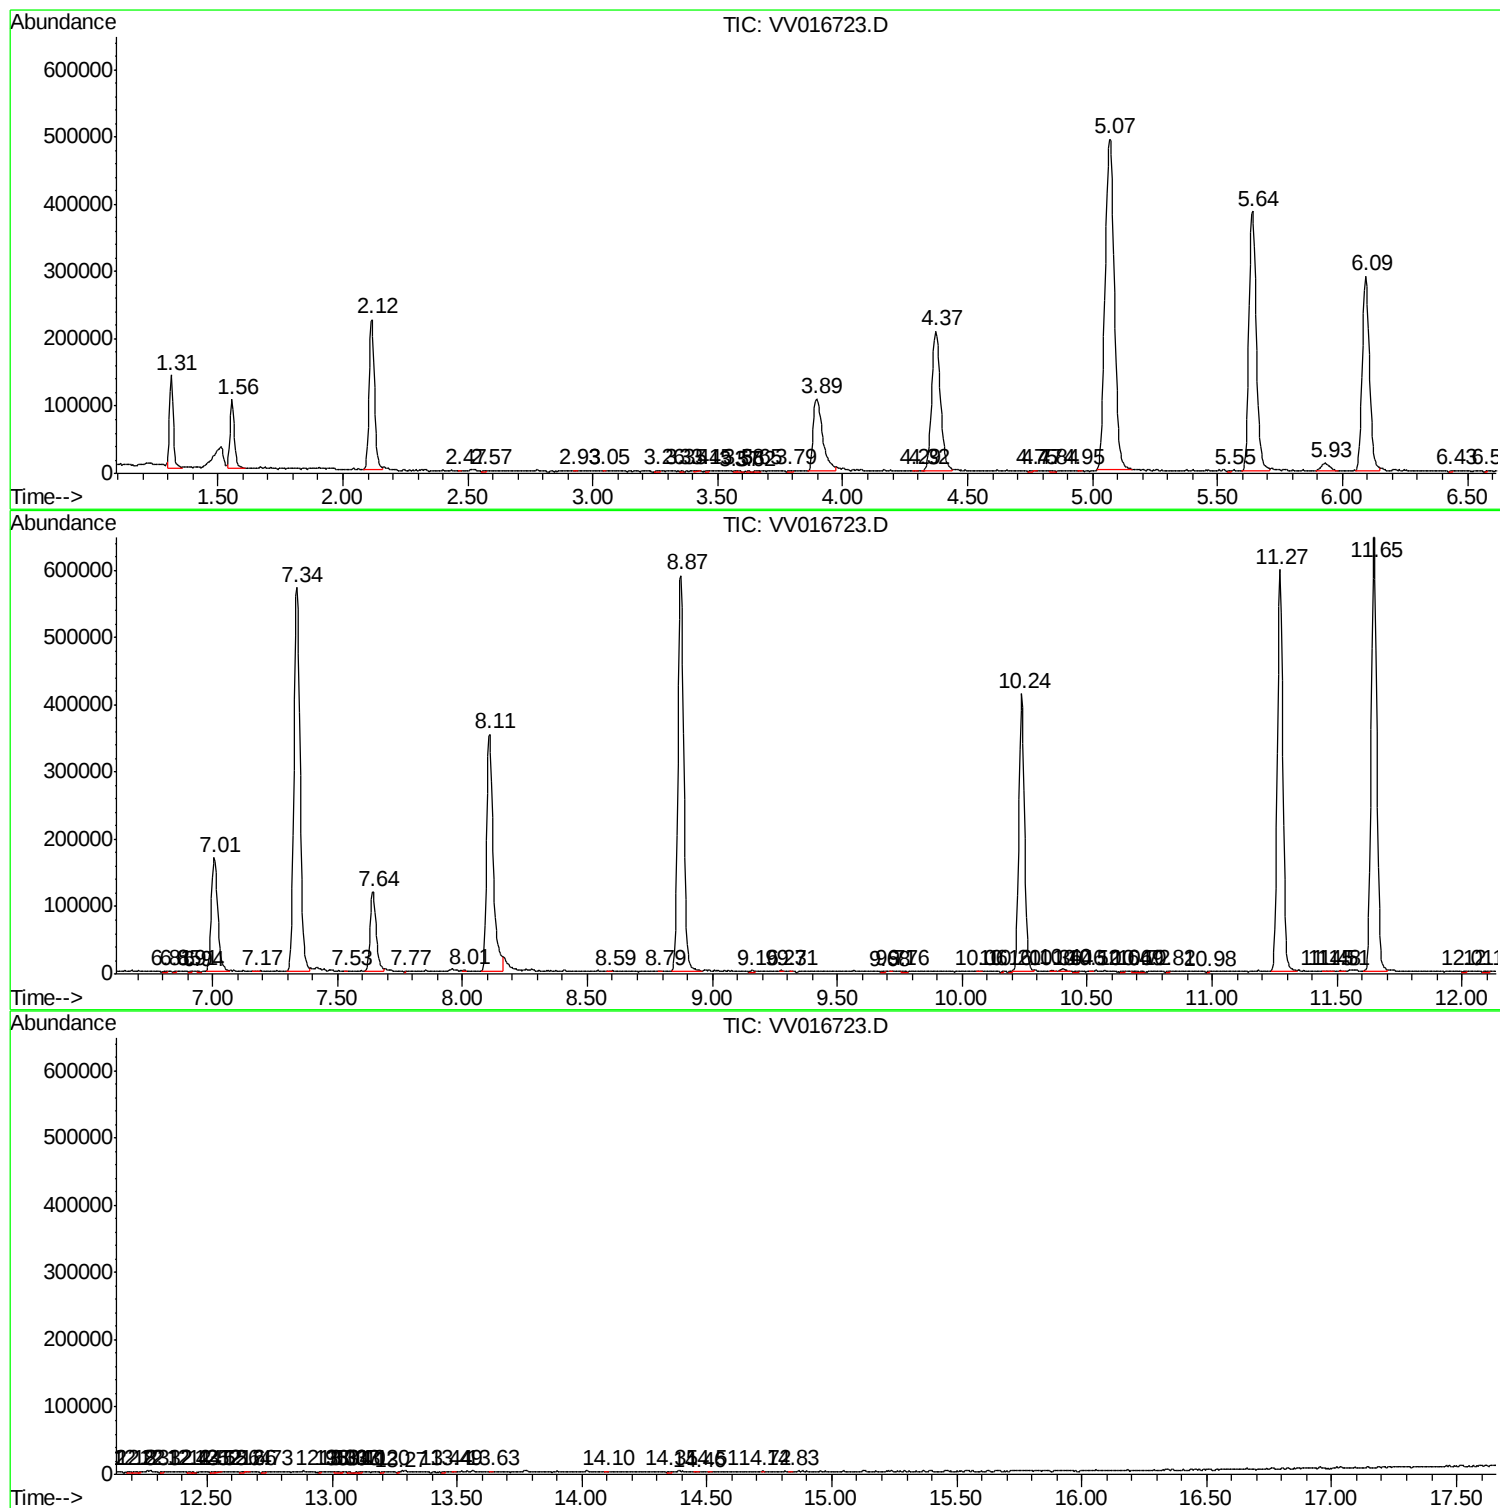

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016723.D
Acq On : 09 Jun 2020 17:37
Operator : SY/MD
Sample : L2901-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTX6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016723.D
Acq On : 09 Jun 2020 17:37
Operator : SY/MD
Sample : L2901-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTX6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc