

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016724.D
 Acq On : 09 Jun 2020 18:01
 Operator : SY/MD
 Sample : L2901-12
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTY5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	63	70	83	rBV2	681907	708875	7.16%	2.880%
2	1.557	139	145	159	rVB	100191	120279	1.22%	0.489%
3	2.119	310	320	343	rVB2	276319	468320	4.73%	1.903%
4	2.457	423	425	429	rBV5	1644	1019	0.01%	0.004%
5	2.775	518	524	538	rVB2	25570	44752	0.45%	0.182%
6	2.894	559	561	564	rBV3	2023	1460	0.01%	0.006%
7	2.959	578	581	585	rVV5	1670	1243	0.01%	0.005%
8	3.061	609	613	615	rBV4	1734	1276	0.01%	0.005%
9	3.113	627	629	633	rVB4	1872	887	0.01%	0.004%
10	3.168	642	646	647	rBV4	1363	963	0.01%	0.004%
11	3.200	653	656	657	rBV3	1811	1002	0.01%	0.004%
12	3.380	708	712	713	rBV3	1735	1287	0.01%	0.005%
13	3.402	716	719	723	rVV4	1332	894	0.01%	0.004%
14	3.463	734	738	740	rBV3	1552	1059	0.01%	0.004%
15	3.528	756	758	760	rVV3	1394	731	0.01%	0.003%
16	3.541	760	762	769	rVB7	1536	1451	0.01%	0.006%
17	3.614	782	785	788	rBV5	2049	1309	0.01%	0.005%
18	3.631	788	790	793	rBV3	1441	1017	0.01%	0.004%
19	3.692	806	809	813	rBV6	1912	1187	0.01%	0.005%
20	3.933	861	884	925	rBV	4010933	9895779	100.00%	40.206%
21	4.373	1005	1021	1043	rBV	209767	518953	5.24%	2.108%
22	4.563	1078	1080	1082	rBV2	1772	859	0.01%	0.003%
23	4.579	1082	1085	1088	rBV5	1953	1185	0.01%	0.005%
24	4.795	1148	1152	1155	rVB5	1318	922	0.01%	0.004%
25	4.856	1167	1171	1177	rBV9	1484	1711	0.02%	0.007%
26	4.981	1207	1210	1213	rBV5	1286	779	0.01%	0.003%
27	5.068	1220	1237	1264	rVV2	494337	1269625	12.83%	5.158%
28	5.251	1290	1294	1297	rBV6	1592	1398	0.01%	0.006%
29	5.354	1323	1326	1328	rBV4	1745	1073	0.01%	0.004%
30	5.418	1344	1346	1350	rBV3	1572	871	0.01%	0.004%
31	5.640	1402	1415	1440	rBV	429638	859035	8.68%	3.490%
32	5.936	1491	1507	1533	rBV	2118703	4044948	40.88%	16.434%
33	6.093	1545	1556	1581	rVB	291278	588420	5.95%	2.391%
34	6.634	1720	1724	1726	rBV4	2019	1607	0.02%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016724.D
 Acq On : 09 Jun 2020 18:01
 Operator : SY/MD
 Sample : L2901-12
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTY5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.894	1800	1805	1806	rBV5	1408	1155	0.01%	0.005%
36	7.007	1826	1840	1859	rBV	169641	305263	3.08%	1.240%
37	7.338	1931	1943	1964	rVV	572304	990655	10.01%	4.025%
38	7.640	2027	2037	2051	rBV	118860	198741	2.01%	0.807%
39	8.048	2162	2164	2168	rVB4	1444	956	0.01%	0.004%
40	8.106	2168	2182	2218	rBV	378400	713000	7.21%	2.897%
41	8.454	2286	2290	2292	rBV4	1762	1127	0.01%	0.005%
42	8.511	2303	2308	2311	rBV6	2568	2966	0.03%	0.012%
43	8.540	2314	2317	2319	rBV3	1317	1001	0.01%	0.004%
44	8.765	2385	2387	2391	rBV3	1283	899	0.01%	0.004%
45	8.823	2402	2405	2408	rBV5	1758	1264	0.01%	0.005%
46	8.875	2408	2421	2446	rVV	648963	1057762	10.69%	4.298%
47	9.074	2480	2483	2485	rBV3	1678	1140	0.01%	0.005%
48	9.158	2507	2509	2510	rBV	1763	653	0.01%	0.003%
49	9.315	2552	2558	2561	rBV7	1390	1472	0.01%	0.006%
50	9.363	2569	2573	2577	rVB6	2051	1462	0.01%	0.006%
51	9.447	2596	2599	2600	rBV3	1374	649	0.01%	0.003%
52	9.553	2628	2632	2633	rBV3	1009	686	0.01%	0.003%
53	9.563	2633	2635	2639	rVV5	1659	1112	0.01%	0.005%
54	9.659	2663	2665	2668	rBV4	1818	1121	0.01%	0.005%
55	9.884	2733	2735	2738	rBV4	1250	697	0.01%	0.003%
56	10.032	2778	2781	2787	rBV8	1503	1505	0.02%	0.006%
57	10.113	2803	2806	2809	rBV4	1104	1123	0.01%	0.005%
58	10.238	2831	2845	2862	rBV	417232	657226	6.64%	2.670%
59	10.592	2950	2955	2957	rBV4	1962	1434	0.01%	0.006%
60	10.621	2962	2964	2967	rVV3	977	665	0.01%	0.003%
61	10.855	3033	3037	3038	rBV4	1247	694	0.01%	0.003%
62	11.000	3079	3082	3085	rBV4	1554	1177	0.01%	0.005%
63	11.035	3090	3093	3098	rVB6	1472	1312	0.01%	0.005%
64	11.180	3134	3138	3139	rBV4	1395	739	0.01%	0.003%
65	11.270	3154	3166	3184	rBV	685697	1039583	10.51%	4.224%
66	11.495	3233	3236	3239	rBV4	1187	684	0.01%	0.003%
67	11.514	3239	3242	3245	rVB5	1365	761	0.01%	0.003%
68	11.646	3272	3283	3298	rBV	667105	1036361	10.47%	4.211%
69	11.865	3349	3351	3354	rVB4	1090	669	0.01%	0.003%
70	11.881	3354	3356	3357	rBV2	1665	856	0.01%	0.003%
71	12.267	3472	3476	3480	rBV5	2179	1986	0.02%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016724.D
 Acq On : 09 Jun 2020 18:01
 Operator : SY/MD
 Sample : L2901-12
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTY5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.376	3507	3510	3515	rVB7	1712	1299	0.01%	0.005%
73	12.415	3519	3522	3530	rBV8	1884	2352	0.02%	0.010%
74	12.453	3530	3534	3538	rBV7	1792	1709	0.02%	0.007%
75	12.563	3563	3568	3570	rBV5	1834	1165	0.01%	0.005%
76	12.601	3576	3580	3586	rVB8	1859	1859	0.02%	0.008%
77	12.630	3586	3589	3590	rBV3	1091	706	0.01%	0.003%
78	12.682	3601	3605	3610	rBV6	1454	1330	0.01%	0.005%
79	12.733	3619	3621	3624	rBV4	1440	849	0.01%	0.003%
80	12.781	3632	3636	3637	rBV4	1728	970	0.01%	0.004%
81	12.810	3642	3645	3649	rBV6	2094	1731	0.02%	0.007%
82	12.855	3656	3659	3663	rBV5	1653	1528	0.02%	0.006%
83	12.910	3673	3676	3678	rBV4	1128	659	0.01%	0.003%
84	13.116	3738	3740	3744	rBV4	1330	748	0.01%	0.003%
85	13.328	3804	3806	3810	rVB4	1346	816	0.01%	0.003%
86	13.360	3814	3816	3818	rBV3	1069	666	0.01%	0.003%
87	13.537	3867	3871	3872	rBV3	2141	1624	0.02%	0.007%
88	13.601	3887	3891	3892	rBV4	1367	1029	0.01%	0.004%
89	13.704	3921	3923	3925	rBV2	1629	1028	0.01%	0.004%
90	13.833	3959	3963	3965	rBV3	1821	1328	0.01%	0.005%
91	13.871	3972	3975	3983	rBV7	1549	1620	0.02%	0.007%
92	13.903	3983	3985	3987	rBV2	1363	668	0.01%	0.003%
93	14.193	4073	4075	4077	rBV3	1457	870	0.01%	0.004%
94	14.244	4089	4091	4094	rBV4	1833	1393	0.01%	0.006%
95	14.328	4114	4117	4119	rBV3	1472	1046	0.01%	0.004%
96	14.386	4133	4135	4137	rBV2	1348	851	0.01%	0.003%
97	14.823	4268	4271	4275	rBV4	1950	1472	0.01%	0.006%
98	14.913	4294	4299	4306	rBV9	1359	1806	0.02%	0.007%
99	15.386	4444	4446	4449	rBV3	1650	1218	0.01%	0.005%
100	15.614	4513	4517	4519	rBV4	1899	1682	0.02%	0.007%


Sum of corrected areas: 24612754

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060920\
Data File : VV016724.D
Acq On : 09 Jun 2020 18:01
Operator : SY/MD
Sample : L2901-12
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTY5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

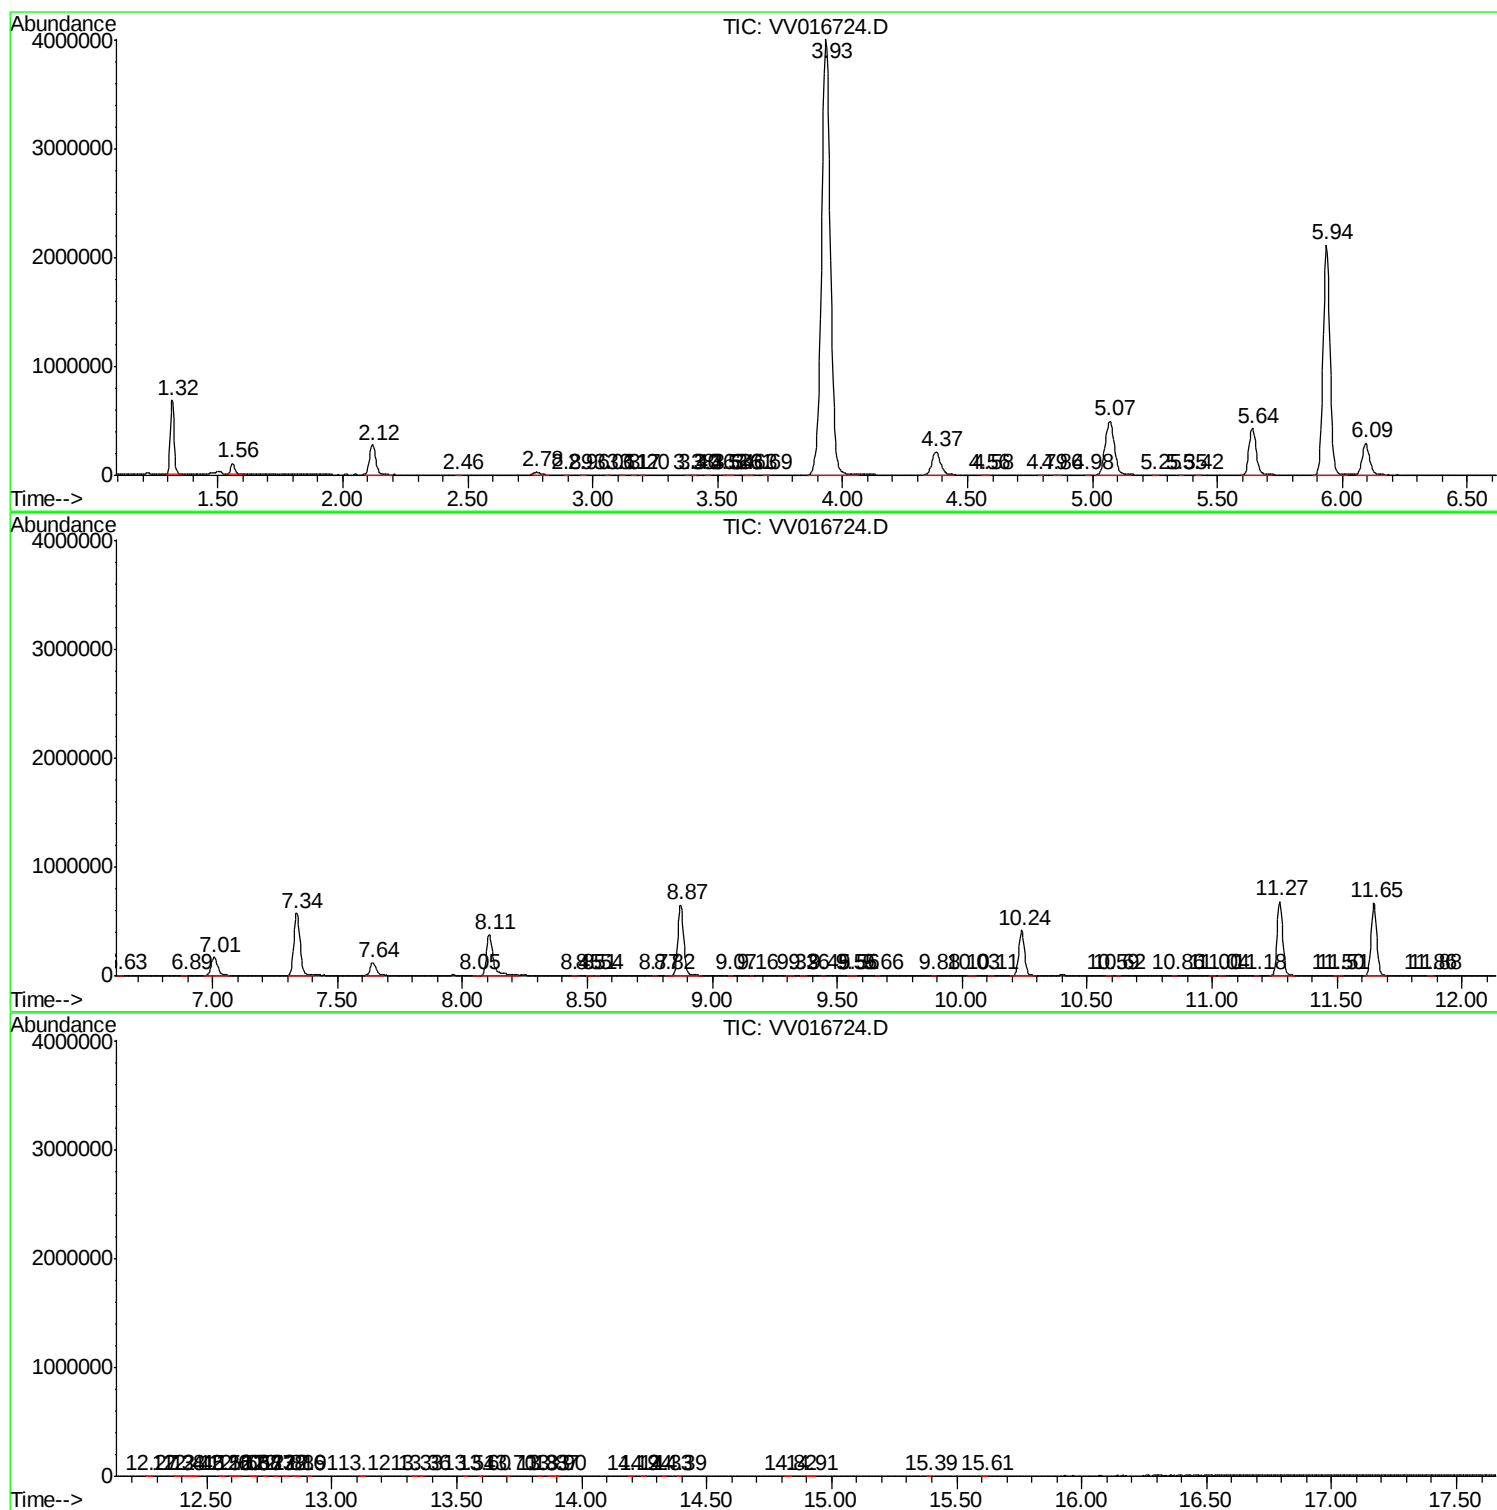

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016724.D
Acq On : 09 Jun 2020 18:01
Operator : SY/MD
Sample : L2901-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTY5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016724.D
Acq On : 09 Jun 2020 18:01
Operator : SY/MD
Sample : L2901-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTY5

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc