

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016726.D
 Acq On : 09 Jun 2020 18:48
 Operator : SY/MD
 Sample : L2901-23
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTS4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	63	71	90	rVB	1887113	1890666	100.00%	14.811%
2	1.560	140	146	159	rVB	99186	118733	6.28%	0.930%
3	2.116	310	319	331	rBV	218455	319605	16.90%	2.504%
4	2.441	416	420	421	rBV5	1397	931	0.05%	0.007%
5	2.987	586	590	591	rBV4	1380	752	0.04%	0.006%
6	3.283	679	682	684	rBV3	1480	1006	0.05%	0.008%
7	3.582	768	775	777	rBV6	1045	1263	0.07%	0.010%
8	3.611	782	784	786	rVV3	1727	798	0.04%	0.006%
9	3.627	786	789	793	rVB4	1429	1022	0.05%	0.008%
10	3.666	798	801	802	rBV2	957	619	0.03%	0.005%
11	3.698	807	811	812	rBV3	1045	866	0.05%	0.007%
12	3.933	862	884	912	rBV2	427743	1287151	68.08%	10.083%
13	4.167	955	957	960	rBV4	1424	640	0.03%	0.005%
14	4.290	993	995	1000	rBV5	1225	869	0.05%	0.007%
15	4.373	1006	1021	1042	rBV	206547	505507	26.74%	3.960%
16	4.679	1112	1116	1117	rBV4	1070	720	0.04%	0.006%
17	4.711	1123	1126	1127	rBV3	1365	730	0.04%	0.006%
18	4.769	1138	1144	1147	rVB8	1853	1859	0.10%	0.015%
19	4.868	1171	1175	1176	rBV4	1300	763	0.04%	0.006%
20	4.913	1186	1189	1190	rBV3	1930	985	0.05%	0.008%
21	4.946	1196	1199	1208	rVB10	2262	2841	0.15%	0.022%
22	4.987	1208	1212	1214	rBV4	1949	1417	0.07%	0.011%
23	5.068	1220	1237	1262	rBV3	482439	1251170	66.18%	9.801%
24	5.293	1304	1307	1309	rBV4	1676	1102	0.06%	0.009%
25	5.527	1376	1380	1382	rBV4	1469	1178	0.06%	0.009%
26	5.640	1402	1415	1441	rBV	430588	850462	44.98%	6.662%
27	6.090	1543	1555	1576	rBV	289192	582293	30.80%	4.562%
28	6.421	1654	1658	1664	rBV8	1663	1822	0.10%	0.014%
29	6.457	1667	1669	1671	rVV3	1337	710	0.04%	0.006%
30	6.479	1674	1676	1680	rVB4	1470	768	0.04%	0.006%
31	6.576	1704	1706	1711	rBV4	1329	898	0.05%	0.007%
32	6.605	1711	1715	1717	rBV4	1313	955	0.05%	0.007%
33	6.634	1720	1724	1726	rBV4	1546	1119	0.06%	0.009%
34	6.775	1763	1768	1769	rBV4	1821	1215	0.06%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016726.D
 Acq On : 09 Jun 2020 18:48
 Operator : SY/MD
 Sample : L2901-23
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTS4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.907	1805	1809	1812	rVB4	1559	1300	0.07%	0.010%
36	7.007	1830	1840	1856	rBV	160947	283095	14.97%	2.218%
37	7.273	1919	1923	1925	rBV4	1592	1015	0.05%	0.008%
38	7.338	1930	1943	1961	rBV	574620	985563	52.13%	7.721%
39	7.640	2027	2037	2055	rBV2	115631	199144	10.53%	1.560%
40	7.756	2071	2073	2078	rBV3	1600	940	0.05%	0.007%
41	7.926	2122	2126	2128	rBV4	1463	1025	0.05%	0.008%
42	7.997	2146	2148	2152	rVB4	1775	1046	0.06%	0.008%
43	8.052	2162	2165	2167	rBV4	1658	993	0.05%	0.008%
44	8.106	2172	2182	2212	rBV	357440	676629	35.79%	5.301%
45	8.534	2313	2315	2319	rVB5	1899	779	0.04%	0.006%
46	8.772	2386	2389	2392	rVB5	1810	1296	0.07%	0.010%
47	8.788	2392	2394	2397	rBV2	1001	753	0.04%	0.006%
48	8.875	2408	2421	2437	rBV	651225	1051638	55.62%	8.238%
49	9.299	2551	2553	2556	rVB4	1517	613	0.03%	0.005%
50	9.357	2569	2571	2572	rBV	1391	598	0.03%	0.005%
51	9.450	2597	2600	2603	rBV3	1611	1045	0.06%	0.008%
52	9.466	2603	2605	2607	rVB3	1486	614	0.03%	0.005%
53	9.502	2612	2616	2619	rBV5	1001	758	0.04%	0.006%
54	9.563	2631	2635	2636	rBV3	1723	766	0.04%	0.006%
55	9.601	2645	2647	2649	rBV3	1963	692	0.04%	0.005%
56	9.691	2672	2675	2679	rVB4	1396	1035	0.05%	0.008%
57	9.717	2679	2683	2684	rBV4	1012	695	0.04%	0.005%
58	10.161	2818	2821	2828	rVB5	1731	2207	0.12%	0.017%
59	10.190	2828	2830	2832	rBV2	1926	1196	0.06%	0.009%
60	10.238	2834	2845	2861	rVV	409113	636410	33.66%	4.986%
61	10.367	2882	2885	2886	rBV2	955	612	0.03%	0.005%
62	10.447	2909	2910	2915	rBV5	915	715	0.04%	0.006%
63	10.485	2920	2922	2925	rBV4	1124	637	0.03%	0.005%
64	10.531	2934	2936	2939	rBV3	1536	1149	0.06%	0.009%
65	10.791	3013	3017	3019	rBV3	1643	1288	0.07%	0.010%
66	10.920	3053	3057	3062	rBV7	1146	926	0.05%	0.007%
67	10.977	3073	3075	3080	rBV5	908	600	0.03%	0.005%
68	11.026	3086	3090	3093	rBV5	1853	1494	0.08%	0.012%
69	11.161	3130	3132	3137	rVB3	1595	1130	0.06%	0.009%
70	11.190	3137	3141	3143	rBV5	2130	1870	0.10%	0.015%
71	11.270	3155	3166	3183	rVV	668881	1023899	54.16%	8.021%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016726.D
 Acq On : 09 Jun 2020 18:48
 Operator : SY/MD
 Sample : L2901-23
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTS4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.466	3225	3227	3230	rBV3	1026	604	0.03%	0.005%
73	11.646	3271	3283	3299	rBV	645460	1014515	53.66%	7.948%
74	11.907	3362	3364	3367	rBV4	1062	680	0.04%	0.005%
75	11.981	3385	3387	3393	rVB7	1596	1126	0.06%	0.009%
76	12.010	3393	3396	3401	rBV6	1151	1148	0.06%	0.009%
77	12.029	3401	3402	3405	rBV2	1141	683	0.04%	0.005%
78	12.074	3413	3416	3419	rBV3	1456	1138	0.06%	0.009%
79	12.164	3442	3444	3447	rVB4	1227	716	0.04%	0.006%
80	12.466	3536	3538	3541	rBV4	994	734	0.04%	0.006%
81	12.611	3580	3583	3586	rBV5	1308	882	0.05%	0.007%
82	12.659	3592	3598	3603	rBV8	2132	2537	0.13%	0.020%
83	12.685	3603	3606	3612	rBV9	2114	2209	0.12%	0.017%
84	12.813	3644	3646	3651	rBV5	1273	1054	0.06%	0.008%
85	13.083	3726	3730	3731	rBV4	1388	954	0.05%	0.007%
86	13.119	3738	3741	3745	rBV5	1583	1256	0.07%	0.010%
87	13.138	3745	3747	3750	rVV4	1728	867	0.05%	0.007%
88	13.228	3773	3775	3779	rVB4	1656	1047	0.06%	0.008%
89	13.273	3783	3789	3790	rBV4	2283	1741	0.09%	0.014%
90	13.354	3812	3814	3816	rBV4	1060	646	0.03%	0.005%
91	13.386	3822	3824	3828	rBV4	1258	631	0.03%	0.005%
92	13.611	3889	3894	3898	rBV6	2045	2120	0.11%	0.017%
93	13.707	3922	3924	3930	rVB7	1724	1422	0.08%	0.011%
94	13.855	3968	3970	3975	rBV3	1373	1200	0.06%	0.009%
95	13.964	4001	4004	4007	rBV2	1116	955	0.05%	0.007%
96	14.325	4114	4116	4117	rBV2	1572	660	0.03%	0.005%
97	14.334	4117	4119	4122	rVV3	1523	766	0.04%	0.006%
98	14.395	4136	4138	4141	rBV2	1297	709	0.04%	0.006%
99	14.543	4180	4184	4187	rBV5	1890	1866	0.10%	0.015%
100	14.781	4255	4258	4259	rBV3	1485	737	0.04%	0.006%


Sum of corrected areas: 12765203

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060920\
Data File : VV016726.D
Acq On : 09 Jun 2020 18:48
Operator : SY/MD
Sample : L2901-23
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTS4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

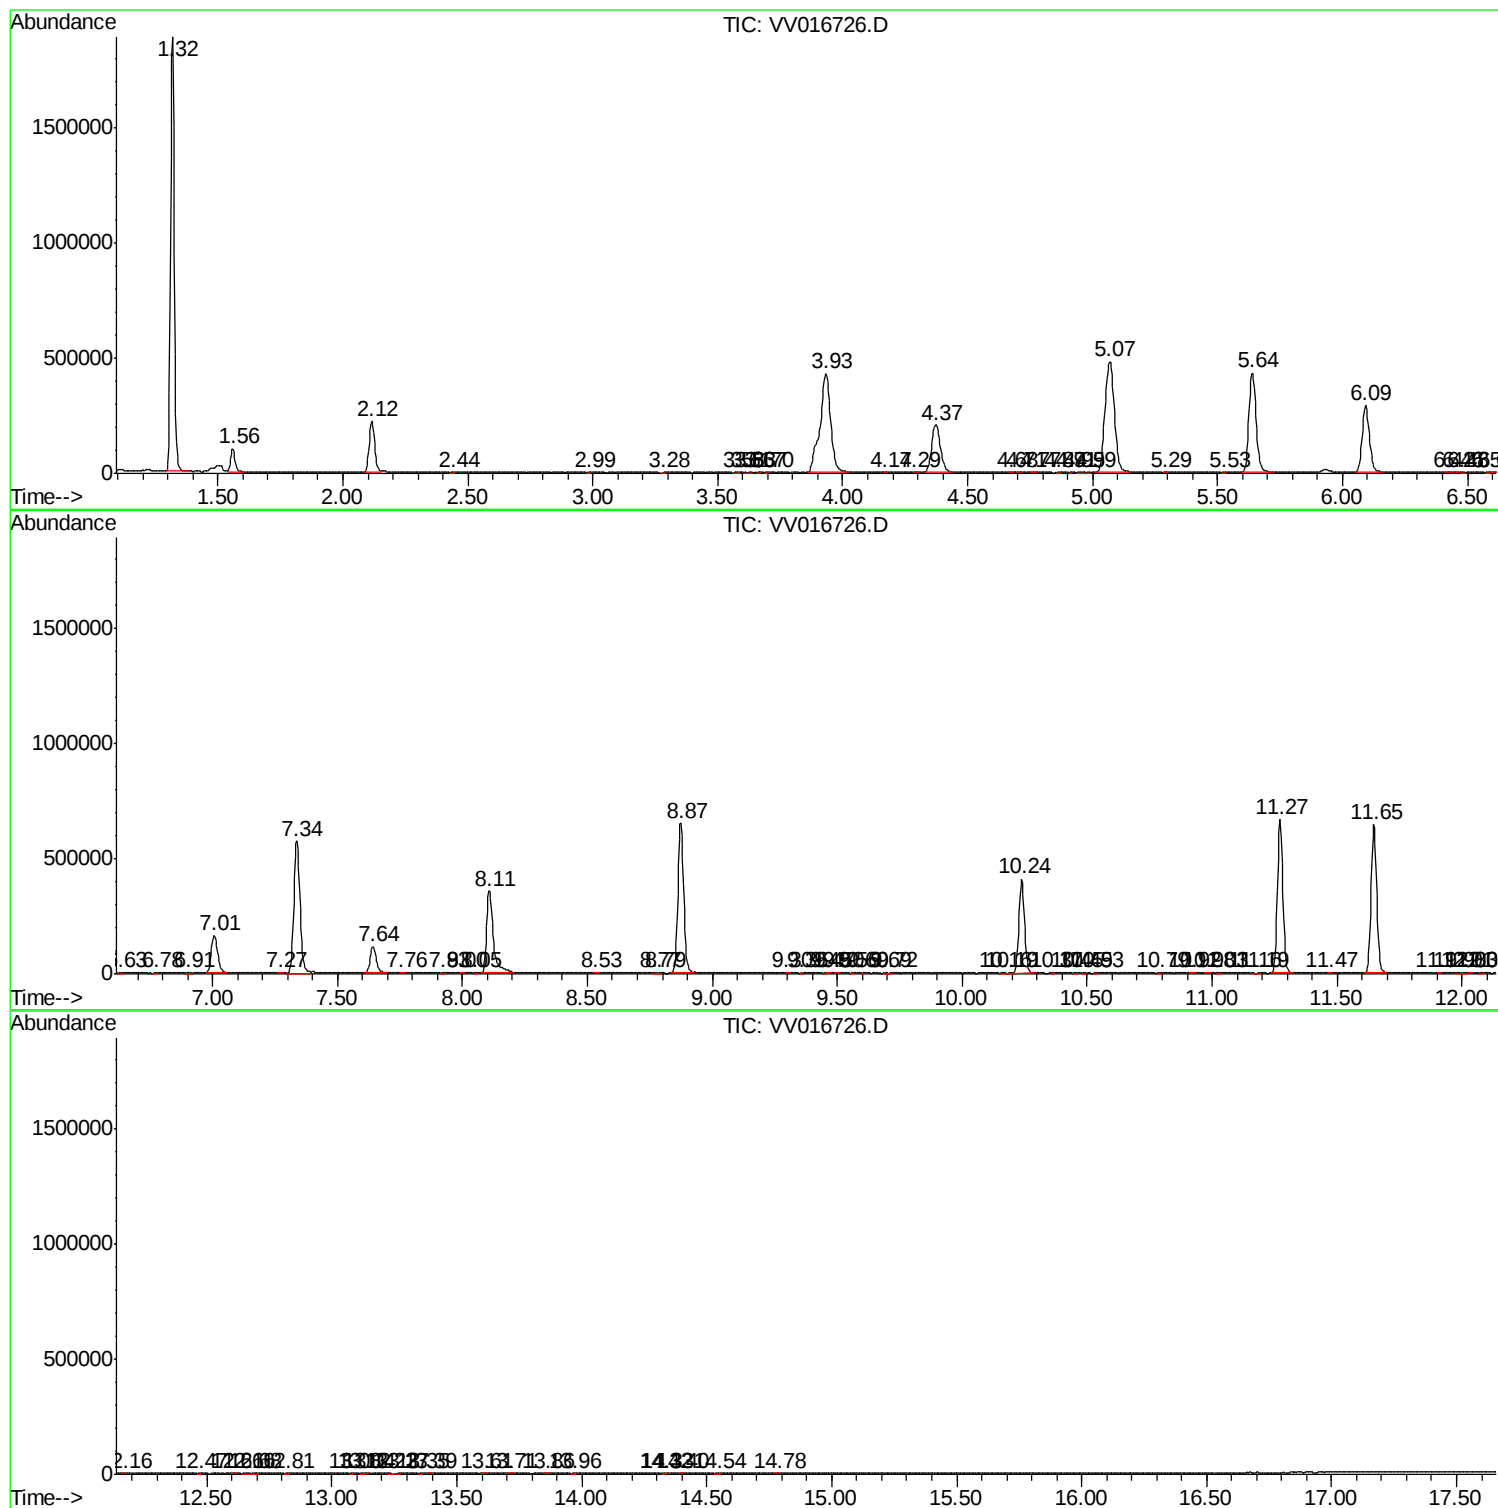

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016726.D
Acq On : 09 Jun 2020 18:48
Operator : SY/MD
Sample : L2901-23
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTS4

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016726.D
Acq On : 09 Jun 2020 18:48
Operator : SY/MD
Sample : L2901-23
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTS4

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc