

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016728.D
 Acq On : 09 Jun 2020 19:36
 Operator : SY/MD
 Sample : L2901-03DL 200X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTR3DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	82	rVB2	213614	220172	16.74%	1.993%
2	1.557	139	145	157	rVB	96749	119089	9.06%	1.078%
3	2.116	310	319	336	rVB	227798	339802	25.84%	3.076%
4	2.425	413	415	419	rBV4	1665	1124	0.09%	0.010%
5	2.518	435	444	446	rBV9	4179	5389	0.41%	0.049%
6	3.026	597	602	606	rVB8	1687	1542	0.12%	0.014%
7	3.055	606	611	612	rBV4	1784	1258	0.10%	0.011%
8	3.084	617	620	623	rVB5	1290	864	0.07%	0.008%
9	3.151	638	641	645	rBV5	1316	966	0.07%	0.009%
10	3.219	660	662	665	rVV3	1797	840	0.06%	0.008%
11	3.257	670	674	676	rVB5	1812	1048	0.08%	0.009%
12	3.273	676	679	680	rBV3	1637	987	0.08%	0.009%
13	3.299	684	687	690	rBV4	1371	972	0.07%	0.009%
14	3.418	722	724	727	rVB2	1141	625	0.05%	0.006%
15	3.441	727	731	733	rBV4	1484	931	0.07%	0.008%
16	3.476	739	742	745	rVB5	1071	659	0.05%	0.006%
17	3.495	745	748	750	rBV3	1126	870	0.07%	0.008%
18	3.537	757	761	763	rBV5	1039	849	0.06%	0.008%
19	3.656	795	798	801	rBV4	1140	918	0.07%	0.008%
20	3.762	830	831	838	rVB6	1959	2042	0.16%	0.018%
21	3.794	838	841	842	rBV3	1514	794	0.06%	0.007%
22	3.933	862	884	907	rBV2	230275	819913	62.36%	7.421%
23	4.235	975	978	979	rBV3	1553	659	0.05%	0.006%
24	4.277	986	991	994	rBV7	2728	2919	0.22%	0.026%
25	4.373	1006	1021	1044	rBV	216182	524346	39.88%	4.746%
26	4.608	1091	1094	1097	rBV5	1374	854	0.06%	0.008%
27	4.781	1144	1148	1150	rBV4	1332	1049	0.08%	0.009%
28	4.855	1169	1171	1173	rBV3	1675	973	0.07%	0.009%
29	4.939	1194	1197	1198	rBV2	1345	631	0.05%	0.006%
30	5.071	1219	1238	1262	rBV2	509282	1314877	100.00%	11.902%
31	5.640	1402	1415	1436	rBV	444953	882904	67.15%	7.992%
32	6.093	1541	1556	1581	rBV	298150	613220	46.64%	5.551%
33	6.357	1636	1638	1641	rBV4	2034	1520	0.12%	0.014%
34	6.415	1655	1656	1662	rVB5	1345	798	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016728.D
 Acq On : 09 Jun 2020 19:36
 Operator : SY/MD
 Sample : L2901-03DL 200X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTR3DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.466	1668	1672	1674	rBV4	1676	1201	0.09%	0.011%
36	6.553	1697	1699	1703	rVB5	2142	1433	0.11%	0.013%
37	6.897	1803	1806	1809	rBV4	1186	720	0.05%	0.007%
38	7.006	1830	1840	1855	rBV	168851	295234	22.45%	2.672%
39	7.338	1931	1943	1964	rBV	591981	1017562	77.39%	9.210%
40	7.640	2027	2037	2052	rBV	120511	203448	15.47%	1.842%
41	7.984	2141	2144	2147	rBV4	1352	1298	0.10%	0.012%
42	8.064	2166	2169	2171	rVB4	2390	1077	0.08%	0.010%
43	8.106	2171	2182	2212	rBV	376041	717414	54.56%	6.494%
44	8.637	2345	2347	2355	rBV9	1508	1559	0.12%	0.014%
45	8.740	2377	2379	2384	rBV6	1315	867	0.07%	0.008%
46	8.875	2408	2421	2444	rBV	660332	1077380	81.94%	9.752%
47	9.067	2479	2481	2484	rBV3	937	638	0.05%	0.006%
48	9.206	2521	2524	2528	rVB6	1846	1479	0.11%	0.013%
49	9.276	2544	2546	2547	rBV2	1561	638	0.05%	0.006%
50	9.479	2605	2609	2611	rBV5	1887	992	0.08%	0.009%
51	9.572	2633	2638	2641	rBV5	1984	1770	0.13%	0.016%
52	9.791	2701	2706	2708	rBV5	1139	1100	0.08%	0.010%
53	9.823	2713	2716	2717	rBV3	1235	631	0.05%	0.006%
54	9.897	2735	2739	2740	rBV3	1945	1153	0.09%	0.010%
55	10.042	2782	2784	2785	rBV3	1457	622	0.05%	0.006%
56	10.186	2826	2829	2830	rBV3	1293	688	0.05%	0.006%
57	10.238	2834	2845	2861	rVV2	423961	656657	49.94%	5.944%
58	10.437	2903	2907	2908	rBV3	943	753	0.06%	0.007%
59	10.521	2928	2933	2935	rBV5	1405	1494	0.11%	0.014%
60	10.547	2939	2941	2946	rBV5	1068	749	0.06%	0.007%
61	10.691	2981	2986	2988	rBV5	1179	1077	0.08%	0.010%
62	10.791	3012	3017	3019	rBV5	1849	1211	0.09%	0.011%
63	10.826	3025	3028	3031	rBV4	1581	977	0.07%	0.009%
64	10.839	3031	3032	3036	rVB4	1042	687	0.05%	0.006%
65	10.891	3046	3048	3052	rVB5	1441	863	0.07%	0.008%
66	10.913	3053	3055	3059	rBV4	1607	1197	0.09%	0.011%
67	10.968	3069	3072	3078	rVB7	1711	1582	0.12%	0.014%
68	11.116	3115	3118	3119	rBV3	1435	752	0.06%	0.007%
69	11.174	3132	3136	3139	rBV4	1421	1194	0.09%	0.011%
70	11.270	3155	3166	3180	rBV	704247	1075543	81.80%	9.735%
71	11.646	3271	3283	3302	rBV	685371	1076401	81.86%	9.743%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016728.D
 Acq On : 09 Jun 2020 19:36
 Operator : SY/MD
 Sample : L2901-03DL 200X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTR3DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.048	3405	3408	3415	rVB6	1959	1961	0.15%	0.018%
73	12.177	3446	3448	3451	rVB4	1764	883	0.07%	0.008%
74	12.350	3499	3502	3505	rBV5	1015	634	0.05%	0.006%
75	12.447	3530	3532	3537	rVB5	1221	676	0.05%	0.006%
76	12.611	3581	3583	3585	rBV3	1271	703	0.05%	0.006%
77	12.665	3595	3600	3602	rBV5	1297	1143	0.09%	0.010%
78	12.685	3602	3606	3607	rBV4	849	676	0.05%	0.006%
79	12.762	3627	3630	3631	rBV3	1636	964	0.07%	0.009%
80	12.791	3636	3639	3643	rVB4	1275	1089	0.08%	0.010%
81	12.868	3660	3663	3666	rVB5	1484	916	0.07%	0.008%
82	12.913	3673	3677	3678	rBV4	1369	849	0.06%	0.008%
83	13.051	3717	3720	3724	rBV3	1986	1273	0.10%	0.012%
84	13.148	3747	3750	3753	rBV4	1439	911	0.07%	0.008%
85	13.225	3772	3774	3778	rVB5	1535	741	0.06%	0.007%
86	13.321	3801	3804	3807	rBV3	1340	798	0.06%	0.007%
87	13.540	3869	3872	3873	rBV3	2366	1155	0.09%	0.010%
88	13.636	3898	3902	3904	rBV5	1611	1125	0.09%	0.010%
89	13.665	3908	3911	3914	rBV5	1286	1095	0.08%	0.010%
90	13.698	3918	3921	3922	rBV3	1057	643	0.05%	0.006%
91	13.781	3945	3947	3950	rBV3	968	638	0.05%	0.006%
92	13.858	3966	3971	3972	rBV4	1646	1240	0.09%	0.011%
93	14.125	4051	4054	4058	rBV4	2152	1768	0.13%	0.016%
94	14.161	4063	4065	4070	rVB4	1750	1443	0.11%	0.013%
95	14.199	4070	4077	4081	rBV8	2578	3567	0.27%	0.032%
96	14.312	4110	4112	4115	rVB4	1293	677	0.05%	0.006%
97	14.434	4147	4150	4155	rBV6	1384	1122	0.09%	0.010%
98	15.000	4324	4326	4328	rBV3	1866	1005	0.08%	0.009%
99	15.135	4366	4368	4372	rBV3	1193	671	0.05%	0.006%
100	15.373	4438	4442	4443	rBV3	1430	1074	0.08%	0.010%


Sum of corrected areas: 11047885

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060920\
Data File : VV016728.D
Acq On : 09 Jun 2020 19:36
Operator : SY/MD
Sample : L2901-03DL 200X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTR3DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

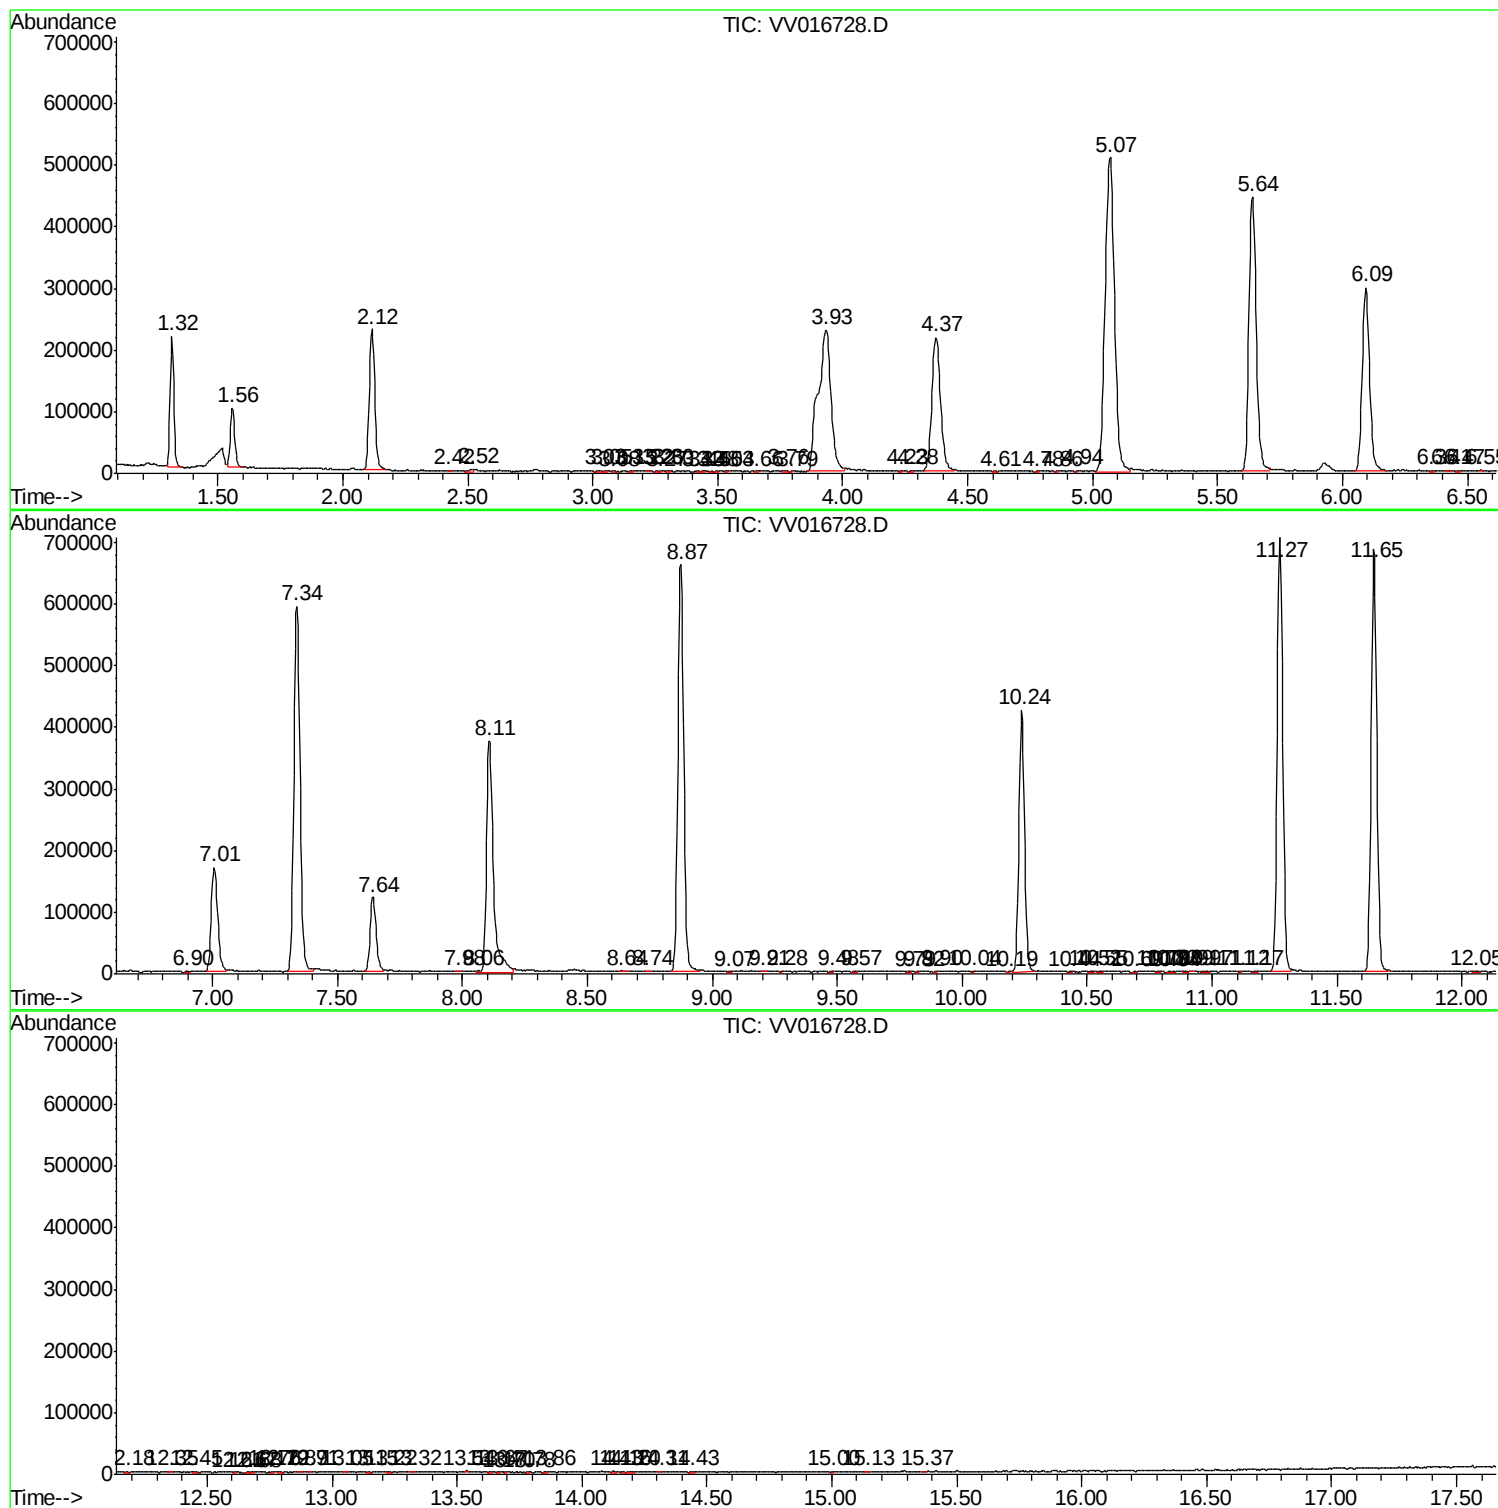

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016728.D
Acq On : 09 Jun 2020 19:36
Operator : SY/MD
Sample : L2901-03DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTR3DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016728.D
Acq On : 09 Jun 2020 19:36
Operator : SY/MD
Sample : L2901-03DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTR3DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc