

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016729.D
 Acq On : 09 Jun 2020 20:00
 Operator : SY/MD
 Sample : L2901-04DL 200X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTR4DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	83	rVB2	201933	212523	16.19%	1.920%
2	1.560	140	146	156	rVB	95247	113975	8.69%	1.029%
3	2.116	310	319	332	rVB	227985	335036	25.53%	3.026%
4	2.412	407	411	413	rBV4	1415	1091	0.08%	0.010%
5	2.685	492	496	499	rBV5	1254	1033	0.08%	0.009%
6	2.721	504	507	509	rBV3	968	753	0.06%	0.007%
7	2.772	519	523	524	rBV3	2263	1878	0.14%	0.017%
8	2.865	549	552	555	rBV4	1544	1158	0.09%	0.010%
9	2.946	571	577	578	rBV6	1612	1554	0.12%	0.014%
10	2.984	586	589	590	rBV3	1335	685	0.05%	0.006%
11	3.042	603	607	609	rBV4	1530	1097	0.08%	0.010%
12	3.106	624	627	628	rBV2	941	547	0.04%	0.005%
13	3.151	640	641	646	rVB4	1283	765	0.06%	0.007%
14	3.177	646	649	653	rBV6	1522	979	0.07%	0.009%
15	3.209	657	659	665	rBV6	1089	954	0.07%	0.009%
16	3.341	697	700	703	rVV5	1286	903	0.07%	0.008%
17	3.518	752	755	758	rVB3	1438	997	0.08%	0.009%
18	3.537	758	761	765	rBV6	1897	1829	0.14%	0.017%
19	3.582	773	775	780	rVB6	1696	1368	0.10%	0.012%
20	3.618	780	786	789	rBV5	1472	1554	0.12%	0.014%
21	3.827	847	851	855	rBV6	1550	1553	0.12%	0.014%
22	3.933	861	884	911	rBV2	235797	839264	63.95%	7.581%
23	4.293	993	996	998	rBV4	1170	697	0.05%	0.006%
24	4.373	1006	1021	1043	rBV	217297	524790	39.99%	4.740%
25	4.556	1075	1078	1080	rBV3	1518	863	0.07%	0.008%
26	4.791	1149	1151	1154	rVV3	1586	905	0.07%	0.008%
27	4.820	1157	1160	1163	rBV5	1044	695	0.05%	0.006%
28	4.875	1174	1177	1179	rBV4	1511	1159	0.09%	0.010%
29	4.917	1187	1190	1191	rBV3	1239	713	0.05%	0.006%
30	5.068	1221	1237	1265	rBV2	509656	1312313	100.00%	11.853%
31	5.511	1373	1375	1378	rBV3	1331	680	0.05%	0.006%
32	5.640	1402	1415	1440	rBV	457431	910494	69.38%	8.224%
33	5.807	1463	1467	1471	rBV6	2327	1869	0.14%	0.017%
34	6.093	1539	1556	1576	rBV	301972	616365	46.97%	5.567%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016729.D
 Acq On : 09 Jun 2020 20:00
 Operator : SY/MD
 Sample : L2901-04DL 200X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTR4DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.225	1593	1597	1600	rBV5	2612	2159	0.16%	0.020%
36	6.347	1631	1635	1637	rBV3	1224	893	0.07%	0.008%
37	6.434	1660	1662	1664	rBV3	925	556	0.04%	0.005%
38	6.585	1706	1709	1714	rVB7	1656	1402	0.11%	0.013%
39	6.608	1714	1716	1718	rBV3	1510	595	0.05%	0.005%
40	6.781	1768	1770	1773	rVB3	1331	822	0.06%	0.007%
41	6.798	1773	1775	1781	rVB6	1395	1020	0.08%	0.009%
42	6.859	1792	1794	1797	rVB3	1467	746	0.06%	0.007%
43	6.900	1802	1807	1809	rBV3	1340	1384	0.11%	0.013%
44	7.007	1829	1840	1856	rBV	172976	303640	23.14%	2.743%
45	7.193	1896	1898	1902	rVB5	1565	954	0.07%	0.009%
46	7.338	1929	1943	1961	rBV	601042	1032123	78.65%	9.322%
47	7.640	2028	2037	2054	rBV	119506	201619	15.36%	1.821%
48	7.868	2106	2108	2111	rBV3	1525	894	0.07%	0.008%
49	8.052	2163	2165	2167	rBV3	1375	707	0.05%	0.006%
50	8.106	2171	2182	2212	rBV	373357	704750	53.70%	6.366%
51	8.691	2362	2364	2368	rBV4	1103	860	0.07%	0.008%
52	8.781	2390	2392	2394	rBV3	1222	682	0.05%	0.006%
53	8.871	2408	2420	2442	rBV	682079	1106208	84.29%	9.992%
54	9.318	2556	2559	2560	rBV3	1195	698	0.05%	0.006%
55	9.421	2588	2591	2596	rVB5	2525	2340	0.18%	0.021%
56	9.450	2596	2600	2601	rBV3	1575	1126	0.09%	0.010%
57	9.466	2603	2605	2610	rVV5	1396	1087	0.08%	0.010%
58	9.505	2615	2617	2622	rBV5	1486	1049	0.08%	0.009%
59	9.527	2622	2624	2625	rBV	1584	585	0.04%	0.005%
60	9.752	2692	2694	2697	rBV3	900	618	0.05%	0.006%
61	9.820	2712	2715	2716	rBV3	1603	703	0.05%	0.006%
62	10.048	2784	2786	2789	rVB3	1166	616	0.05%	0.006%
63	10.187	2826	2829	2832	rBV5	1400	1174	0.09%	0.011%
64	10.238	2833	2845	2859	rVV	419512	651179	49.62%	5.882%
65	10.360	2880	2883	2885	rBV3	1705	915	0.07%	0.008%
66	10.408	2896	2898	2902	rBV3	1491	1037	0.08%	0.009%
67	10.457	2910	2913	2915	rBV3	1690	942	0.07%	0.009%
68	10.473	2915	2918	2922	rVB5	1946	1233	0.09%	0.011%
69	10.527	2928	2935	2939	rVB7	1603	1700	0.13%	0.015%
70	10.595	2954	2956	2958	rBV3	1527	886	0.07%	0.008%
71	11.010	3083	3085	3088	rVV3	1153	721	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016729.D
 Acq On : 09 Jun 2020 20:00
 Operator : SY/MD
 Sample : L2901-04DL 200X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTR4DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.071	3101	3104	3107	rBV3	1894	1428	0.11%	0.013%
73	11.270	3154	3166	3186	rBV	692768	1067407	81.34%	9.641%
74	11.572	3258	3260	3264	rVB3	1159	771	0.06%	0.007%
75	11.646	3272	3283	3299	rBV	670626	1057699	80.60%	9.553%
76	12.000	3390	3393	3398	rBV7	999	1026	0.08%	0.009%
77	12.055	3406	3410	3412	rBV5	1422	728	0.06%	0.007%
78	12.074	3412	3416	3418	rBV5	1688	1252	0.10%	0.011%
79	12.251	3466	3471	3472	rBV4	1439	1031	0.08%	0.009%
80	12.482	3540	3543	3547	rBV5	1284	1175	0.09%	0.011%
81	12.547	3562	3563	3566	rVB3	1354	557	0.04%	0.005%
82	12.685	3604	3606	3607	rBV3	1430	582	0.04%	0.005%
83	12.739	3621	3623	3625	rBV2	962	534	0.04%	0.005%
84	12.939	3683	3685	3687	rBV2	1020	536	0.04%	0.005%
85	13.029	3710	3713	3714	rBV3	1075	624	0.05%	0.006%
86	13.132	3742	3745	3748	rBV3	1177	878	0.07%	0.008%
87	13.241	3777	3779	3781	rBV2	1549	676	0.05%	0.006%
88	13.431	3834	3838	3839	rBV3	1436	892	0.07%	0.008%
89	13.575	3881	3883	3888	rBV4	1359	1280	0.10%	0.012%
90	13.665	3908	3911	3914	rBV4	895	707	0.05%	0.006%
91	13.778	3945	3946	3948	rBV2	1464	691	0.05%	0.006%
92	13.942	3995	3997	4000	rVB2	1162	561	0.04%	0.005%
93	14.003	4012	4016	4019	rBV6	1458	993	0.08%	0.009%
94	14.016	4019	4020	4023	rBV3	1277	606	0.05%	0.005%
95	14.186	4071	4073	4075	rBV3	1068	627	0.05%	0.006%
96	14.456	4155	4157	4160	rBV5	1188	551	0.04%	0.005%
97	14.714	4233	4237	4238	rBV3	1580	1058	0.08%	0.010%
98	14.752	4247	4249	4251	rVB3	1569	798	0.06%	0.007%
99	15.128	4362	4366	4368	rBV3	1779	1368	0.10%	0.012%
100	15.347	4431	4434	4435	rBV3	1195	628	0.05%	0.006%


Sum of corrected areas: 11071326

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060920\
Data File : VV016729.D
Acq On : 09 Jun 2020 20:00
Operator : SY/MD
Sample : L2901-04DL 200X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTR4DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

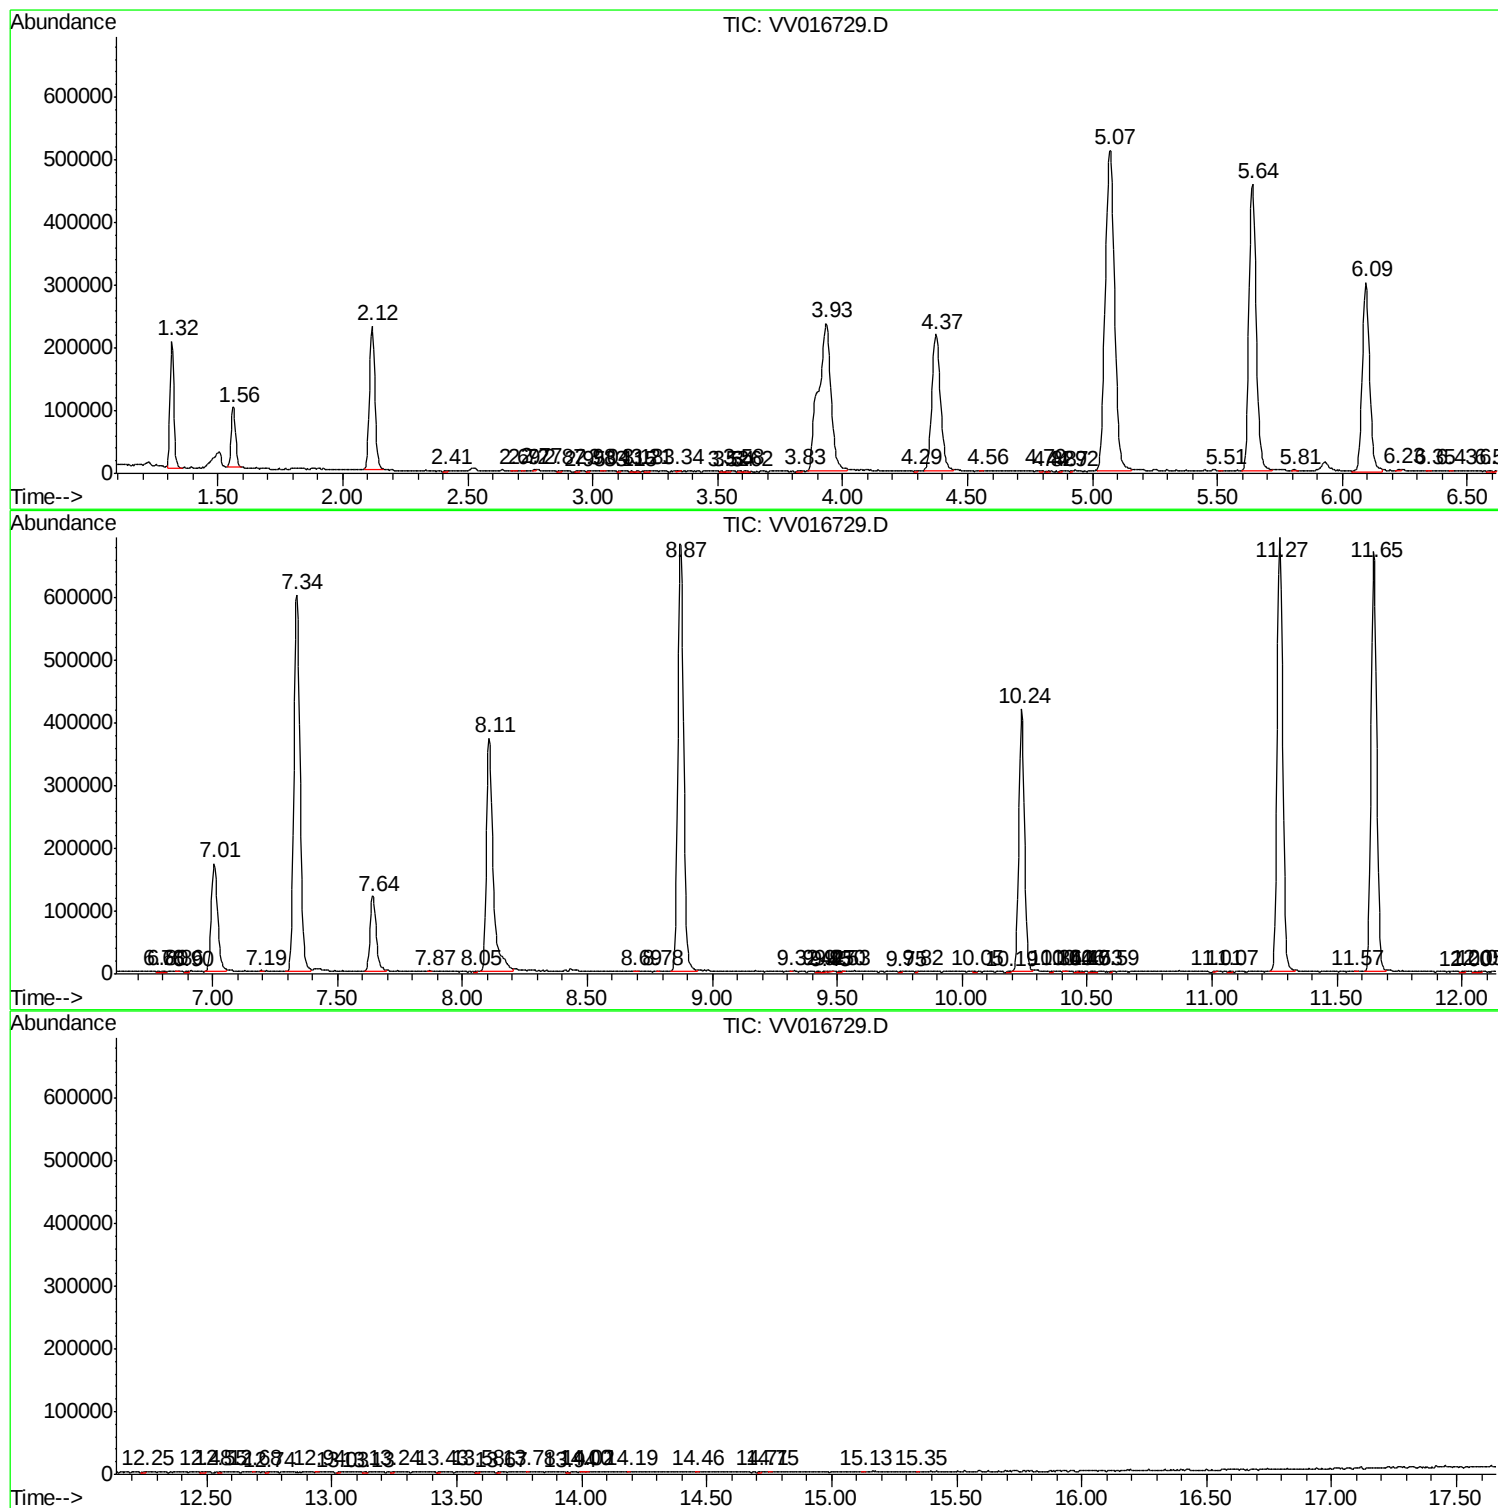

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016729.D
Acq On : 09 Jun 2020 20:00
Operator : SY/MD
Sample : L2901-04DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTR4DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016729.D
Acq On : 09 Jun 2020 20:00
Operator : SY/MD
Sample : L2901-04DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTR4DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc