

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016731.D
 Acq On : 09 Jun 2020 20:48
 Operator : SY/MD
 Sample : L2914-20
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E73

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	64	69	81	rVB	120774	122448	9.89%	1.245%
2	1.560	139	146	158	rVB	96788	116048	9.38%	1.180%
3	2.116	310	319	332	rBV	207498	308272	24.91%	3.135%
4	2.351	389	392	395	rBV5	2078	1468	0.12%	0.015%
5	2.415	410	412	414	rBV3	1419	883	0.07%	0.009%
6	2.595	463	468	470	rBV5	2284	1356	0.11%	0.014%
7	2.746	511	515	517	rVV4	1521	1309	0.11%	0.013%
8	3.055	606	611	612	rBV4	1032	869	0.07%	0.009%
9	3.106	624	627	631	rVB5	1253	855	0.07%	0.009%
10	3.254	670	673	677	rBV6	1683	1320	0.11%	0.013%
11	3.364	704	707	708	rBV2	1416	745	0.06%	0.008%
12	3.399	715	718	721	rBV6	1489	1198	0.10%	0.012%
13	3.611	781	784	790	rBV7	1951	2266	0.18%	0.023%
14	3.695	805	810	813	rBV5	1592	1310	0.11%	0.013%
15	3.765	829	832	835	rBV5	1272	1192	0.10%	0.012%
16	3.804	842	844	847	rBV4	1242	627	0.05%	0.006%
17	3.894	862	872	898	rBV	106304	284794	23.01%	2.896%
18	4.373	1003	1021	1046	rBV	212906	533446	43.10%	5.425%
19	4.762	1140	1142	1144	rBV3	1421	704	0.06%	0.007%
20	4.817	1154	1159	1161	rBV6	1297	1203	0.10%	0.012%
21	4.910	1183	1188	1190	rBV4	1689	1631	0.13%	0.017%
22	4.936	1194	1196	1201	rVV6	1310	1096	0.09%	0.011%
23	4.974	1205	1208	1209	rBV3	1361	811	0.07%	0.008%
24	5.068	1220	1237	1266	rBV2	478028	1237673	100.00%	12.587%
25	5.518	1374	1377	1379	rVB3	2227	999	0.08%	0.010%
26	5.640	1401	1415	1435	rBV	424399	843430	68.15%	8.578%
27	5.823	1469	1472	1474	rBV4	1621	1289	0.10%	0.013%
28	5.855	1480	1482	1486	rBV5	1674	1073	0.09%	0.011%
29	6.093	1543	1556	1576	rBV	281651	566299	45.76%	5.759%
30	6.351	1634	1636	1641	rBV6	1269	1043	0.08%	0.011%
31	6.634	1721	1724	1726	rBV3	2119	1425	0.12%	0.014%
32	6.746	1756	1759	1760	rBV3	1175	634	0.05%	0.006%
33	6.814	1777	1780	1781	rBV3	1907	792	0.06%	0.008%
34	7.007	1830	1840	1860	rVV	160251	280585	22.67%	2.854%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016731.D
 Acq On : 09 Jun 2020 20:48
 Operator : SY/MD
 Sample : L2914-20
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E73

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	7.177	1889	1893	1895	rBV5	1450	1176	0.10%	0.012%
36	7.267	1919	1921	1923	rBV3	1365	699	0.06%	0.007%
37	7.338	1931	1943	1961	rVV	551275	952658	76.97%	9.689%
38	7.466	1980	1983	1985	rBV2	1958	908	0.07%	0.009%
39	7.643	2028	2038	2056	rBV	112712	190001	15.35%	1.932%
40	7.936	2125	2129	2132	rBV5	1137	1067	0.09%	0.011%
41	8.035	2158	2160	2164	rVB5	980	589	0.05%	0.006%
42	8.064	2164	2169	2172	rBV6	1628	1869	0.15%	0.019%
43	8.109	2172	2183	2213	rBV2	337444	665580	53.78%	6.769%
44	8.466	2292	2294	2298	rBV6	1388	1119	0.09%	0.011%
45	8.527	2310	2313	2314	rBV3	1493	844	0.07%	0.009%
46	8.585	2327	2331	2336	rBV5	2001	2327	0.19%	0.024%
47	8.675	2357	2359	2364	rBV5	2025	1910	0.15%	0.019%
48	8.875	2410	2421	2437	rBV	635449	1029894	83.21%	10.474%
49	9.283	2546	2548	2549	rBV2	1455	665	0.05%	0.007%
50	9.370	2572	2575	2577	rBV4	1305	1065	0.09%	0.011%
51	9.614	2649	2651	2655	rBV4	1107	886	0.07%	0.009%
52	9.698	2675	2677	2681	rVB3	1495	1203	0.10%	0.012%
53	9.727	2681	2686	2688	rBV5	1924	1547	0.12%	0.016%
54	9.842	2719	2722	2724	rBV4	1296	756	0.06%	0.008%
55	10.087	2796	2798	2802	rVB5	1955	1203	0.10%	0.012%
56	10.238	2833	2845	2862	rBV	390039	615649	49.74%	6.261%
57	10.399	2890	2895	2896	rBV3	2330	1803	0.15%	0.018%
58	10.450	2909	2911	2916	rBV6	1308	1207	0.10%	0.012%
59	10.550	2938	2942	2944	rBV4	1255	699	0.06%	0.007%
60	10.566	2945	2947	2952	rVV5	1105	798	0.06%	0.008%
61	10.736	2997	3000	3001	rBV3	1319	764	0.06%	0.008%
62	11.270	3156	3166	3183	rBV	658027	997089	80.56%	10.141%
63	11.376	3195	3199	3201	rBV4	1509	1035	0.08%	0.011%
64	11.553	3251	3254	3256	rBV3	2503	1655	0.13%	0.017%
65	11.646	3271	3283	3300	rBV	635970	993818	80.30%	10.107%
66	11.717	3303	3305	3306	rBV2	1883	612	0.05%	0.006%
67	11.788	3325	3327	3329	rBV2	1930	1194	0.10%	0.012%
68	11.829	3338	3340	3345	rBV5	1474	1065	0.09%	0.011%
69	12.048	3406	3408	3410	rBV2	1320	663	0.05%	0.007%
70	12.177	3446	3448	3453	rVB5	1266	710	0.06%	0.007%
71	12.273	3471	3478	3481	rBV5	2062	2505	0.20%	0.025%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016731.D
 Acq On : 09 Jun 2020 20:48
 Operator : SY/MD
 Sample : L2914-20
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E73

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.296	3482	3485	3491	rVB7	1891	1429	0.12%	0.015%
73	12.341	3491	3499	3502	rBV9	1393	2223	0.18%	0.023%
74	12.373	3505	3509	3513	rBV7	1498	1365	0.11%	0.014%
75	12.463	3533	3537	3539	rBV5	1107	936	0.08%	0.010%
76	12.540	3559	3561	3565	rBV6	1955	1120	0.09%	0.011%
77	12.588	3574	3576	3578	rBV3	1131	662	0.05%	0.007%
78	12.601	3578	3580	3582	rBV3	1066	596	0.05%	0.006%
79	12.669	3599	3601	3603	rBV2	2146	1351	0.11%	0.014%
80	12.981	3695	3698	3700	rBV4	1319	862	0.07%	0.009%
81	12.997	3700	3703	3705	rBV4	1252	766	0.06%	0.008%
82	13.119	3739	3741	3743	rBV3	1957	895	0.07%	0.009%
83	13.331	3803	3807	3811	rVB7	1722	1323	0.11%	0.013%
84	13.360	3811	3816	3821	rBV10	1435	1297	0.10%	0.013%
85	13.411	3829	3832	3834	rBV4	1089	937	0.08%	0.010%
86	13.440	3839	3841	3844	rBV4	1186	720	0.06%	0.007%
87	13.524	3865	3867	3869	rBV2	2211	1357	0.11%	0.014%
88	13.733	3928	3932	3934	rBV5	1374	1041	0.08%	0.011%
89	13.852	3967	3969	3971	rBV3	1499	834	0.07%	0.008%
90	13.977	4002	4008	4009	rBV5	1934	2031	0.16%	0.021%
91	14.122	4051	4053	4057	rBV6	1253	758	0.06%	0.008%
92	14.225	4083	4085	4090	rVB5	2108	1326	0.11%	0.013%
93	14.321	4113	4115	4118	rVB3	1990	1024	0.08%	0.010%
94	14.353	4121	4125	4127	rBV4	1173	1094	0.09%	0.011%
95	14.447	4152	4154	4157	rVB4	1472	606	0.05%	0.006%
96	14.466	4157	4160	4162	rBV3	1606	1129	0.09%	0.011%
97	14.591	4197	4199	4201	rBV2	1314	892	0.07%	0.009%
98	14.675	4222	4225	4229	rBV6	1495	1302	0.11%	0.013%
99	14.868	4283	4285	4288	rBV3	1745	1181	0.10%	0.012%
100	15.096	4353	4356	4359	rBV3	1745	1261	0.10%	0.013%


Sum of corrected areas: 9832643

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060920\
Data File : VV016731.D
Acq On : 09 Jun 2020 20:48
Operator : SY/MD
Sample : L2914-20
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E73

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

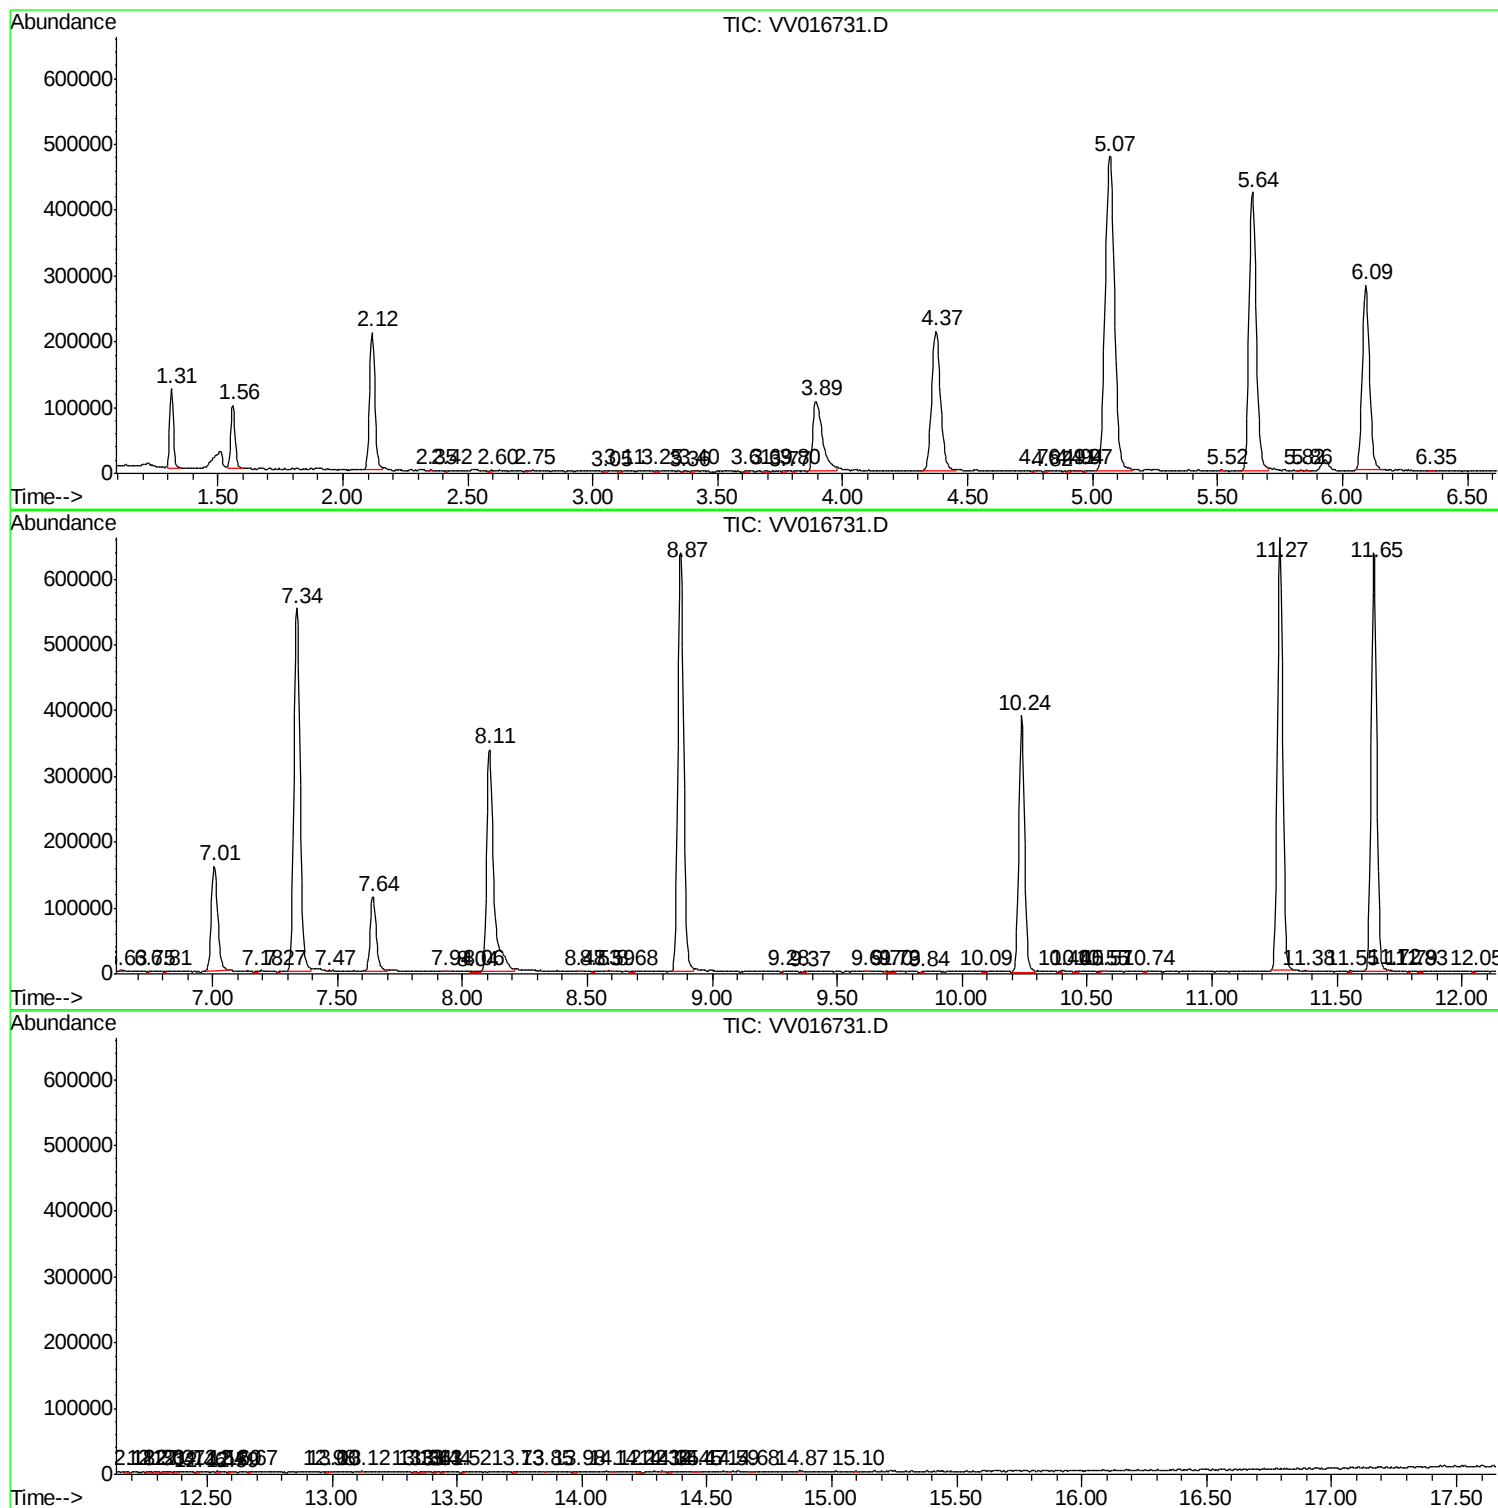

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016731.D
Acq On : 09 Jun 2020 20:48
Operator : SY/MD
Sample : L2914-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E73

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016731.D
Acq On : 09 Jun 2020 20:48
Operator : SY/MD
Sample : L2914-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E73

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc