

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016735.D
 Acq On : 09 Jun 2020 22:23
 Operator : SY/MD
 Sample : L2914-19
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E66

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	79	rVB	150532	149034	10.86%	1.393%
2	1.560	139	146	161	rVB	113252	140058	10.20%	1.309%
3	2.116	309	319	332	rBV	249760	373563	27.21%	3.491%
4	2.495	435	437	441	rBV4	1353	1055	0.08%	0.010%
5	2.582	457	464	466	rBV8	1337	1512	0.11%	0.014%
6	2.672	490	492	495	rBV4	854	568	0.04%	0.005%
7	2.756	514	518	521	rBV5	2352	2238	0.16%	0.021%
8	2.817	535	537	541	rVB5	1216	640	0.05%	0.006%
9	2.923	567	570	572	rVV5	1063	567	0.04%	0.005%
10	3.039	602	606	610	rVB7	1535	1441	0.10%	0.013%
11	3.103	623	626	627	rBV3	1245	606	0.04%	0.006%
12	3.142	632	638	640	rBV7	1446	1363	0.10%	0.013%
13	3.283	677	682	685	rBV4	2406	1687	0.12%	0.016%
14	3.331	694	697	700	rBV5	1385	950	0.07%	0.009%
15	3.399	715	718	721	rVB4	1615	1017	0.07%	0.010%
16	3.418	721	724	726	rBV4	1181	702	0.05%	0.007%
17	3.482	739	744	746	rBV4	1500	1038	0.08%	0.010%
18	3.505	749	751	753	rBV2	1115	555	0.04%	0.005%
19	3.566	768	770	775	rVB3	1068	926	0.07%	0.009%
20	3.589	775	777	778	rBV2	1284	541	0.04%	0.005%
21	3.614	783	785	790	rBV5	841	670	0.05%	0.006%
22	3.637	790	792	795	rBV4	1059	517	0.04%	0.005%
23	3.656	797	798	802	rVB4	1068	521	0.04%	0.005%
24	3.679	802	805	809	rBV5	1109	810	0.06%	0.008%
25	3.711	813	815	819	rBV3	1120	831	0.06%	0.008%
26	3.762	829	831	833	rBV3	1795	774	0.06%	0.007%
27	3.804	841	844	846	rVB4	1249	583	0.04%	0.005%
28	3.823	846	850	853	rVB4	1255	824	0.06%	0.008%
29	3.843	853	856	858	rBV4	902	576	0.04%	0.005%
30	3.894	862	872	896	rBV	117166	302679	22.05%	2.829%
31	4.209	967	970	971	rBV3	1130	606	0.04%	0.006%
32	4.299	996	998	1001	rBV3	1082	766	0.06%	0.007%
33	4.373	1007	1021	1042	rVB	225142	535309	38.99%	5.003%
34	4.640	1101	1104	1108	rVB5	1732	1233	0.09%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016735.D
 Acq On : 09 Jun 2020 22:23
 Operator : SY/MD
 Sample : L2914-19
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E66

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	4.662	1108	1111	1112	rBV2	1001	659	0.05%	0.006%
36	4.794	1149	1152	1154	rBV4	1808	1031	0.08%	0.010%
37	4.833	1162	1164	1169	rVB5	1470	829	0.06%	0.008%
38	4.859	1169	1172	1177	rBV7	1892	1356	0.10%	0.013%
39	5.068	1221	1237	1260	rBV2	542269	1372803	100.00%	12.830%
40	5.396	1336	1339	1340	rBV3	1655	1092	0.08%	0.010%
41	5.444	1350	1354	1360	rVB8	1976	2633	0.19%	0.025%
42	5.486	1363	1367	1371	rBV6	1745	1373	0.10%	0.013%
43	5.592	1397	1400	1402	rBV3	1150	865	0.06%	0.008%
44	5.640	1402	1415	1435	rVV	427309	852123	62.07%	7.964%
45	5.849	1478	1480	1486	rVB6	2044	1210	0.09%	0.011%
46	6.000	1525	1527	1529	rBV3	1301	726	0.05%	0.007%
47	6.093	1542	1556	1581	rBV	313106	637097	46.41%	5.954%
48	6.267	1608	1610	1617	rVB7	2029	2038	0.15%	0.019%
49	6.351	1633	1636	1637	rBV3	1519	656	0.05%	0.006%
50	6.511	1684	1686	1688	rVB3	1606	710	0.05%	0.007%
51	6.531	1688	1692	1696	rBV6	1367	973	0.07%	0.009%
52	6.559	1696	1701	1703	rBV6	1967	1586	0.12%	0.015%
53	6.762	1761	1764	1765	rBV3	1148	681	0.05%	0.006%
54	6.804	1770	1777	1780	rBV8	1527	1768	0.13%	0.017%
55	6.878	1798	1800	1803	rBV4	1703	909	0.07%	0.008%
56	6.926	1813	1815	1817	rBV3	1059	664	0.05%	0.006%
57	6.955	1823	1824	1829	rVB5	1838	636	0.05%	0.006%
58	7.006	1829	1840	1861	rBV	175545	315970	23.02%	2.953%
59	7.338	1929	1943	1961	rBV	626189	1075113	78.32%	10.048%
60	7.502	1992	1994	2000	rBV7	1201	926	0.07%	0.009%
61	7.640	2028	2037	2055	rBV	117974	197960	14.42%	1.850%
62	7.862	2103	2106	2110	rBV5	1707	1731	0.13%	0.016%
63	8.106	2172	2182	2213	rBV	397462	744976	54.27%	6.963%
64	8.437	2282	2285	2288	rBV4	1399	909	0.07%	0.008%
65	8.711	2368	2370	2372	rBV3	1397	751	0.05%	0.007%
66	8.874	2410	2421	2442	rBV	645911	1041874	75.89%	9.737%
67	9.100	2489	2491	2492	rBV2	1654	798	0.06%	0.007%
68	9.157	2507	2509	2513	rBV5	1416	1011	0.07%	0.009%
69	9.286	2540	2549	2556	rBV5	10019	16910	1.23%	0.158%
70	9.379	2576	2578	2581	rBV4	1145	769	0.06%	0.007%
71	9.399	2581	2584	2585	rBV3	1201	582	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016735.D
 Acq On : 09 Jun 2020 22:23
 Operator : SY/MD
 Sample : L2914-19
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E66

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	9.450	2598	2600	2601	rBV2	1470	624	0.05%	0.006%
73	9.460	2601	2603	2606	rVV4	1101	678	0.05%	0.006%
74	9.559	2632	2634	2638	rBV5	1666	1441	0.10%	0.013%
75	9.701	2674	2678	2680	rBV4	1953	1564	0.11%	0.015%
76	9.736	2682	2689	2691	rBV7	4029	4848	0.35%	0.045%
77	10.032	2779	2781	2783	rBV3	1559	725	0.05%	0.007%
78	10.048	2783	2786	2788	rBV4	1473	902	0.07%	0.008%
79	10.090	2797	2799	2800	rBV2	1611	690	0.05%	0.006%
80	10.183	2822	2828	2829	rBV4	3144	3024	0.22%	0.028%
81	10.238	2834	2845	2859	rVV	441513	695177	50.64%	6.497%
82	10.527	2928	2935	2943	rVB	4067	5948	0.43%	0.056%
83	10.569	2943	2948	2950	rBV5	2170	2012	0.15%	0.019%
84	10.701	2982	2989	2990	rBV6	2311	2137	0.16%	0.020%
85	10.833	3026	3030	3031	rBV3	3647	2566	0.19%	0.024%
86	11.270	3155	3166	3183	rBV	679357	1042811	75.96%	9.746%
87	11.453	3221	3223	3226	rBV3	2703	1702	0.12%	0.016%
88	11.646	3272	3283	3298	rVB	697271	1108236	80.73%	10.358%
89	11.971	3381	3384	3385	rBV4	1848	1008	0.07%	0.009%
90	12.177	3446	3448	3449	rBV2	1511	788	0.06%	0.007%
91	12.726	3617	3619	3620	rBV2	1290	522	0.04%	0.005%
92	13.035	3713	3715	3716	rBV2	1184	522	0.04%	0.005%
93	13.161	3751	3754	3757	rBV4	1637	1322	0.10%	0.012%
94	13.775	3942	3945	3947	rBV3	1572	1221	0.09%	0.011%
95	13.810	3954	3956	3959	rBV3	1960	1299	0.09%	0.012%
96	14.369	4127	4130	4132	rBV3	1955	1513	0.11%	0.014%
97	14.463	4156	4159	4161	rBV3	1608	1008	0.07%	0.009%
98	14.556	4184	4188	4192	rVB7	2135	2008	0.15%	0.019%
99	15.312	4421	4423	4427	rBV5	1390	843	0.06%	0.008%
100	15.340	4429	4432	4435	rVB5	1720	1064	0.08%	0.010%


Sum of corrected areas: 10699661

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060920\
Data File : VV016735.D
Acq On : 09 Jun 2020 22:23
Operator : SY/MD
Sample : L2914-19
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E66

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

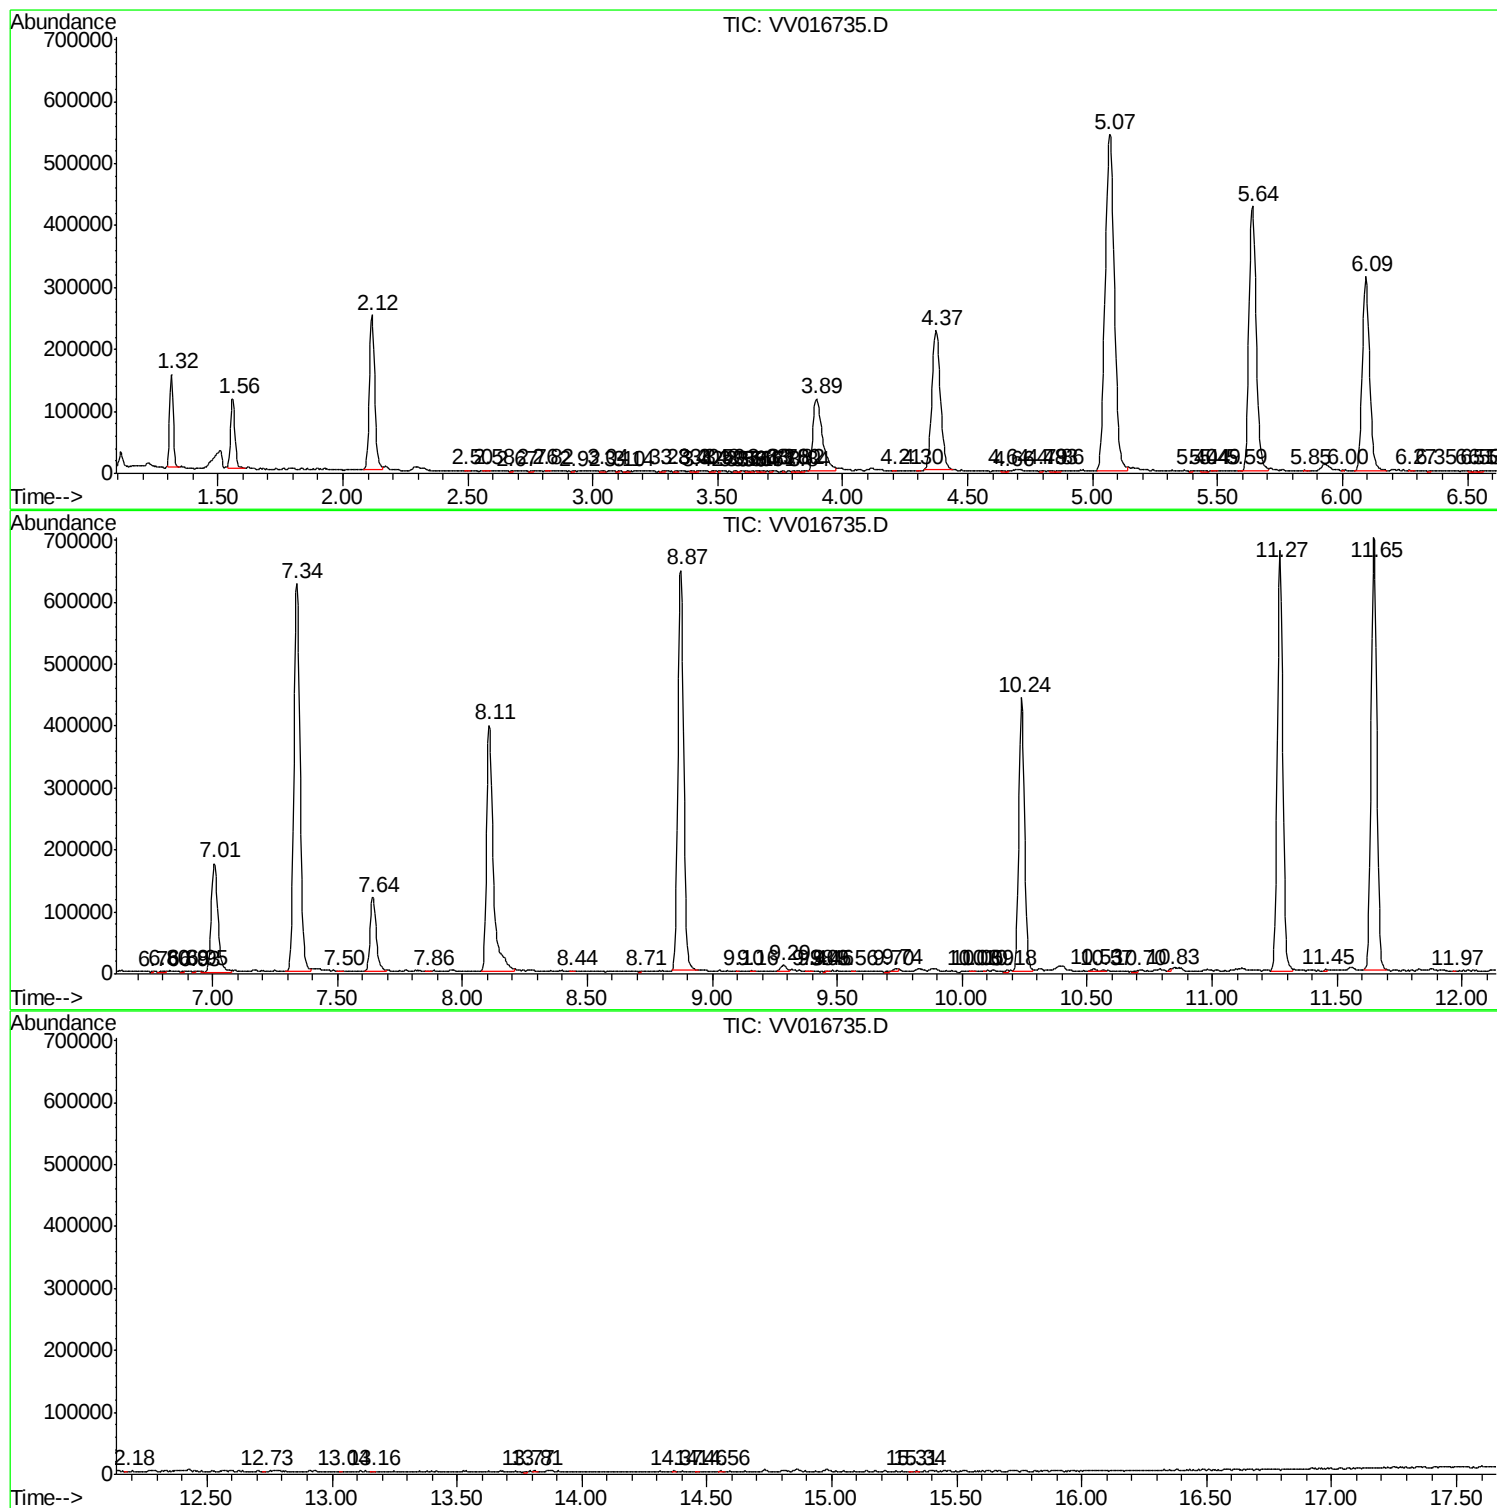

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016735.D
Acq On : 09 Jun 2020 22:23
Operator : SY/MD
Sample : L2914-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E66

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016735.D
Acq On : 09 Jun 2020 22:23
Operator : SY/MD
Sample : L2914-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E66

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc