

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016736.D
 Acq On : 09 Jun 2020 22:46
 Operator : SY/MD
 Sample : L2914-01DL 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9D86DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	80	rVB	210754	217883	17.06%	1.969%
2	1.557	139	145	158	rVB	114968	137325	10.75%	1.241%
3	2.116	310	319	333	rVB	237645	351180	27.49%	3.173%
4	2.914	560	567	571	rBV10	1578	1879	0.15%	0.017%
5	2.959	576	581	582	rBV5	1595	951	0.07%	0.009%
6	3.029	600	603	606	rBV3	1555	1117	0.09%	0.010%
7	3.052	606	610	612	rBV3	1085	994	0.08%	0.009%
8	3.161	642	644	647	rBV3	996	677	0.05%	0.006%
9	3.225	661	664	669	rBV6	1666	1785	0.14%	0.016%
10	3.357	702	705	708	rVB6	1278	863	0.07%	0.008%
11	3.377	708	711	713	rBV4	1305	877	0.07%	0.008%
12	3.653	792	797	800	rVB7	1263	982	0.08%	0.009%
13	3.714	813	816	819	rVB4	1359	936	0.07%	0.008%
14	3.733	819	822	823	rBV3	1030	628	0.05%	0.006%
15	3.894	859	872	902	rBV	121573	354483	27.75%	3.203%
16	4.258	980	985	988	rBV6	1768	1630	0.13%	0.015%
17	4.373	1006	1021	1042	rBV	221704	539746	42.25%	4.877%
18	4.804	1152	1155	1160	rBV7	1999	2310	0.18%	0.021%
19	4.913	1184	1189	1193	rVB8	1168	1063	0.08%	0.010%
20	4.987	1210	1212	1214	rBV3	1347	716	0.06%	0.006%
21	5.071	1219	1238	1244	rBV2	529351	1277444	100.00%	11.543%
22	5.640	1403	1415	1435	rBV	412833	813970	63.72%	7.355%
23	5.933	1492	1506	1524	rBV4	14203	34668	2.71%	0.313%
24	6.093	1544	1556	1582	rVB	307061	619816	48.52%	5.601%
25	6.290	1614	1617	1618	rBV3	1222	641	0.05%	0.006%
26	6.556	1697	1700	1702	rBV4	1569	1362	0.11%	0.012%
27	6.775	1765	1768	1773	rBV3	1672	1310	0.10%	0.012%
28	6.801	1773	1776	1777	rBV2	1283	704	0.06%	0.006%
29	6.859	1792	1794	1798	rBV5	1407	1050	0.08%	0.009%
30	6.952	1821	1823	1827	rVB5	1240	890	0.07%	0.008%
31	7.007	1830	1840	1858	rVV	167675	295153	23.10%	2.667%
32	7.241	1910	1913	1915	rBV5	1463	1055	0.08%	0.010%
33	7.338	1931	1943	1956	rBV	594791	1006654	78.80%	9.096%
34	7.412	1958	1966	1985	rVB	115172	201375	15.76%	1.820%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016736.D
 Acq On : 09 Jun 2020 22:46
 Operator : SY/MD
 Sample : L2914-01DL 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleID :
 F9D86DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	7.640	2028	2037	2054	rBV	123297	201193	15.75%	1.818%
36	7.830	2092	2096	2097	rBV5	1439	857	0.07%	0.008%
37	8.106	2171	2182	2216	rBV	396142	748733	58.61%	6.766%
38	8.543	2312	2318	2320	rBV6	1550	1452	0.11%	0.013%
39	8.595	2332	2334	2338	rVB5	1081	775	0.06%	0.007%
40	8.614	2338	2340	2342	rBV2	1589	1057	0.08%	0.010%
41	8.810	2398	2401	2403	rBV3	1234	850	0.07%	0.008%
42	8.823	2403	2405	2408	rVV3	2022	1125	0.09%	0.010%
43	8.875	2409	2421	2449	rVV	610843	1015084	79.46%	9.173%
44	9.035	2460	2471	2487	rBV	179129	284687	22.29%	2.573%
45	9.386	2578	2580	2582	rBV3	1263	744	0.06%	0.007%
46	9.566	2627	2636	2650	rVB	62226	95154	7.45%	0.860%
47	9.682	2669	2672	2675	rBV5	1347	1141	0.09%	0.010%
48	9.736	2685	2689	2692	rBV4	2160	2341	0.18%	0.021%
49	9.797	2701	2708	2711	rBV7	2587	3098	0.24%	0.028%
50	9.878	2729	2733	2736	rBV5	3483	3506	0.27%	0.032%
51	10.109	2798	2805	2814	rVB5	3606	6490	0.51%	0.059%
52	10.164	2818	2822	2826	rBV6	904	835	0.07%	0.008%
53	10.238	2833	2845	2862	rBV	435842	683825	53.53%	6.179%
54	10.675	2978	2981	2983	rBV4	1228	905	0.07%	0.008%
55	10.717	2990	2994	2997	rBV5	1581	1407	0.11%	0.013%
56	10.765	3002	3009	3017	rVV3	7050	10819	0.85%	0.098%
57	10.939	3055	3063	3071	rBV5	10214	15944	1.25%	0.144%
58	11.045	3093	3096	3098	rBV4	1557	928	0.07%	0.008%
59	11.199	3142	3144	3150	rBV6	1824	2154	0.17%	0.019%
60	11.270	3156	3166	3185	rVB	653713	978629	76.61%	8.843%
61	11.547	3245	3252	3262	rBV10	6644	12024	0.94%	0.109%
62	11.649	3272	3284	3297	rBV	685820	1072247	83.94%	9.689%
63	11.759	3316	3318	3321	rBV4	2216	1586	0.12%	0.014%
64	11.932	3368	3372	3374	rBV5	1306	786	0.06%	0.007%
65	12.019	3397	3399	3403	rVB5	1705	1159	0.09%	0.010%
66	12.045	3403	3407	3409	rBV4	1148	883	0.07%	0.008%
67	12.113	3425	3428	3429	rBV2	1696	887	0.07%	0.008%
68	12.235	3465	3466	3469	rBV3	1628	934	0.07%	0.008%
69	12.354	3499	3503	3505	rVB6	1736	1043	0.08%	0.009%
70	12.437	3526	3529	3532	rBV4	1622	1188	0.09%	0.011%
71	12.485	3542	3544	3546	rBV3	1123	712	0.06%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016736.D
 Acq On : 09 Jun 2020 22:46
 Operator : SY/MD
 Sample : L2914-01DL 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9D86DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.749	3622	3626	3629	rVB3	1246	750	0.06%	0.007%
73	12.817	3644	3647	3649	rBV3	1461	925	0.07%	0.008%
74	12.836	3649	3653	3655	rBV5	1565	1100	0.09%	0.010%
75	12.916	3676	3678	3680	rBV3	1831	938	0.07%	0.008%
76	12.968	3692	3694	3698	rBV5	1062	770	0.06%	0.007%
77	13.151	3749	3751	3755	rVB4	1329	801	0.06%	0.007%
78	13.251	3781	3782	3786	rVB4	1423	716	0.06%	0.006%
79	13.289	3788	3794	3797	rVV6	1584	1210	0.09%	0.011%
80	13.309	3798	3800	3803	rVB3	1109	639	0.05%	0.006%
81	13.354	3808	3814	3815	rBV4	1501	1427	0.11%	0.013%
82	13.376	3819	3821	3824	rVB4	1762	1094	0.09%	0.010%
83	13.405	3824	3830	3834	rBV9	1960	2232	0.17%	0.020%
84	13.592	3882	3888	3890	rBV7	1292	1298	0.10%	0.012%
85	13.981	4007	4009	4011	rBV4	1271	747	0.06%	0.007%
86	14.026	4020	4023	4028	rBV7	1901	1665	0.13%	0.015%
87	14.093	4040	4044	4046	rBV4	1638	983	0.08%	0.009%
88	14.177	4067	4070	4073	rVB3	2106	1289	0.10%	0.012%
89	14.196	4073	4076	4080	rBV3	1116	1152	0.09%	0.010%
90	14.254	4092	4094	4096	rVB3	1381	698	0.05%	0.006%
91	14.270	4096	4099	4103	rBV5	2162	1576	0.12%	0.014%
92	14.395	4136	4138	4142	rVB5	1618	1019	0.08%	0.009%
93	14.453	4154	4156	4159	rBV3	1258	923	0.07%	0.008%
94	14.691	4227	4230	4232	rBV4	1487	777	0.06%	0.007%
95	14.900	4290	4295	4299	rBV6	1854	1774	0.14%	0.016%
96	15.022	4331	4333	4336	rBV4	1338	732	0.06%	0.007%
97	15.090	4350	4354	4358	rBV5	2226	1719	0.13%	0.016%
98	15.112	4358	4361	4366	rVV6	2277	1985	0.16%	0.018%
99	15.267	4406	4409	4417	rBV9	2044	2865	0.22%	0.026%
100	15.447	4460	4465	4466	rBV5	1465	1322	0.10%	0.012%


Sum of corrected areas: 11066425

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060920\
Data File : VV016736.D
Acq On : 09 Jun 2020 22:46
Operator : SY/MD
Sample : L2914-01DL 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9D86DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

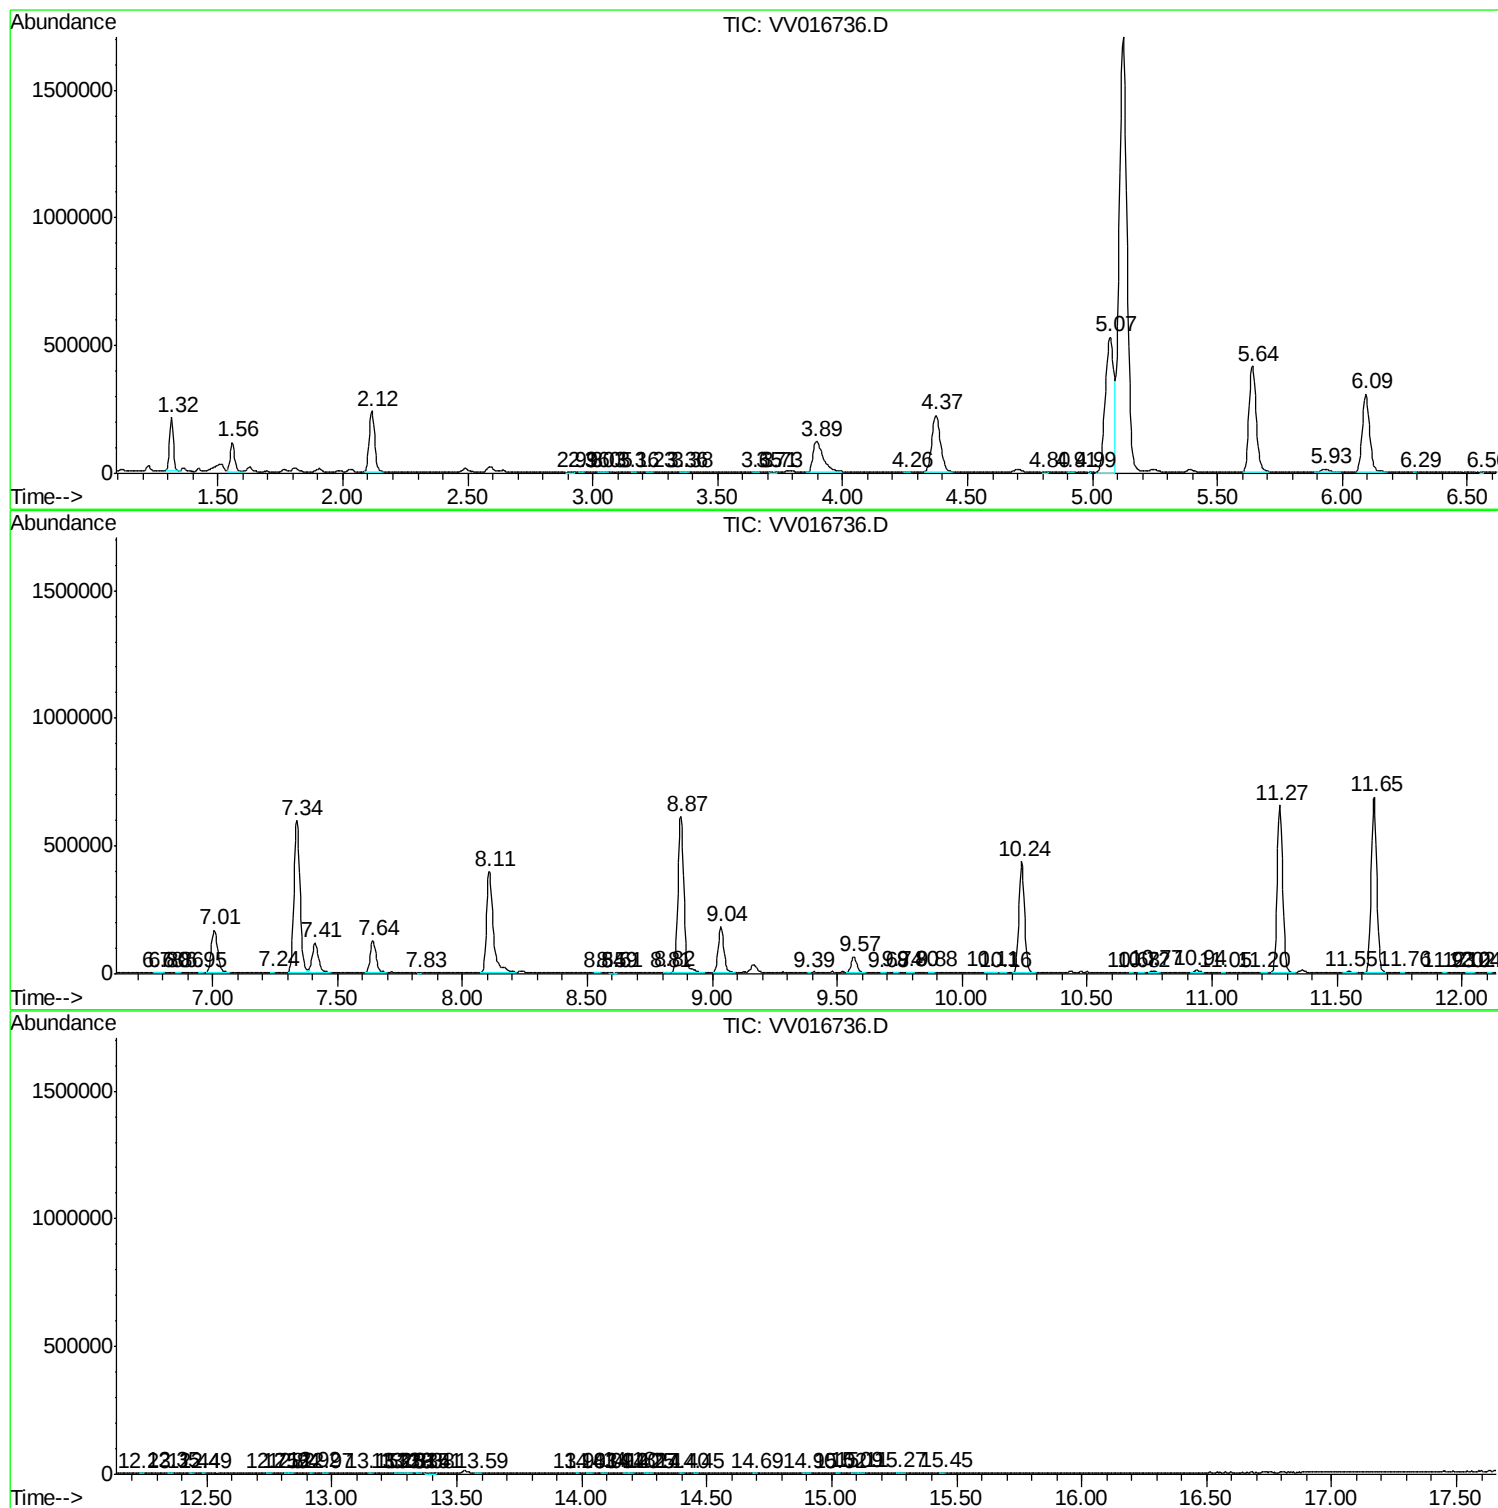

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016736.D
Acq On : 09 Jun 2020 22:46
Operator : SY/MD
Sample : L2914-01DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9D86DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016736.D
Acq On : 09 Jun 2020 22:46
Operator : SY/MD
Sample : L2914-01DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9D86DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc