

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016738.D
 Acq On : 09 Jun 2020 23:34
 Operator : SY/MD
 Sample : L2914-03 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9D96

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	79	rVB	163508	171644	13.04%	1.579%
2	1.553	138	144	158	rVB	111588	131680	10.00%	1.211%
3	2.116	309	319	332	rBV	232909	353213	26.84%	3.248%
4	2.418	412	413	414	rBV	764	282	0.02%	0.003%
5	2.585	457	465	473	rBV2	9575	17413	1.32%	0.160%
6	2.830	537	541	545	rVB6	1194	968	0.07%	0.009%
7	2.875	552	555	556	rBV2	913	360	0.03%	0.003%
8	2.917	565	568	569	rBV3	1021	501	0.04%	0.005%
9	2.942	574	576	577	rBV2	955	443	0.03%	0.004%
10	3.058	611	612	615	rBV3	908	438	0.03%	0.004%
11	3.100	618	625	628	rBV8	1504	1981	0.15%	0.018%
12	3.155	640	642	644	rBV3	1447	819	0.06%	0.008%
13	3.521	750	756	759	rBV7	1224	1265	0.10%	0.012%
14	3.585	773	776	780	rBV3	1101	964	0.07%	0.009%
15	3.627	788	789	792	rBV3	804	322	0.02%	0.003%
16	3.666	795	801	804	rBV8	1525	1513	0.11%	0.014%
17	3.743	823	825	826	rBV2	1049	383	0.03%	0.004%
18	3.855	853	860	861	rBV6	1796	2010	0.15%	0.018%
19	3.894	862	872	906	rVV2	119709	338554	25.72%	3.114%
20	4.109	938	939	941	rBV2	1141	444	0.03%	0.004%
21	4.312	1001	1002	1003	rBV	989	342	0.03%	0.003%
22	4.373	1004	1021	1041	rVV2	225302	553752	42.07%	5.093%
23	4.656	1106	1109	1110	rBV3	1843	1129	0.09%	0.010%
24	4.923	1190	1192	1196	rVB5	1733	1007	0.08%	0.009%
25	4.949	1196	1200	1204	rBV6	1423	1280	0.10%	0.012%
26	5.068	1218	1237	1245	rBV2	531336	1316221	100.00%	12.105%
27	5.640	1402	1415	1433	rBV	434148	856284	65.06%	7.875%
28	5.868	1484	1486	1489	rBV5	1186	515	0.04%	0.005%
29	6.093	1541	1556	1578	rBV	311078	627371	47.66%	5.770%
30	6.508	1682	1685	1686	rBV3	1484	719	0.05%	0.007%
31	6.547	1695	1697	1698	rBV2	1006	368	0.03%	0.003%
32	6.717	1748	1750	1751	rBV2	1389	580	0.04%	0.005%
33	6.756	1759	1762	1763	rBV3	1567	1063	0.08%	0.010%
34	6.868	1796	1797	1799	rBV2	819	333	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016738.D
 Acq On : 09 Jun 2020 23:34
 Operator : SY/MD
 Sample : L2914-03 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9D96

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.916	1809	1812	1814	rBV4	1366	805	0.06%	0.007%
36	7.006	1828	1840	1862	rBV	169203	303953	23.09%	2.795%
37	7.135	1876	1880	1883	rBV4	2128	1423	0.11%	0.013%
38	7.167	1883	1890	1892	rBV7	2392	2931	0.22%	0.027%
39	7.232	1908	1910	1912	rBV3	1748	925	0.07%	0.009%
40	7.248	1912	1915	1917	rBV3	3380	2473	0.19%	0.023%
41	7.338	1930	1943	1957	rBV	595803	1024039	77.80%	9.418%
42	7.412	1959	1966	1983	rVB	85793	150817	11.46%	1.387%
43	7.640	2028	2037	2049	rBV	119645	201136	15.28%	1.850%
44	7.920	2122	2124	2125	rBV2	1069	378	0.03%	0.003%
45	8.010	2148	2152	2153	rBV3	1442	1030	0.08%	0.009%
46	8.106	2172	2182	2213	rBV	388869	748857	56.89%	6.887%
47	8.421	2278	2280	2281	rBV2	1767	689	0.05%	0.006%
48	8.579	2328	2329	2331	rVB2	1272	357	0.03%	0.003%
49	8.604	2335	2337	2339	rBV2	1123	676	0.05%	0.006%
50	8.701	2366	2367	2369	rVB2	1165	244	0.02%	0.002%
51	8.765	2385	2387	2389	rBV3	1174	577	0.04%	0.005%
52	8.788	2389	2394	2397	rBV6	1502	1659	0.13%	0.015%
53	8.804	2397	2399	2402	rBV4	1395	957	0.07%	0.009%
54	8.875	2410	2421	2434	rBV	642149	1030000	78.25%	9.473%
55	9.035	2462	2471	2486	rBV	82192	133306	10.13%	1.226%
56	9.405	2580	2586	2597	rBV	6165	11043	0.84%	0.102%
57	9.569	2629	2637	2650	rVB2	22785	36755	2.79%	0.338%
58	9.682	2669	2672	2673	rBV3	1147	515	0.04%	0.005%
59	9.694	2674	2676	2679	rVB3	1752	881	0.07%	0.008%
60	9.720	2681	2684	2687	rBV4	2096	1785	0.14%	0.016%
61	10.103	2794	2803	2814	rBV4	5220	9804	0.74%	0.090%
62	10.238	2834	2845	2861	rBV	428872	667180	50.69%	6.136%
63	10.701	2987	2989	2993	rBV4	2665	2355	0.18%	0.022%
64	11.270	3155	3166	3185	rBV	677198	1034909	78.63%	9.518%
65	11.479	3229	3231	3233	rBV3	1067	521	0.04%	0.005%
66	11.530	3243	3247	3248	rBV4	2731	1574	0.12%	0.014%
67	11.646	3270	3283	3299	rBV	677239	1077676	81.88%	9.911%
68	11.929	3368	3371	3376	rBV7	2264	2350	0.18%	0.022%
69	12.038	3402	3405	3408	rBV4	1399	885	0.07%	0.008%
70	12.054	3408	3410	3412	rBV3	945	660	0.05%	0.006%
71	12.267	3473	3476	3479	rVB4	2354	1162	0.09%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016738.D
 Acq On : 09 Jun 2020 23:34
 Operator : SY/MD
 Sample : L2914-03 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9D96

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.286	3479	3482	3483	rBV3	897	459	0.03%	0.004%
73	12.302	3485	3487	3491	rVB5	1853	1182	0.09%	0.011%
74	12.517	3551	3554	3556	rBV3	1896	1135	0.09%	0.010%
75	12.550	3561	3564	3565	rBV2	1014	570	0.04%	0.005%
76	12.707	3611	3613	3615	rBV3	1441	730	0.06%	0.007%
77	12.768	3630	3632	3634	rBV3	1382	734	0.06%	0.007%
78	13.058	3716	3722	3729	rBV3	2479	3937	0.30%	0.036%
79	13.112	3735	3739	3742	rBV5	1330	1115	0.08%	0.010%
80	13.154	3750	3752	3753	rBV2	897	383	0.03%	0.004%
81	13.289	3792	3794	3796	rBV3	1011	414	0.03%	0.004%
82	13.321	3802	3804	3805	rBV2	761	356	0.03%	0.003%
83	13.373	3815	3820	3821	rBV3	1364	1032	0.08%	0.009%
84	13.398	3826	3828	3830	rVV3	1120	534	0.04%	0.005%
85	13.443	3840	3842	3844	rBV3	1186	789	0.06%	0.007%
86	13.662	3905	3910	3913	rBV7	1888	2143	0.16%	0.020%
87	13.807	3953	3955	3959	rVB5	1472	635	0.05%	0.006%
88	13.932	3990	3994	3998	rBV5	1903	1354	0.10%	0.012%
89	14.045	4025	4029	4033	rBV6	1942	1742	0.13%	0.016%
90	14.161	4061	4065	4066	rBV4	1369	901	0.07%	0.008%
91	14.186	4071	4073	4076	rVV4	1573	678	0.05%	0.006%
92	14.202	4076	4078	4080	rVB2	1451	562	0.04%	0.005%
93	14.218	4080	4083	4087	rBV5	1373	1127	0.09%	0.010%
94	14.302	4105	4109	4118	rVB5	1481	2325	0.18%	0.021%
95	14.595	4197	4200	4203	rBV5	1280	1059	0.08%	0.010%
96	15.032	4334	4336	4337	rBV3	1224	424	0.03%	0.004%
97	15.093	4353	4355	4357	rBV3	1627	630	0.05%	0.006%
98	15.318	4423	4425	4428	rBV4	1677	976	0.07%	0.009%
99	15.678	4536	4537	4538	rBV	1050	282	0.02%	0.003%
100	15.932	4614	4616	4619	rBV3	2879	1631	0.12%	0.015%


Sum of corrected areas: 10873287

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060920\
Data File : VV016738.D
Acq On : 09 Jun 2020 23:34
Operator : SY/MD
Sample : L2914-03 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9D96

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

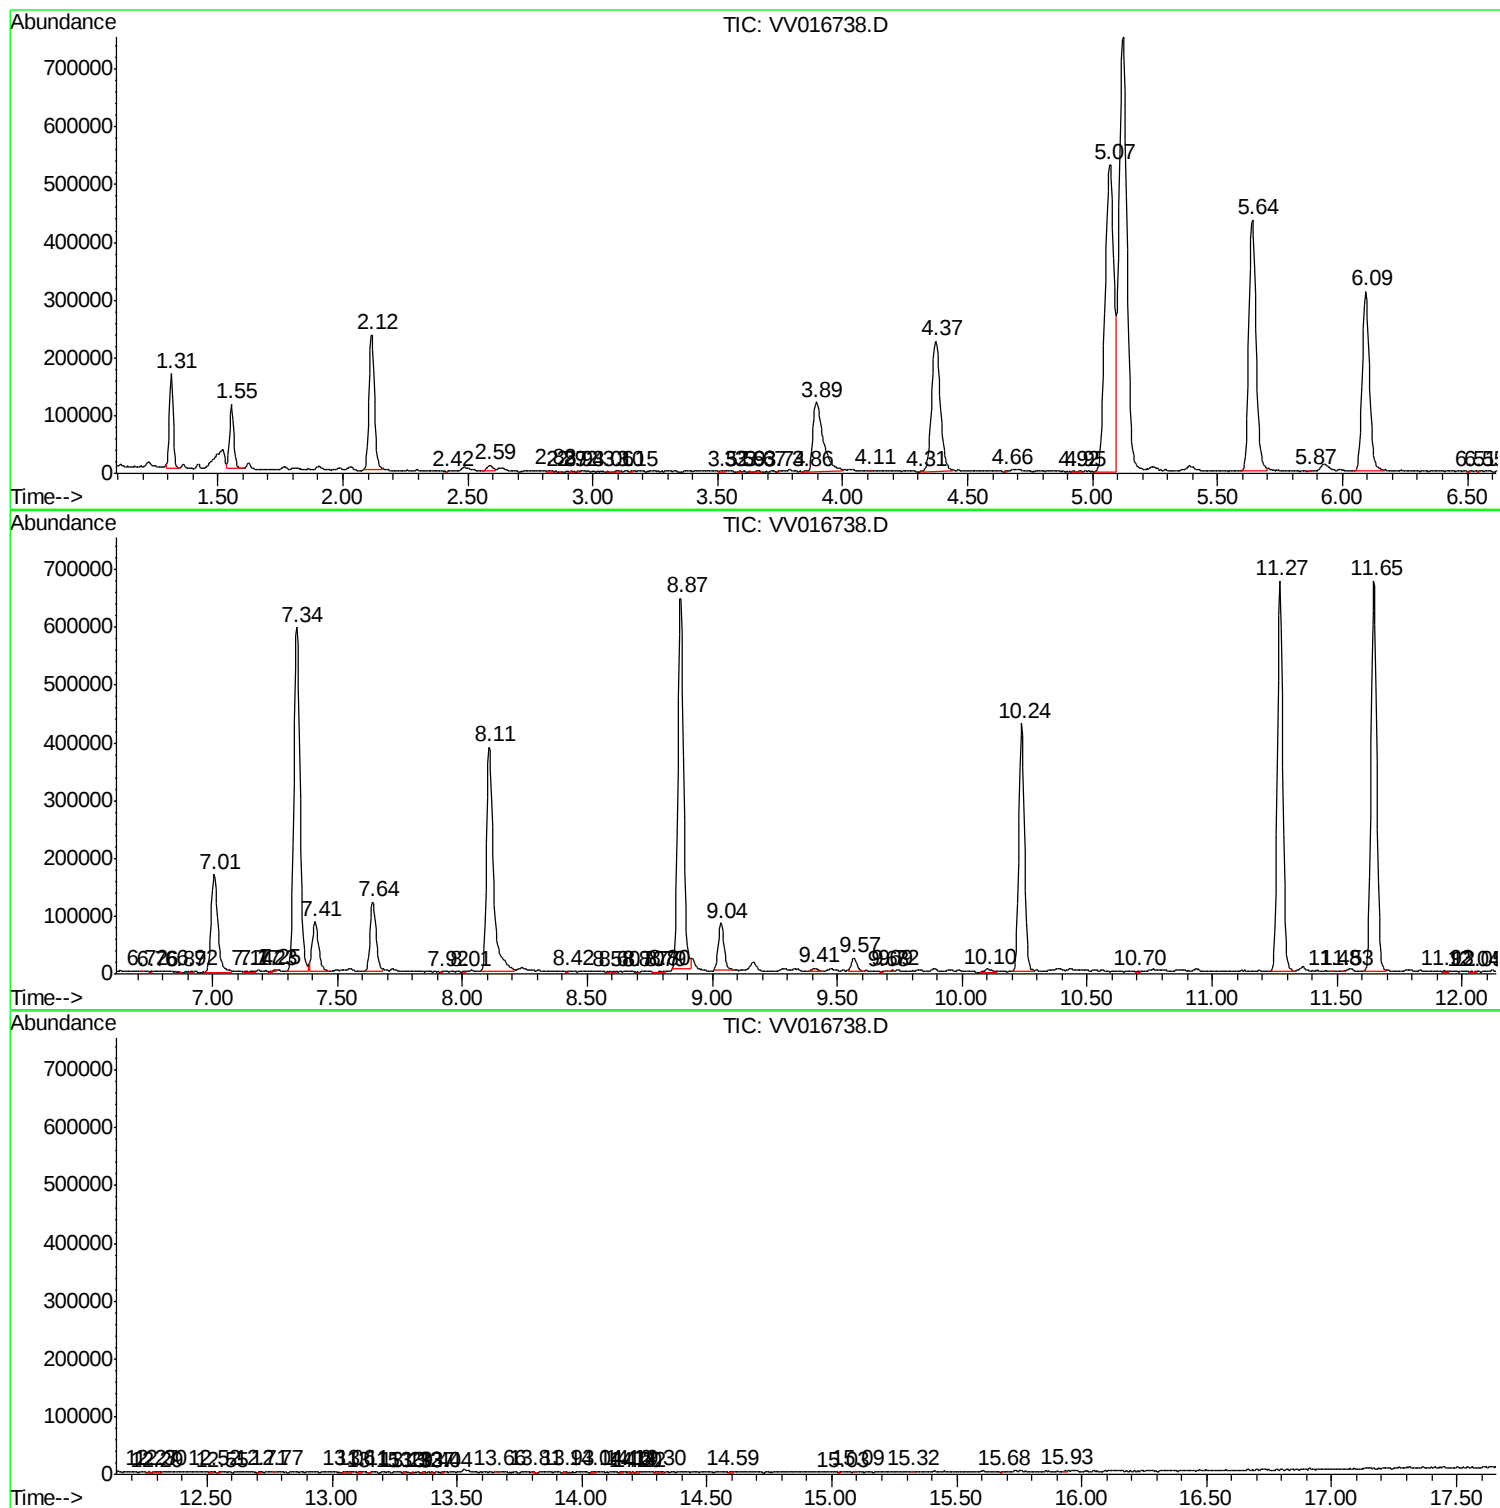

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016738.D
Acq On : 09 Jun 2020 23:34
Operator : SY/MD
Sample : L2914-03 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9D96

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016738.D
Acq On : 09 Jun 2020 23:34
Operator : SY/MD
Sample : L2914-03 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9D96

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc