

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016741.D
 Acq On : 10 Jun 2020 00:45
 Operator : SY/MD
 Sample : L2914-06 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	80	rVB	174199	184935	13.29%	1.699%
2	1.557	140	145	160	rVB	109708	136789	9.83%	1.257%
3	2.116	310	319	333	rBV	252062	367436	26.40%	3.375%
4	2.762	514	520	522	rBV6	1830	1807	0.13%	0.017%
5	2.836	540	543	548	rBV7	1523	966	0.07%	0.009%
6	2.859	548	550	555	rBV4	1221	1013	0.07%	0.009%
7	2.901	560	563	564	rBV2	903	551	0.04%	0.005%
8	3.209	656	659	661	rBV3	1307	575	0.04%	0.005%
9	3.241	666	669	671	rBV3	1745	1074	0.08%	0.010%
10	3.566	766	770	772	rBV4	1859	1669	0.12%	0.015%
11	3.614	784	785	791	rVB4	1469	706	0.05%	0.006%
12	3.647	791	795	798	rBV6	955	901	0.06%	0.008%
13	3.852	858	859	861	rBV3	1254	587	0.04%	0.005%
14	3.894	862	872	904	rVV	118341	333480	23.96%	3.063%
15	4.257	983	985	988	rVB5	1560	803	0.06%	0.007%
16	4.373	1008	1021	1051	rVB	228395	553594	39.78%	5.085%
17	4.663	1108	1111	1112	rBV3	1622	870	0.06%	0.008%
18	4.782	1145	1148	1151	rBV5	1186	946	0.07%	0.009%
19	4.978	1207	1209	1213	rVB4	1005	706	0.05%	0.006%
20	5.068	1219	1237	1247	rBV2	545059	1391728	100.00%	12.785%
21	5.450	1352	1356	1365	rVB2	2807	3492	0.25%	0.032%
22	5.492	1365	1369	1373	rBV6	2305	2745	0.20%	0.025%
23	5.640	1401	1415	1444	rBV	454959	909072	65.32%	8.351%
24	5.839	1475	1477	1480	rBV4	987	586	0.04%	0.005%
25	5.926	1494	1504	1513	rBV3	15250	30175	2.17%	0.277%
26	6.093	1543	1556	1576	rBV	317323	636590	45.74%	5.848%
27	6.376	1642	1644	1650	rVB5	1589	1325	0.10%	0.012%
28	6.402	1650	1652	1655	rBV3	921	560	0.04%	0.005%
29	6.441	1662	1664	1670	rVB6	1884	1311	0.09%	0.012%
30	6.476	1670	1675	1680	rBV9	1734	1988	0.14%	0.018%
31	6.524	1688	1690	1693	rBV4	1339	643	0.05%	0.006%
32	6.643	1721	1727	1728	rBV5	2341	2407	0.17%	0.022%
33	6.720	1749	1751	1754	rVB4	1538	663	0.05%	0.006%
34	6.765	1762	1765	1770	rBV7	1437	1188	0.09%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016741.D
 Acq On : 10 Jun 2020 00:45
 Operator : SY/MD
 Sample : L2914-06 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.807	1775	1778	1779	rBV3	912	551	0.04%	0.005%
36	7.007	1830	1840	1861	rBV	169756	301576	21.67%	2.770%
37	7.170	1887	1891	1893	rBV3	2234	1530	0.11%	0.014%
38	7.338	1931	1943	1959	rBV	620124	1069546	76.85%	9.825%
39	7.592	2020	2022	2025	rBV3	1602	1139	0.08%	0.010%
40	7.640	2028	2037	2054	rVV	121219	207797	14.93%	1.909%
41	7.875	2108	2110	2115	rVB5	1703	1135	0.08%	0.010%
42	8.106	2172	2182	2214	rBV	386534	737976	53.03%	6.779%
43	8.379	2265	2267	2269	rBV2	1327	648	0.05%	0.006%
44	8.756	2380	2384	2386	rBV5	1375	1049	0.08%	0.010%
45	8.875	2409	2421	2442	rBV	677154	1104415	79.36%	10.145%
46	9.006	2460	2462	2464	rBV3	1173	689	0.05%	0.006%
47	9.254	2536	2539	2540	rBV3	1422	964	0.07%	0.009%
48	9.469	2600	2606	2607	rBV4	3087	2681	0.19%	0.025%
49	9.672	2666	2669	2672	rBV3	1773	1340	0.10%	0.012%
50	9.736	2682	2689	2692	rBV8	2312	2790	0.20%	0.026%
51	9.794	2705	2707	2713	rBV7	1275	1533	0.11%	0.014%
52	9.852	2723	2725	2728	rBV3	1160	639	0.05%	0.006%
53	9.942	2749	2753	2754	rBV3	1001	629	0.05%	0.006%
54	10.174	2824	2825	2828	rVB3	1234	642	0.05%	0.006%
55	10.238	2834	2845	2866	rVB	427422	666534	47.89%	6.123%
56	10.608	2957	2960	2962	rBV4	1645	1125	0.08%	0.010%
57	10.669	2975	2979	2981	rBV4	1859	1612	0.12%	0.015%
58	10.743	2999	3002	3003	rBV3	2162	1013	0.07%	0.009%
59	10.939	3056	3063	3072	rBV6	7287	11866	0.85%	0.109%
60	11.006	3079	3084	3087	rBV7	1291	1454	0.10%	0.013%
61	11.042	3091	3095	3099	rBV5	2019	2225	0.16%	0.020%
62	11.270	3153	3166	3186	rBV	698518	1057194	75.96%	9.711%
63	11.473	3225	3229	3230	rBV4	1373	972	0.07%	0.009%
64	11.534	3246	3248	3249	rBV2	1436	687	0.05%	0.006%
65	11.646	3271	3283	3301	rBV	695470	1093829	78.60%	10.048%
66	11.826	3334	3339	3341	rBV3	1886	1518	0.11%	0.014%
67	11.900	3359	3362	3363	rBV2	1446	611	0.04%	0.006%
68	11.939	3372	3374	3376	rVB3	1641	656	0.05%	0.006%
69	11.984	3384	3388	3392	rVB6	1982	1575	0.11%	0.014%
70	12.006	3392	3395	3397	rBV4	1227	1015	0.07%	0.009%
71	12.116	3425	3429	3432	rBV5	1419	1401	0.10%	0.013%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016741.D
 Acq On : 10 Jun 2020 00:45
 Operator : SY/MD
 Sample : L2914-06 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.247	3467	3470	3472	rBV3	811	657	0.05%	0.006%
73	12.331	3493	3496	3499	rVB5	1821	1348	0.10%	0.012%
74	12.347	3499	3501	3503	rBV4	1261	574	0.04%	0.005%
75	12.469	3537	3539	3542	rBV3	1864	1119	0.08%	0.010%
76	12.508	3548	3551	3554	rBV4	1540	969	0.07%	0.009%
77	12.656	3594	3597	3599	rBV4	1246	918	0.07%	0.008%
78	12.743	3619	3624	3625	rBV4	1661	1043	0.07%	0.010%
79	12.820	3643	3648	3650	rBV5	1216	1231	0.09%	0.011%
80	12.897	3670	3672	3674	rBV3	1437	957	0.07%	0.009%
81	13.051	3717	3720	3722	rBV3	1778	849	0.06%	0.008%
82	13.186	3759	3762	3763	rBV3	1113	557	0.04%	0.005%
83	13.476	3850	3852	3858	rBV7	871	683	0.05%	0.006%
84	13.730	3929	3931	3935	rVB3	1391	767	0.06%	0.007%
85	13.755	3935	3939	3940	rBV3	1695	1417	0.10%	0.013%
86	13.871	3971	3975	3977	rBV6	1408	961	0.07%	0.009%
87	13.903	3983	3985	3988	rBV3	1447	687	0.05%	0.006%
88	13.948	3994	3999	4001	rBV6	2214	1968	0.14%	0.018%
89	14.090	4040	4043	4046	rBV3	1347	792	0.06%	0.007%
90	14.202	4073	4078	4079	rBV4	1638	1111	0.08%	0.010%
91	14.218	4081	4083	4085	rVB3	1396	532	0.04%	0.005%
92	14.392	4135	4137	4141	rVB5	1114	748	0.05%	0.007%
93	14.460	4156	4158	4159	rBV2	1390	746	0.05%	0.007%
94	14.662	4218	4221	4223	rBV4	1492	824	0.06%	0.008%
95	14.807	4264	4266	4269	rBV4	1734	1421	0.10%	0.013%
96	15.074	4347	4349	4351	rBV3	864	567	0.04%	0.005%
97	15.112	4358	4361	4363	rBV3	1057	704	0.05%	0.006%
98	15.283	4410	4414	4416	rBV4	1158	786	0.06%	0.007%
99	15.299	4416	4419	4421	rBV4	2281	1640	0.12%	0.015%
100	15.987	4631	4633	4636	rBV4	1562	1010	0.07%	0.009%


Sum of corrected areas: 10886023

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060920\
Data File : VV016741.D
Acq On : 10 Jun 2020 00:45
Operator : SY/MD
Sample : L2914-06 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

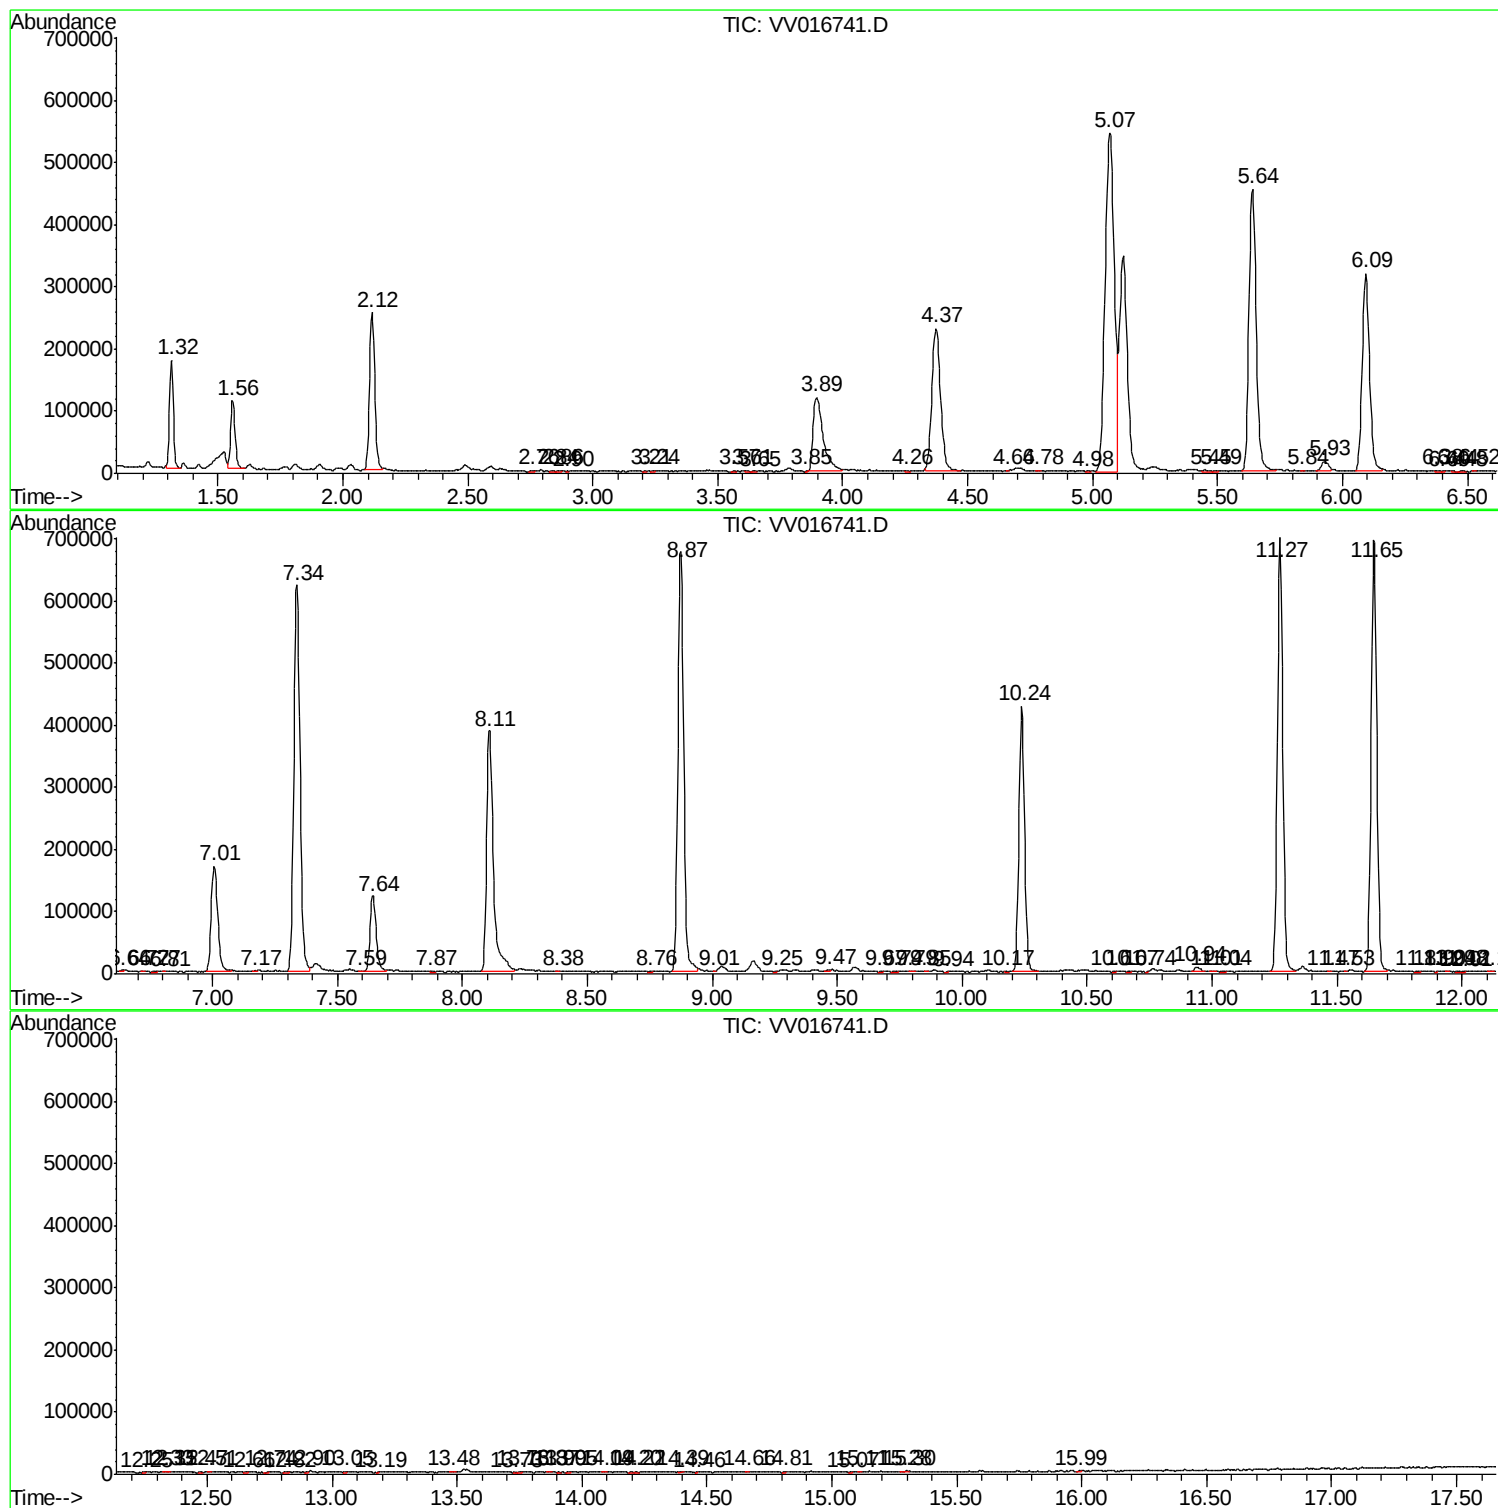

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016741.D
Acq On : 10 Jun 2020 00:45
Operator : SY/MD
Sample : L2914-06 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016741.D
Acq On : 10 Jun 2020 00:45
Operator : SY/MD
Sample : L2914-06 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc