

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016743.D
 Acq On : 10 Jun 2020 01:33
 Operator : SY/MD
 Sample : L2901-07 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTT2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	63	70	82	rVB2	277641	292846	11.65%	1.929%
2	1.557	139	145	158	rVB	105787	130167	5.18%	0.857%
3	2.116	309	319	336	rVB	244101	361599	14.39%	2.382%
4	2.428	413	416	418	rBV4	1304	892	0.04%	0.006%
5	2.602	466	470	471	rBV3	1422	782	0.03%	0.005%
6	2.721	504	507	510	rBV5	1475	751	0.03%	0.005%
7	2.849	542	547	551	rVB8	1742	2022	0.08%	0.013%
8	2.872	551	554	557	rBV5	1591	1245	0.05%	0.008%
9	2.971	581	585	588	rVB4	1602	1056	0.04%	0.007%
10	3.039	602	606	608	rBV5	1271	1143	0.05%	0.008%
11	3.061	611	613	620	rBV8	1404	1214	0.05%	0.008%
12	3.116	628	630	633	rBV3	713	625	0.02%	0.004%
13	3.174	645	648	650	rBV4	1593	1095	0.04%	0.007%
14	3.357	702	705	710	rVB6	1477	834	0.03%	0.005%
15	3.402	717	719	723	rBV7	1287	790	0.03%	0.005%
16	3.450	731	734	736	rBV4	1612	867	0.03%	0.006%
17	3.534	756	760	764	rBV6	1314	1344	0.05%	0.009%
18	3.637	787	792	794	rBV4	1293	1170	0.05%	0.008%
19	3.714	815	816	820	rBV3	1113	888	0.04%	0.006%
20	3.791	838	840	844	rVB5	1686	766	0.03%	0.005%
21	3.933	861	884	918	rBV2	866579	2354057	93.68%	15.505%
22	4.303	996	999	1002	rBV4	1527	968	0.04%	0.006%
23	4.373	1008	1021	1046	rVB	221749	541113	21.53%	3.564%
24	4.547	1073	1075	1078	rVB4	1986	1012	0.04%	0.007%
25	4.647	1102	1106	1107	rBV2	1631	1013	0.04%	0.007%
26	4.888	1179	1181	1184	rVB3	1724	760	0.03%	0.005%
27	5.068	1219	1237	1269	rBV2	520876	1354556	53.90%	8.922%
28	5.640	1402	1415	1438	rVB	428359	854759	34.01%	5.630%
29	5.936	1493	1507	1538	rVB	1305682	2512952	100.00%	16.552%
30	6.093	1544	1556	1576	rVB	306527	614244	24.44%	4.046%
31	6.492	1678	1680	1683	rVV4	1544	836	0.03%	0.006%
32	6.508	1683	1685	1688	rVB3	1450	731	0.03%	0.005%
33	6.576	1704	1706	1707	rBV2	1352	621	0.02%	0.004%
34	6.627	1719	1722	1723	rBV3	1401	882	0.04%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016743.D
 Acq On : 10 Jun 2020 01:33
 Operator : SY/MD
 Sample : L2901-07 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTT2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.746	1755	1759	1763	rBV7	1560	1395	0.06%	0.009%
36	6.939	1817	1819	1822	rBV4	914	629	0.03%	0.004%
37	7.007	1829	1840	1864	rVV	164805	298578	11.88%	1.967%
38	7.338	1930	1943	1963	rBV	606506	1043582	41.53%	6.874%
39	7.640	2028	2037	2052	rBV	116305	197105	7.84%	1.298%
40	7.984	2142	2144	2146	rBV3	1662	731	0.03%	0.005%
41	8.042	2160	2162	2165	rVB3	1365	760	0.03%	0.005%
42	8.106	2172	2182	2215	rVV	382937	729582	29.03%	4.805%
43	8.396	2270	2272	2274	rBV3	1667	833	0.03%	0.005%
44	8.428	2278	2282	2283	rBV3	2990	1871	0.07%	0.012%
45	8.492	2299	2302	2305	rBV5	1882	1397	0.06%	0.009%
46	8.540	2313	2317	2320	rBV5	1716	993	0.04%	0.007%
47	8.875	2409	2421	2442	rBV	641613	1036163	41.23%	6.825%
48	9.164	2509	2511	2512	rBV2	1285	638	0.03%	0.004%
49	9.479	2602	2609	2611	rBV7	1811	1816	0.07%	0.012%
50	9.643	2657	2660	2662	rBV4	1173	632	0.03%	0.004%
51	9.672	2667	2669	2671	rBV2	1537	775	0.03%	0.005%
52	10.019	2774	2777	2778	rBV3	1978	1254	0.05%	0.008%
53	10.238	2830	2845	2859	rBV	422345	659404	26.24%	4.343%
54	10.379	2887	2889	2893	rBV4	1237	738	0.03%	0.005%
55	10.582	2950	2952	2955	rVB4	1668	708	0.03%	0.005%
56	10.598	2955	2957	2960	rVB3	1918	925	0.04%	0.006%
57	10.675	2975	2981	2989	rBV10	1467	1951	0.08%	0.013%
58	10.724	2993	2996	2997	rBV2	1337	633	0.03%	0.004%
59	10.765	3005	3009	3011	rBV4	1750	1347	0.05%	0.009%
60	10.936	3057	3062	3064	rBV5	1024	866	0.03%	0.006%
61	10.978	3070	3075	3077	rBV7	1680	1160	0.05%	0.008%
62	10.990	3077	3079	3083	rVB5	2158	1364	0.05%	0.009%
63	11.071	3102	3104	3107	rBV3	1114	778	0.03%	0.005%
64	11.164	3129	3133	3134	rBV2	1259	750	0.03%	0.005%
65	11.203	3142	3145	3149	rVB4	1354	949	0.04%	0.006%
66	11.225	3149	3152	3153	rBV3	989	663	0.03%	0.004%
67	11.270	3155	3166	3184	rVV	675218	1028132	40.91%	6.772%
68	11.405	3204	3208	3212	rBV6	2251	1621	0.06%	0.011%
69	11.543	3248	3251	3253	rBV4	1107	678	0.03%	0.004%
70	11.601	3266	3269	3270	rBV3	1452	868	0.03%	0.006%
71	11.646	3272	3283	3299	rVV	682621	1088819	43.33%	7.172%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016743.D
 Acq On : 10 Jun 2020 01:33
 Operator : SY/MD
 Sample : L2901-07 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTT2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.810	3333	3334	3339	rVB4	2207	1313	0.05%	0.009%
73	11.868	3349	3352	3354	rBV4	1258	715	0.03%	0.005%
74	12.016	3395	3398	3400	rBV3	1351	886	0.04%	0.006%
75	12.113	3425	3428	3433	rBV6	1761	1296	0.05%	0.009%
76	12.408	3514	3520	3523	rBV6	1365	1487	0.06%	0.010%
77	12.547	3560	3563	3566	rBV4	1297	1039	0.04%	0.007%
78	12.588	3572	3576	3578	rBV3	1746	1259	0.05%	0.008%
79	12.717	3611	3616	3617	rBV5	1637	1109	0.04%	0.007%
80	12.743	3622	3624	3627	rBV3	1171	746	0.03%	0.005%
81	12.788	3637	3638	3642	rVB3	1163	811	0.03%	0.005%
82	12.810	3643	3645	3650	rVB6	1644	952	0.04%	0.006%
83	12.968	3692	3694	3700	rVB3	1298	753	0.03%	0.005%
84	13.039	3713	3716	3718	rVB3	1215	766	0.03%	0.005%
85	13.096	3730	3734	3735	rBV4	1301	763	0.03%	0.005%
86	13.186	3760	3762	3768	rVB7	2233	1677	0.07%	0.011%
87	13.228	3768	3775	3778	rBV8	1799	1794	0.07%	0.012%
88	13.273	3785	3789	3790	rBV3	1100	617	0.02%	0.004%
89	13.305	3795	3799	3802	rVB4	2004	1531	0.06%	0.010%
90	13.328	3802	3806	3808	rVB4	1566	1122	0.04%	0.007%
91	13.344	3808	3811	3813	rBV3	1451	1042	0.04%	0.007%
92	13.421	3832	3835	3839	rVB6	906	661	0.03%	0.004%
93	13.627	3895	3899	3901	rBV3	1679	920	0.04%	0.006%
94	13.640	3901	3903	3905	rBV3	1263	784	0.03%	0.005%
95	13.707	3922	3924	3928	rVB4	1996	1183	0.05%	0.008%
96	13.736	3929	3933	3935	rBV4	1702	1220	0.05%	0.008%
97	13.894	3979	3982	3986	rVB3	1522	899	0.04%	0.006%
98	13.981	4007	4009	4013	rBV5	1654	1179	0.05%	0.008%
99	15.228	4396	4397	4401	rBV4	1330	978	0.04%	0.006%
100	15.366	4436	4440	4441	rBV3	1522	1199	0.05%	0.008%


Sum of corrected areas: 15182389

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060920\
Data File : VV016743.D
Acq On : 10 Jun 2020 01:33
Operator : SY/MD
Sample : L2901-07 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTT2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

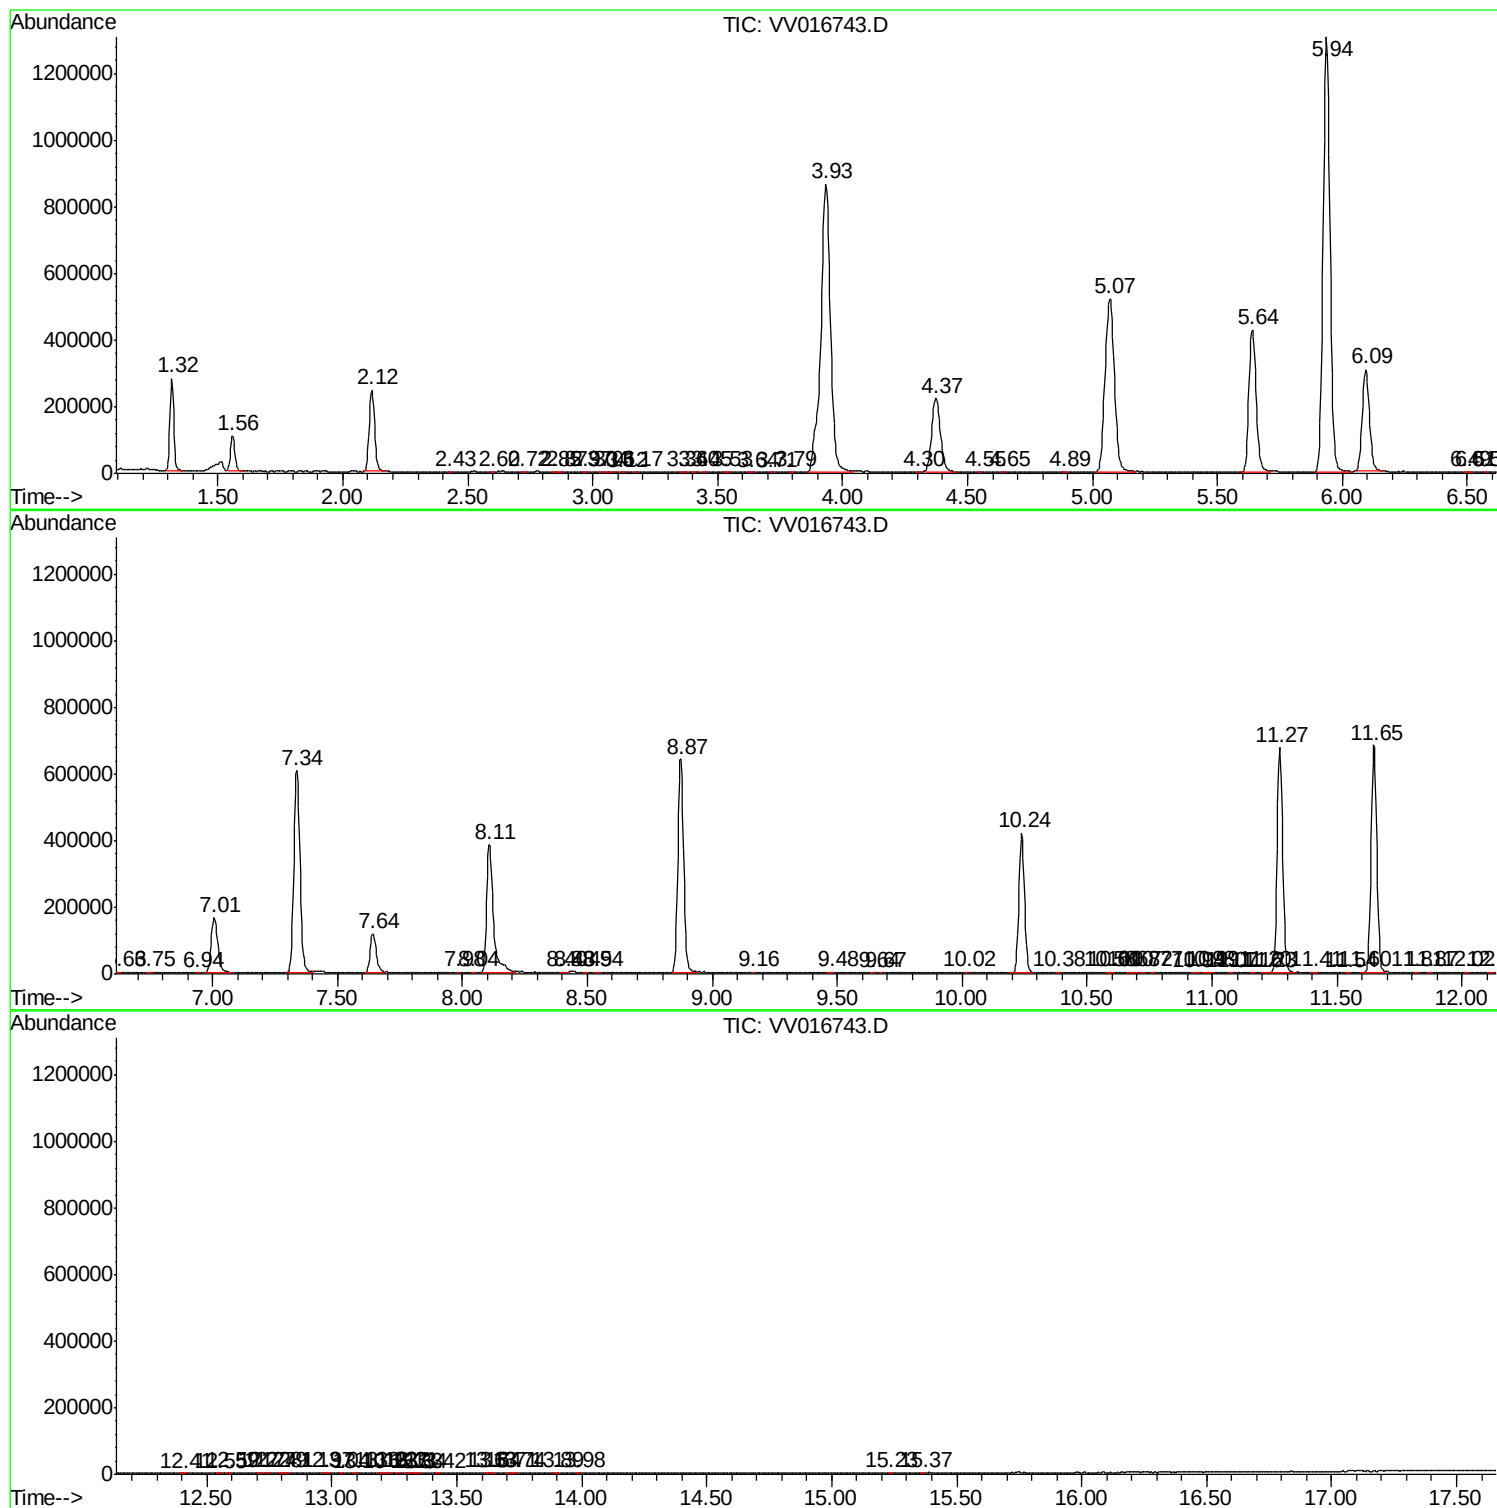

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016743.D
Acq On : 10 Jun 2020 01:33
Operator : SY/MD
Sample : L2901-07 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTT2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016743.D
Acq On : 10 Jun 2020 01:33
Operator : SY/MD
Sample : L2901-07 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTT2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc