

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016745.D
 Acq On : 10 Jun 2020 02:20
 Operator : SY/MD
 Sample : L2914-08 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E03

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M

Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	79	rVB	180787	185861	13.78%	1.732%
2	1.557	138	145	159	rVB	105321	132811	9.85%	1.237%
3	2.116	310	319	333	rVB	241522	350393	25.98%	3.264%
4	2.219	347	351	355	rBV6	2130	1797	0.13%	0.017%
5	2.293	372	374	378	rBV5	1662	1345	0.10%	0.013%
6	2.746	510	515	518	rBV7	1976	1734	0.13%	0.016%
7	2.865	548	552	554	rBV4	2154	1848	0.14%	0.017%
8	2.907	560	565	568	rBV5	1695	1763	0.13%	0.016%
9	3.100	623	625	628	rBV4	1308	758	0.06%	0.007%
10	3.216	658	661	664	rBV	6027	3502	0.26%	0.033%
11	3.431	726	728	729	rBV2	1799	681	0.05%	0.006%
12	3.524	751	757	761	rBV8	1546	1697	0.13%	0.016%
13	3.585	774	776	780	rBV4	1148	678	0.05%	0.006%
14	3.650	794	796	798	rVB4	1262	605	0.04%	0.006%
15	3.659	798	799	802	rBV3	1378	749	0.06%	0.007%
16	3.691	806	809	811	rBV3	973	675	0.05%	0.006%
17	3.720	814	818	820	rBV4	1116	1186	0.09%	0.011%
18	3.859	858	861	862	rBV3	1130	651	0.05%	0.006%
19	3.894	862	872	905	rVV	115801	330469	24.50%	3.079%
20	4.199	961	967	968	rBV4	1909	1600	0.12%	0.015%
21	4.373	1005	1021	1043	rBV	223663	542111	40.20%	5.050%
22	4.621	1096	1098	1102	rBV4	1354	849	0.06%	0.008%
23	4.868	1169	1175	1177	rBV6	1563	1539	0.11%	0.014%
24	5.007	1213	1218	1220	rBV4	1691	1446	0.11%	0.013%
25	5.068	1220	1237	1246	rBV2	529320	1348590	100.00%	12.564%
26	5.640	1402	1415	1438	rVV	447231	883457	65.51%	8.230%
27	6.093	1543	1556	1579	rBV	304672	617026	45.75%	5.748%
28	6.312	1623	1624	1628	rBV3	1258	673	0.05%	0.006%
29	6.367	1640	1641	1645	rBV4	1369	792	0.06%	0.007%
30	6.415	1654	1656	1660	rVB4	1165	789	0.06%	0.007%
31	6.453	1666	1668	1669	rBV2	1176	586	0.04%	0.005%
32	6.560	1697	1701	1702	rBV3	1382	1014	0.08%	0.009%
33	6.630	1719	1723	1726	rBV6	2193	2089	0.15%	0.019%
34	6.752	1759	1761	1764	rBV3	1788	1076	0.08%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016745.D
 Acq On : 10 Jun 2020 02:20
 Operator : SY/MD
 Sample : L2914-08 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E03

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.855	1791	1793	1794	rBV2	1530	722	0.05%	0.007%
36	6.891	1800	1804	1807	rVB5	1525	994	0.07%	0.009%
37	6.907	1807	1809	1812	rVB4	1257	617	0.05%	0.006%
38	6.952	1819	1823	1826	rBV6	1458	1067	0.08%	0.010%
39	6.968	1826	1828	1829	rBV2	1489	618	0.05%	0.006%
40	7.006	1829	1840	1858	rVV	165326	291358	21.60%	2.714%
41	7.267	1918	1921	1922	rBV2	2042	1014	0.08%	0.009%
42	7.338	1931	1943	1958	rBV	603914	1038476	77.00%	9.675%
43	7.640	2028	2037	2056	rBV	118934	197835	14.67%	1.843%
44	7.865	2103	2107	2110	rBV5	1329	1205	0.09%	0.011%
45	7.945	2129	2132	2133	rBV3	1441	898	0.07%	0.008%
46	8.106	2172	2182	2212	rVV	376852	721909	53.53%	6.725%
47	8.437	2283	2285	2287	rBV3	1505	647	0.05%	0.006%
48	8.482	2296	2299	2301	rBV4	1144	890	0.07%	0.008%
49	8.543	2315	2318	2320	rBV4	1071	634	0.05%	0.006%
50	8.556	2320	2322	2325	rVV4	1253	598	0.04%	0.006%
51	8.746	2379	2381	2383	rBV3	1653	814	0.06%	0.008%
52	8.762	2383	2386	2387	rVV3	1680	850	0.06%	0.008%
53	8.830	2403	2407	2408	rBV4	1723	1108	0.08%	0.010%
54	8.875	2409	2421	2447	rVV	659849	1096030	81.27%	10.211%
55	9.164	2495	2511	2526	rBV2	32933	66043	4.90%	0.615%
56	9.286	2541	2549	2557	rBV2	5828	9928	0.74%	0.092%
57	9.656	2662	2664	2667	rBV4	1514	698	0.05%	0.007%
58	9.727	2682	2686	2687	rBV4	1837	1471	0.11%	0.014%
59	9.926	2745	2748	2750	rBV3	1616	1043	0.08%	0.010%
60	10.042	2780	2784	2789	rBV7	1590	1640	0.12%	0.015%
61	10.106	2795	2804	2811	rVB7	5327	8410	0.62%	0.078%
62	10.238	2834	2845	2861	rVB	418014	650835	48.26%	6.063%
63	10.637	2965	2969	2973	rBV5	1929	1328	0.10%	0.012%
64	10.669	2975	2979	2981	rBV5	1597	1165	0.09%	0.011%
65	10.939	3056	3063	3072	rVB3	12378	17709	1.31%	0.165%
66	11.093	3107	3111	3113	rBV4	1517	1278	0.09%	0.012%
67	11.270	3153	3166	3183	rBV	700044	1062149	78.76%	9.895%
68	11.553	3248	3254	3266	rVB	6052	9788	0.73%	0.091%
69	11.646	3272	3283	3305	rVB	690881	1086649	80.58%	10.123%
70	11.752	3314	3316	3318	rBV3	1564	885	0.07%	0.008%
71	11.878	3351	3355	3360	rBV7	2130	2481	0.18%	0.023%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
Data File : VV016745.D
Acq On : 10 Jun 2020 02:20
Operator : SY/MD
Sample : L2914-08 50X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E03

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Title : VOC Analysis

72	11.923	3367	3369	3370	rBV2	1572	710	0.05%	0.007%
73	12.035	3401	3404	3408	rVB5	2032	1571	0.12%	0.015%
74	12.302	3484	3487	3490	rBV4	1196	953	0.07%	0.009%
75	12.672	3599	3602	3605	rBV3	2480	1265	0.09%	0.012%
76	12.691	3605	3608	3610	rBV3	1013	730	0.05%	0.007%
77	12.971	3690	3695	3696	rBV5	1363	1040	0.08%	0.010%
78	13.128	3741	3744	3749	rVB6	1622	900	0.07%	0.008%
79	13.238	3772	3778	3781	rBV7	2425	2302	0.17%	0.021%
80	13.350	3810	3813	3816	rBV4	1487	1463	0.11%	0.014%
81	13.386	3823	3824	3828	rVB4	1530	901	0.07%	0.008%
82	13.431	3833	3838	3839	rBV5	1460	822	0.06%	0.008%
83	13.495	3856	3858	3861	rBV4	1492	1064	0.08%	0.010%
84	13.707	3921	3924	3927	rBV4	968	781	0.06%	0.007%
85	13.726	3929	3930	3933	rBV2	1082	724	0.05%	0.007%
86	13.784	3946	3948	3952	rVB4	1610	706	0.05%	0.007%
87	13.894	3979	3982	3986	rVB4	992	935	0.07%	0.009%
88	14.048	4027	4030	4032	rBV5	1028	666	0.05%	0.006%
89	14.061	4032	4034	4037	rVV4	1285	602	0.04%	0.006%
90	14.116	4048	4051	4055	rBV5	1496	1094	0.08%	0.010%
91	14.170	4065	4068	4069	rBV3	1111	617	0.05%	0.006%
92	14.386	4133	4135	4142	rVB7	1643	1327	0.10%	0.012%
93	14.415	4142	4144	4148	rVB4	1216	646	0.05%	0.006%
94	14.492	4165	4168	4171	rVB5	2016	1253	0.09%	0.012%
95	14.604	4199	4203	4206	rBV5	2024	1628	0.12%	0.015%
96	14.624	4206	4209	4212	rBV3	1495	948	0.07%	0.009%
97	14.669	4219	4223	4225	rBV5	1392	1295	0.10%	0.012%
98	15.077	4348	4350	4352	rBV3	1157	678	0.05%	0.006%
99	15.363	4435	4439	4440	rBV3	1631	1178	0.09%	0.011%
100	15.495	4478	4480	4483	rBV4	999	585	0.04%	0.005%


Sum of corrected areas: 10734008

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060920\
Data File : VV016745.D
Acq On : 10 Jun 2020 02:20
Operator : SY/MD
Sample : L2914-08 50X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E03

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

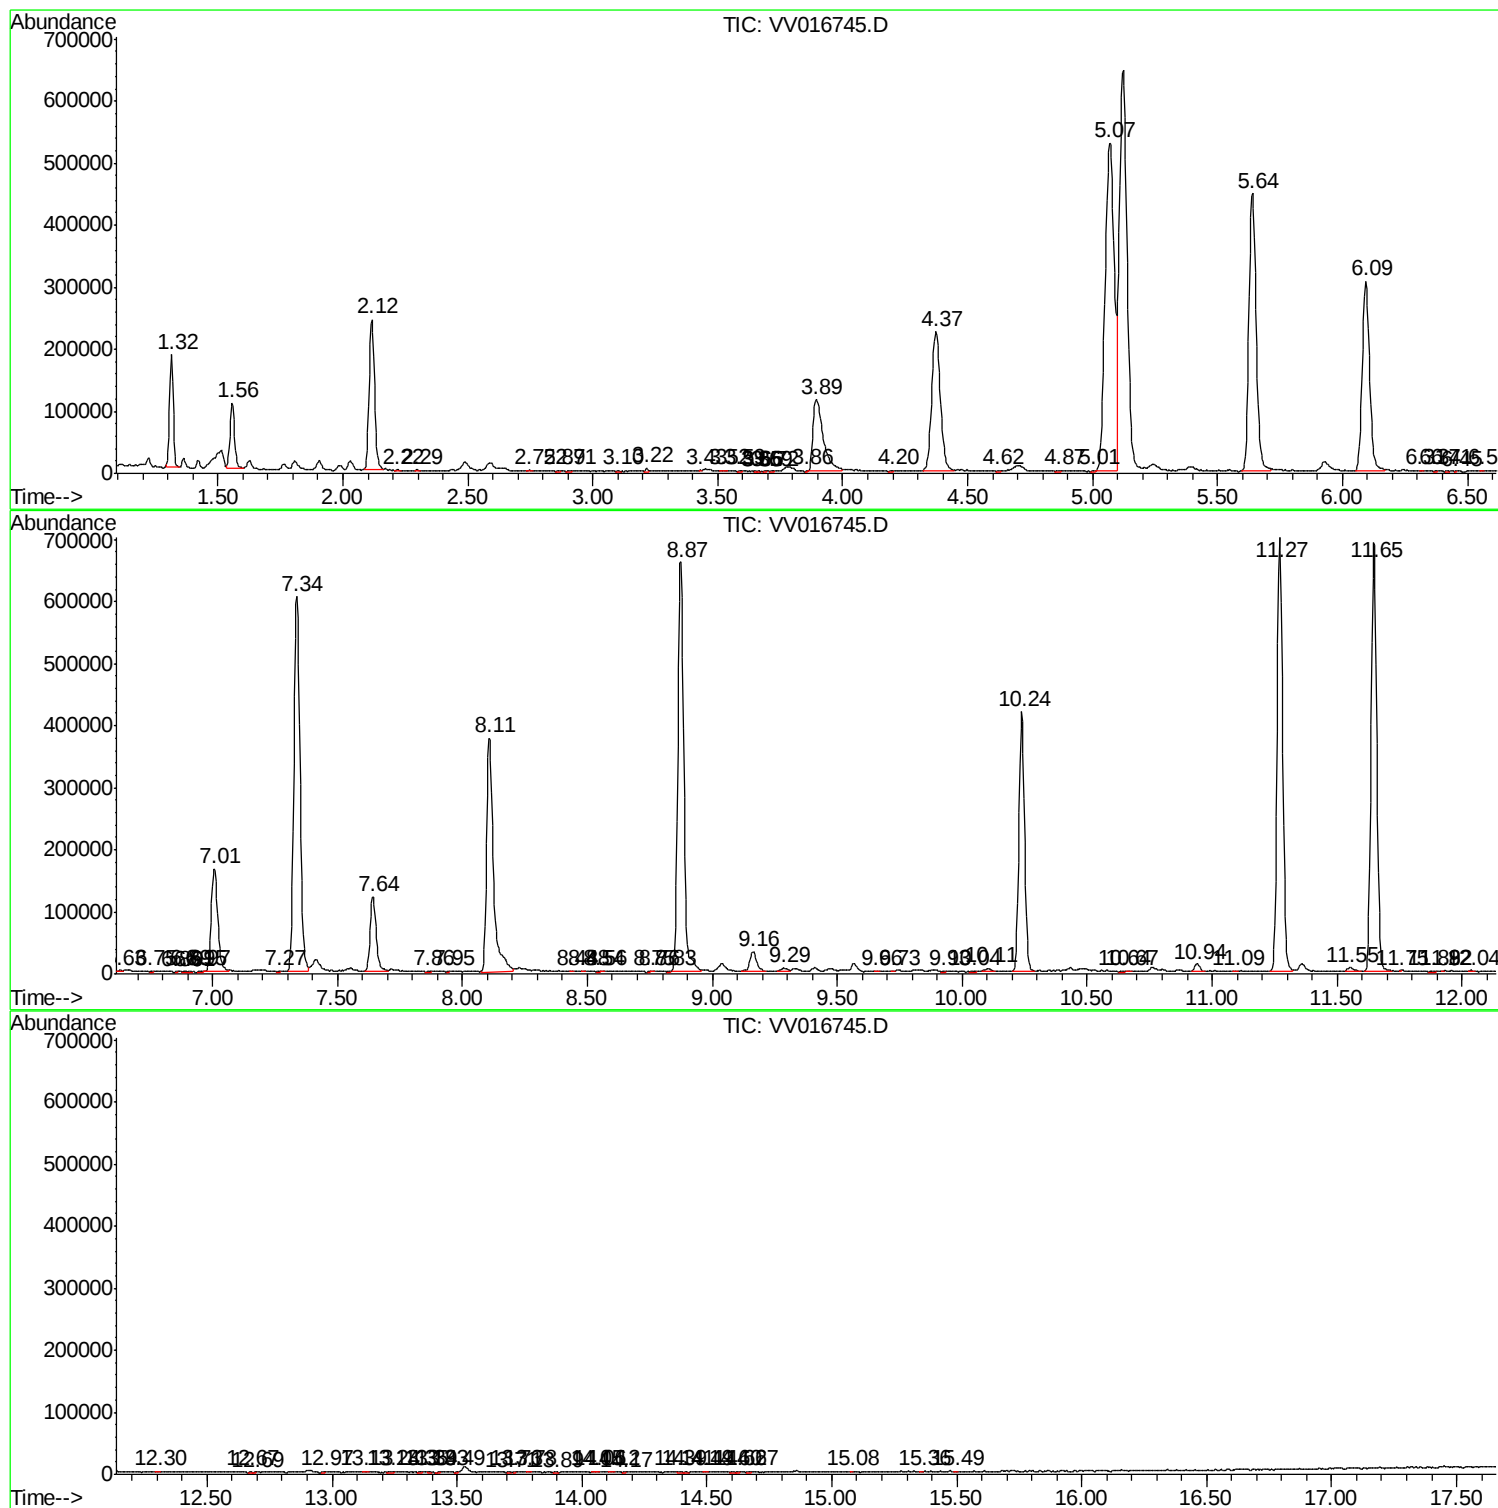

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016745.D
Acq On : 10 Jun 2020 02:20
Operator : SY/MD
Sample : L2914-08 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E03

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016745.D
Acq On : 10 Jun 2020 02:20
Operator : SY/MD
Sample : L2914-08 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E03

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
