

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016747.D
 Acq On : 10 Jun 2020 03:55
 Operator : SY/MD
 Sample : VV0609WBL03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK77

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	83	rVB	154839	158600	11.22%	1.480%
2	1.560	139	146	158	rVB	113644	137472	9.72%	1.283%
3	2.116	310	319	339	rVB	259010	382207	27.03%	3.566%
4	2.733	509	511	515	rBV3	1482	1152	0.08%	0.011%
5	2.907	559	565	567	rBV7	1782	1564	0.11%	0.015%
6	2.962	579	582	584	rBV4	1226	609	0.04%	0.006%
7	2.987	588	590	592	rBV3	881	346	0.02%	0.003%
8	3.048	605	609	612	rBV4	1998	1542	0.11%	0.014%
9	3.119	629	631	636	rVB5	1650	1218	0.09%	0.011%
10	3.145	636	639	641	rBV4	1731	1182	0.08%	0.011%
11	3.216	658	661	664	rVB4	1320	928	0.07%	0.009%
12	3.232	664	666	667	rBV2	1521	717	0.05%	0.007%
13	3.370	707	709	711	rBV3	985	460	0.03%	0.004%
14	3.415	721	723	728	rBV4	1293	892	0.06%	0.008%
15	3.457	733	736	738	rBV3	2085	1363	0.10%	0.013%
16	3.482	742	744	746	rBV3	891	474	0.03%	0.004%
17	3.499	746	749	751	rBV4	1075	653	0.05%	0.006%
18	3.592	775	778	780	rBV5	1036	593	0.04%	0.006%
19	3.621	784	787	788	rBV4	1073	588	0.04%	0.005%
20	3.669	798	802	804	rBV5	1527	1185	0.08%	0.011%
21	3.759	828	830	836	rVB6	1850	1191	0.08%	0.011%
22	3.810	843	846	847	rBV3	874	468	0.03%	0.004%
23	3.839	853	855	859	rBV4	902	619	0.04%	0.006%
24	3.894	859	872	903	rBV	120401	331649	23.46%	3.094%
25	4.187	961	963	965	rBV2	1676	823	0.06%	0.008%
26	4.251	981	983	987	rBV3	1644	1011	0.07%	0.009%
27	4.273	987	990	993	rVV5	1598	1328	0.09%	0.012%
28	4.373	1006	1021	1046	rBV	233509	563781	39.88%	5.260%
29	4.785	1145	1149	1152	rBV5	1941	1962	0.14%	0.018%
30	4.952	1199	1201	1204	rVB4	1407	679	0.05%	0.006%
31	5.068	1221	1237	1265	rBV2	548038	1413794	100.00%	13.191%
32	5.405	1339	1342	1343	rBV3	1259	743	0.05%	0.007%
33	5.457	1355	1358	1360	rBV4	1754	853	0.06%	0.008%
34	5.473	1360	1363	1364	rBV3	1330	640	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016747.D
 Acq On : 10 Jun 2020 03:55
 Operator : SY/MD
 Sample : VV0609WBL03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK77

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	5.640	1403	1415	1441	rBV	415261	824271	58.30%	7.691%
36	6.093	1541	1556	1581	rBV	320771	660018	46.68%	6.158%
37	6.392	1647	1649	1652	rBV4	916	468	0.03%	0.004%
38	6.434	1660	1662	1664	rBV4	883	337	0.02%	0.003%
39	6.576	1704	1706	1710	rBV5	1299	959	0.07%	0.009%
40	6.797	1774	1775	1777	rBV2	1206	601	0.04%	0.006%
41	6.897	1804	1806	1810	rVB5	2073	1052	0.07%	0.010%
42	6.916	1810	1812	1813	rBV2	910	386	0.03%	0.004%
43	7.006	1829	1840	1855	rBV2	168564	300572	21.26%	2.804%
44	7.338	1931	1943	1960	rBV	632248	1088738	77.01%	10.158%
45	7.643	2027	2038	2051	rBV	121061	209017	14.78%	1.950%
46	7.868	2104	2108	2111	rBV4	1870	1886	0.13%	0.018%
47	7.936	2127	2129	2136	rBV7	1276	1234	0.09%	0.012%
48	8.106	2172	2182	2213	rBV	405033	764049	54.04%	7.129%
49	8.875	2409	2421	2445	rBV	631583	1011810	71.57%	9.441%
50	9.273	2543	2545	2550	rBV4	1675	1243	0.09%	0.012%
51	9.338	2558	2565	2566	rBV6	1724	1744	0.12%	0.016%
52	9.547	2628	2630	2631	rBV	1047	368	0.03%	0.003%
53	9.675	2669	2670	2671	rBV	1038	344	0.02%	0.003%
54	9.704	2676	2679	2680	rBV2	1131	611	0.04%	0.006%
55	9.829	2716	2718	2724	rVB5	1186	766	0.05%	0.007%
56	9.862	2724	2728	2733	rVB7	2232	1891	0.13%	0.018%
57	9.891	2733	2737	2738	rBV4	882	642	0.05%	0.006%
58	9.920	2745	2746	2748	rBV2	1044	387	0.03%	0.004%
59	9.993	2767	2769	2771	rBV2	888	449	0.03%	0.004%
60	10.006	2771	2773	2776	rBV4	1721	1049	0.07%	0.010%
61	10.125	2808	2810	2813	rBV3	1223	845	0.06%	0.008%
62	10.177	2823	2826	2829	rBV4	1778	1209	0.09%	0.011%
63	10.238	2833	2845	2863	rVV	437177	682381	48.27%	6.367%
64	10.318	2868	2870	2874	rVB4	745	497	0.04%	0.005%
65	10.460	2912	2914	2915	rBV2	1220	593	0.04%	0.006%
66	10.476	2918	2919	2920	rBV	1100	376	0.03%	0.004%
67	10.820	3023	3026	3028	rBV4	1472	1079	0.08%	0.010%
68	10.919	3052	3057	3058	rBV5	1117	868	0.06%	0.008%
69	11.074	3102	3105	3109	rBV5	870	870	0.06%	0.008%
70	11.186	3136	3140	3141	rBV3	2285	1534	0.11%	0.014%
71	11.270	3155	3166	3183	rBV	646296	986632	69.79%	9.206%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016747.D
 Acq On : 10 Jun 2020 03:55
 Operator : SY/MD
 Sample : VV0609WBL03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK77

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.521	3242	3244	3247	rBV4	1107	518	0.04%	0.005%
73	11.572	3257	3260	3262	rBV4	1019	685	0.05%	0.006%
74	11.649	3272	3284	3300	rVB	710063	1119371	79.17%	10.444%
75	11.884	3355	3357	3358	rBV	1020	474	0.03%	0.004%
76	12.029	3401	3402	3405	rVB3	950	474	0.03%	0.004%
77	12.051	3405	3409	3410	rBV4	1068	817	0.06%	0.008%
78	12.543	3560	3562	3564	rBV2	1086	357	0.03%	0.003%
79	12.755	3625	3628	3629	rBV3	745	337	0.02%	0.003%
80	12.768	3629	3632	3634	rBV3	858	519	0.04%	0.005%
81	12.823	3647	3649	3653	rBV3	1147	649	0.05%	0.006%
82	12.868	3661	3663	3664	rBV2	1242	512	0.04%	0.005%
83	12.900	3670	3673	3678	rBV6	2811	2716	0.19%	0.025%
84	12.980	3694	3698	3700	rBV4	1758	1164	0.08%	0.011%
85	13.058	3717	3722	3725	rBV7	1865	1918	0.14%	0.018%
86	13.202	3764	3767	3769	rVB4	1275	579	0.04%	0.005%
87	13.218	3771	3772	3776	rVV4	1150	667	0.05%	0.006%
88	13.296	3789	3796	3802	rBV4	3929	6320	0.45%	0.059%
89	13.334	3805	3808	3812	rBV5	2119	1419	0.10%	0.013%
90	13.398	3827	3828	3831	rBV3	807	544	0.04%	0.005%
91	13.974	4005	4007	4009	rBV3	1096	461	0.03%	0.004%
92	14.058	4030	4033	4037	rBV4	2511	2076	0.15%	0.019%
93	14.090	4042	4043	4046	rBV3	941	558	0.04%	0.005%
94	14.456	4155	4157	4160	rBV3	1529	1106	0.08%	0.010%
95	14.646	4215	4216	4218	rBV2	1027	447	0.03%	0.004%
96	14.855	4278	4281	4283	rBV4	2478	1502	0.11%	0.014%
97	15.045	4338	4340	4341	rBV	1310	492	0.03%	0.005%
98	15.115	4356	4362	4366	rBV7	2926	3189	0.23%	0.030%
99	15.260	4405	4407	4409	rBV3	1496	656	0.05%	0.006%
100	15.431	4458	4460	4466	rBV7	2181	1955	0.14%	0.018%


Sum of corrected areas: 10717544

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060920\
Data File : VV016747.D
Acq On : 10 Jun 2020 03:55
Operator : SY/MD
Sample : VV0609WBL03
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK77

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

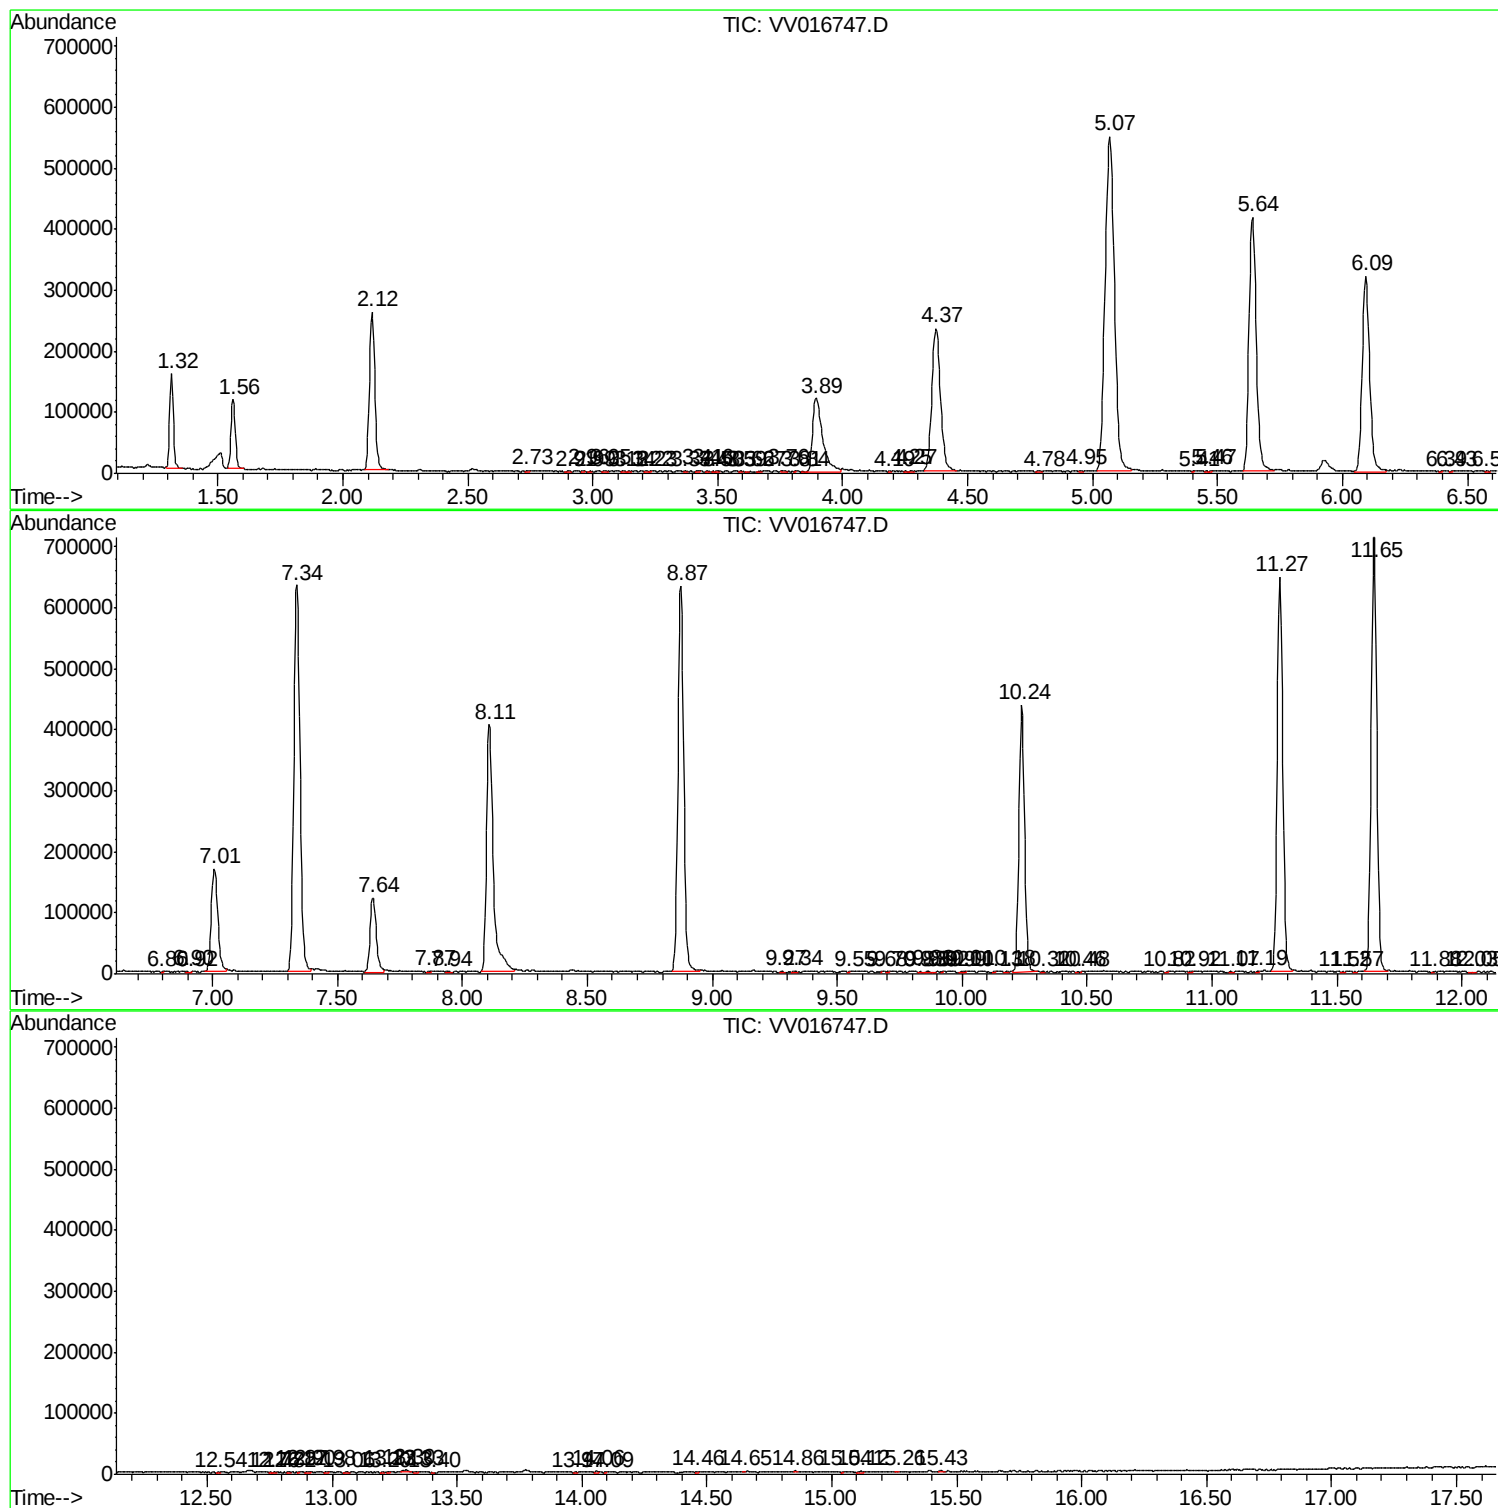

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016747.D
Acq On : 10 Jun 2020 03:55
Operator : SY/MD
Sample : VV0609WBL03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK77

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV060920\
Data File : VV016747.D
Acq On : 10 Jun 2020 03:55
Operator : SY/MD
Sample : VV0609WBL03
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VBLK77

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc