

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016751.D
 Acq On : 10 Jun 2020 05:30
 Operator : SY/MD
 Sample : L2914-12 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E15

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	62	70	79	rVB2	205134	222402	19.09%	1.847%
2	1.364	80	85	91	rVB	30404	27947	2.40%	0.232%
3	1.421	99	103	110	rVB	25715	21982	1.89%	0.183%
4	1.557	140	145	156	rVB	114514	138113	11.85%	1.147%
5	2.116	309	319	333	rBV	247265	368973	31.66%	3.064%
6	2.415	408	412	413	rBV4	1652	1050	0.09%	0.009%
7	2.740	510	513	514	rBV2	2078	1215	0.10%	0.010%
8	2.801	531	532	533	rBV	955	294	0.03%	0.002%
9	2.862	548	551	553	rBV3	2073	1350	0.12%	0.011%
10	2.881	555	557	558	rBV2	921	368	0.03%	0.003%
11	2.946	573	577	579	rBV5	1835	1670	0.14%	0.014%
12	2.994	591	592	596	rVB4	1156	432	0.04%	0.004%
13	3.013	596	598	600	rBV3	718	361	0.03%	0.003%
14	3.122	630	632	633	rBV2	724	320	0.03%	0.003%
15	3.788	823	839	852	rBV6	10717	30281	2.60%	0.251%
16	3.894	862	872	898	rBV	117197	312348	26.80%	2.594%
17	4.373	1007	1021	1043	rVB	224310	535224	45.93%	4.444%
18	4.659	1108	1110	1112	rBV2	1811	1112	0.10%	0.009%
19	4.962	1199	1204	1205	rBV4	1323	1093	0.09%	0.009%
20	5.010	1212	1219	1220	rBV6	1681	1740	0.15%	0.014%
21	5.071	1220	1238	1242	rBV3	539994	1165299	100.00%	9.677%
22	5.640	1402	1415	1434	rBV	434689	863686	74.12%	7.172%
23	5.884	1488	1491	1492	rBV3	1042	555	0.05%	0.005%
24	6.093	1544	1556	1580	rBV	302004	606941	52.08%	5.040%
25	6.547	1694	1697	1700	rBV5	1334	1103	0.09%	0.009%
26	7.006	1829	1840	1856	rBV	165523	290499	24.93%	2.412%
27	7.338	1931	1943	1955	rBV	612377	1049461	90.06%	8.715%
28	7.408	1956	1965	1984	rVB	504424	844487	72.47%	7.013%
29	7.640	2028	2037	2053	rBV	118909	201577	17.30%	1.674%
30	7.929	2125	2127	2129	rBV3	982	415	0.04%	0.003%
31	7.977	2138	2142	2144	rBV5	1662	1148	0.10%	0.010%
32	8.032	2156	2159	2162	rVB5	1904	1299	0.11%	0.011%
33	8.055	2162	2166	2169	rBV5	2016	1800	0.15%	0.015%
34	8.106	2172	2182	2217	rVV	385102	730676	62.70%	6.067%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016751.D
 Acq On : 10 Jun 2020 05:30
 Operator : SY/MD
 Sample : L2914-12 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E15

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	8.466	2292	2294	2299	rBV4	1076	945	0.08%	0.008%
36	8.621	2340	2342	2345	rVB4	1183	531	0.05%	0.004%
37	8.701	2365	2367	2368	rBV2	1046	431	0.04%	0.004%
38	8.736	2376	2378	2379	rBV2	961	347	0.03%	0.003%
39	8.875	2409	2421	2433	rBV	648983	1060833	91.04%	8.809%
40	9.032	2460	2470	2487	rBV	307179	482680	41.42%	4.008%
41	9.566	2629	2636	2651	rVB2	42032	71412	6.13%	0.593%
42	9.739	2681	2690	2691	rBV9	3449	4318	0.37%	0.036%
43	9.958	2750	2758	2765	rVB6	5917	9380	0.80%	0.078%
44	10.006	2771	2773	2777	rVB5	1636	757	0.06%	0.006%
45	10.106	2797	2804	2816	rVB5	6558	12581	1.08%	0.104%
46	10.238	2834	2845	2860	rBV	435827	680358	58.38%	5.650%
47	10.325	2869	2872	2873	rBV2	1430	786	0.07%	0.007%
48	10.620	2962	2964	2965	rBV2	1557	678	0.06%	0.006%
49	10.762	3001	3008	3013	rBV2	11288	17086	1.47%	0.142%
50	10.939	3055	3063	3073	rVB3	15804	28797	2.47%	0.239%
51	11.270	3155	3166	3185	rVB	684475	1053470	90.40%	8.748%
52	11.550	3242	3253	3264	rBV6	9643	20411	1.75%	0.169%
53	11.646	3272	3283	3304	rVB	704405	1104612	94.79%	9.173%
54	11.768	3316	3321	3322	rBV4	3595	3059	0.26%	0.025%
55	11.942	3372	3375	3380	rBV7	1375	1561	0.13%	0.013%
56	12.193	3449	3453	3454	rBV4	1141	578	0.05%	0.005%
57	12.260	3471	3474	3475	rBV2	1644	883	0.08%	0.007%
58	12.315	3488	3491	3492	rBV3	1030	571	0.05%	0.005%
59	12.431	3523	3527	3528	rBV3	1906	1511	0.13%	0.013%
60	12.563	3566	3568	3573	rVB6	2090	1396	0.12%	0.012%
61	12.585	3573	3575	3577	rBV3	924	479	0.04%	0.004%
62	12.627	3585	3588	3590	rBV3	2045	1110	0.10%	0.009%
63	12.746	3620	3625	3627	rBV3	1710	1713	0.15%	0.014%
64	12.826	3648	3650	3652	rBV3	1146	700	0.06%	0.006%
65	12.910	3669	3676	3682	rBV3	4337	6050	0.52%	0.050%
66	13.074	3721	3727	3729	rBV6	2379	2215	0.19%	0.018%
67	13.135	3744	3746	3748	rVB3	843	277	0.02%	0.002%
68	13.386	3820	3824	3826	rBV3	1159	961	0.08%	0.008%
69	13.530	3860	3869	3878	rBV	12443	21817	1.87%	0.181%
70	13.653	3900	3907	3908	rBV5	3327	3487	0.30%	0.029%
71	13.762	3938	3941	3944	rBV5	1340	988	0.08%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016751.D
 Acq On : 10 Jun 2020 05:30
 Operator : SY/MD
 Sample : L2914-12 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E15

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	13.842	3963	3966	3970	rBV4	815	644	0.06%	0.005%
73	14.016	4017	4020	4023	rVB4	1434	899	0.08%	0.007%
74	14.051	4028	4031	4033	rBV4	1810	1130	0.10%	0.009%
75	14.119	4050	4052	4054	rBV3	1336	676	0.06%	0.006%
76	14.222	4082	4084	4085	rBV2	952	350	0.03%	0.003%
77	14.334	4116	4119	4120	rBV2	1409	623	0.05%	0.005%
78	14.415	4141	4144	4146	rBV4	1402	1066	0.09%	0.009%
79	14.460	4151	4158	4161	rBV6	1988	2323	0.20%	0.019%
80	14.476	4161	4163	4165	rBV3	1278	712	0.06%	0.006%
81	14.498	4169	4170	4173	rBV3	1549	634	0.05%	0.005%
82	14.556	4184	4188	4190	rBV4	1969	1109	0.10%	0.009%
83	15.106	4357	4359	4362	rBV4	1345	888	0.08%	0.007%
84	15.331	4426	4429	4430	rBV3	1376	783	0.07%	0.007%
85	15.366	4437	4440	4444	rBV5	1511	1260	0.11%	0.010%
86	15.437	4460	4462	4464	rBV2	1476	648	0.06%	0.005%
87	15.485	4473	4477	4481	rBV5	1879	1735	0.15%	0.014%


Sum of corrected areas: 12042470

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060920\
Data File : VV016751.D
Acq On : 10 Jun 2020 05:30
Operator : SY/MD
Sample : L2914-12 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 58 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E15

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

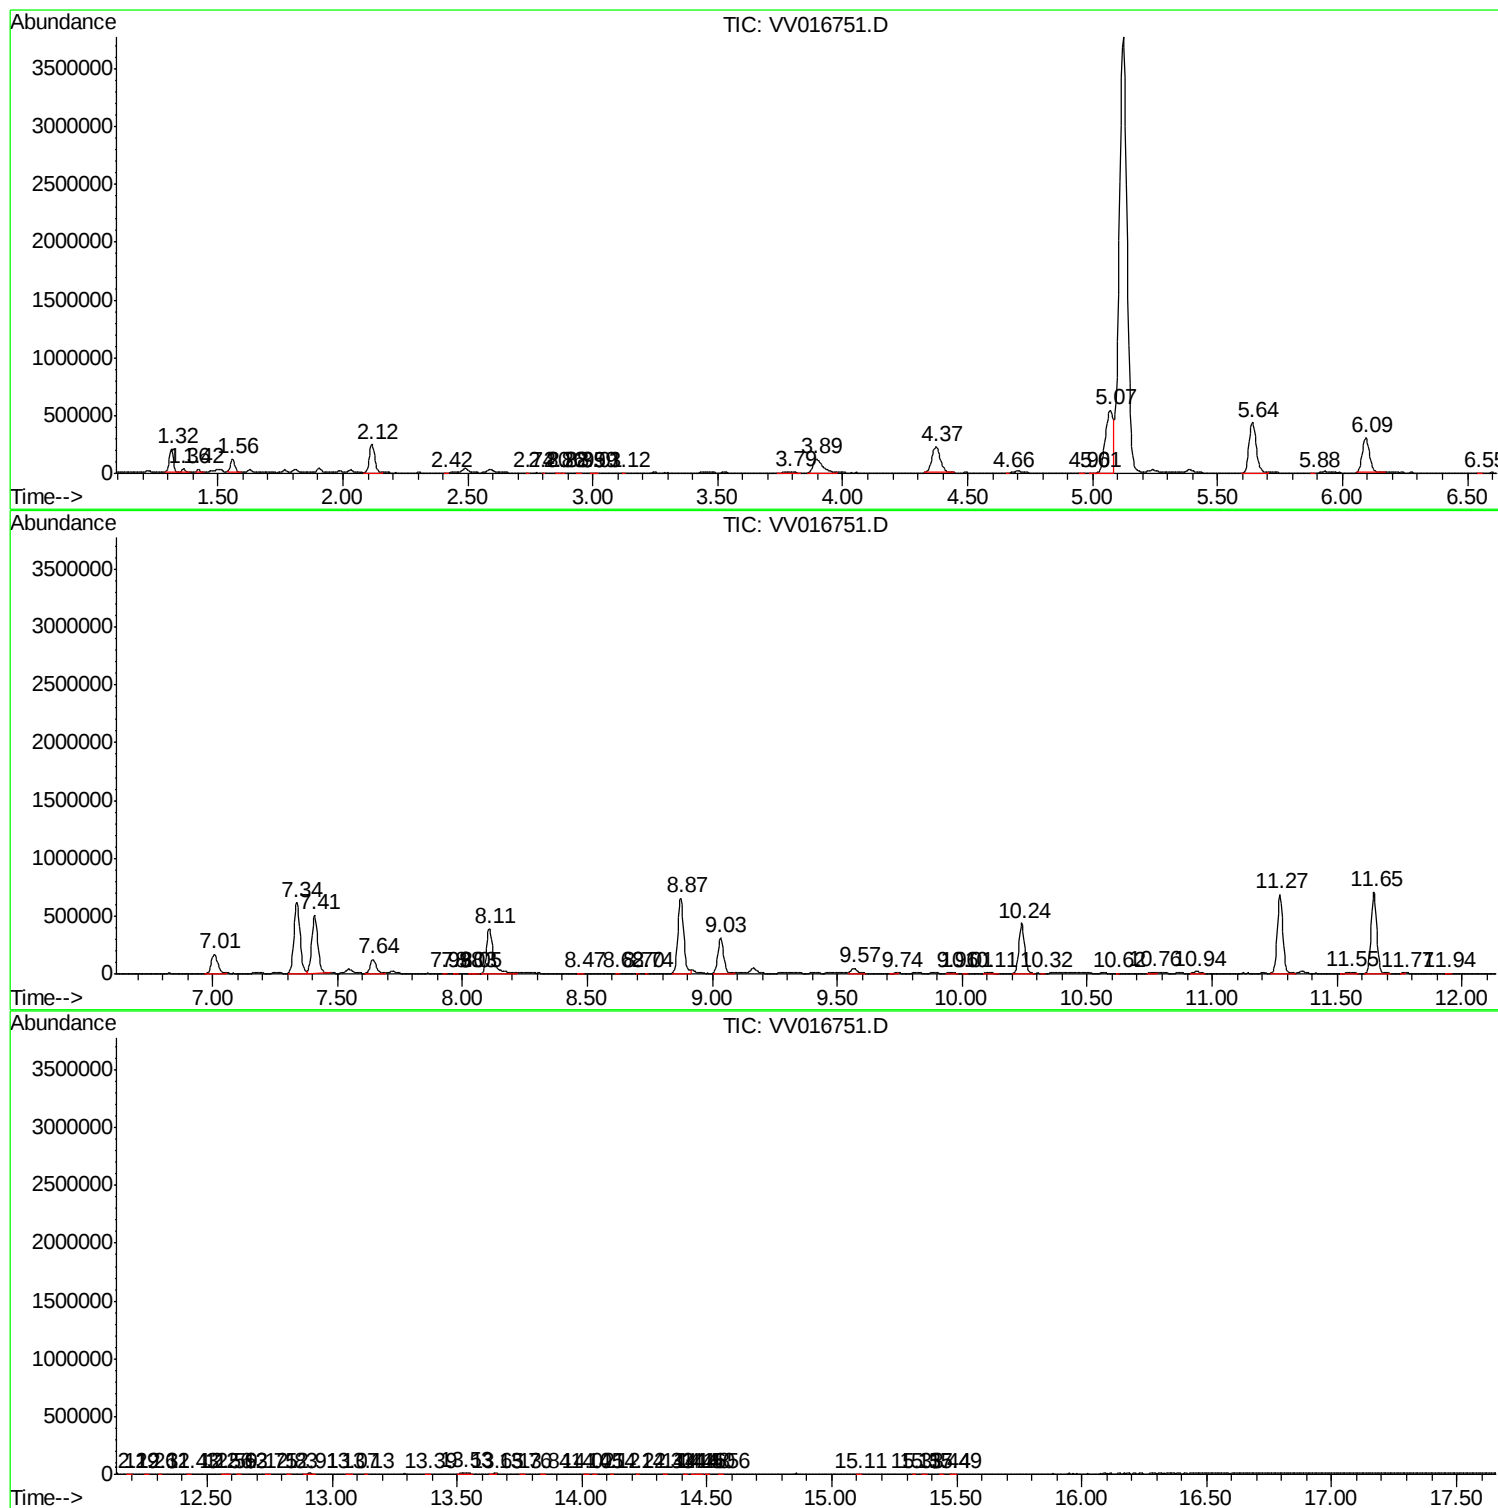

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016751.D
Acq On : 10 Jun 2020 05:30
Operator : SY/MD
Sample : L2914-12 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 58 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E15

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016751.D
Acq On : 10 Jun 2020 05:30
Operator : SY/MD
Sample : L2914-12 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 58 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E15

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc